

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041822\
 Data File : PP046269.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Apr 2022 02:47
 Operator : YP\AJ
 Sample : N2452-01
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 WC-15-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/19/2022
 Supervised By :mohammad ahmed 04/19/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 19 05:04:46 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP041222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 12 05:31:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.874	3.142	26537209	22690046	10.789	14.280m#
2) SA Decachlor...	9.995f	8.500f	25391625	21450376	15.468	15.050m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041822\
Data File : PP046269.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Apr 2022 02:47
Operator : YP\AJ
Sample : N2452-01
Misc :
ALS Vial : 38 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
WC-15-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/19/2022
Supervised By :mohammad ahmed 04/19/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 19 05:04:46 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP041222.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 12 05:31:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

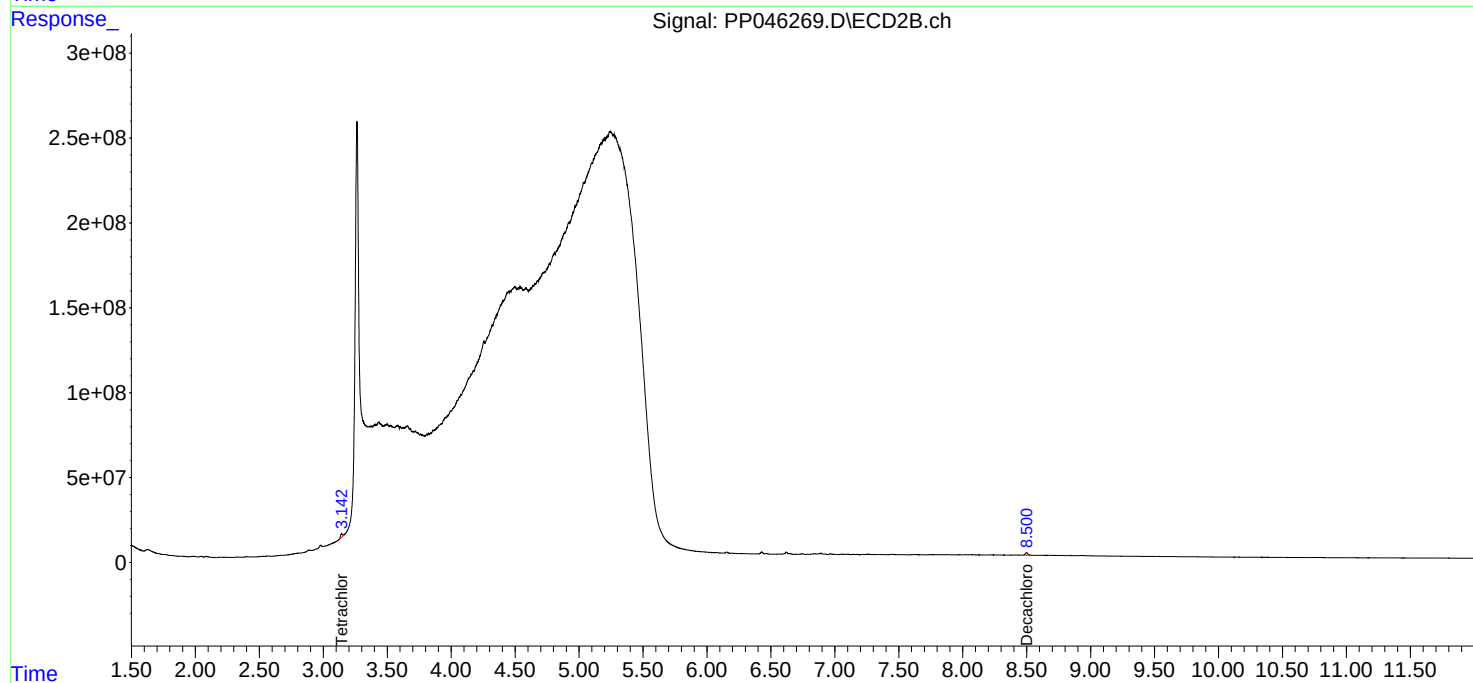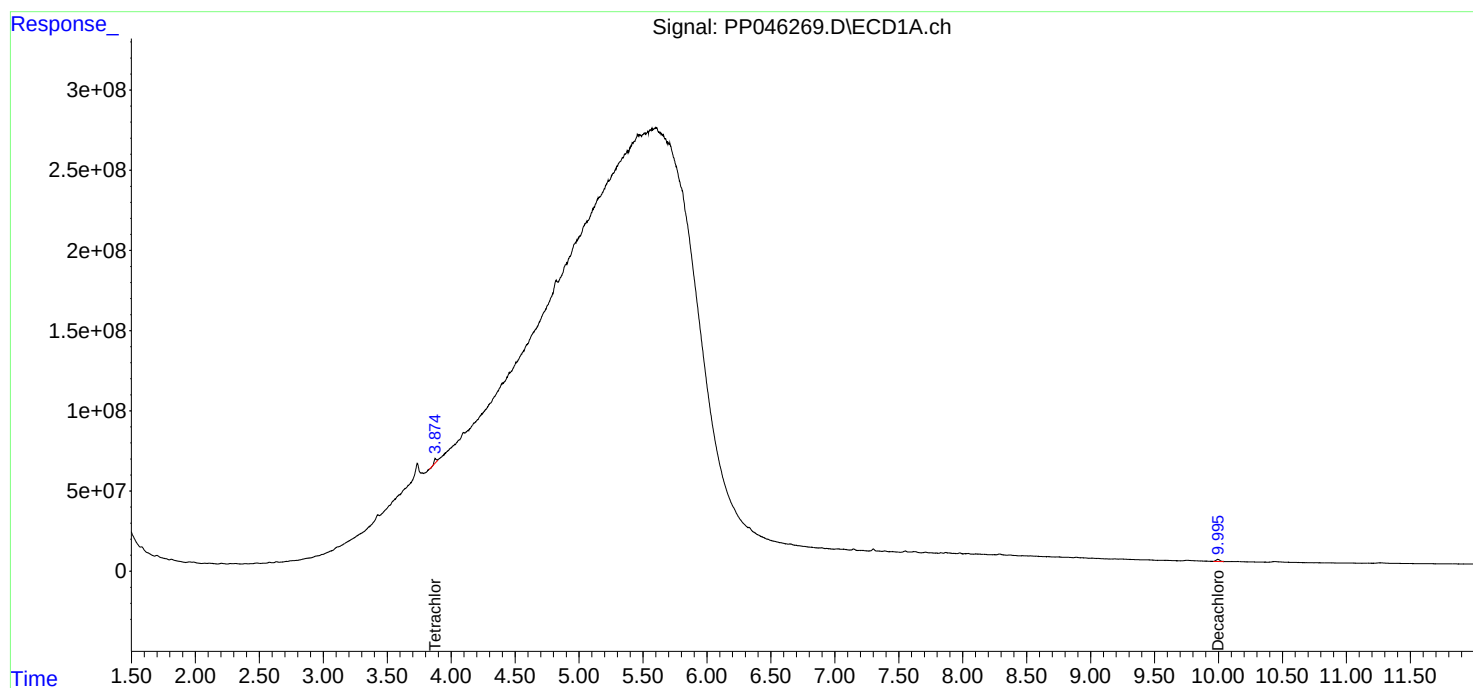

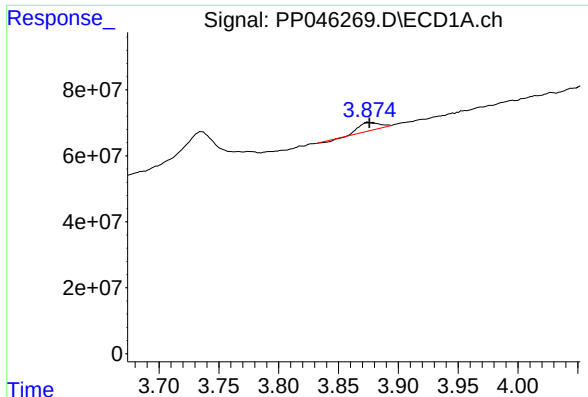


#1 Tetrachloro-m-xylene

R.T.: 3.874 min
Delta R.T.: -0.002 min
Response: 26537209
Conc: 10.79 ng/ml

Instrument :
ECD_P
ClientSampleId :
WC-15-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/19/2022
Supervised By :mohammad ahmed 04/19/2022

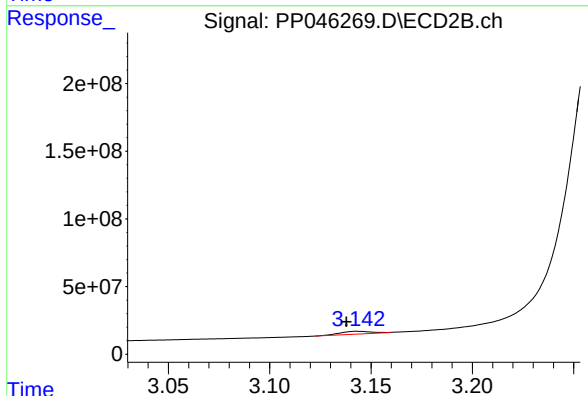


#1 Tetrachloro-m-xylene

R.T.: 3.142 min
Delta R.T.: 0.005 min
Response: 22690046
Conc: 14.28 ng/ml m

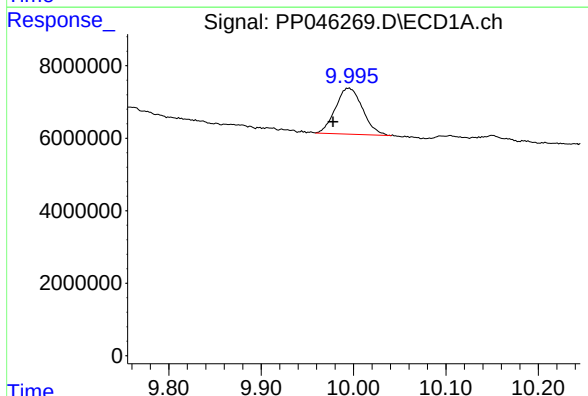

#2 Decachlorobiphenyl

R.T.: 9.995 min
Delta R.T.: 0.017 min
Response: 25391625
Conc: 15.47 ng/ml

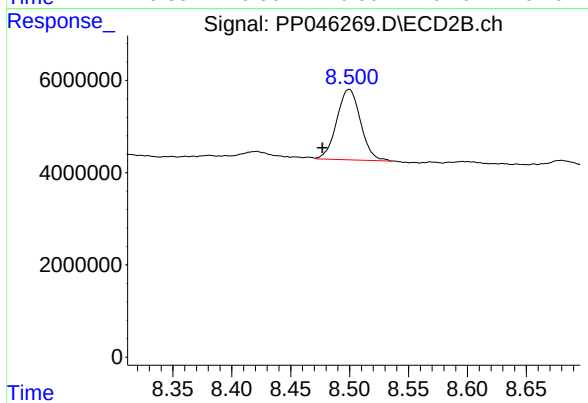

#2 Decachlorobiphenyl

R.T.: 8.500 min
Delta R.T.: 0.023 min
Response: 21450376
Conc: 15.05 ng/ml m