

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041825\
 Data File : PP071365.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Apr 2025 11:43
 Operator : YP\AJ
 Sample : Q1794-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 40325-A-B-COMP

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/18/2025
 Supervised By :mohammad ahmed 04/23/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 18 13:09:04 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032725.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 28 03:13:46 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.514	3.812	12649058	7725395	8.654m	7.452
2) SA Decachlor...	10.233	8.848	21331078	11717738	20.265	14.867 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041825\
Data File : PP071365.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Apr 2025 11:43
Operator : YP\AJ
Sample : Q1794-04
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
40325-A-B-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/18/2025
Supervised By :mohammad ahmed 04/23/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 18 13:09:04 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032725.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 28 03:13:46 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

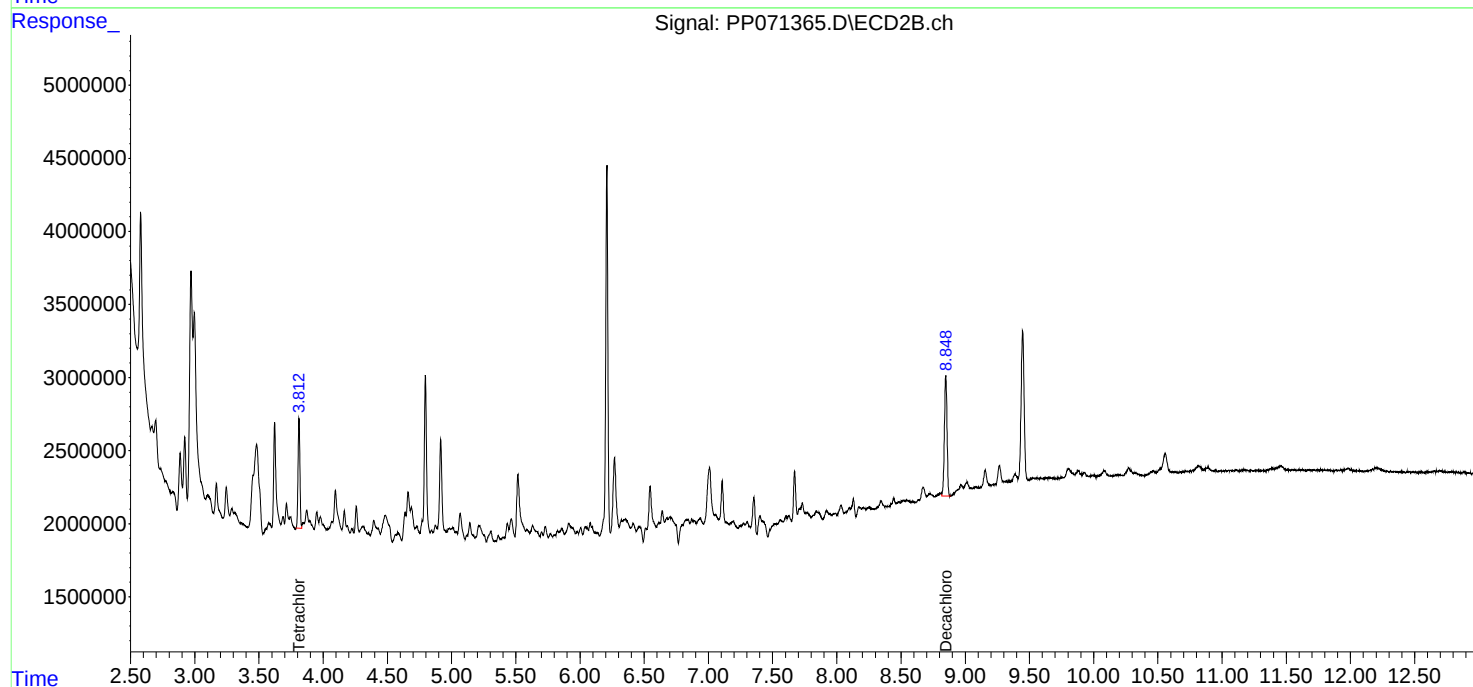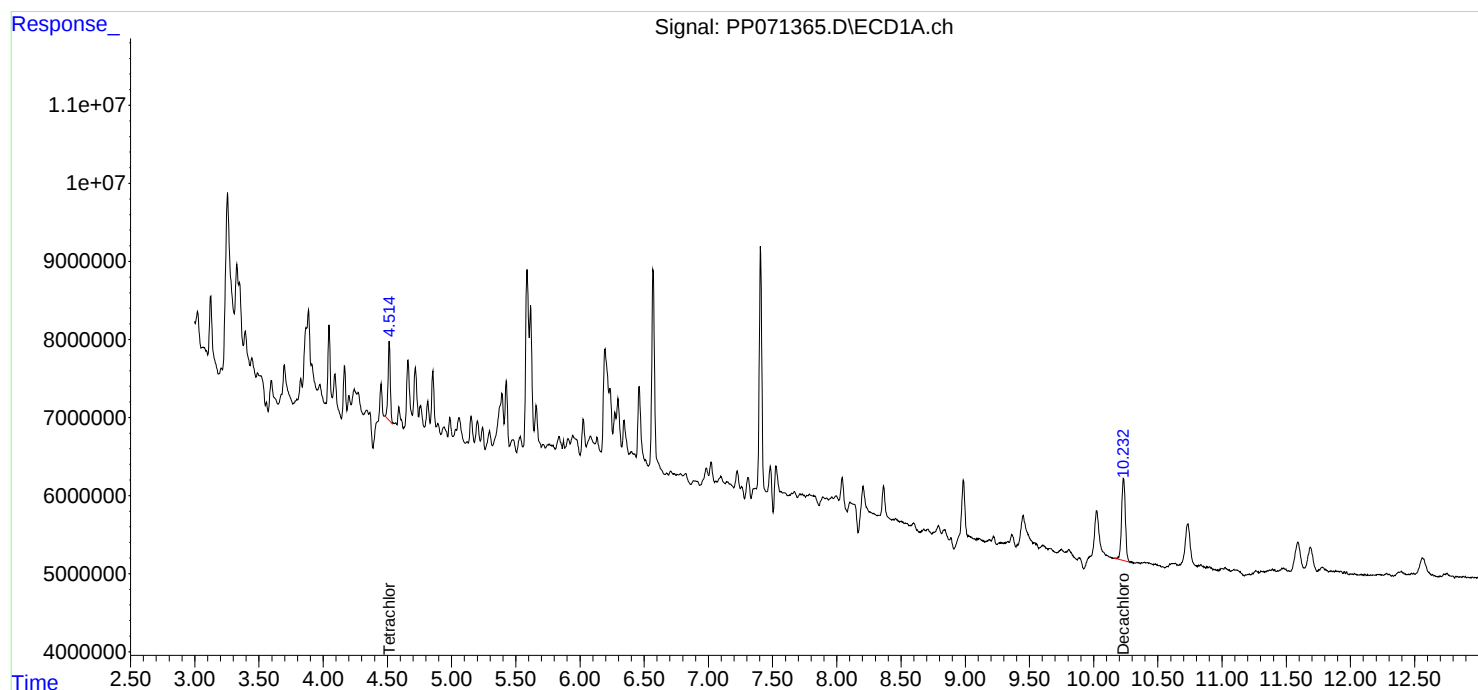

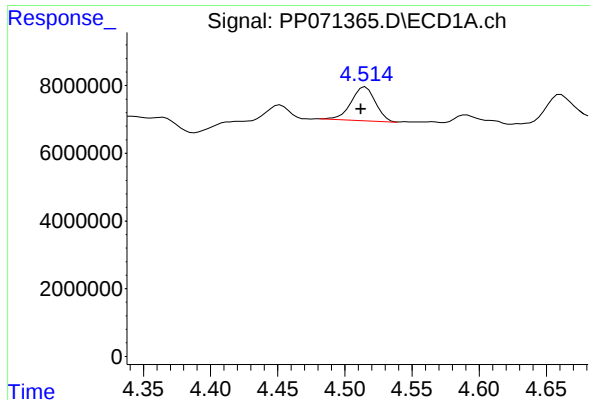


#1 Tetrachloro-m-xylene

R.T.: 4.514 min
Delta R.T.: 0.002 min
Response: 12649058
Conc: 8.65 ng/ml

Instrument :
ECD_P
ClientSampleId :
40325-A-B-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/18/2025
Supervised By :mohammad ahmed 04/23/2025

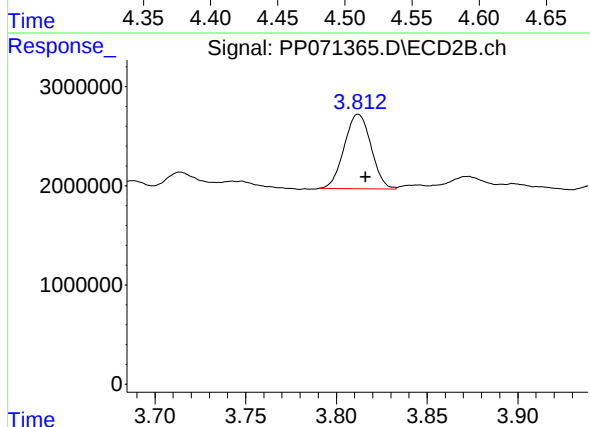


#1 Tetrachloro-m-xylene

R.T.: 3.812 min
Delta R.T.: -0.004 min
Response: 7725395
Conc: 7.45 ng/ml

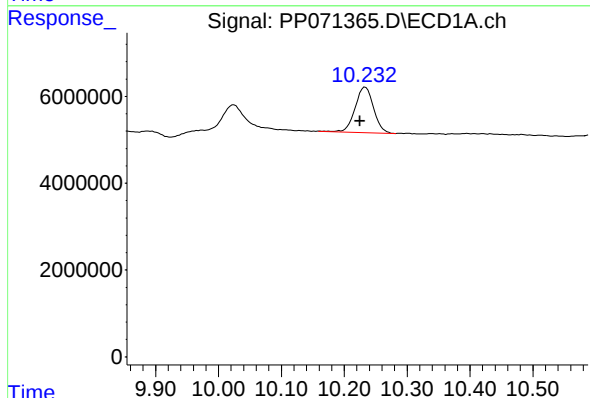

#2 Decachlorobiphenyl

R.T.: 10.233 min
Delta R.T.: 0.008 min
Response: 21331078
Conc: 20.26 ng/ml

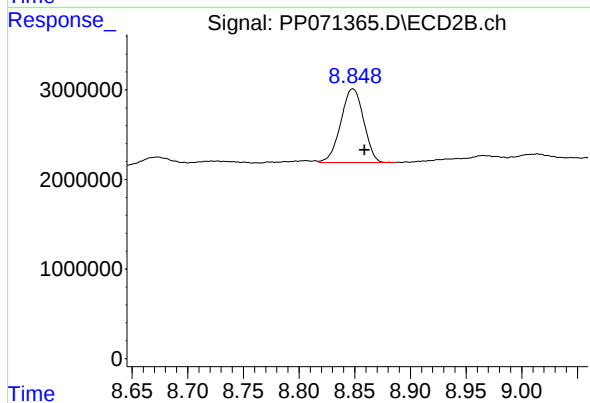

#2 Decachlorobiphenyl

R.T.: 8.848 min
Delta R.T.: -0.010 min
Response: 11717738
Conc: 14.87 ng/ml