

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041825\
 Data File : PP071381.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Apr 2025 17:20
 Operator : YP\AJ
 Sample : Q1832-37
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PL-714-COMP-07

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/21/2025
 Supervised By :mohammad ahmed 04/23/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 19 02:50:57 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032725.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 28 03:13:46 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.513	3.813	27352898	24995906	18.715m	24.112 #
2) SA Decachlor...	10.233	8.850	17629916	12116641	16.749	15.373

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041825\
Data File : PP071381.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Apr 2025 17:20
Operator : YP\AJ
Sample : Q1832-37
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
PL-714-COMP-07


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/21/2025
Supervised By :mohammad ahmed 04/23/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 19 02:50:57 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP032725.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 28 03:13:46 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

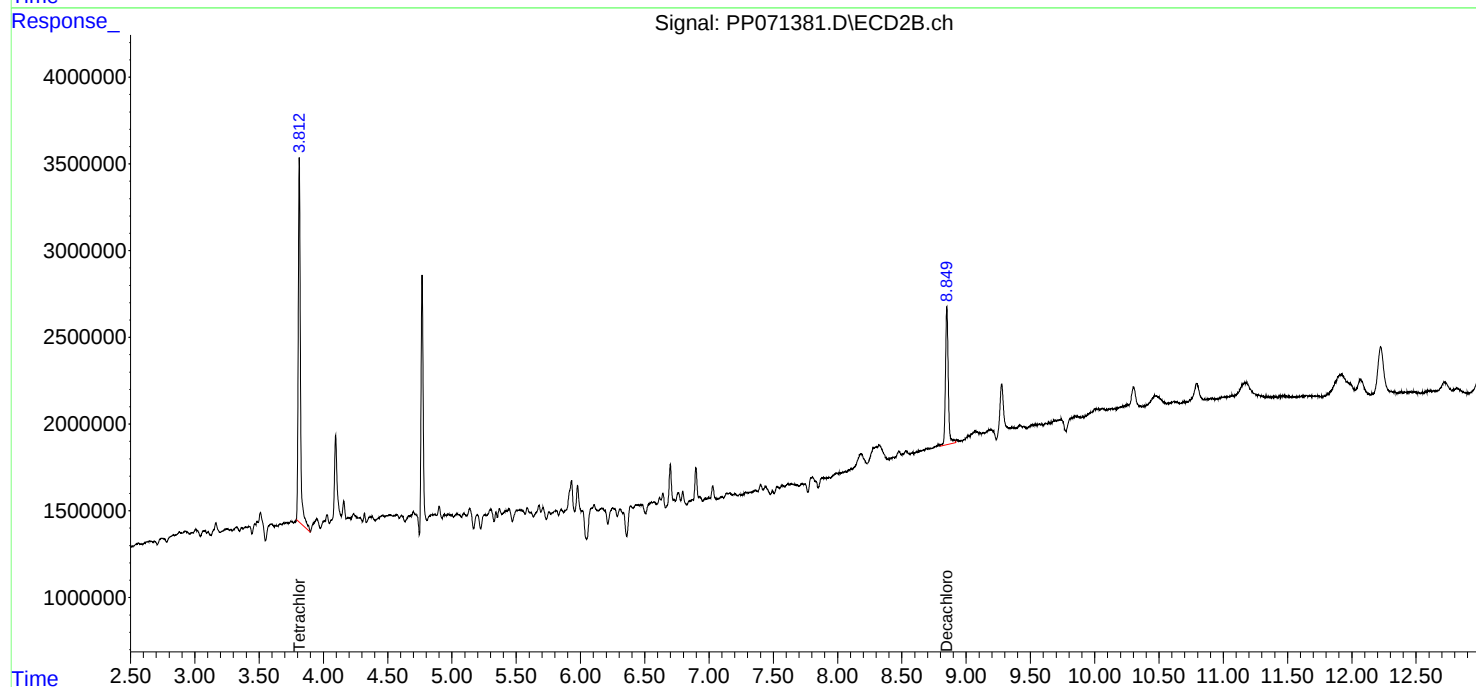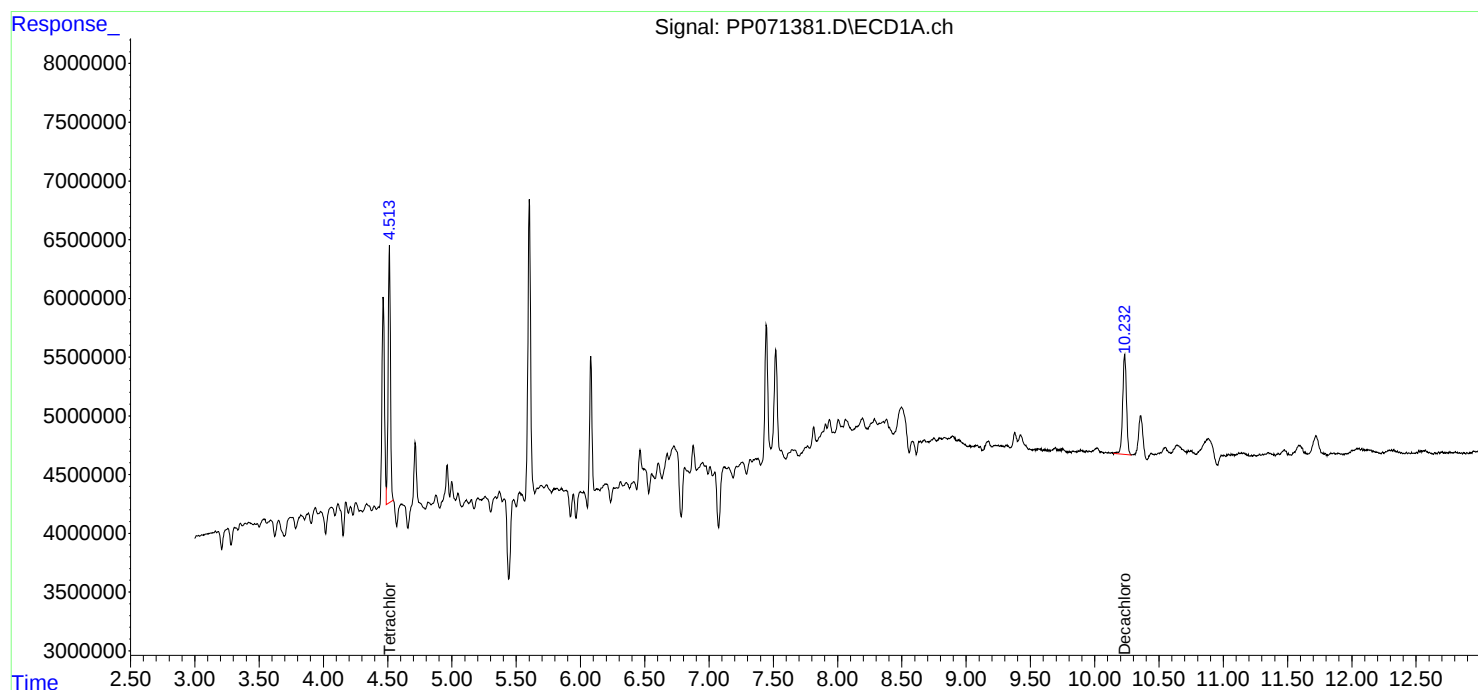

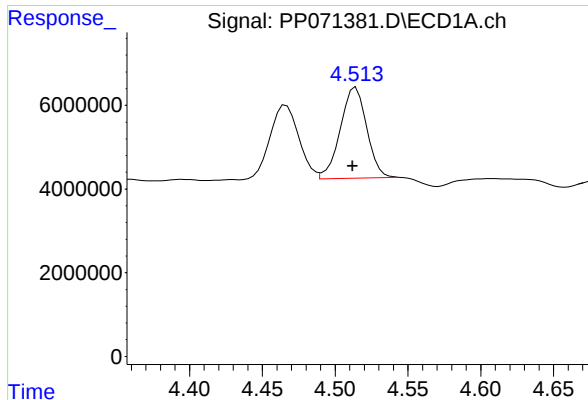


#1 Tetrachloro-m-xylene

R.T.: 4.513 min
Delta R.T.: 0.000 min
Response: 27352898
Conc: 18.71 ng/ml

Instrument :
ECD_P
ClientSampleId :
PL-714-COMP-07


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/21/2025
Supervised By :mohammad ahmed 04/23/2025

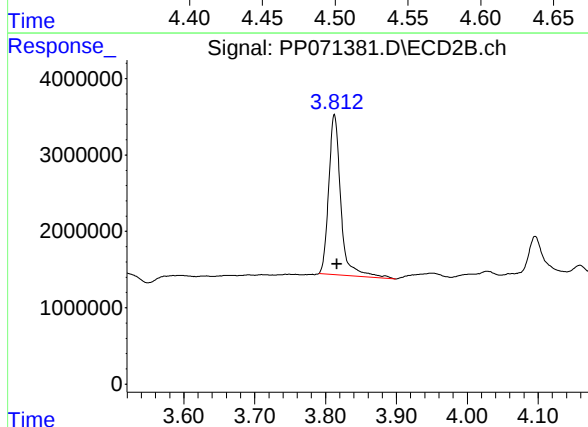


#1 Tetrachloro-m-xylene

R.T.: 3.813 min
Delta R.T.: -0.003 min
Response: 24995906
Conc: 24.11 ng/ml

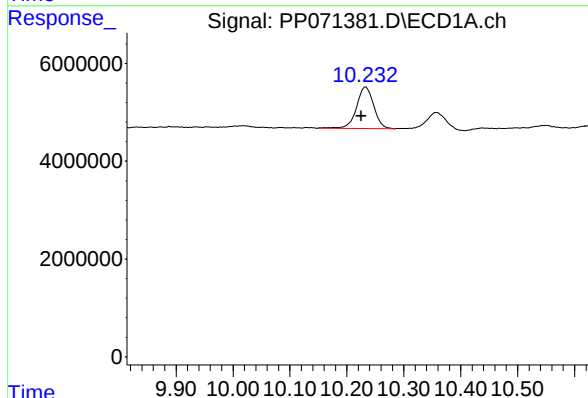

#2 Decachlorobiphenyl

R.T.: 10.233 min
Delta R.T.: 0.008 min
Response: 17629916
Conc: 16.75 ng/ml

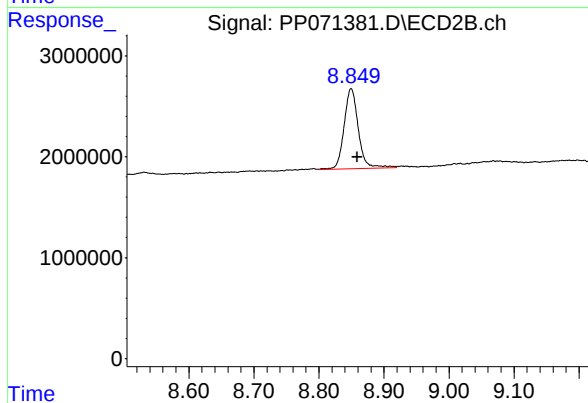

#2 Decachlorobiphenyl

R.T.: 8.850 min
Delta R.T.: -0.009 min
Response: 12116641
Conc: 15.37 ng/ml