

Data Path : P:\HPCHEM1\ECD_P\Data\PP041918\
Data File : PP025149.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Apr 2018 12:41
Operator : UA/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 20 06:54:26 2018
Quant Method : P:\HPCHEM1\ECD_P\methods\PP032918.M
Quant Title : 8080.M
QLast Update : Mon Apr 02 02:18:04 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.417	11.117	304.9E6	290.9E6	576.146	490.169
Target Compounds							
15) T	Picloram	16.972	0.000	12274879	0	2.097	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : P:\HPCHEM1\ECD_P\Data\PP041918\
Data File : PP025149.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Apr 2018 12:41
Operator : UA/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 20 06:54:26 2018
Quant Method : P:\HPCHEM1\ECD_P\methods\PP032918.M
Quant Title : 8080.M
QLast Update : Mon Apr 02 02:18:04 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

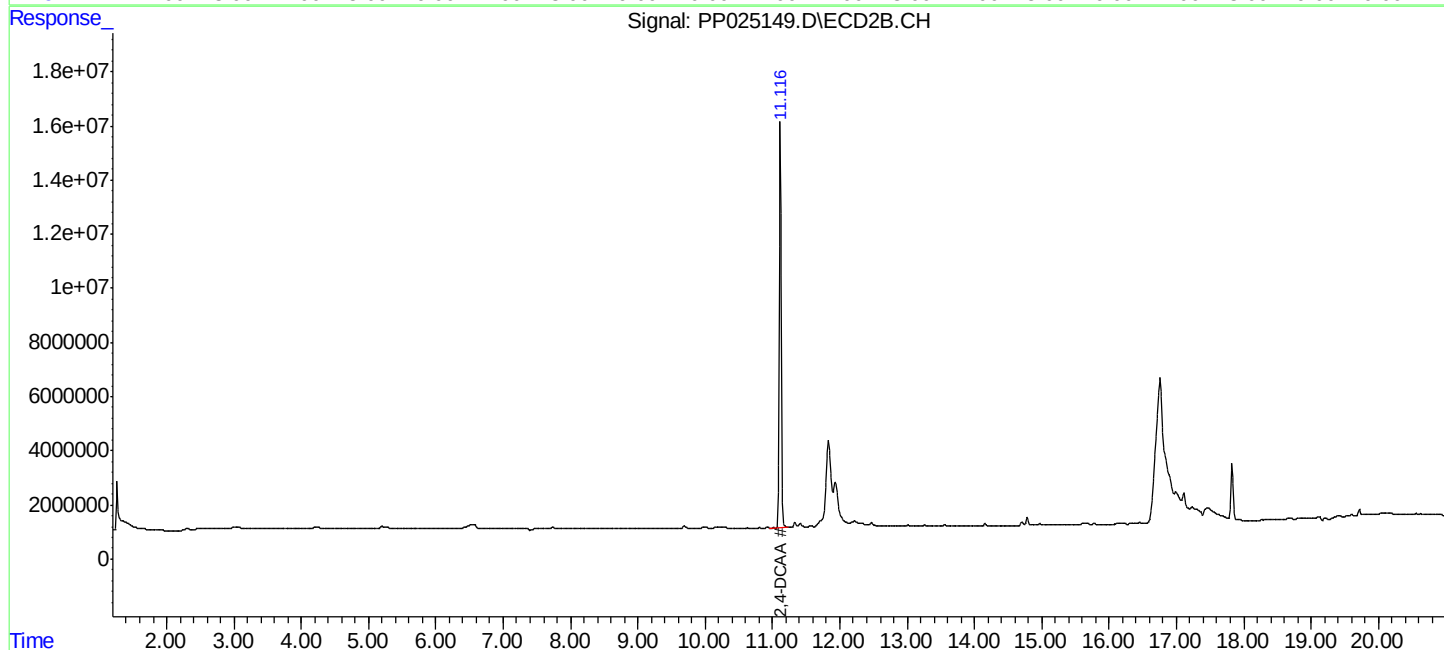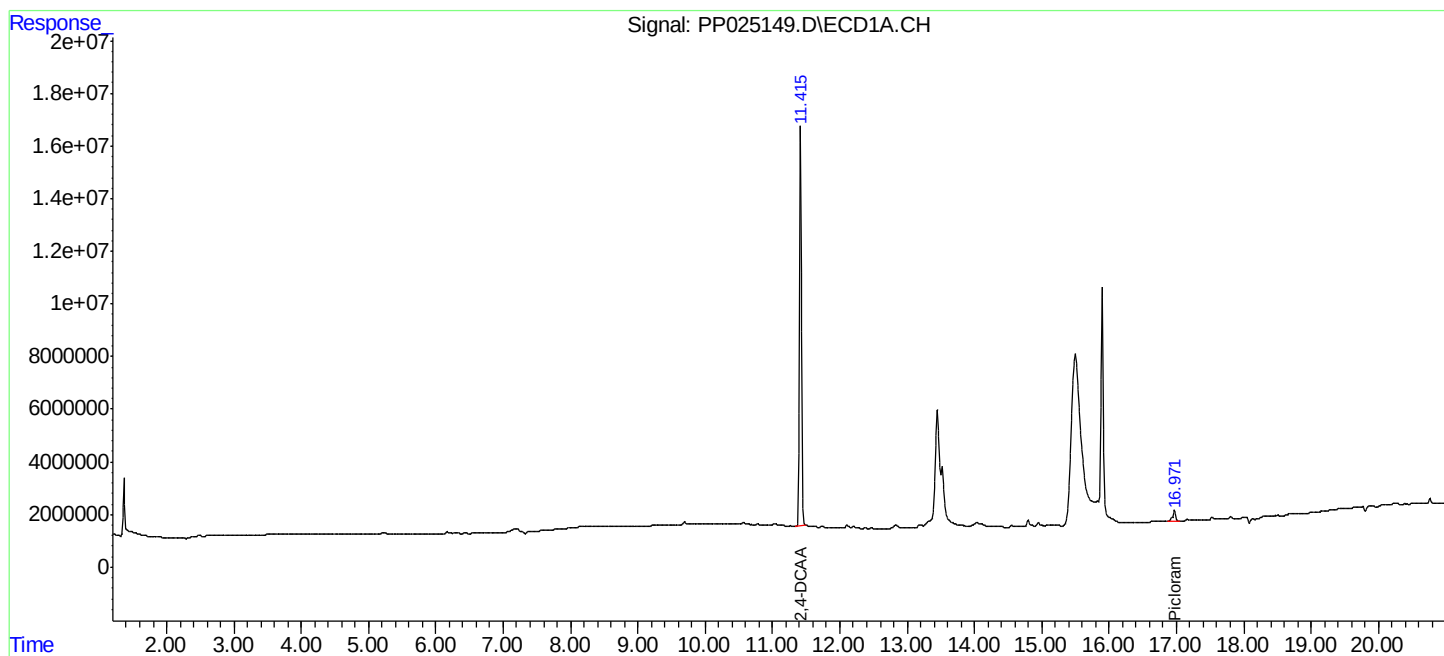


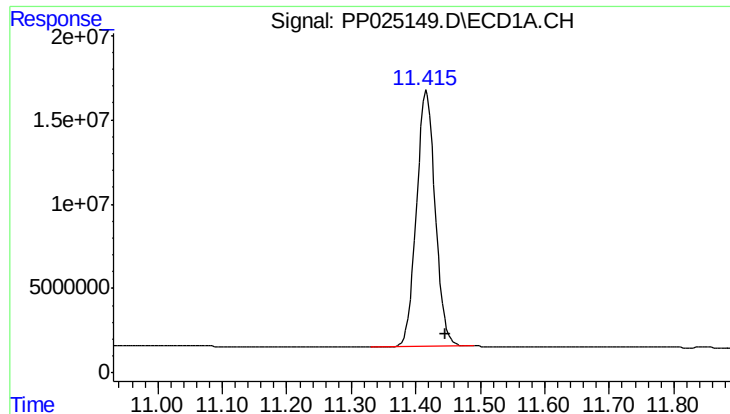

#4 2,4-DCAA


R.T.: 11.417 min
Delta R.T.: -0.030 min
Response: 304938228
Conc: 576.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

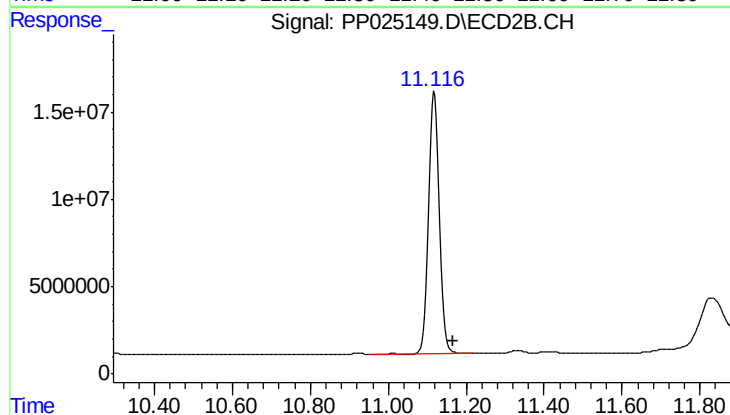


#4 2,4-DCAA

R.T.: 11.117 min
Delta R.T.: -0.050 min
Response: 290872713
Conc: 490.17 ng/ml

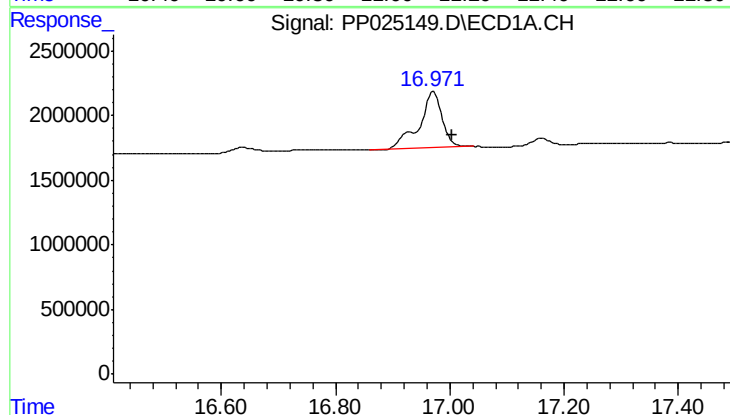

#15 Picloram

R.T.: 16.972 min
Delta R.T.: -0.033 min
Response: 12274879
Conc: 2.10 ng/ml

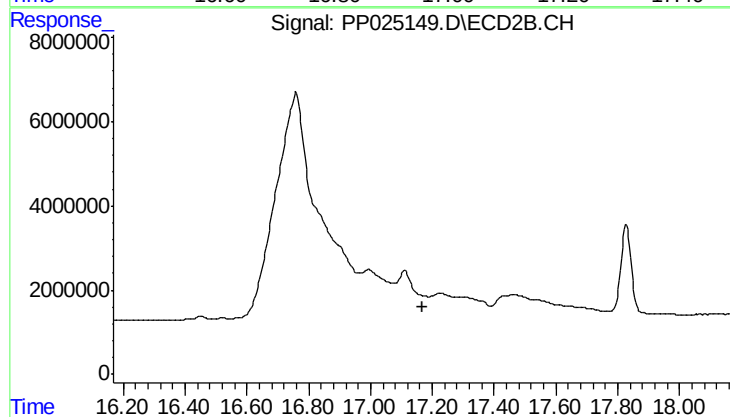

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 17.167 min
Response: 0
Conc: N.D.