

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041921\
 Data File : PP034993.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Apr 2021 16:23
 Operator : DD\AJ
 Sample : M2030-02RE
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 04-14-21-WATERRE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 19 16:23:27 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 31 06:02:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.842	4.259	1333493	845031	17.481m	18.811
2) SA Decachlor...	10.753	9.551	350364	156119	4.551m	5.529

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041921\
Data File : PP034993.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Apr 2021 16:23
Operator : DD\AJ
Sample : M2030-02RE
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
04-14-21-WATERRE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 19 16:23:27 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 31 06:02:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

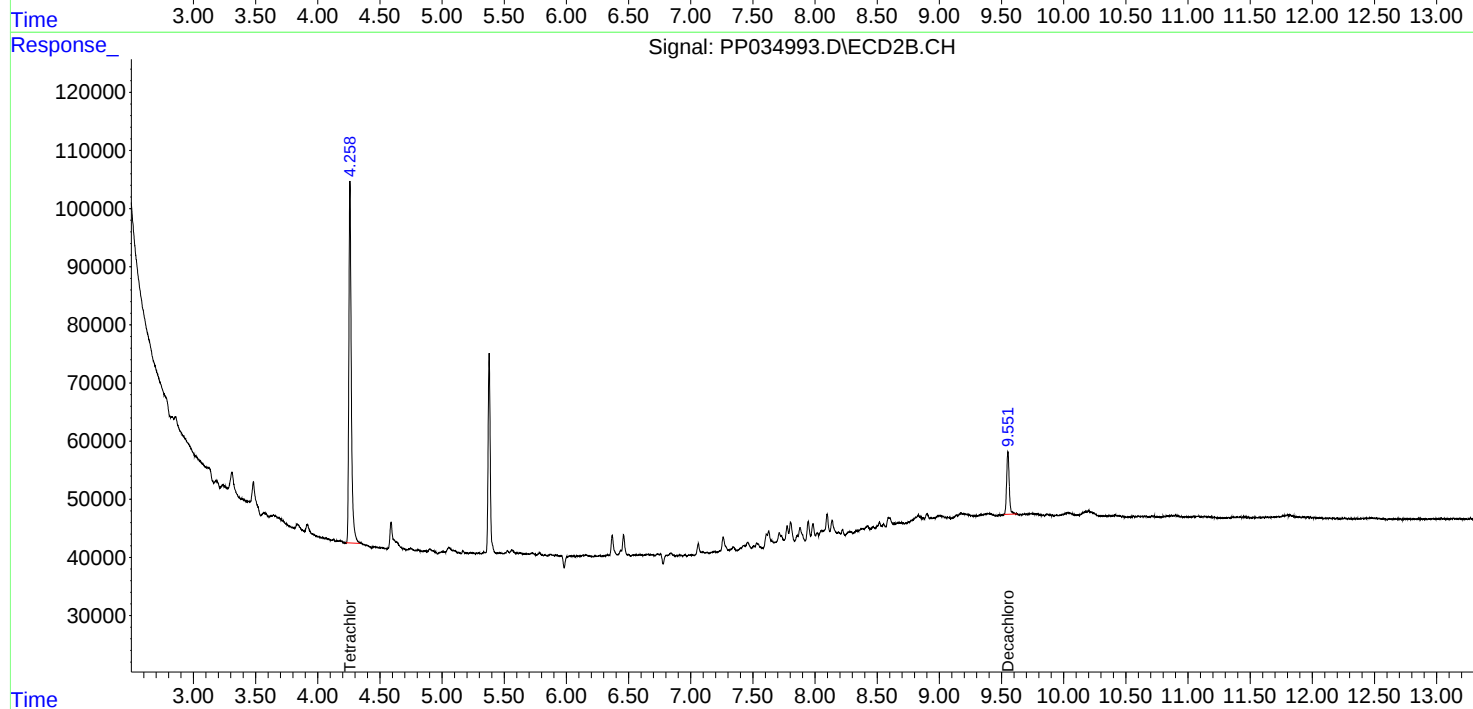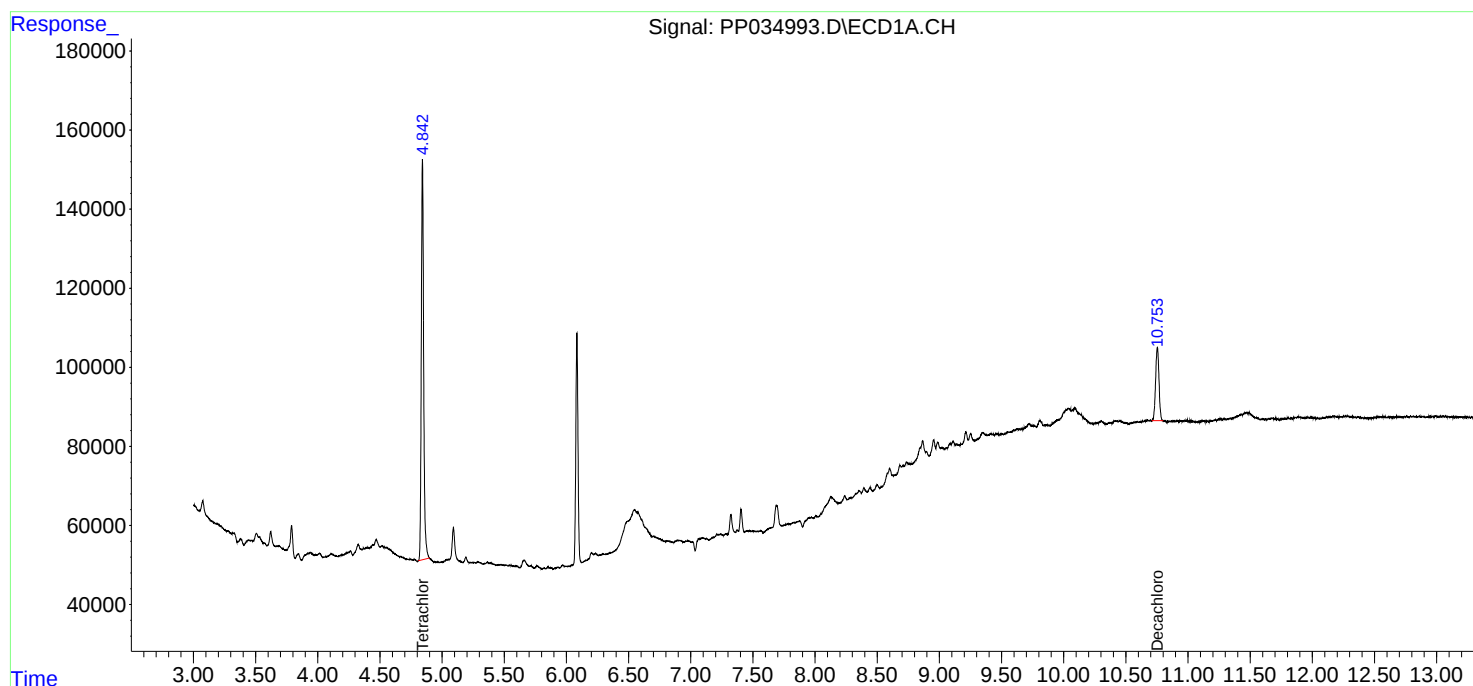

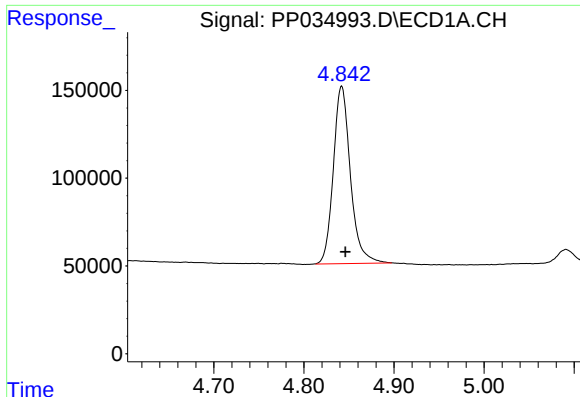

#1 Tetrachloro-m-xylene


R.T.: 4.842 min

Delta R.T.: -0.004 min

Response: 1333493

Conc: 17.48 ng/ml m

Instrument :
ECD_P
ClientSampleId :
04-14-21-WATERRE

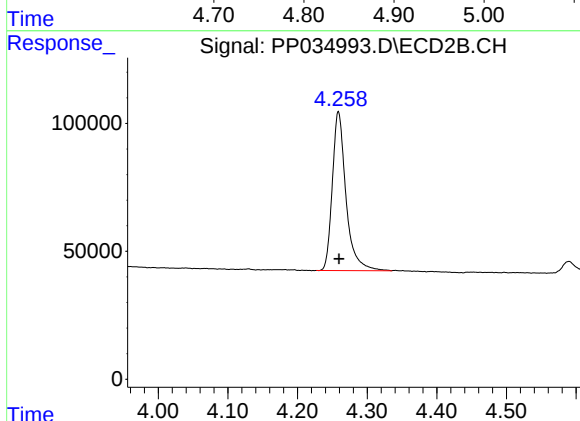


#1 Tetrachloro-m-xylene

R.T.: 4.259 min

Delta R.T.: -0.001 min

Response: 845031

Conc: 18.81 ng/ml

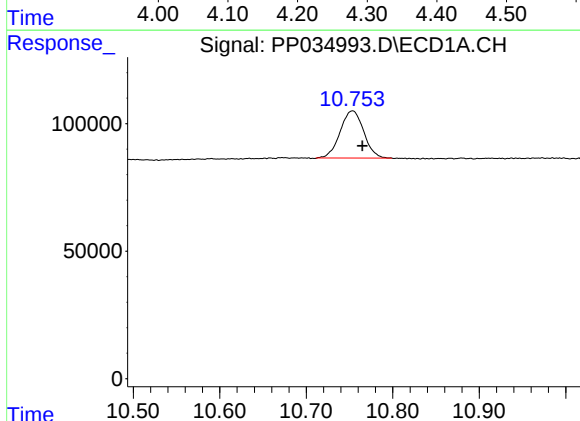


#2 Decachlorobiphenyl

R.T.: 10.753 min

Delta R.T.: -0.012 min

Response: 350364

Conc: 4.55 ng/ml m

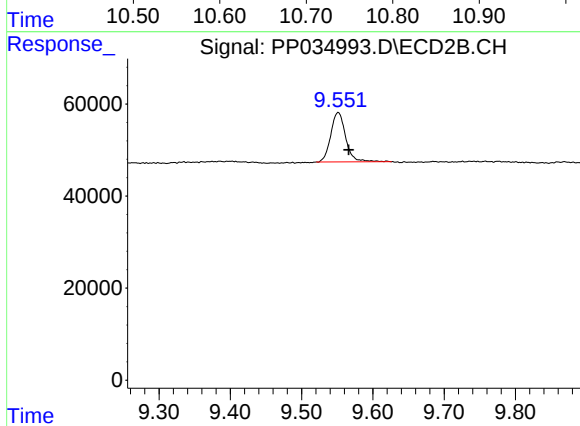

#2 Decachlorobiphenyl

R.T.: 9.551 min

Delta R.T.: -0.015 min

Response: 156119

Conc: 5.53 ng/ml