

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP041921\  
 Data File : PP035011.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 19 Apr 2021 22:02  
 Operator : DD\AJ  
 Sample : M2070-01  
 Misc :  
 ALS Vial : 25 Sample Multiplier: 1

Instrument :  
 ECD\_P  
 ClientSampleId :  
 JGD-3150-D3550-A

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 20 09:35:09 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP033021.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Mar 31 06:02:19 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound                    | RT#1   | RT#2   | Resp#1  | Resp#2  | ng/ml  | ng/ml  |
|-----------------------------|--------|--------|---------|---------|--------|--------|
| -----                       |        |        |         |         |        |        |
| System Monitoring Compounds |        |        |         |         |        |        |
| 1) SA Tetrachlo...          | 4.841  | 4.258  | 1608407 | 1012625 | 21.084 | 22.542 |
| 2) SA Decachlor...          | 10.755 | 9.550f | 1120489 | 471361  | 14.556 | 16.694 |

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP041921\  
Data File : PP035011.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 19 Apr 2021 22:02  
Operator : DD\AJ  
Sample : M2070-01  
Misc :  
ALS Vial : 25 Sample Multiplier: 1

Instrument :  
ECD\_P  
ClientSampleId :  
JGD-3150-D3550-A

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Apr 20 09:35:09 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP033021.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Wed Mar 31 06:02:19 2021  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

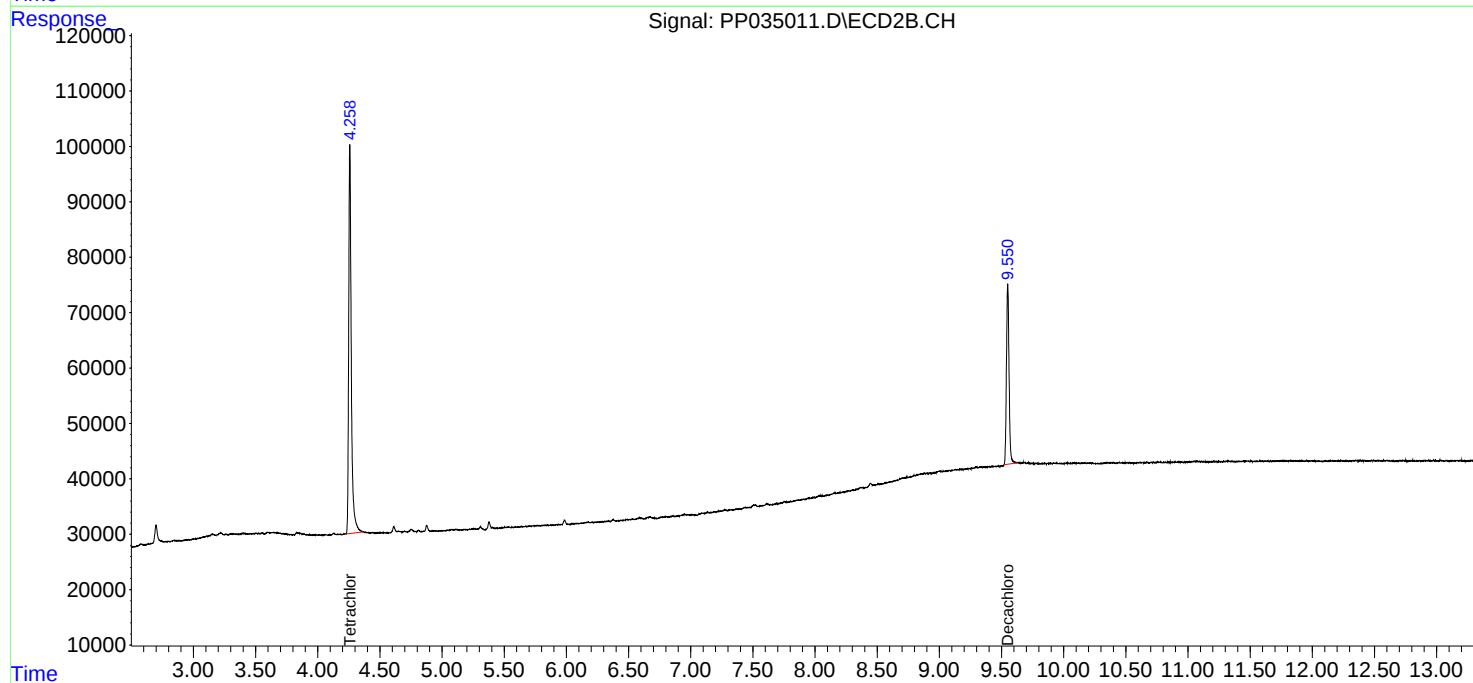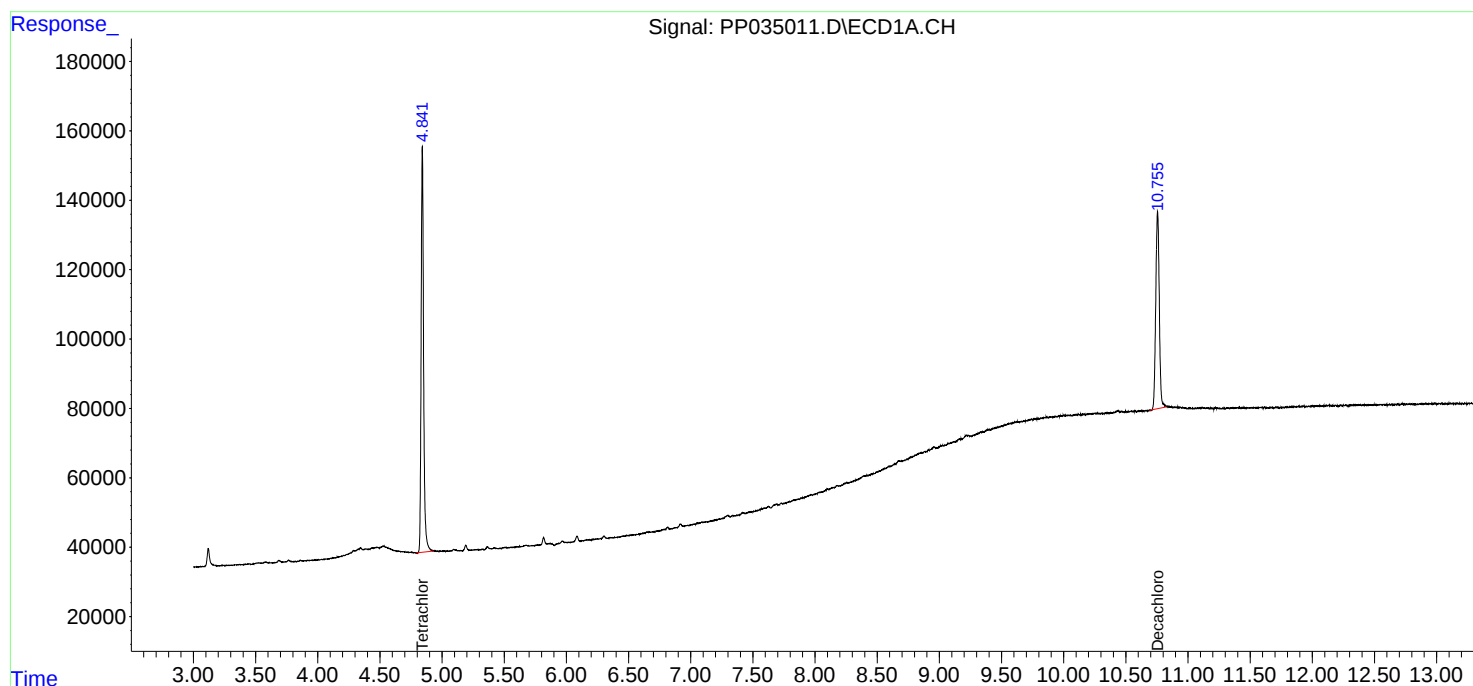


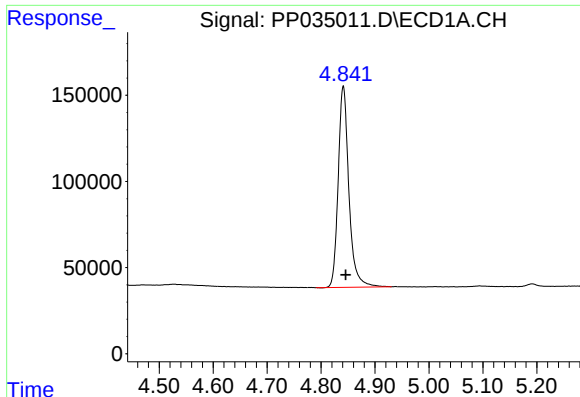

#1 Tetrachloro-m-xylene


R.T.: 4.841 min  
Delta R.T.: -0.005 min  
Response: 1608407  
Conc: 21.08 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
JGD-3150-D3550-A

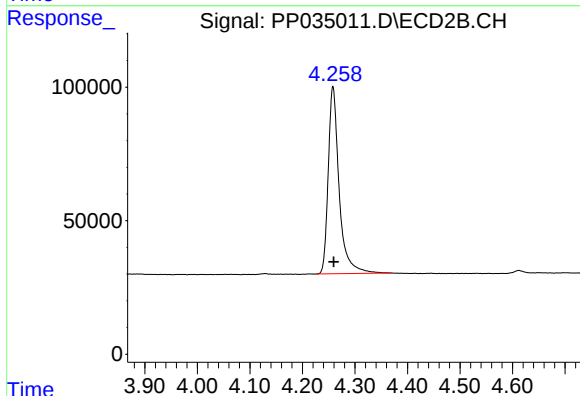


#1 Tetrachloro-m-xylene

R.T.: 4.258 min  
Delta R.T.: -0.002 min  
Response: 1012625  
Conc: 22.54 ng/ml

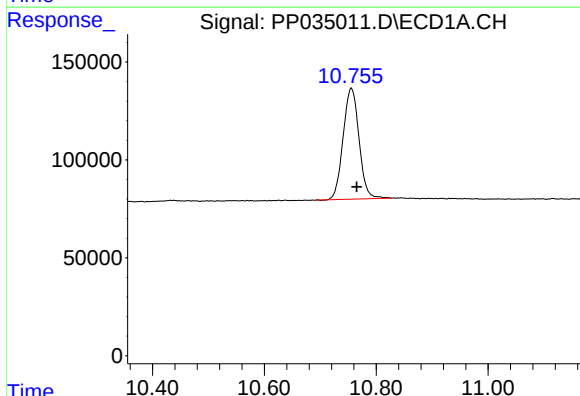

#2 Decachlorobiphenyl

R.T.: 10.755 min  
Delta R.T.: -0.010 min  
Response: 1120489  
Conc: 14.56 ng/ml

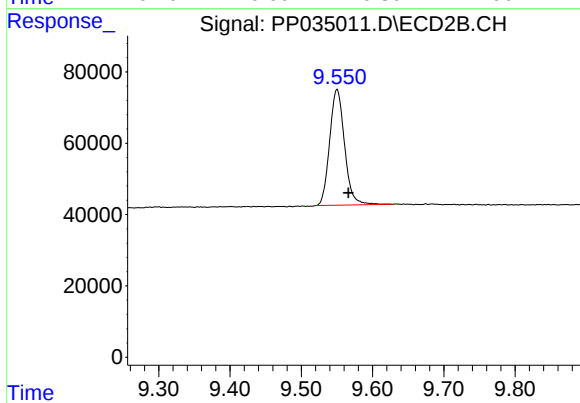

#2 Decachlorobiphenyl

R.T.: 9.550 min  
Delta R.T.: -0.016 min  
Response: 471361  
Conc: 16.69 ng/ml