

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041921\
 Data File : PP035028.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Apr 2021 2:49
 Operator : DD\AJ
 Sample : M2070-05
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 JGD-3150-D3550-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 20 08:37:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 31 06:02:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.841	4.258	1455200	949243	19.076	21.131
2) SA Decachlor...	10.753	9.550f	885687	375670	11.505	13.305

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041921\
Data File : PP035028.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Apr 2021 2:49
Operator : DD\AJ
Sample : M2070-05
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
JGD-3150-D3550-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 20 08:37:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP033021.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 31 06:02:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

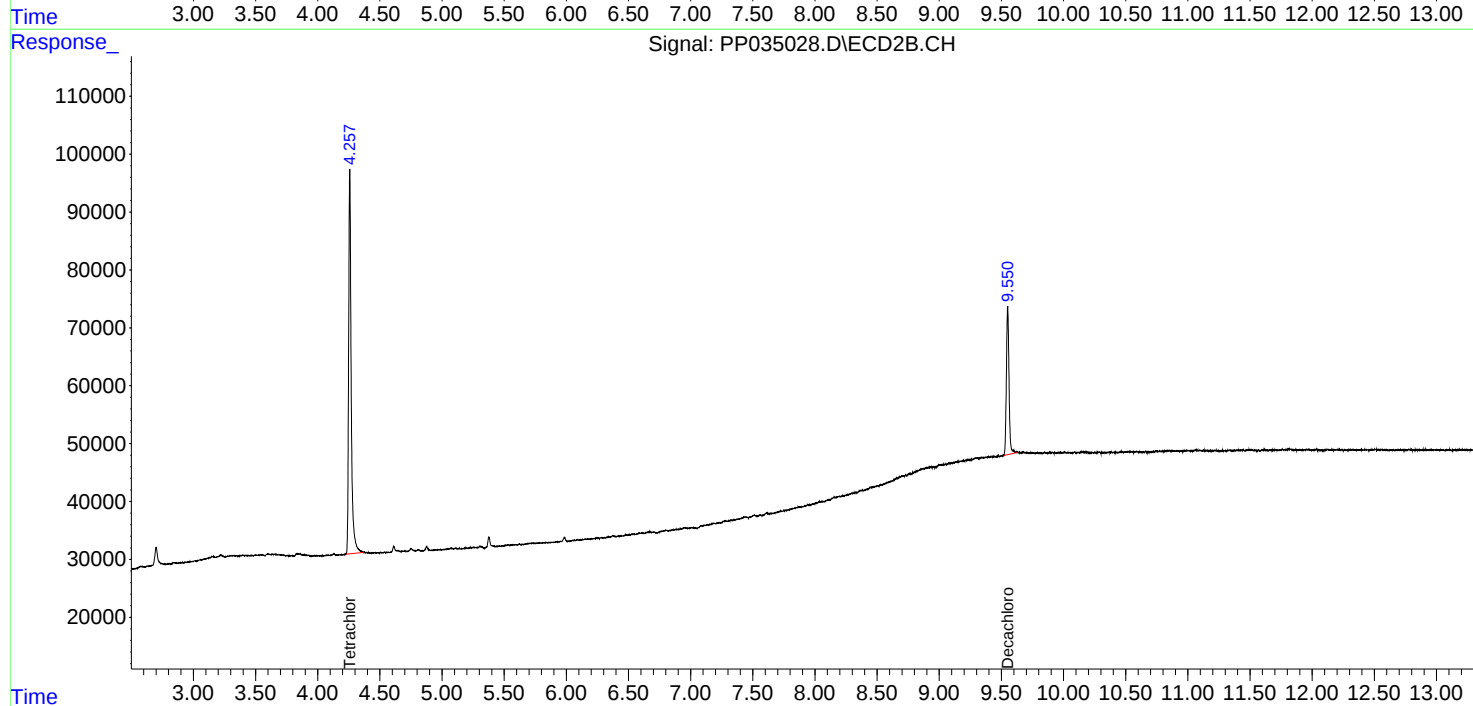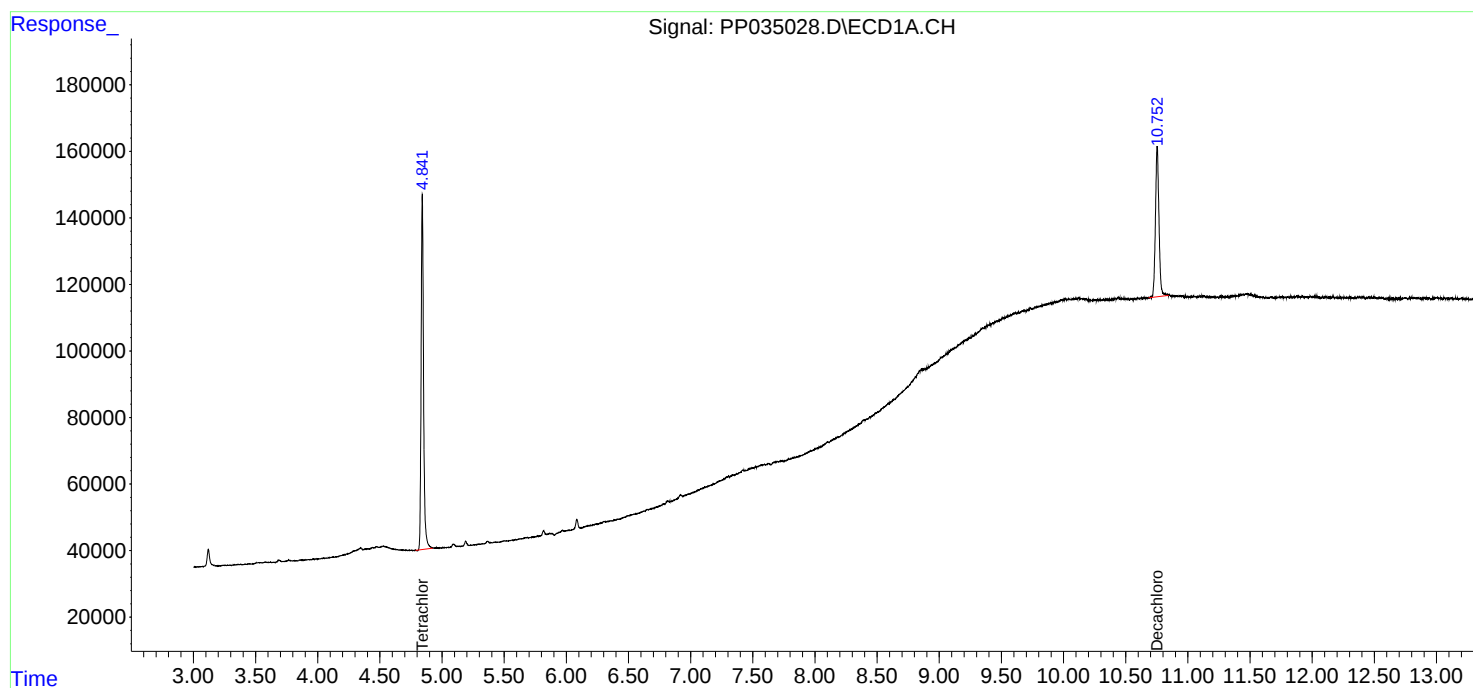


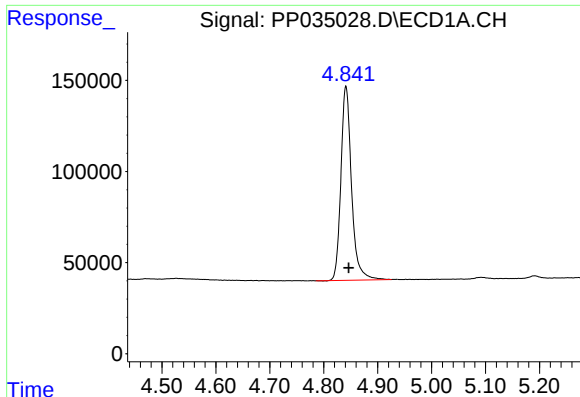

#1 Tetrachloro-m-xylene


R.T.: 4.841 min
Delta R.T.: -0.005 min
Response: 1455200
Conc: 19.08 ng/ml

Instrument :
ECD_P
ClientSampleId :
JGD-3150-D3550-B

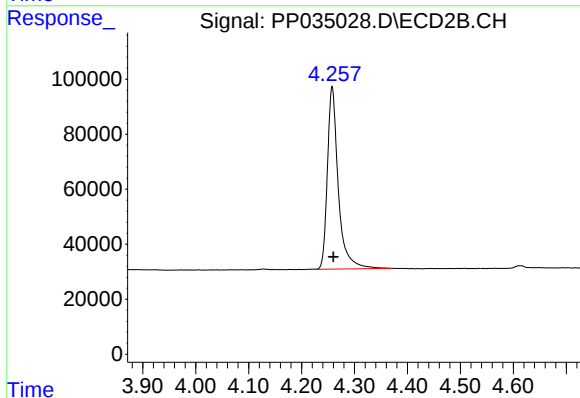


#1 Tetrachloro-m-xylene

R.T.: 4.258 min
Delta R.T.: -0.002 min
Response: 949243
Conc: 21.13 ng/ml

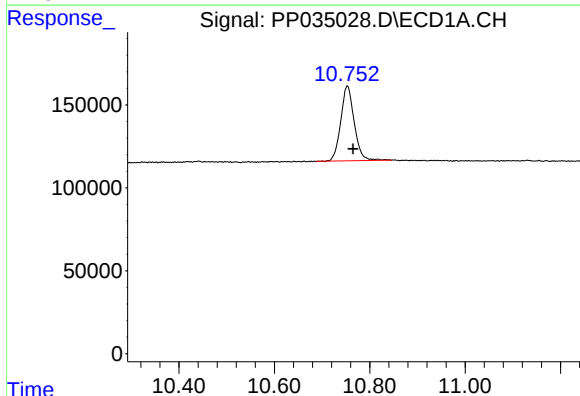

#2 Decachlorobiphenyl

R.T.: 10.753 min
Delta R.T.: -0.012 min
Response: 885687
Conc: 11.51 ng/ml

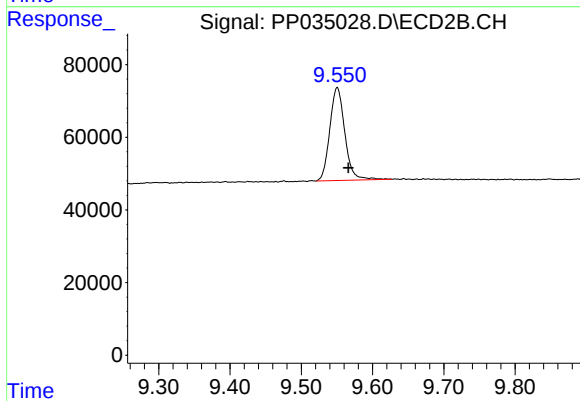

#2 Decachlorobiphenyl

R.T.: 9.550 min
Delta R.T.: -0.016 min
Response: 375670
Conc: 13.30 ng/ml