

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041922\
 Data File : PP046316.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Apr 2022 23:47
 Operator : YP\AJ
 Sample : N2459-17
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 31581-84

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/20/2022
 Supervised By :mohammad ahmed 04/20/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 20 05:33:23 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP041222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 19 10:41:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.871	3.136	43989540	30801975	17.884	19.385m
2) SA Decachlor...	9.961	8.462	21890208	23909702	13.335	16.775 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041922\
Data File : PP046316.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Apr 2022 23:47
Operator : YP\AJ
Sample : N2459-17
Misc :
ALS Vial : 29 Sample Multiplier: 1


Instrument :
ECD_P
ClientSampleId :
31581-84


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/20/2022
Supervised By :mohammad ahmed 04/20/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 20 05:33:23 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP041222.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 19 10:41:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

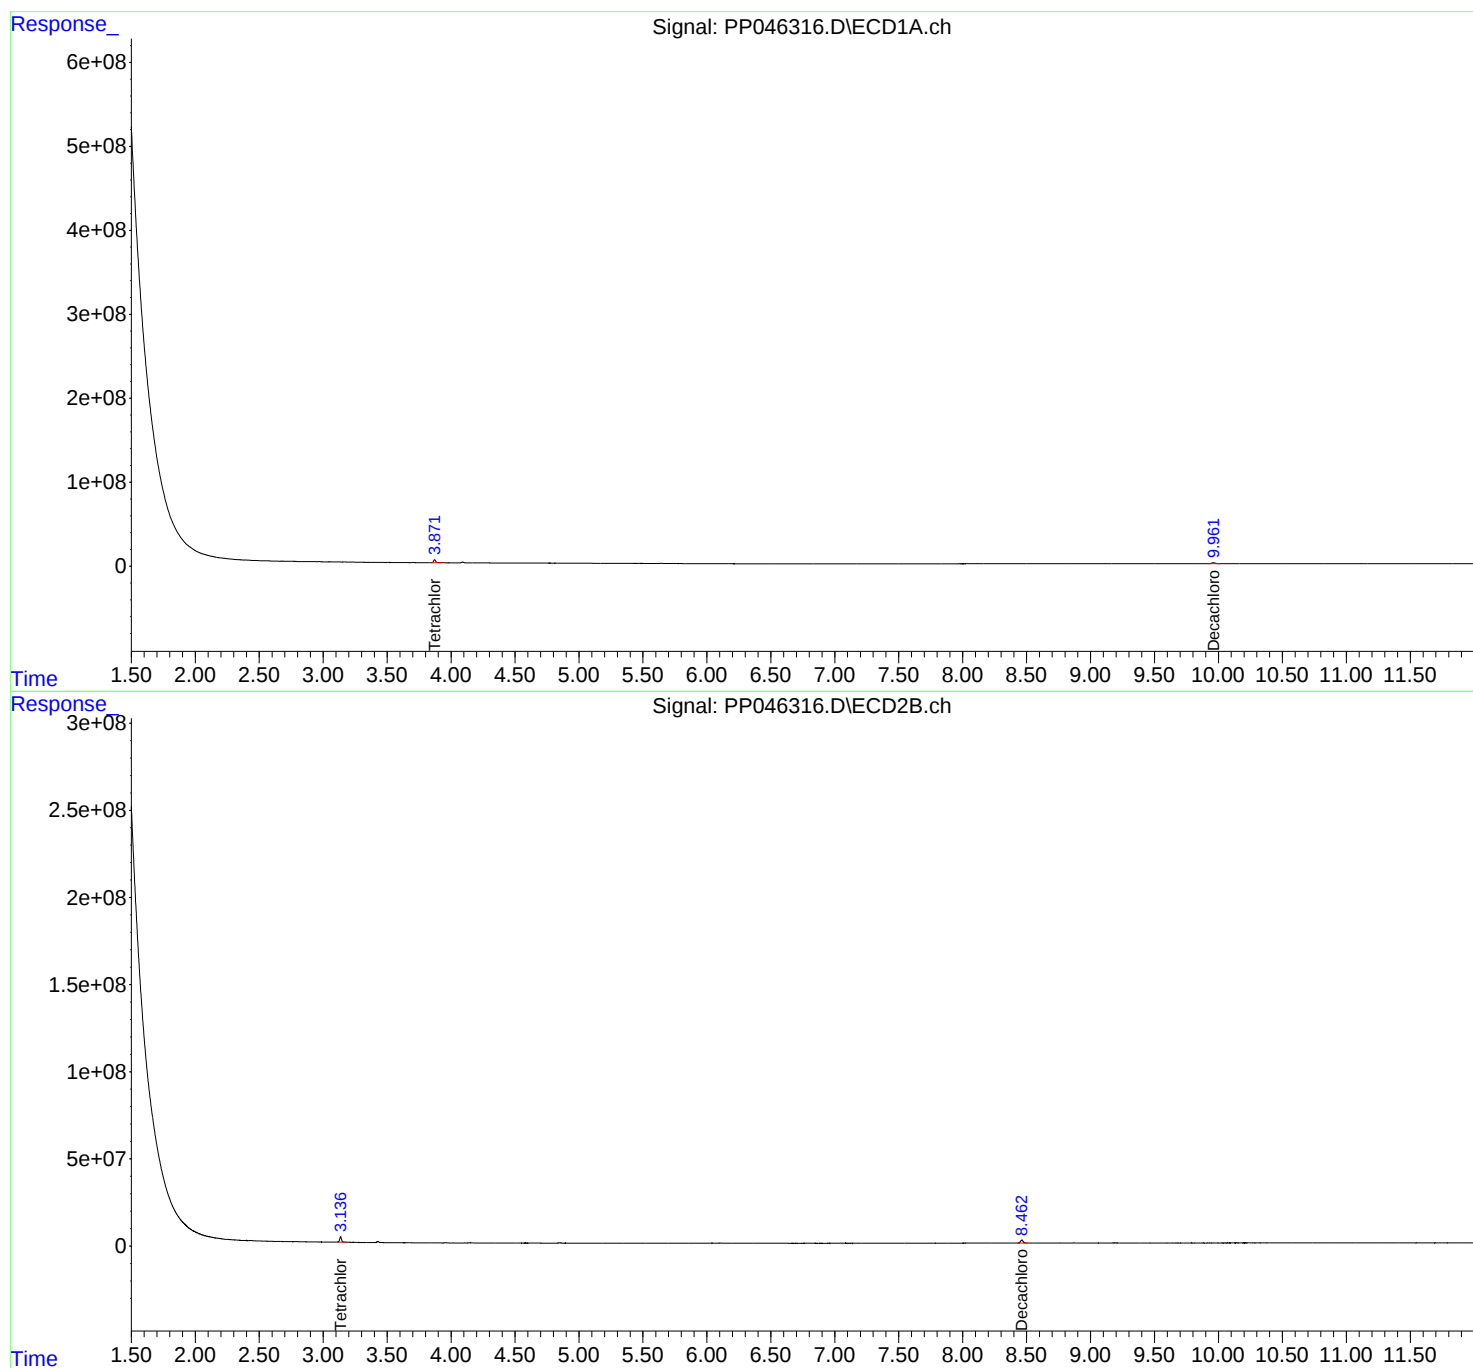

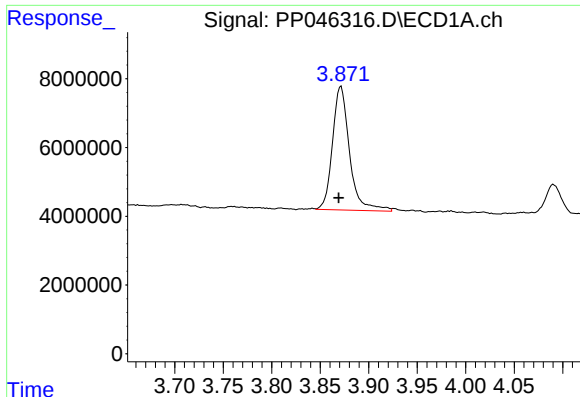


#1 Tetrachloro-m-xylene

R.T.: 3.871 min
Delta R.T.: 0.002 min
Response: 43989540
Conc: 17.88 ng/ml

Instrument :
ECD_P
ClientSampleId :
31581-84


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/20/2022
Supervised By :mohammad ahmed 04/20/2022

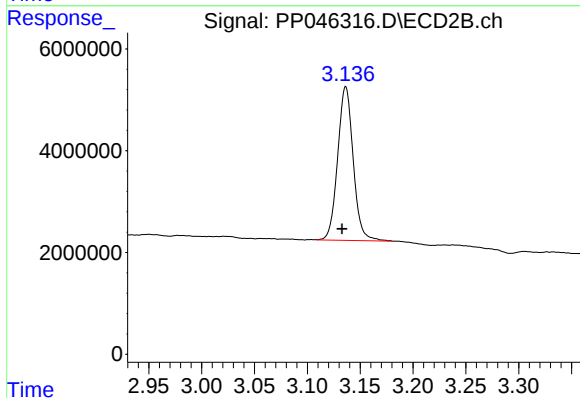


#1 Tetrachloro-m-xylene

R.T.: 3.136 min
Delta R.T.: 0.003 min
Response: 30801975
Conc: 19.38 ng/ml m

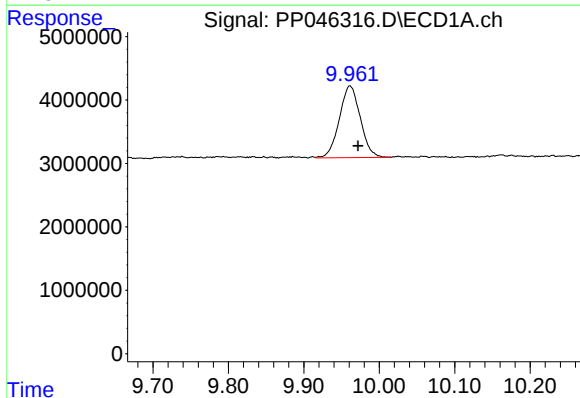

#2 Decachlorobiphenyl

R.T.: 9.961 min
Delta R.T.: -0.011 min
Response: 21890208
Conc: 13.33 ng/ml

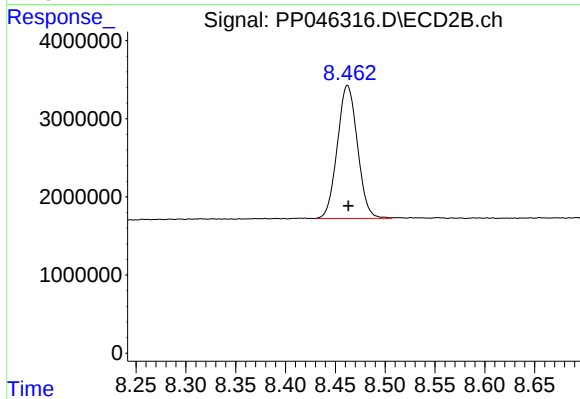

#2 Decachlorobiphenyl

R.T.: 8.462 min
Delta R.T.: 0.000 min
Response: 23909702
Conc: 16.77 ng/ml