

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041922\
 Data File : PP046321.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Apr 2022 01:03
 Operator : YP\AJ
 Sample : N2461-02 10X
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 KMH249C-END-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/20/2022
 Supervised By :mohammad ahmed 04/20/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 20 05:35:22 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP041222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 19 10:41:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.871	3.135	3427515	2929243	1.393m	1.843m#
2) SA Decachlor...	9.962	8.465	4157259	3462681	2.532	2.429

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041922\
Data File : PP046321.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Apr 2022 01:03
Operator : YP\AJ
Sample : N2461-02 10X
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
KMH249C-END-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/20/2022
Supervised By :mohammad ahmed 04/20/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 20 05:35:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP041222.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 19 10:41:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

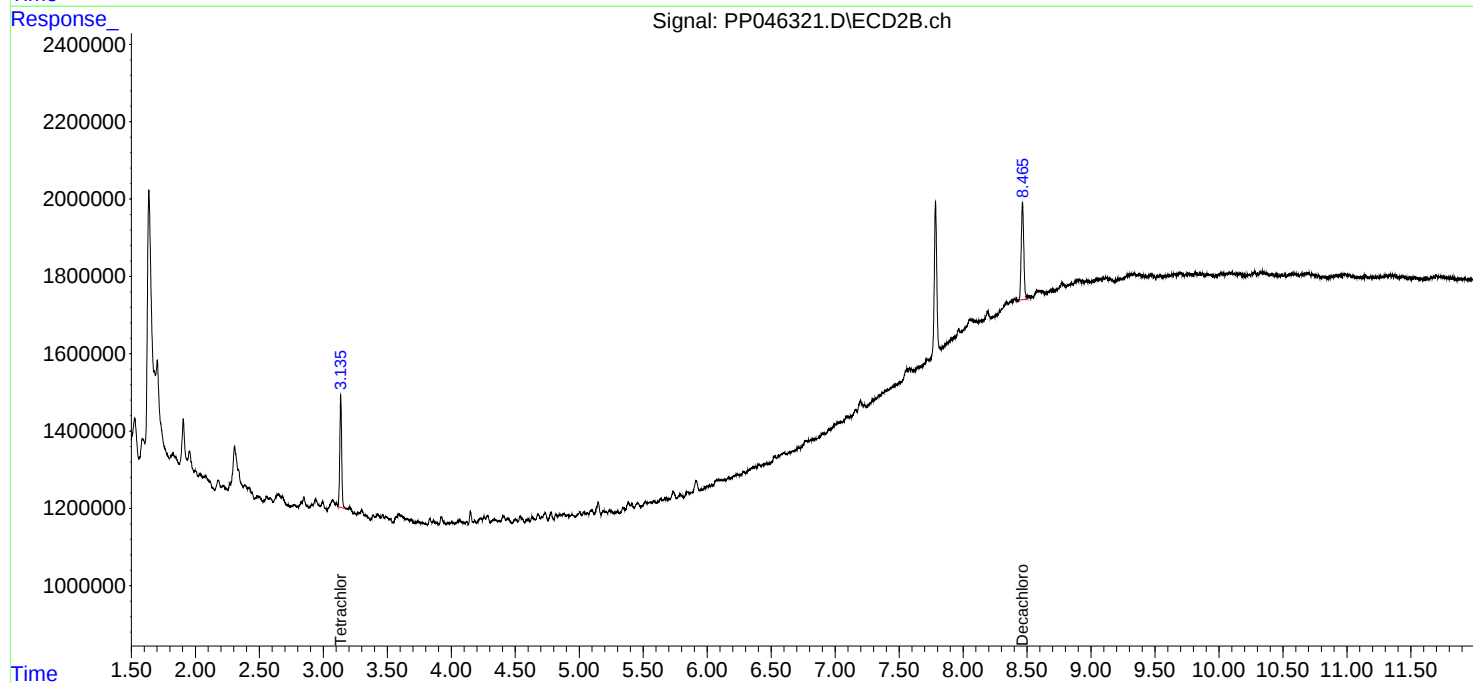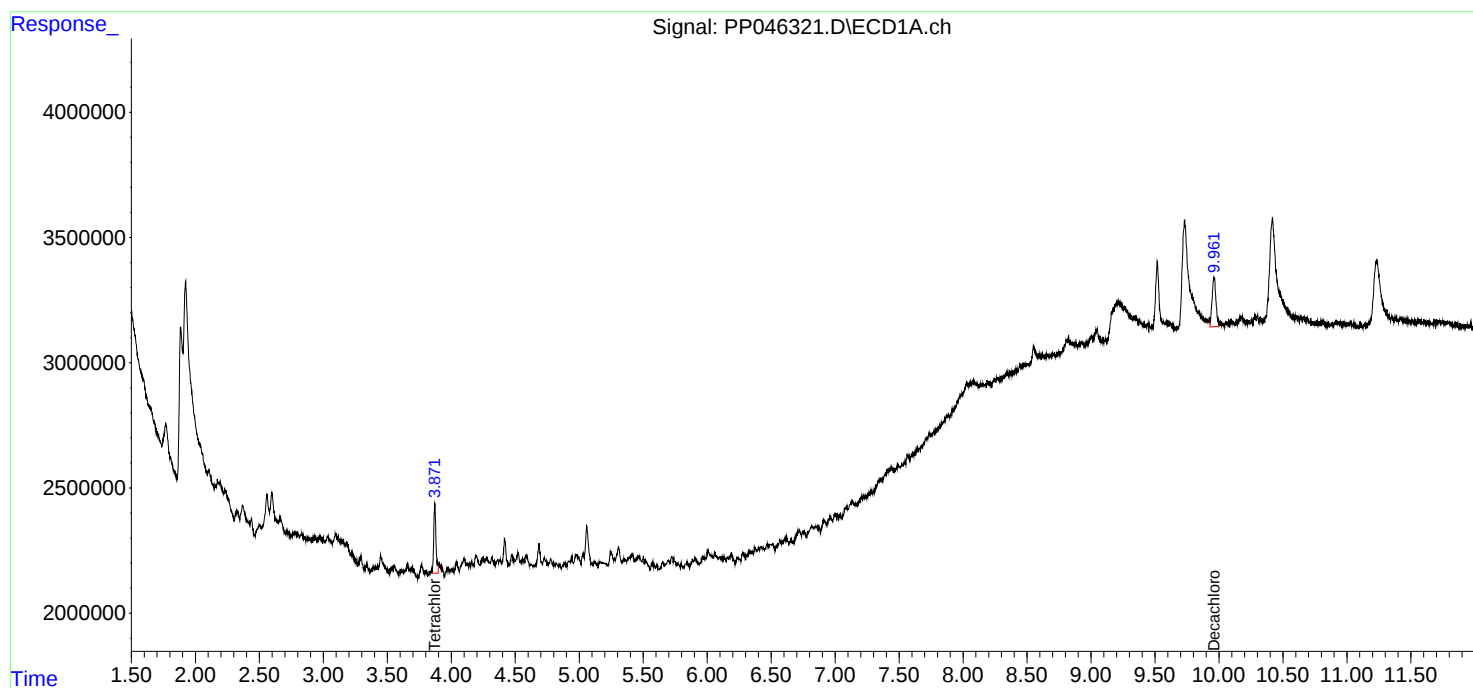

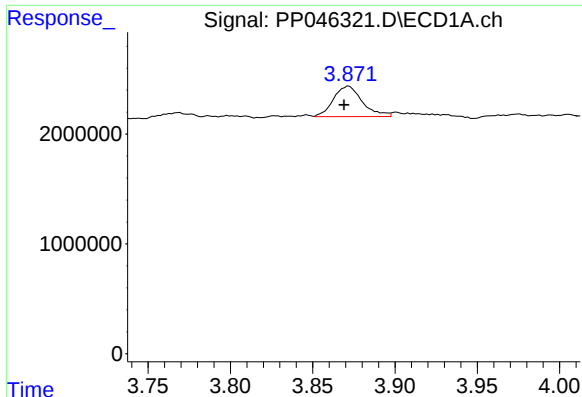


#1 Tetrachloro-m-xylene

R.T.: 3.871 min
Delta R.T.: 0.002 min
Response: 3427515
Conc: 1.39 ng/ml

Instrument :
ECD_P
ClientSampleId :
KMH249C-END-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/20/2022
Supervised By :mohammad ahmed 04/20/2022

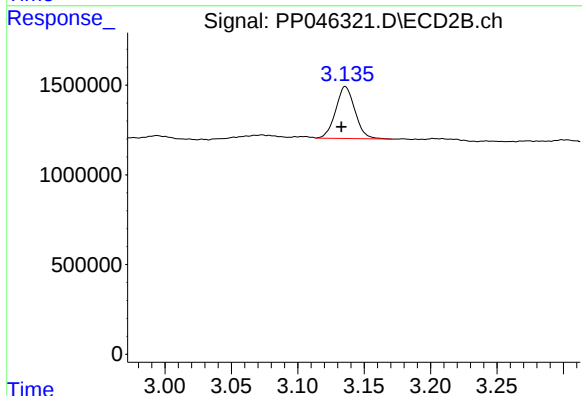


#1 Tetrachloro-m-xylene

R.T.: 3.135 min
Delta R.T.: 0.002 min
Response: 2929243
Conc: 1.84 ng/ml m

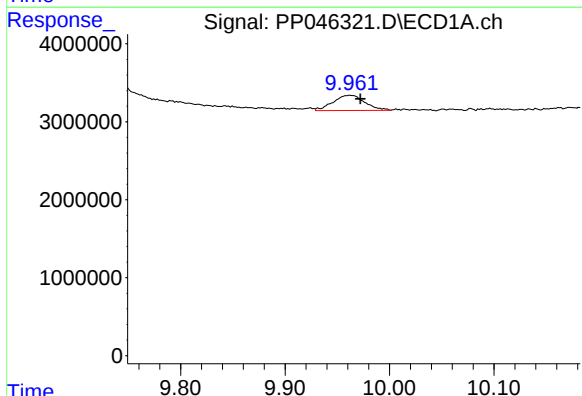

#2 Decachlorobiphenyl

R.T.: 9.962 min
Delta R.T.: -0.010 min
Response: 4157259
Conc: 2.53 ng/ml

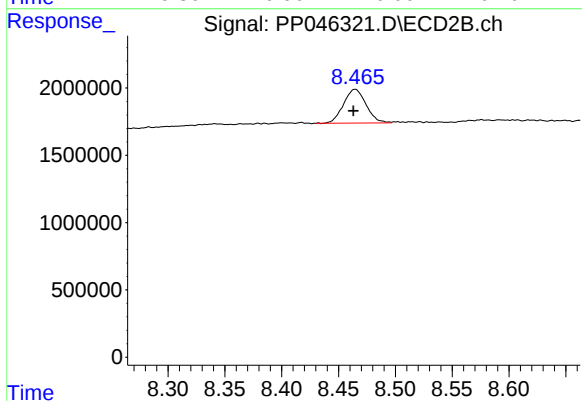

#2 Decachlorobiphenyl

R.T.: 8.465 min
Delta R.T.: 0.002 min
Response: 3462681
Conc: 2.43 ng/ml