

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041923\
 Data File : PP057007.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Apr 2023 14:59
 Operator : YP\AJ
 Sample : 02270-11
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SB-27-8-10-20230411

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/20/2023
 Supervised By :Ankita Jodhani 04/20/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 19 22:11:53 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP041823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 19 04:08:43 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.401	3.628	40808834	30271576	17.069	17.039
2) SA Decachlor...	10.220	8.687	31081331	33490266	33.796	24.220 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP041923\
Data File : PP057007.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Apr 2023 14:59
Operator : YP\AJ
Sample : 02270-11
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
SB-27-8-10-20230411


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/20/2023
Supervised By :Ankita Jodhani 04/20/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 19 22:11:53 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP041823.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 19 04:08:43 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

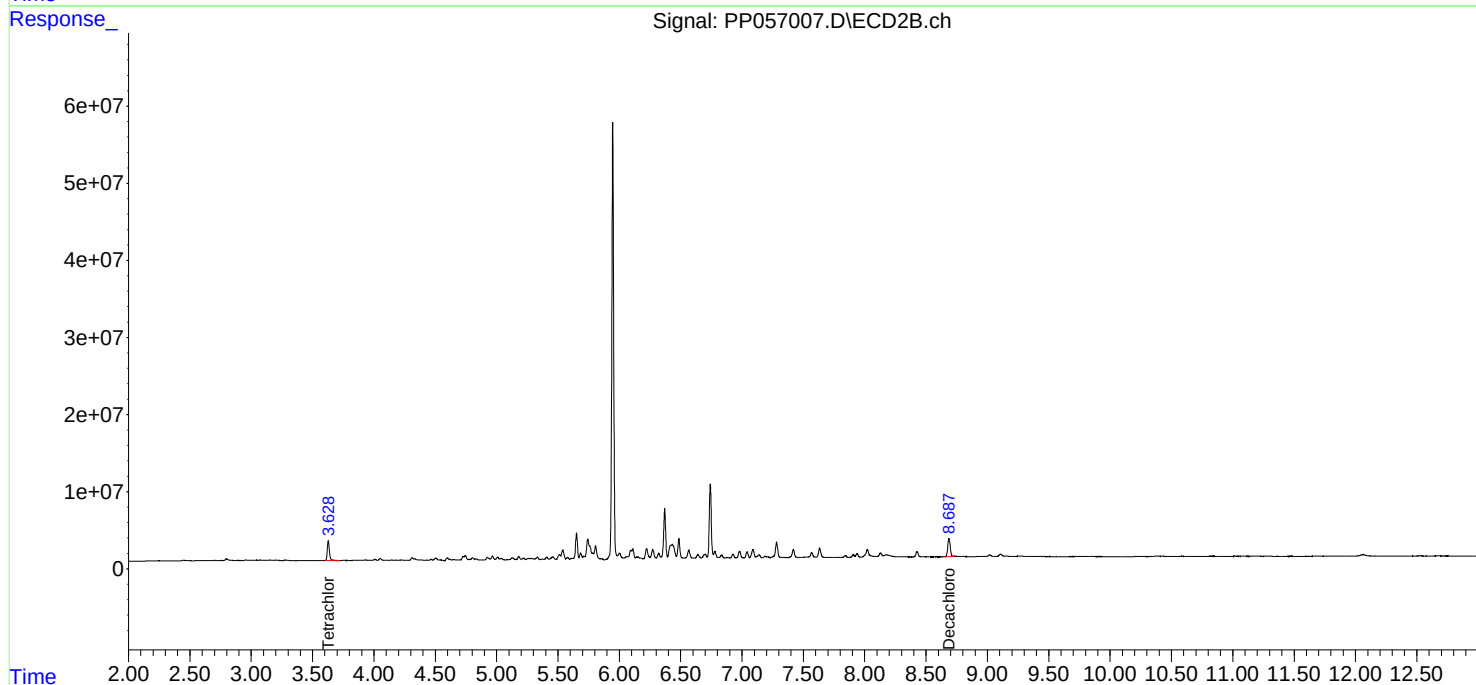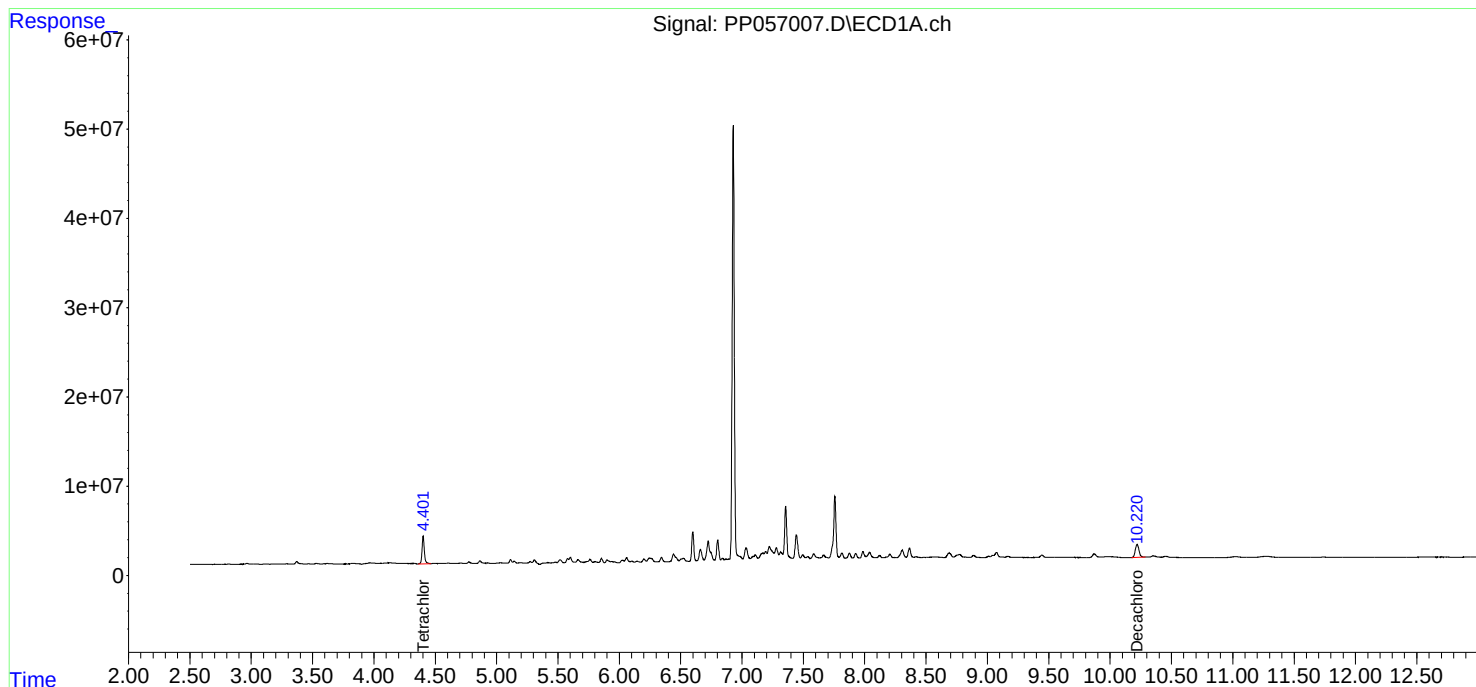

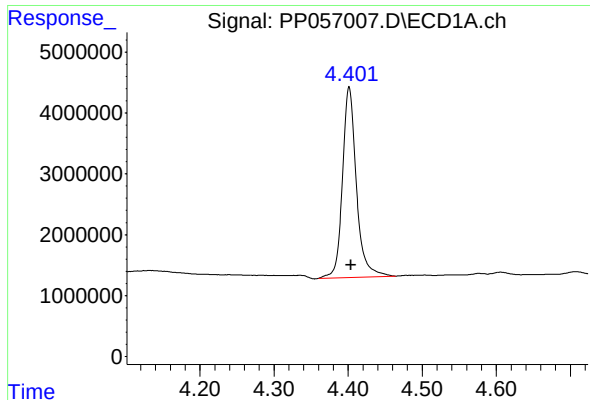


#1 Tetrachloro-m-xylene

R.T.: 4.401 min
Delta R.T.: -0.003 min
Response: 40808834
Conc: 17.07 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-27-8-10-20230411


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/20/2023
Supervised By :Ankita Jodhani 04/20/2023

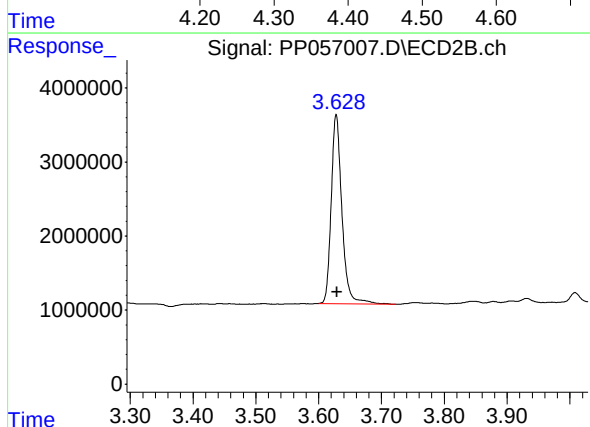


#1 Tetrachloro-m-xylene

R.T.: 3.628 min
Delta R.T.: -0.001 min
Response: 30271576
Conc: 17.04 ng/ml

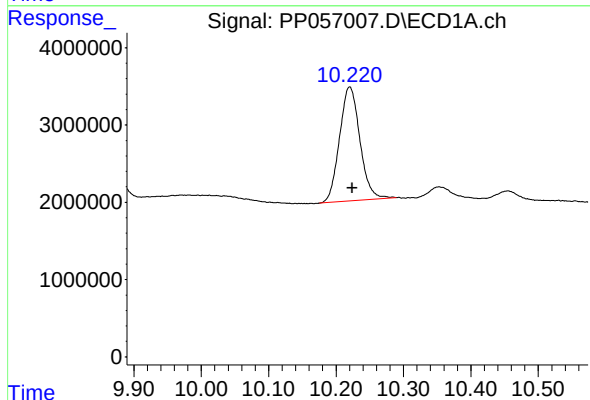

#2 Decachlorobiphenyl

R.T.: 10.220 min
Delta R.T.: -0.004 min
Response: 31081331
Conc: 33.80 ng/ml

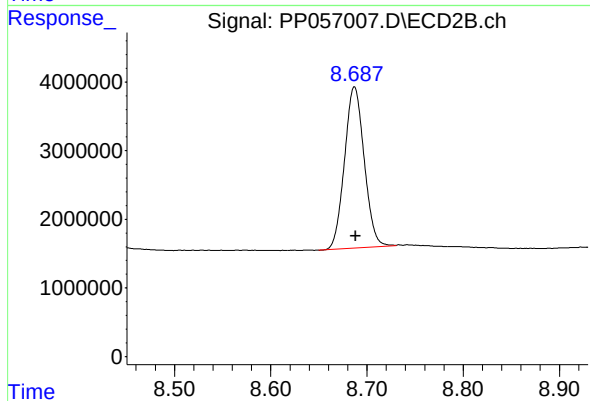

#2 Decachlorobiphenyl

R.T.: 8.687 min
Delta R.T.: 0.000 min
Response: 33490266
Conc: 24.22 ng/ml