

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042022\
 Data File : PP046370.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Apr 2022 19:20
 Operator : YP\AJ
 Sample : N2474-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TMS-JET-GROUT-SPOILS-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 21 08:21:24 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP041222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Apr 21 08:16:42 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.870	3.135	51936825	37058687	21.115	23.322
2) SA Decachlor...	9.956	8.459	29899588	31072356	18.214	21.800

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042022\
Data File : PP046370.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Apr 2022 19:20
Operator : YP\AJ
Sample : N2474-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
TMS-JET-GROUT-SPOILS-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 21 08:21:24 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP041222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 21 08:16:42 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

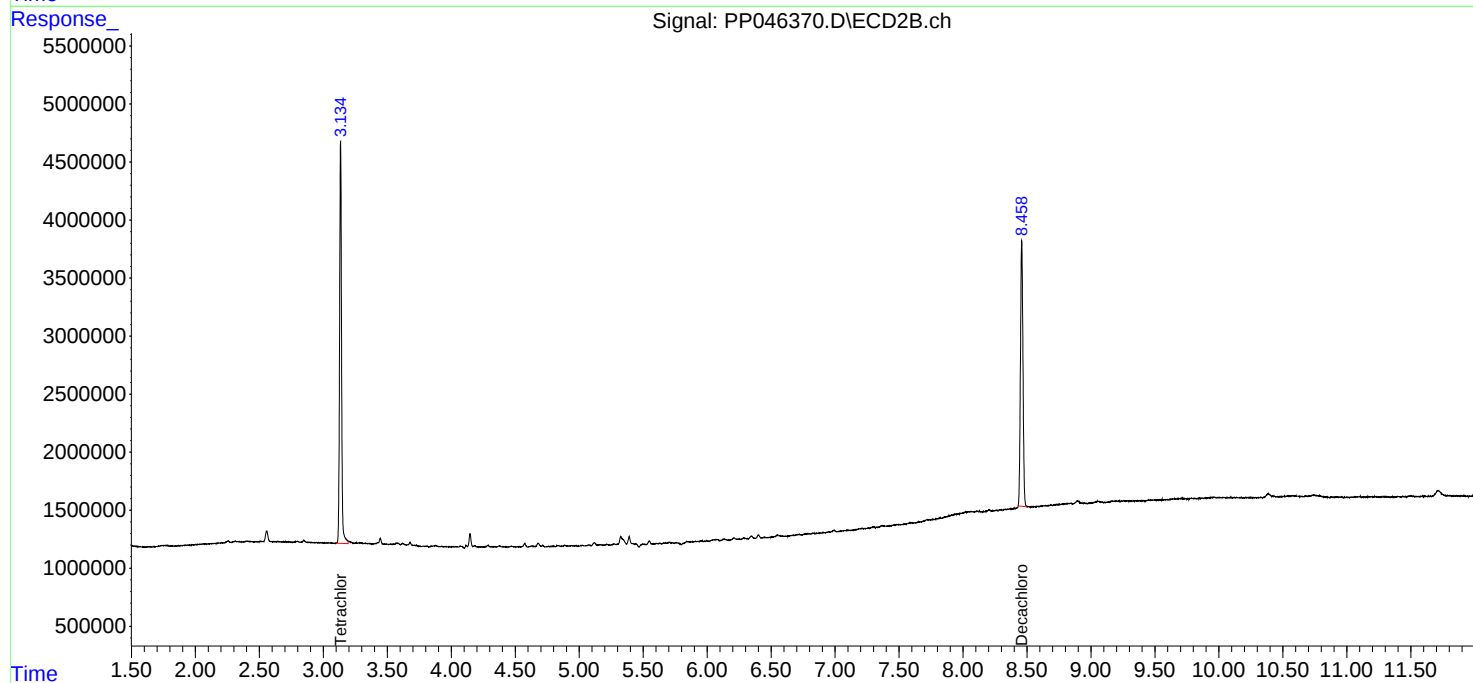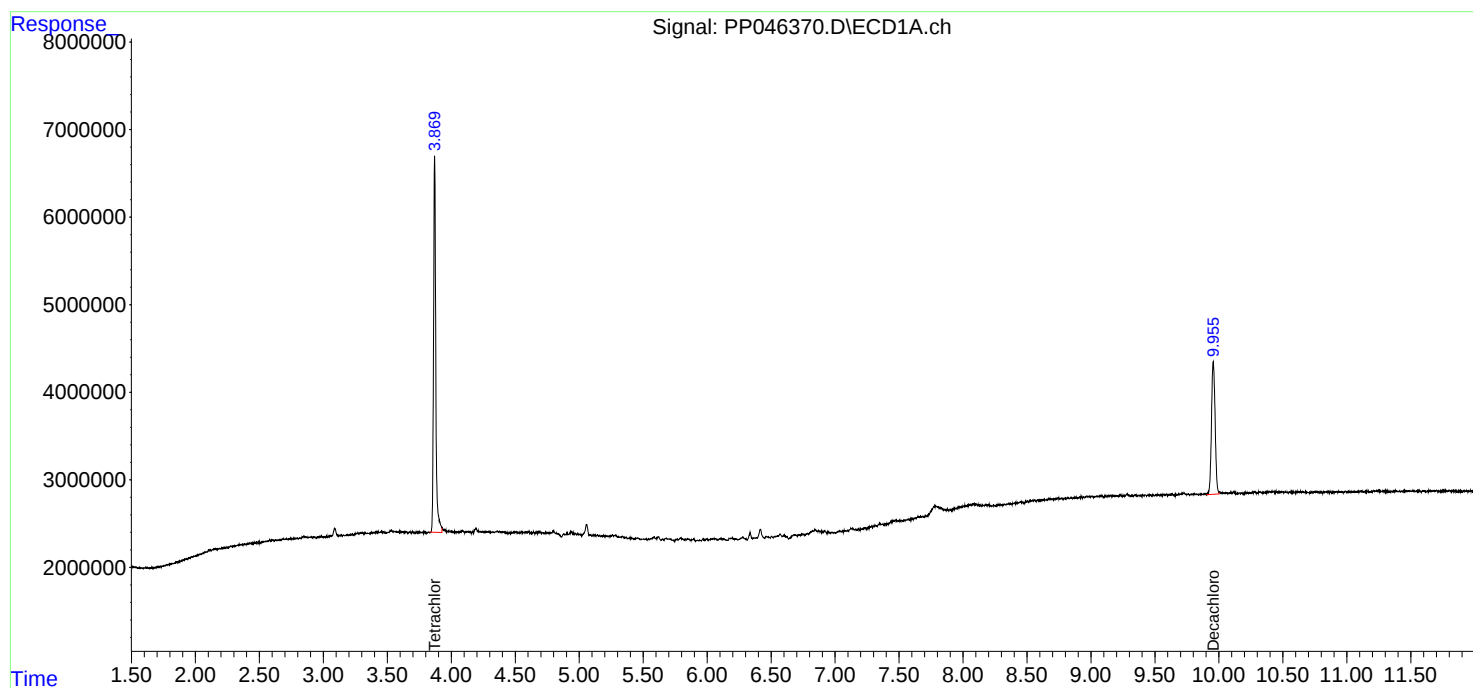


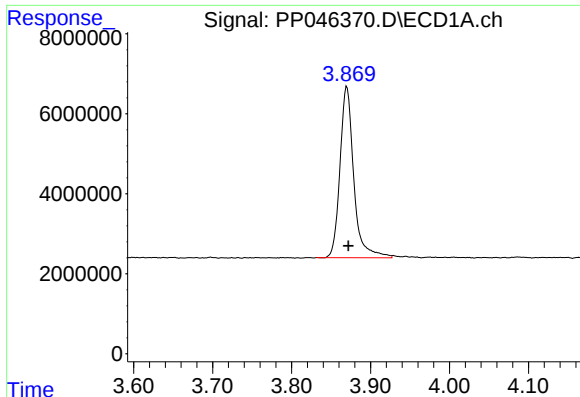

#1 Tetrachloro-m-xylene


R.T.: 3.870 min
Delta R.T.: -0.002 min
Response: 51936825
Conc: 21.12 ng/ml

Instrument :
ECD_P
ClientSampleId :
TMS-JET-GROUT-SPOILS-A

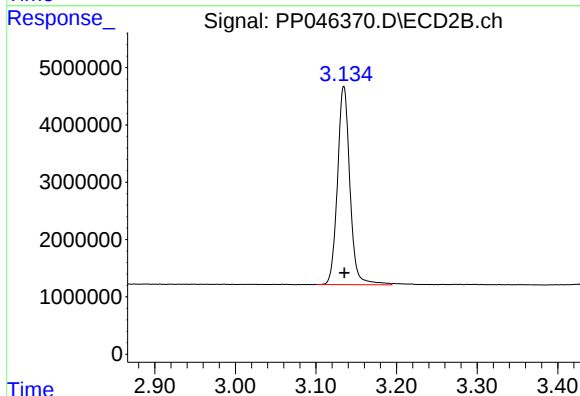


#1 Tetrachloro-m-xylene

R.T.: 3.135 min
Delta R.T.: 0.000 min
Response: 37058687
Conc: 23.32 ng/ml

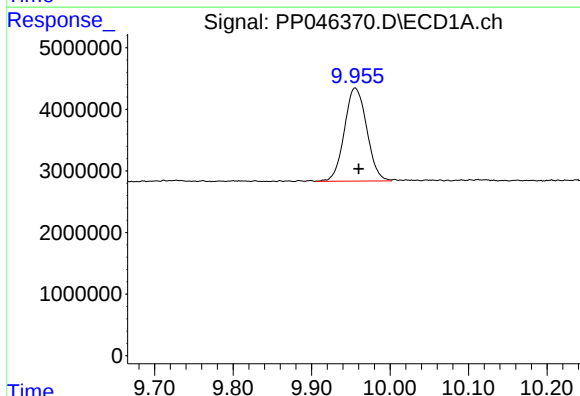

#2 Decachlorobiphenyl

R.T.: 9.956 min
Delta R.T.: -0.004 min
Response: 29899588
Conc: 18.21 ng/ml

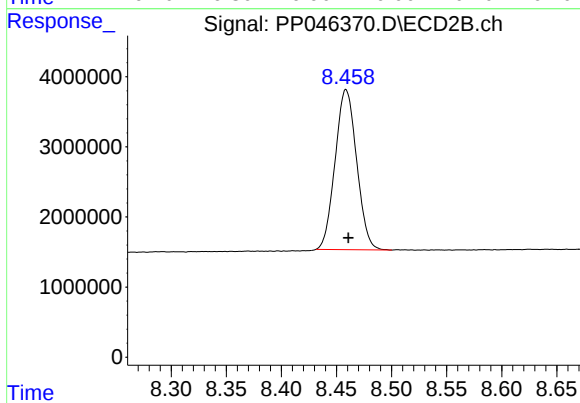

#2 Decachlorobiphenyl

R.T.: 8.459 min
Delta R.T.: -0.002 min
Response: 31072356
Conc: 21.80 ng/ml