

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042022\
 Data File : PP046378.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Apr 2022 23:36
 Operator : YP\AJ
 Sample : N2476-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PAT-02-041922

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/21/2022
 Supervised By :mohammad ahmed 04/21/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 21 08:34:21 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP041222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Apr 21 08:16:42 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.868	3.134	38270957	34274332	15.559m	21.570 #
2) SA Decachlor...	9.954	8.459	24723787	23615483	15.061	16.569

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042022\
Data File : PP046378.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Apr 2022 23:36
Operator : YP\AJ
Sample : N2476-03
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
PAT-02-041922


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/21/2022
Supervised By :mohammad ahmed 04/21/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 21 08:34:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP041222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 21 08:16:42 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

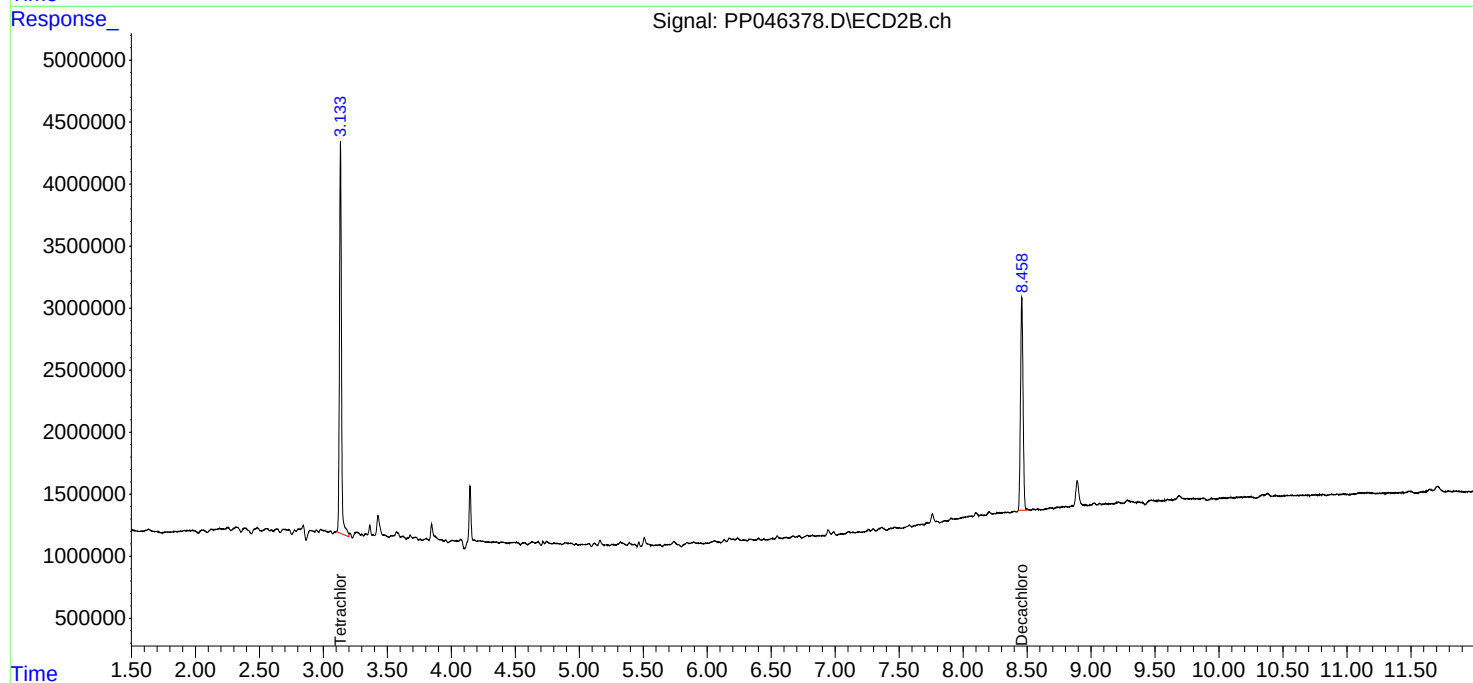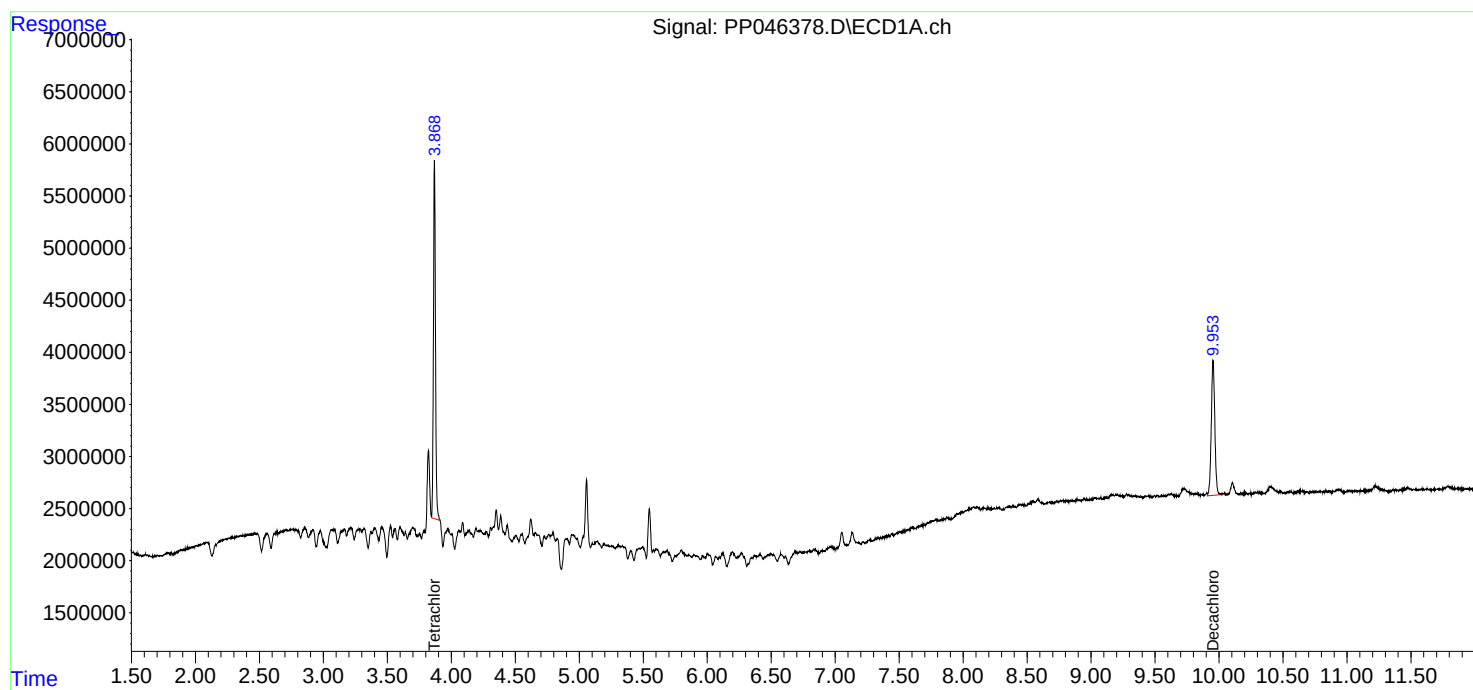

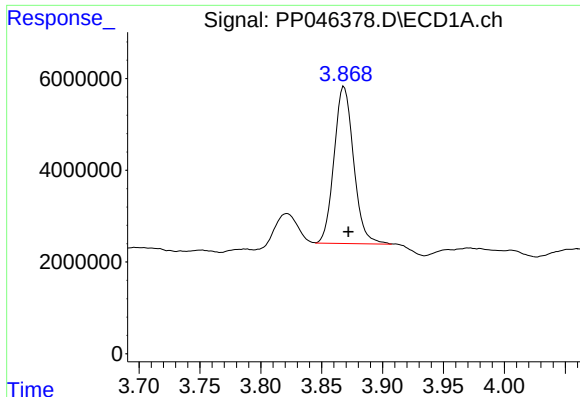


#1 Tetrachloro-m-xylene

R.T.: 3.868 min
Delta R.T.: -0.004 min
Response: 38270957
Conc: 15.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
PAT-02-041922


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/21/2022
Supervised By :mohammad ahmed 04/21/2022

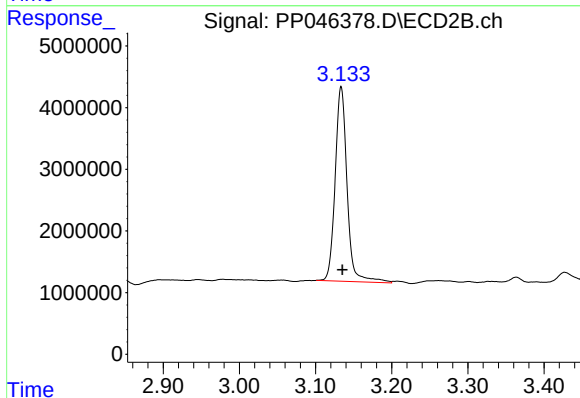


#1 Tetrachloro-m-xylene

R.T.: 3.134 min
Delta R.T.: -0.001 min
Response: 34274332
Conc: 21.57 ng/ml

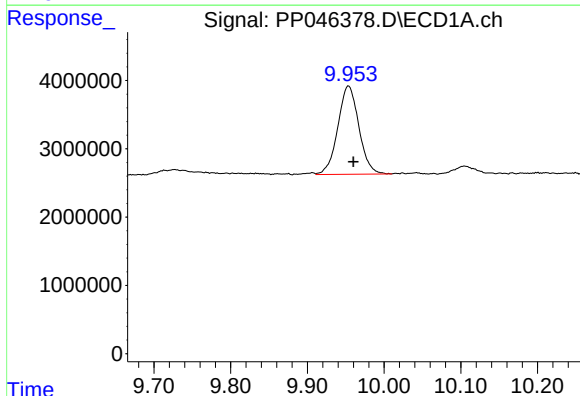

#2 Decachlorobiphenyl

R.T.: 9.954 min
Delta R.T.: -0.007 min
Response: 24723787
Conc: 15.06 ng/ml

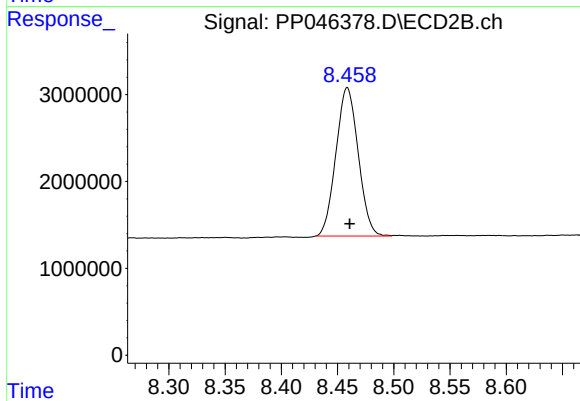

#2 Decachlorobiphenyl

R.T.: 8.459 min
Delta R.T.: -0.002 min
Response: 23615483
Conc: 16.57 ng/ml