

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042022\
 Data File : PP046379.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Apr 2022 23:51
 Operator : YP\AJ
 Sample : N2476-05
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PAT-03-041922

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/21/2022
 Supervised By :mohammad ahmed 04/21/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 21 08:35:53 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP041222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Apr 21 08:16:42 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.867	3.133	34396039	32255289	13.984m	20.299 #
2) SA Decachlor...	9.955	8.459	24648963	23853761	15.015	16.736

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042022\
Data File : PP046379.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Apr 2022 23:51
Operator : YP\AJ
Sample : N2476-05
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
PAT-03-041922


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/21/2022
Supervised By :mohammad ahmed 04/21/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 21 08:35:53 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP041222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 21 08:16:42 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

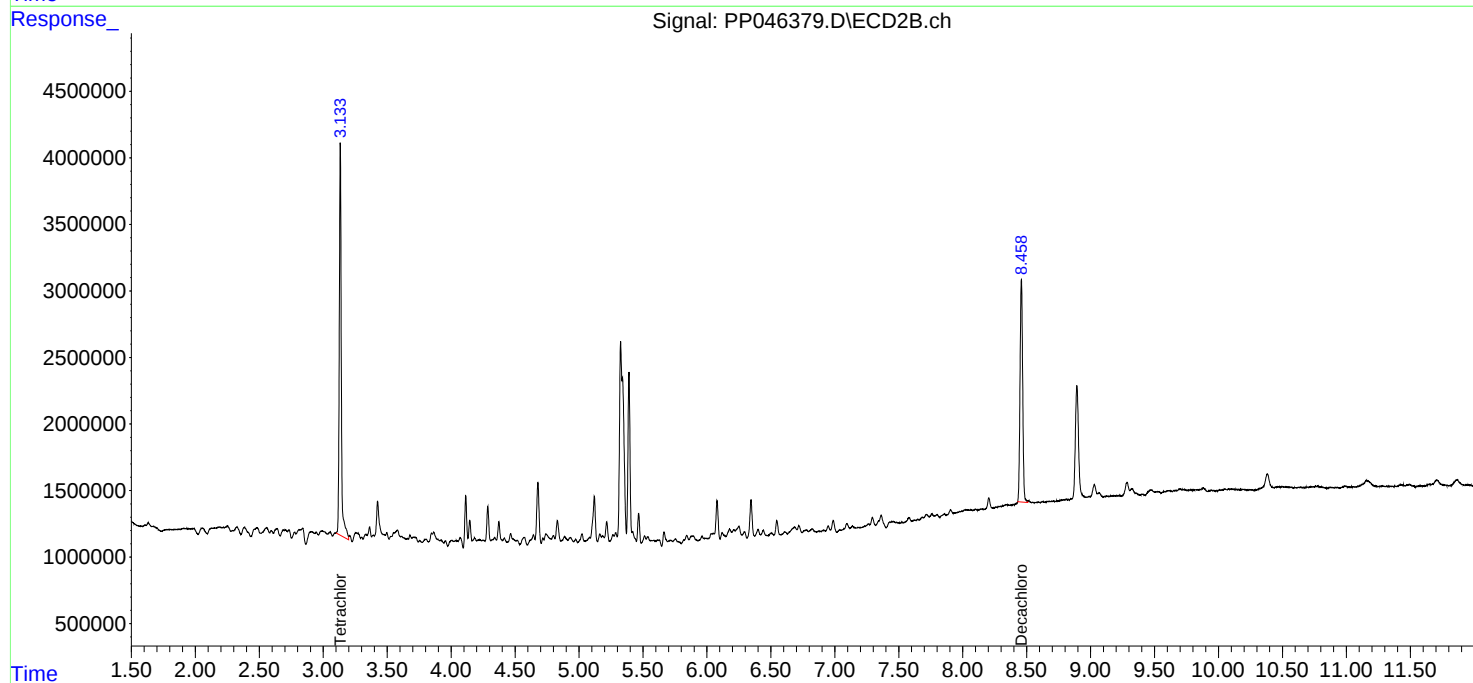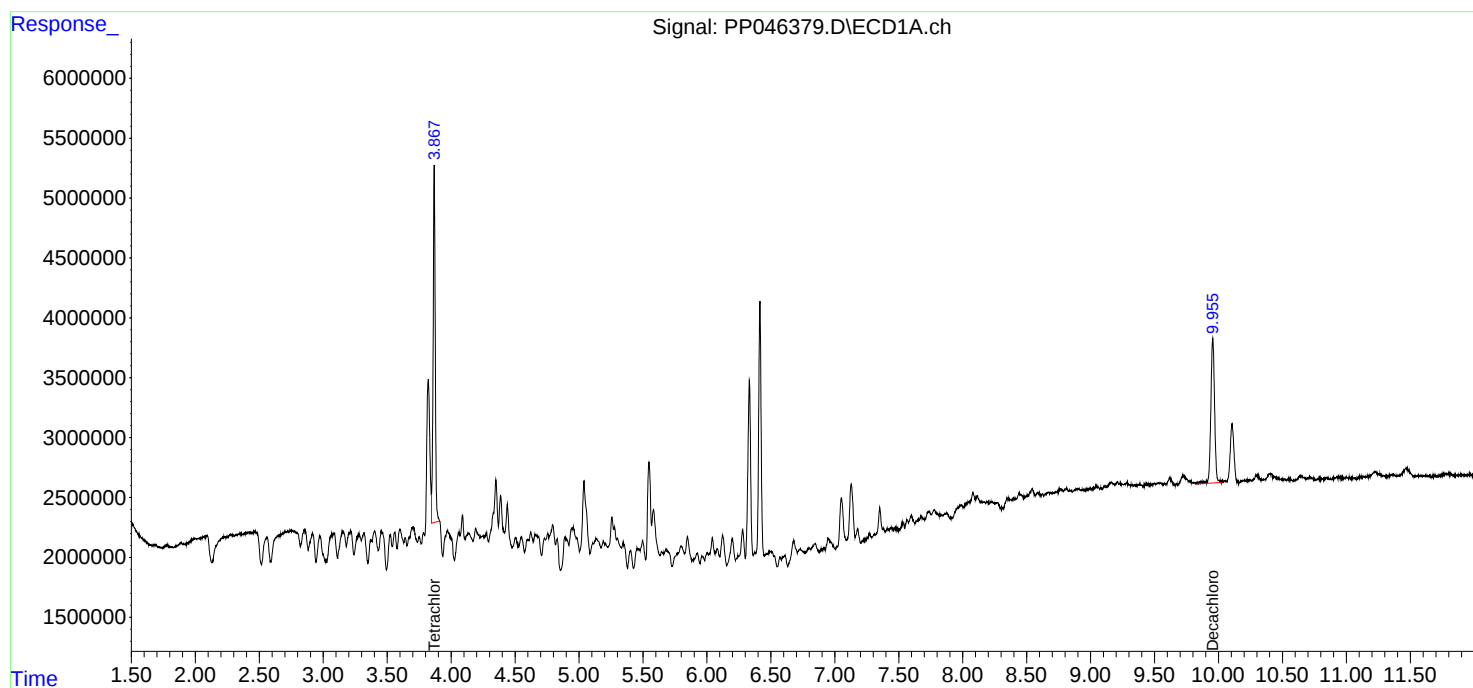

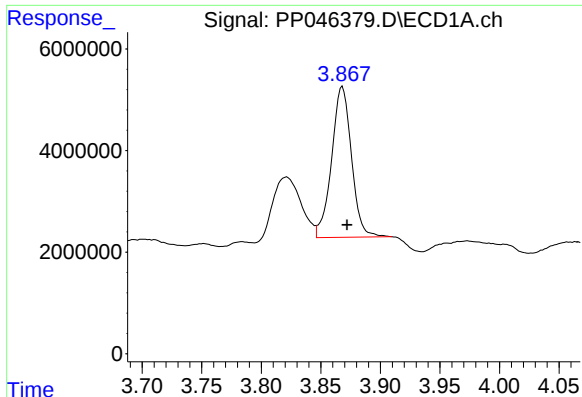


#1 Tetrachloro-m-xylene

R.T.: 3.867 min
Delta R.T.: -0.005 min
Response: 34396039
Conc: 13.98 ng/ml

Instrument :
ECD_P
ClientSampleId :
PAT-03-041922


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/21/2022
Supervised By :mohammad ahmed 04/21/2022

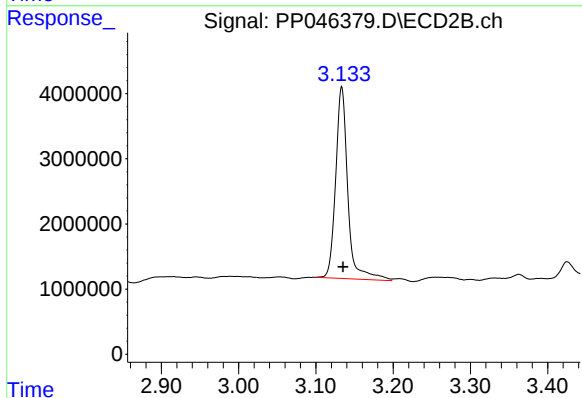


#1 Tetrachloro-m-xylene

R.T.: 3.133 min
Delta R.T.: -0.002 min
Response: 32255289
Conc: 20.30 ng/ml

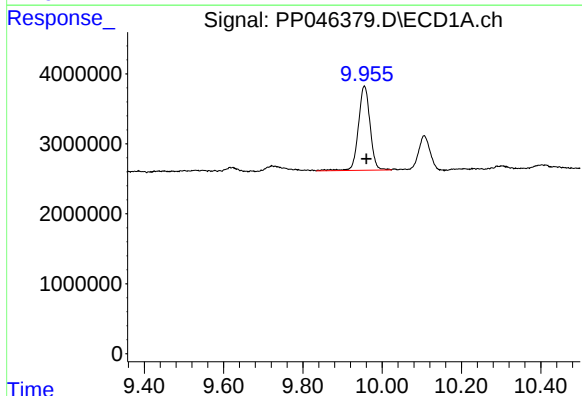

#2 Decachlorobiphenyl

R.T.: 9.955 min
Delta R.T.: -0.005 min
Response: 24648963
Conc: 15.02 ng/ml

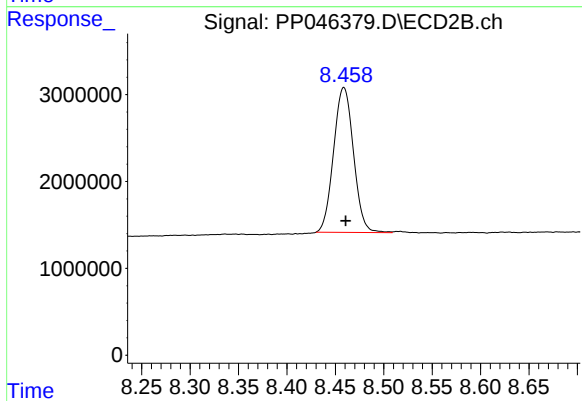

#2 Decachlorobiphenyl

R.T.: 8.459 min
Delta R.T.: -0.002 min
Response: 23853761
Conc: 16.74 ng/ml