

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042022\
 Data File : PP046396.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Apr 2022 06:25
 Operator : YP\AJ
 Sample : N2468-07RE
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 WC-15-1-7RE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/21/2022
 Supervised By :mohammad ahmed 04/21/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 21 09:15:13 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP041222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Apr 21 08:16:42 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.872	3.137	32605705	27071833	13.256m	17.037m#
2) SA Decachlor...	9.985f	8.488f	24599528	21767799	14.985m	15.272m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042022\
Data File : PP046396.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Apr 2022 06:25
Operator : YP\AJ
Sample : N2468-07RE
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
WC-15-1-7RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/21/2022
Supervised By :mohammad ahmed 04/21/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 21 09:15:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP041222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 21 08:16:42 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

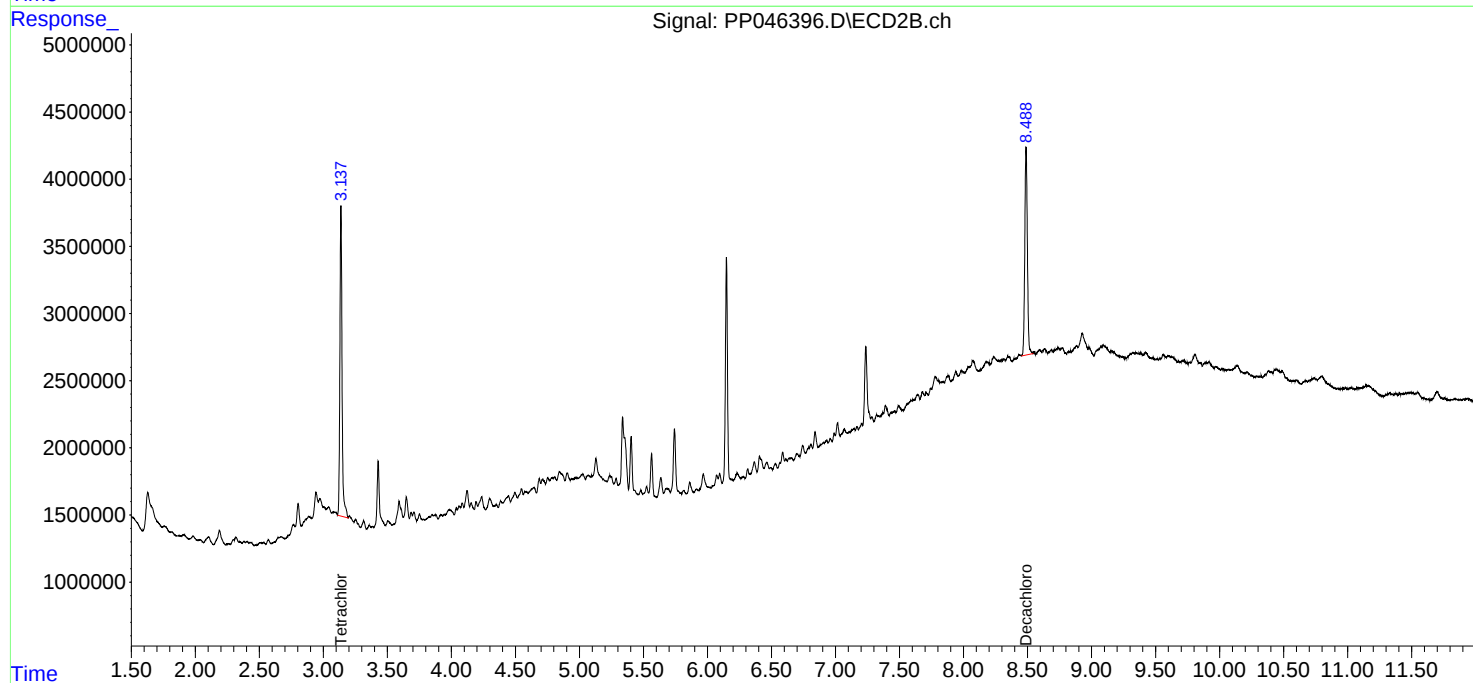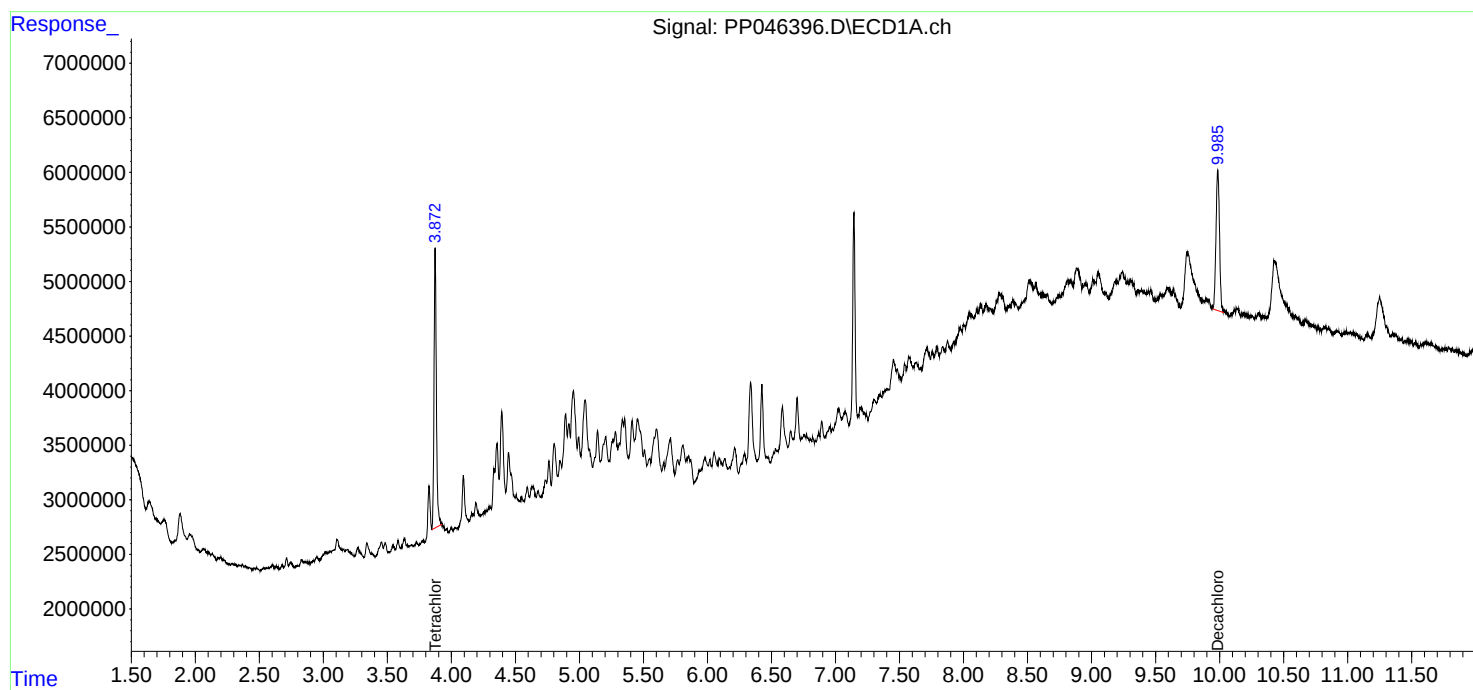

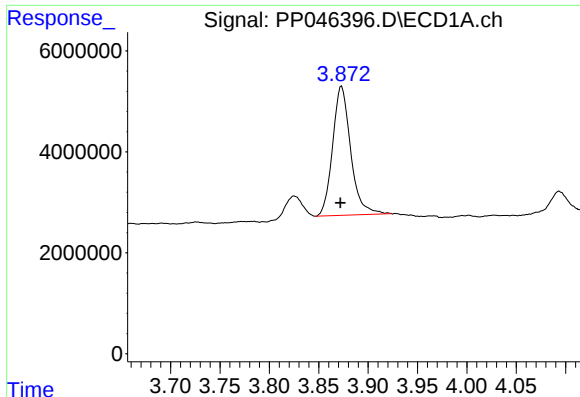


#1 Tetrachloro-m-xylene

R.T.: 3.872 min
Delta R.T.: 0.000 min
Response: 32605705
Conc: 13.26 ng/ml

Instrument :
ECD_P
ClientSampleId :
WC-15-1-7RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/21/2022
Supervised By :mohammad ahmed 04/21/2022

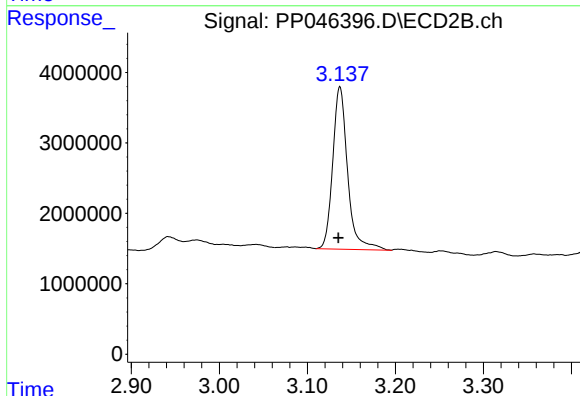


#1 Tetrachloro-m-xylene

R.T.: 3.137 min
Delta R.T.: 0.001 min
Response: 27071833
Conc: 17.04 ng/ml m

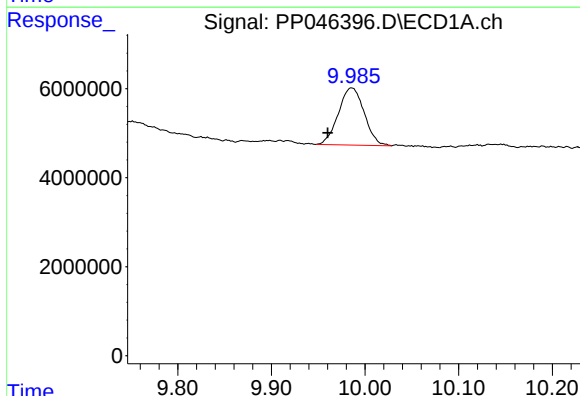

#2 Decachlorobiphenyl

R.T.: 9.985 min
Delta R.T.: 0.025 min
Response: 24599528
Conc: 14.99 ng/ml m

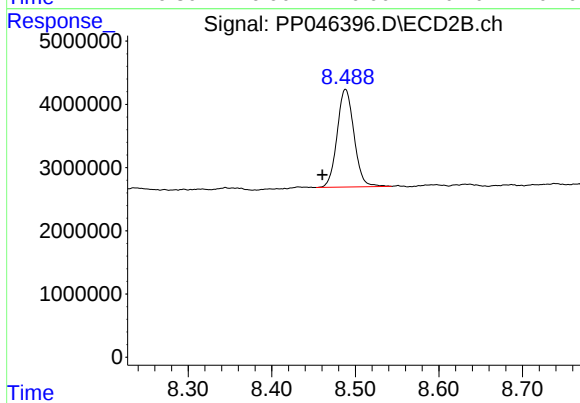

#2 Decachlorobiphenyl

R.T.: 8.488 min
Delta R.T.: 0.027 min
Response: 21767799
Conc: 15.27 ng/ml m