

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042022\
 Data File : PP046397.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Apr 2022 06:41
 Operator : YP\AJ
 Sample : N2468-11RE
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 WC-15-1-8RE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/21/2022
 Supervised By :mohammad ahmed 04/21/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 21 09:17:12 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP041222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Apr 21 08:16:42 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.873	3.138	32085511	27891139	13.045m	17.553 #
2) SA Decachlor...	9.984f	8.488f	26001217	20147792	15.839	14.136

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042022\
Data File : PP046397.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Apr 2022 06:41
Operator : YP\AJ
Sample : N2468-11RE
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
WC-15-1-8RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/21/2022
Supervised By :mohammad ahmed 04/21/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 21 09:17:12 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP041222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 21 08:16:42 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

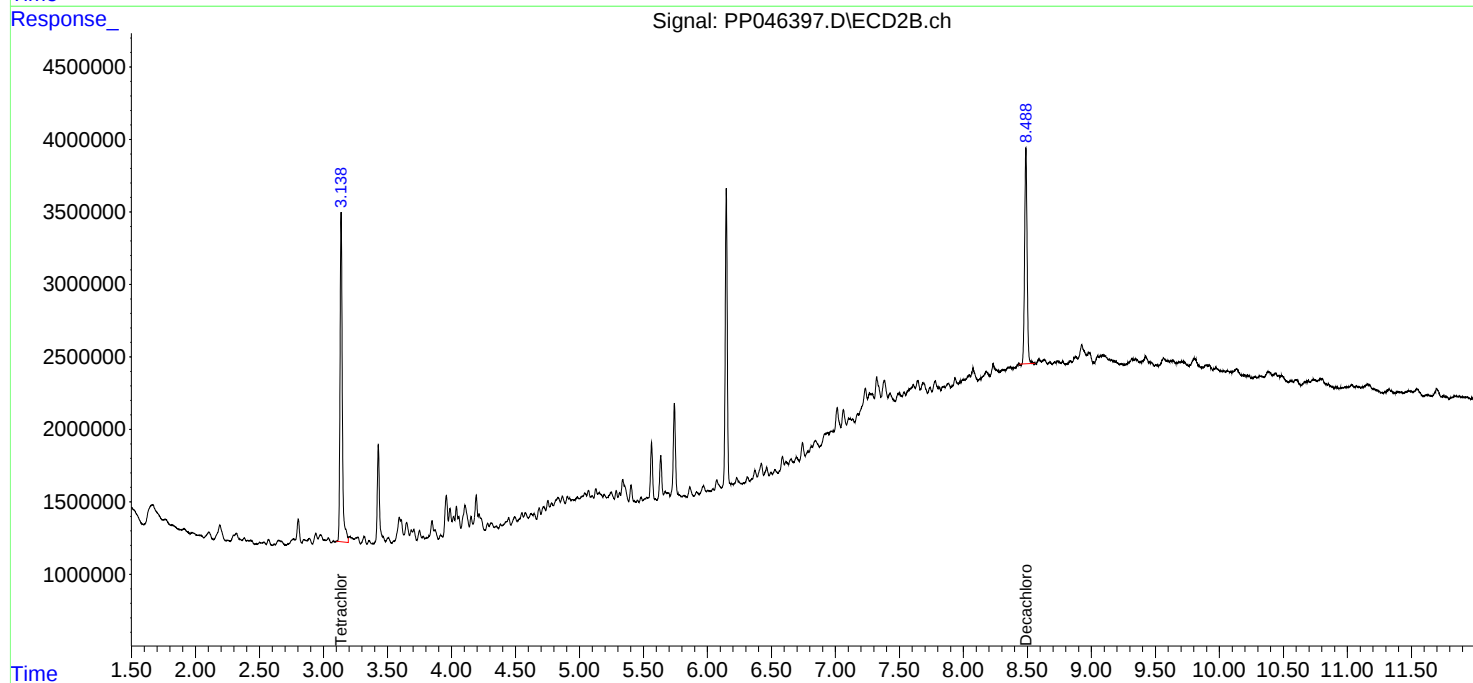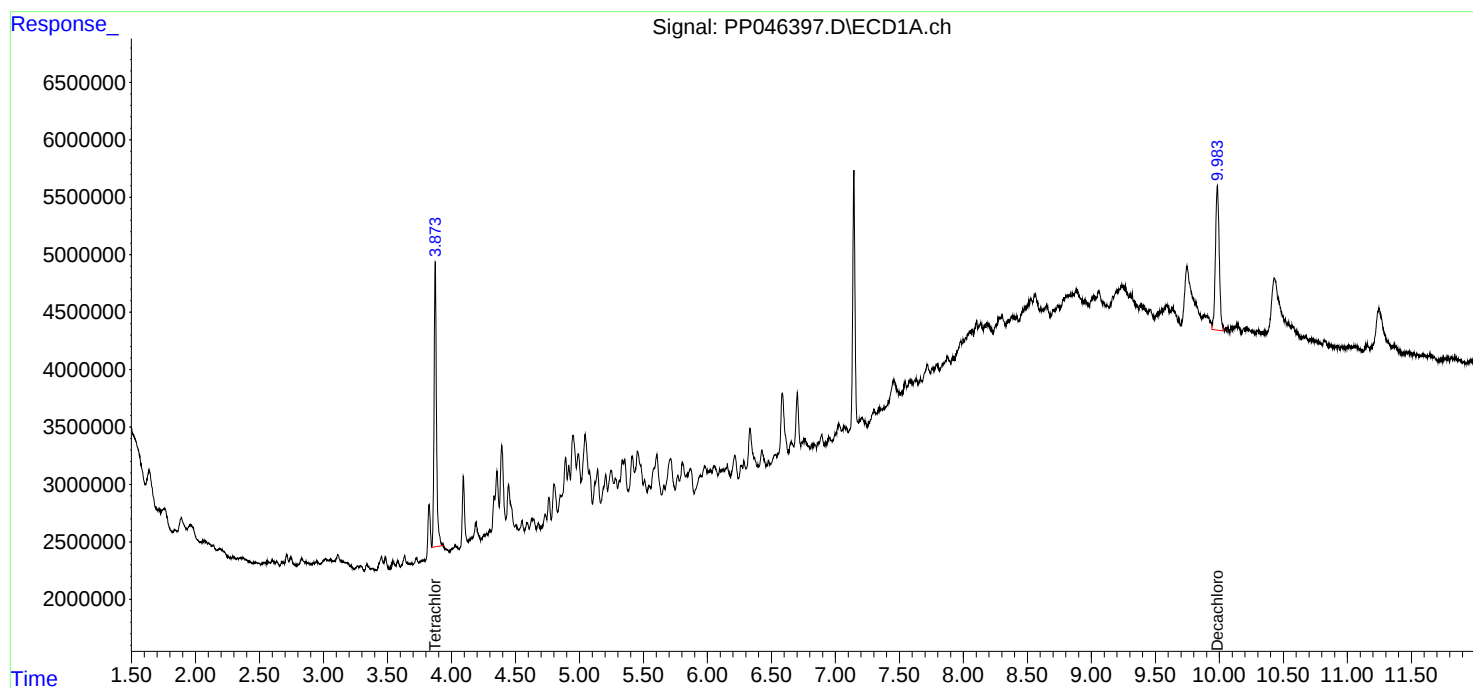

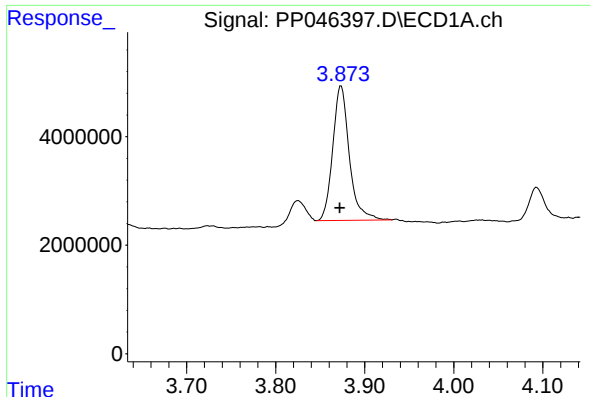


#1 Tetrachloro-m-xylene

R.T.: 3.873 min
Delta R.T.: 0.000 min
Response: 32085511
Conc: 13.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
WC-15-1-8RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/21/2022
Supervised By :mohammad ahmed 04/21/2022

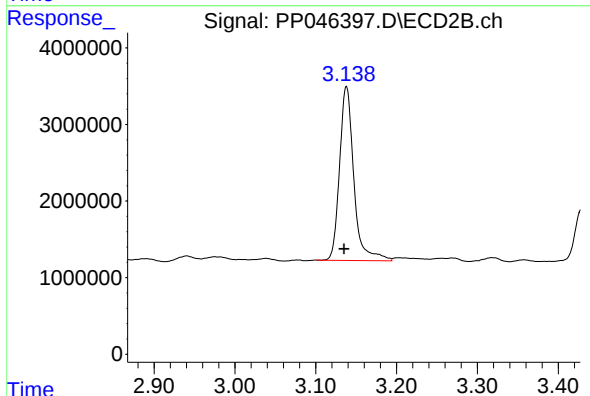


#1 Tetrachloro-m-xylene

R.T.: 3.138 min
Delta R.T.: 0.003 min
Response: 27891139
Conc: 17.55 ng/ml

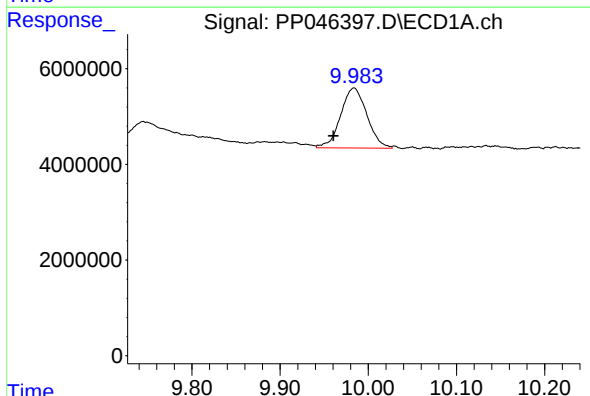

#2 Decachlorobiphenyl

R.T.: 9.984 min
Delta R.T.: 0.024 min
Response: 26001217
Conc: 15.84 ng/ml

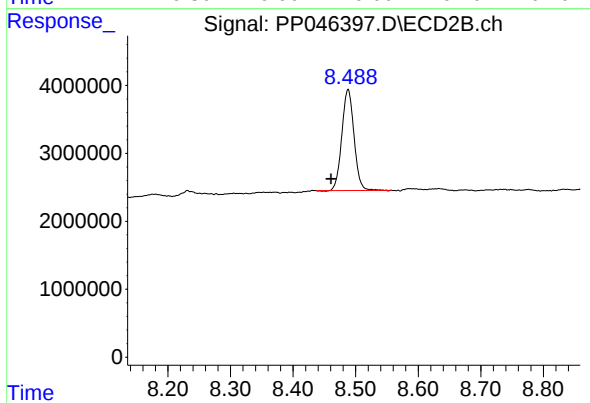

#2 Decachlorobiphenyl

R.T.: 8.488 min
Delta R.T.: 0.027 min
Response: 20147792
Conc: 14.14 ng/ml