

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042023\
 Data File : PP057045.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Apr 2023 10:31
 Operator : YP\AJ
 Sample : AR1221ICC500
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1221ICC500

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/21/2023
 Supervised By :Ankita Jodhani 04/21/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 20 12:29:51 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042023.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Apr 20 12:29:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.404	3.631	114.8E6	87218689	50.000	50.012m
2) SA Decachlor...	10.217	8.686	80692156	89969427	50.000	50.000
Target Compounds						
8) L2 AR-1221-1	4.613	3.847	13347456	10671999	500.000	500.000
9) L2 AR-1221-2	4.699	3.933	9731040	8040577	500.000	500.000
10) L2 AR-1221-3	4.776	4.010	29322432	24577783	500.000	500.000

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042023\
Data File : PP057045.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Apr 2023 10:31
Operator : YP\AJ
Sample : AR1221ICC500
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1221ICC500


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/21/2023
Supervised By :Ankita Jodhani 04/21/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 20 12:29:51 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042023.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 20 12:29:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

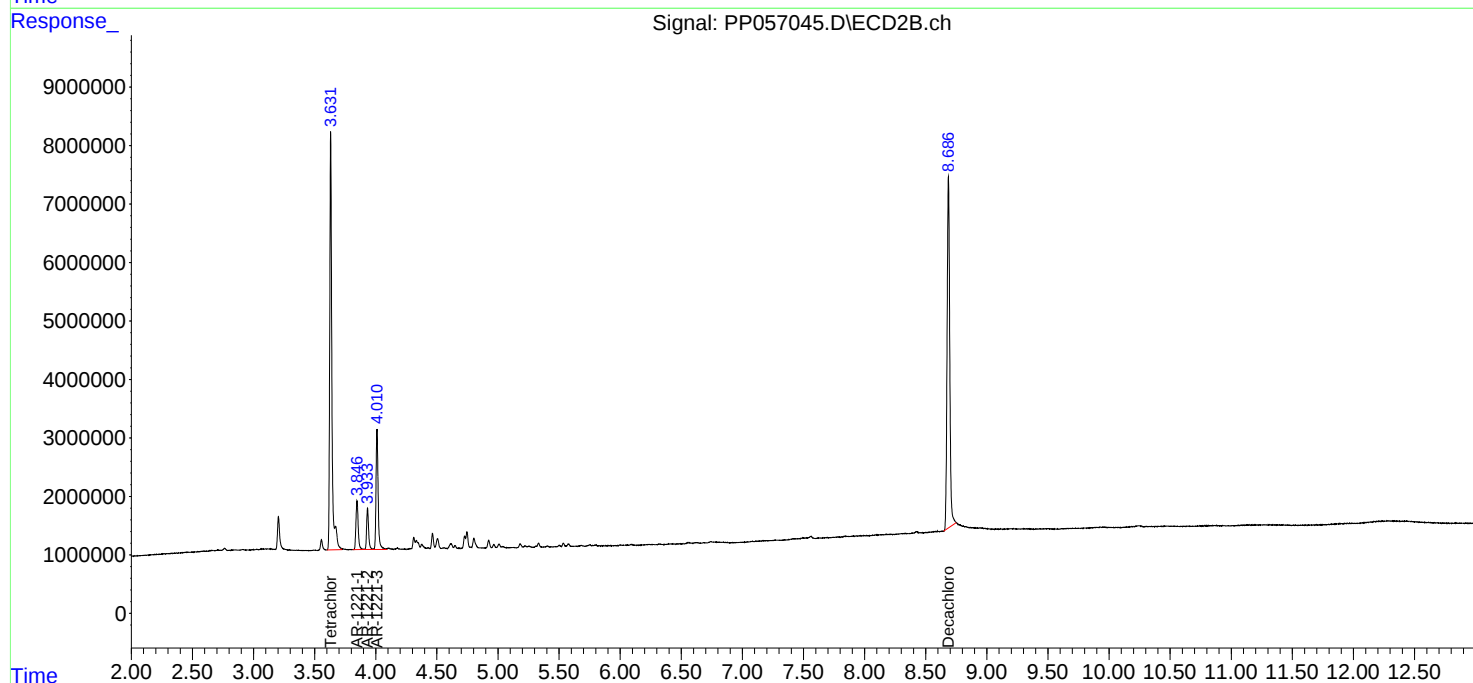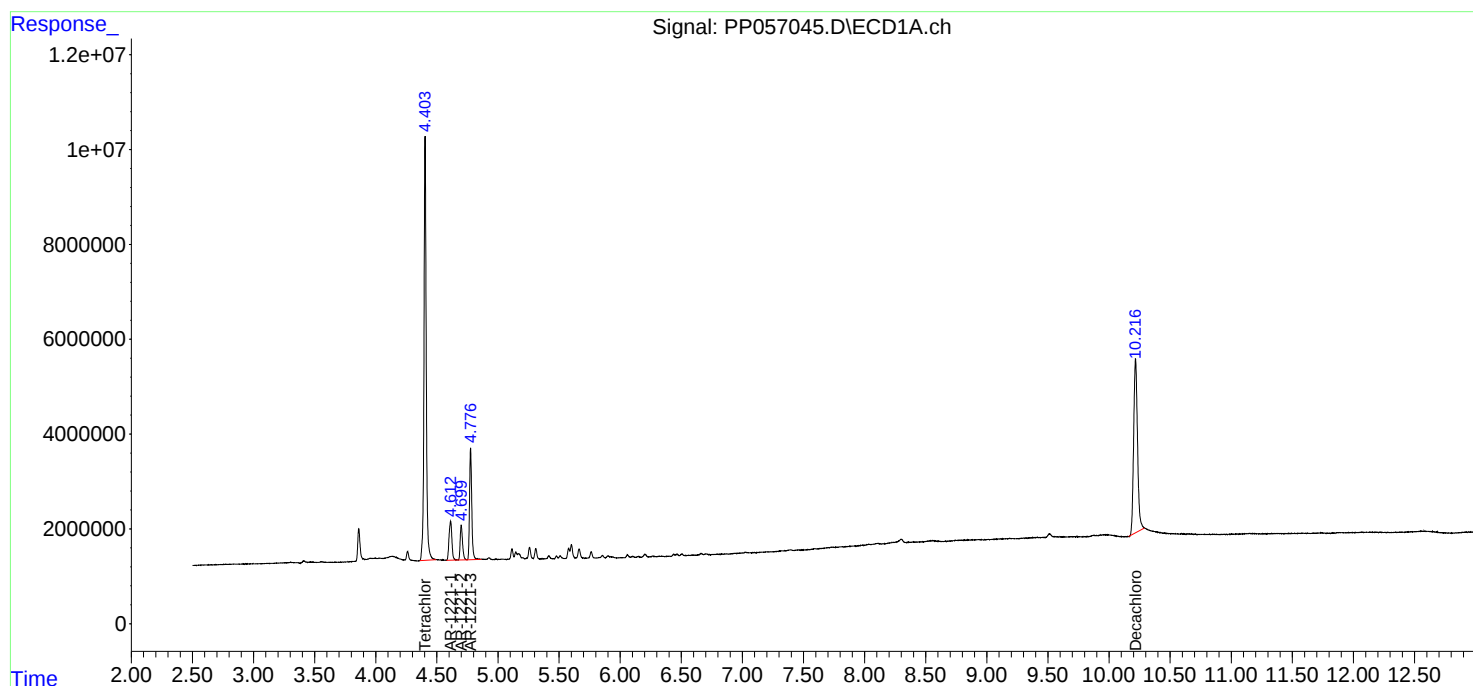

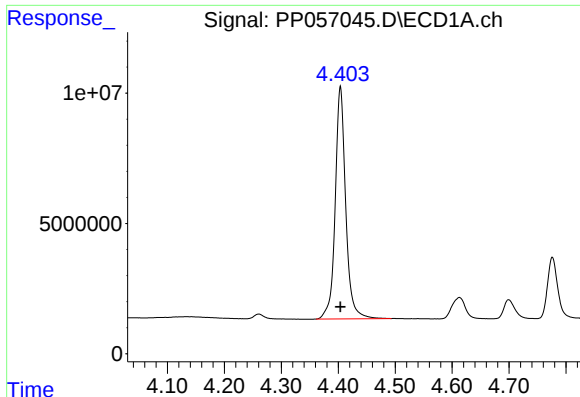


#1 Tetrachloro-m-xylene

R.T.: 4.404 min
Delta R.T.: 0.000 min
Response: 114822850
Conc: 50.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1221ICC500


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/21/2023
Supervised By :Ankita Jodhani 04/21/2023

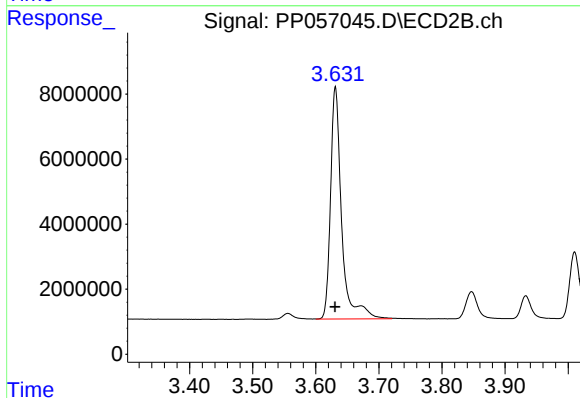


#1 Tetrachloro-m-xylene

R.T.: 3.631 min
Delta R.T.: 0.000 min
Response: 87218689
Conc: 50.01 ng/ml m

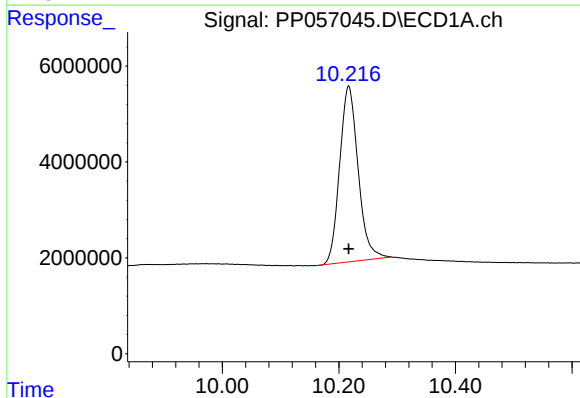


#2 Decachlorobiphenyl

R.T.: 10.217 min
Delta R.T.: 0.000 min
Response: 80692156
Conc: 50.00 ng/ml

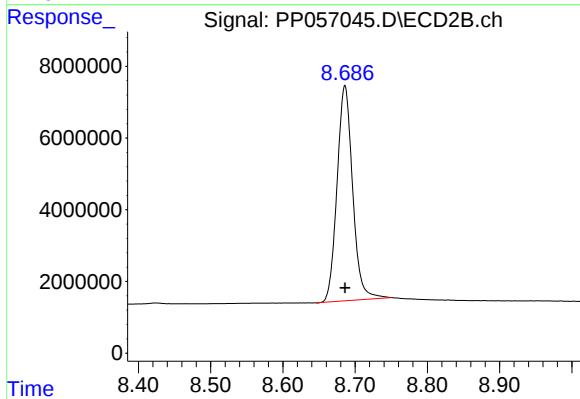

#2 Decachlorobiphenyl

R.T.: 8.686 min
Delta R.T.: 0.000 min
Response: 89969427
Conc: 50.00 ng/ml

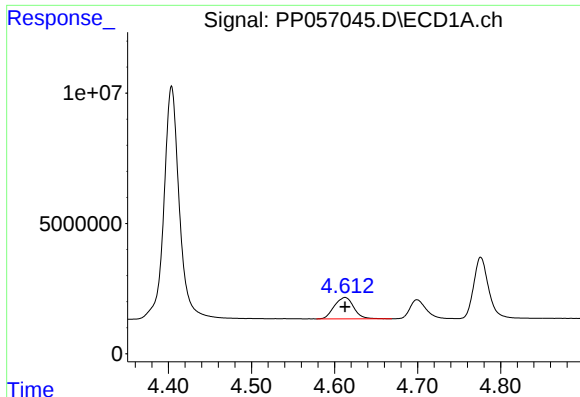


#8 AR-1221-1

R.T.: 4.613 min
Delta R.T.: 0.000 min
Response: 13347456
Conc: 500.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1221ICC500


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/21/2023
Supervised By :Ankita Jodhani 04/21/2023

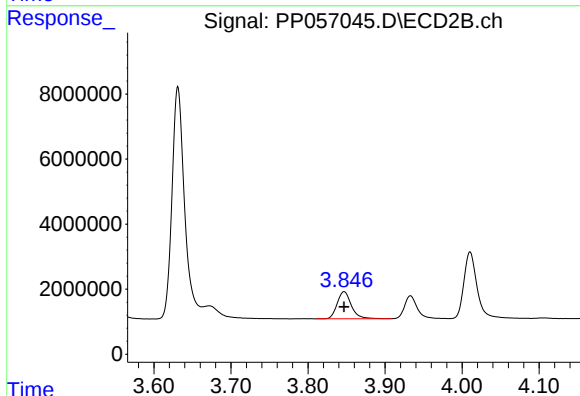


#8 AR-1221-1

R.T.: 3.847 min
Delta R.T.: 0.000 min
Response: 10671999
Conc: 500.00 ng/ml

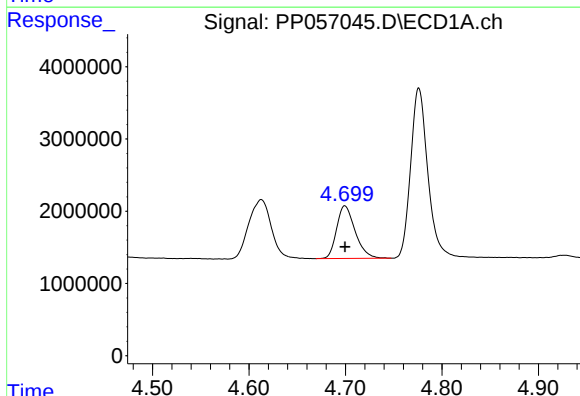


#9 AR-1221-2

R.T.: 4.699 min
Delta R.T.: 0.000 min
Response: 9731040
Conc: 500.00 ng/ml

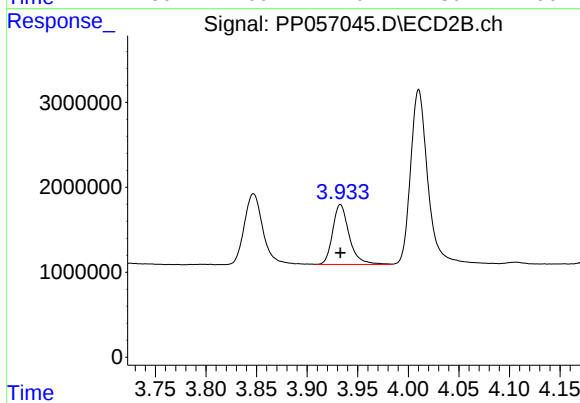

#9 AR-1221-2

R.T.: 3.933 min
Delta R.T.: 0.000 min
Response: 8040577
Conc: 500.00 ng/ml

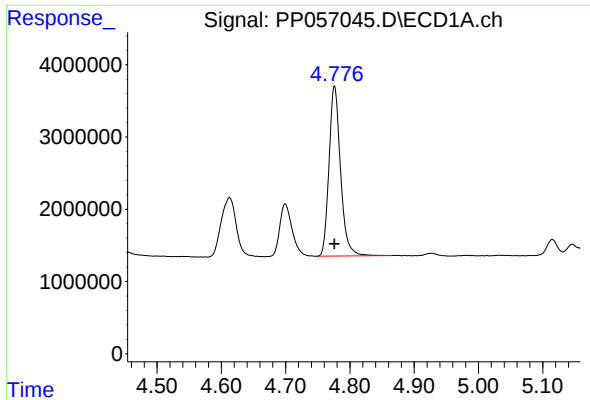


#10 AR-1221-3

R.T.: 4.776 min
Delta R.T.: 0.000 min
Response: 29322432
Conc: 500.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1221ICC500

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/21/2023
Supervised By :Ankita Jodhani 04/21/2023

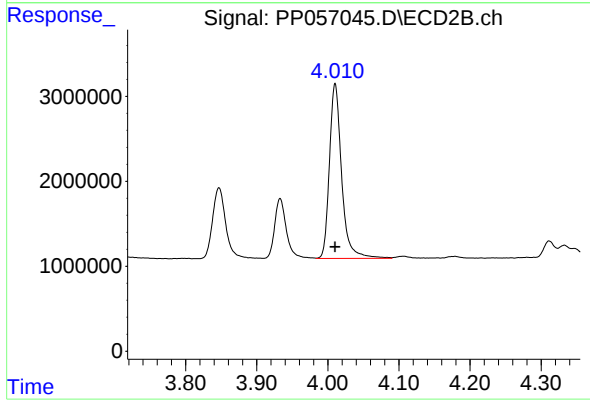

#10 AR-1221-3

R.T.: 4.010 min
Delta R.T.: 0.000 min
Response: 24577783
Conc: 500.00 ng/ml