

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042023\
 Data File : PP057081.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Apr 2023 20:29
 Operator : YP\AJ
 Sample : 02420-01 10X
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HEE193L-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/21/2023
 Supervised By :Ankita Jodhani 04/21/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 21 01:13:33 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042023.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Apr 20 16:59:40 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.404	3.630	3973353	2907067	1.796	1.721m
2) SA Decachlor...	10.218	8.687	3836906	3559865	2.391	1.990

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042023\
Data File : PP057081.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Apr 2023 20:29
Operator : YP\AJ
Sample : 02420-01 10X
Misc :
ALS Vial : 39 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
HEE193L-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/21/2023
Supervised By :Ankita Jodhani 04/21/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 21 01:13:33 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042023.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 20 16:59:40 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

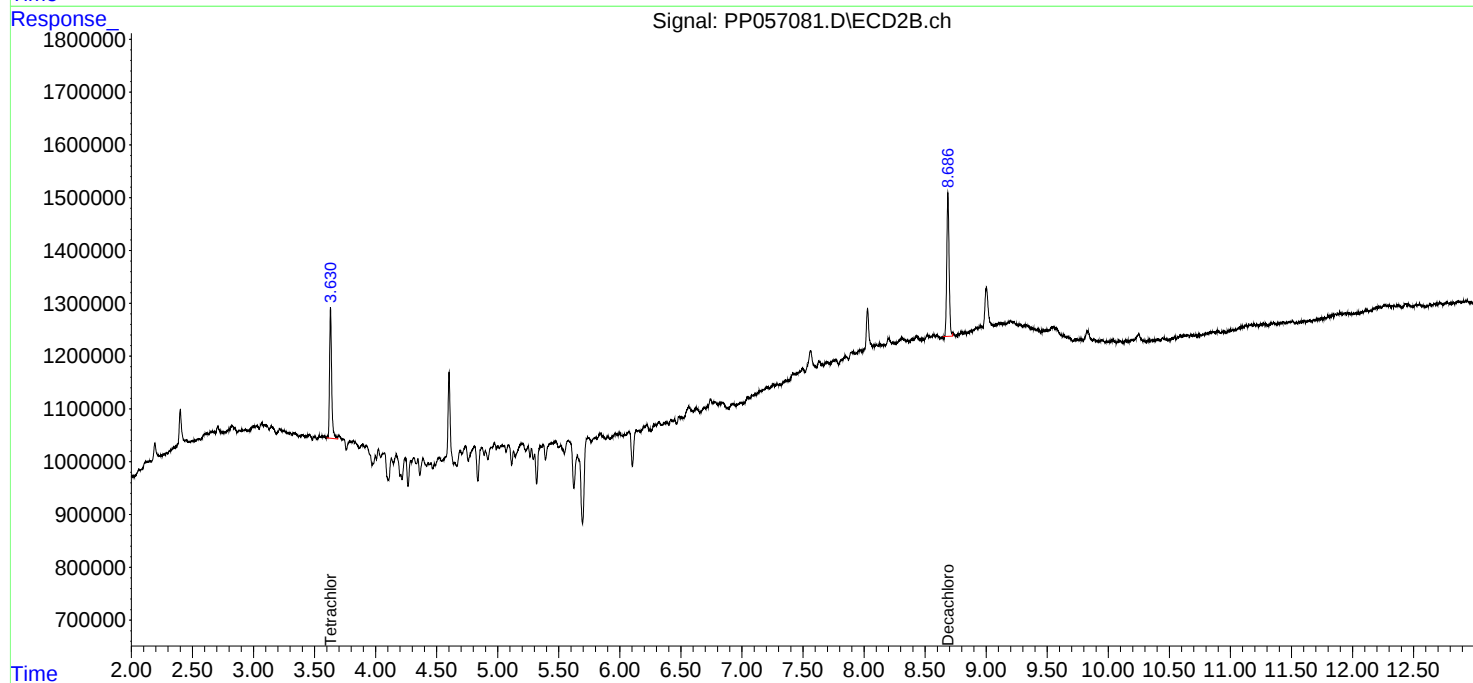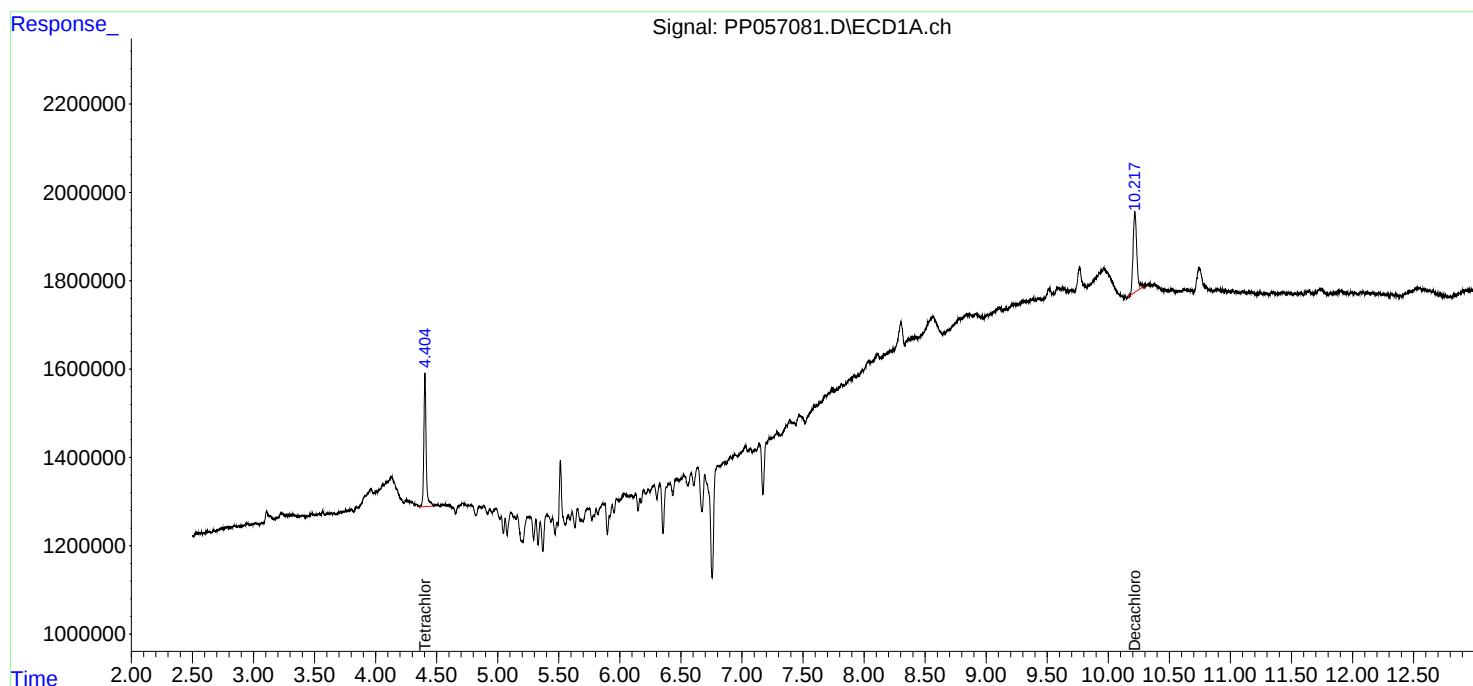

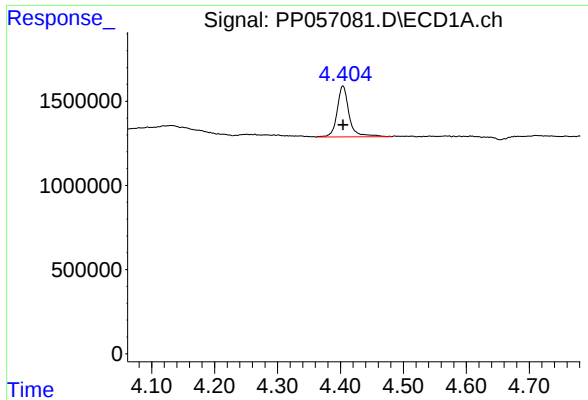


#1 Tetrachloro-m-xylene

R.T.: 4.404 min
Delta R.T.: 0.000 min
Response: 3973353
Conc: 1.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEE193L-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/21/2023
Supervised By :Ankita Jodhani 04/21/2023

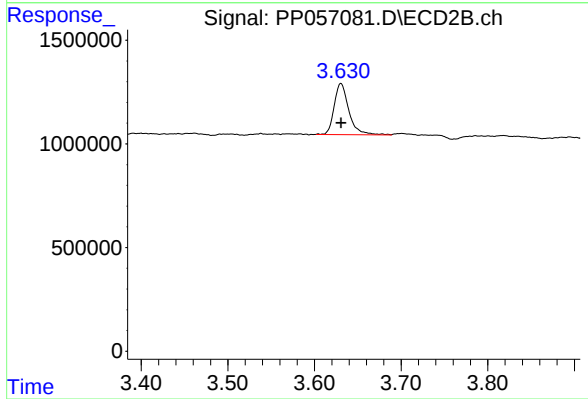


#1 Tetrachloro-m-xylene

R.T.: 3.630 min
Delta R.T.: 0.000 min
Response: 2907067
Conc: 1.72 ng/ml m

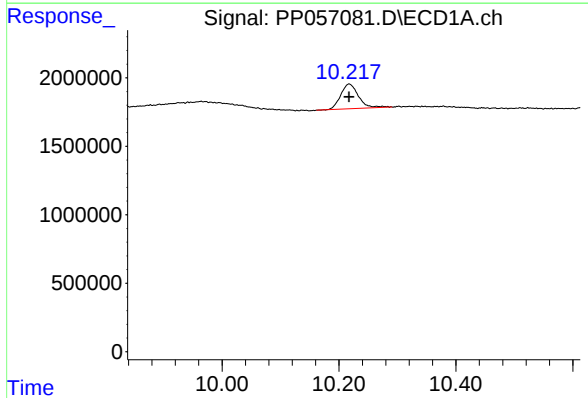

#2 Decachlorobiphenyl

R.T.: 10.218 min
Delta R.T.: 0.000 min
Response: 3836906
Conc: 2.39 ng/ml

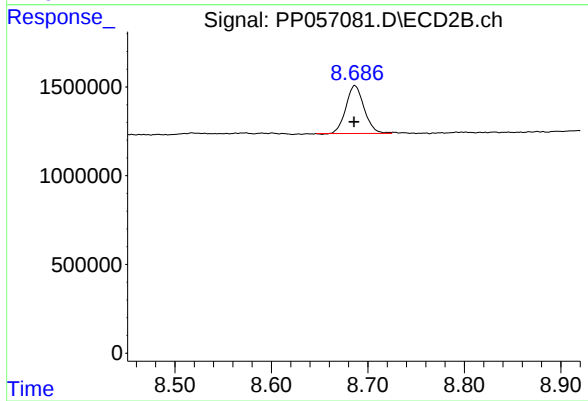

#2 Decachlorobiphenyl

R.T.: 8.687 min
Delta R.T.: 0.000 min
Response: 3559865
Conc: 1.99 ng/ml