

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042023\
 Data File : PP057112.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Apr 2023 06:07
 Operator : YP\AJ
 Sample : 02422-08 10X
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SOM041923R-END-2-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 21 07:10:42 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042023.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Apr 20 16:59:40 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.403	3.631	2740656	2732624	1.239	1.618 #
2) SA Decachlor...	10.221	8.689	3292006	2693475	2.051	1.506 #

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042023\
Data File : PP057112.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Apr 2023 06:07
Operator : YP\AJ
Sample : 02422-08 10X
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
SOM041923R-END-2-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 21 07:10:42 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042023.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 20 16:59:40 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

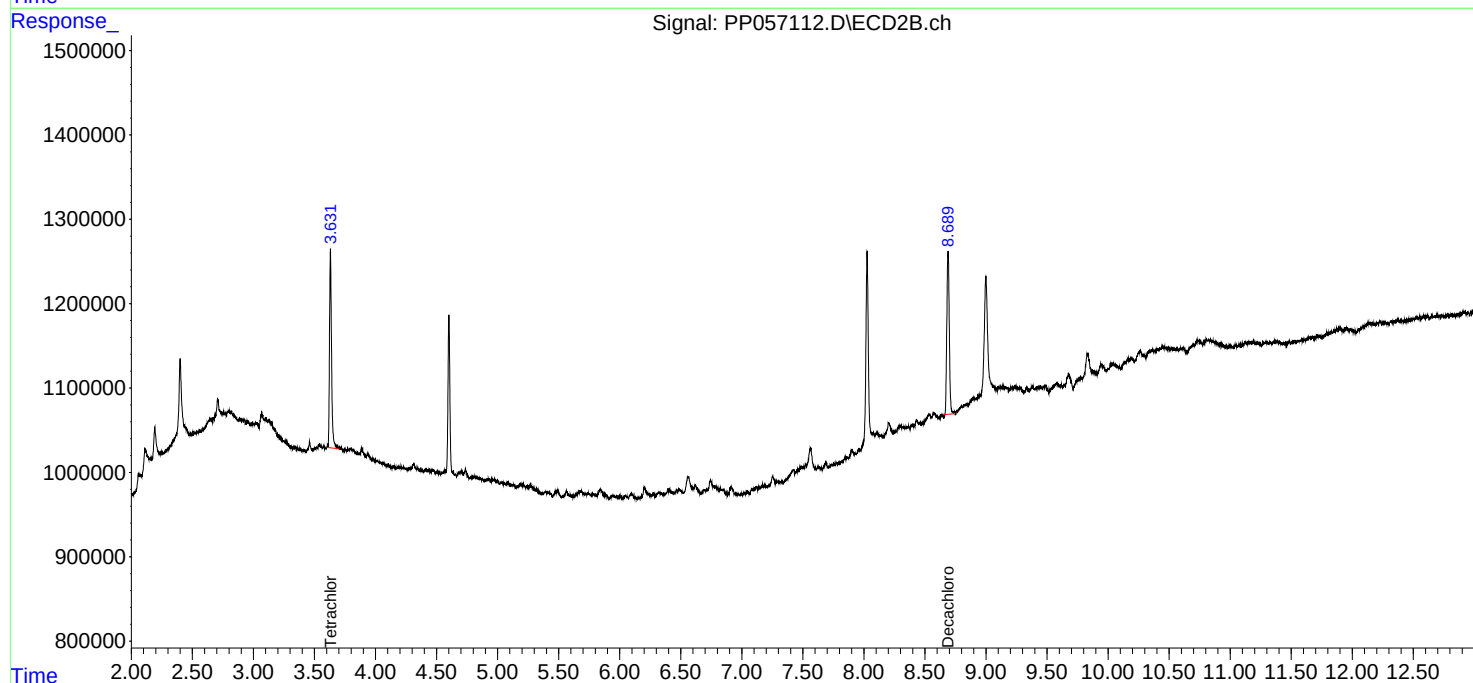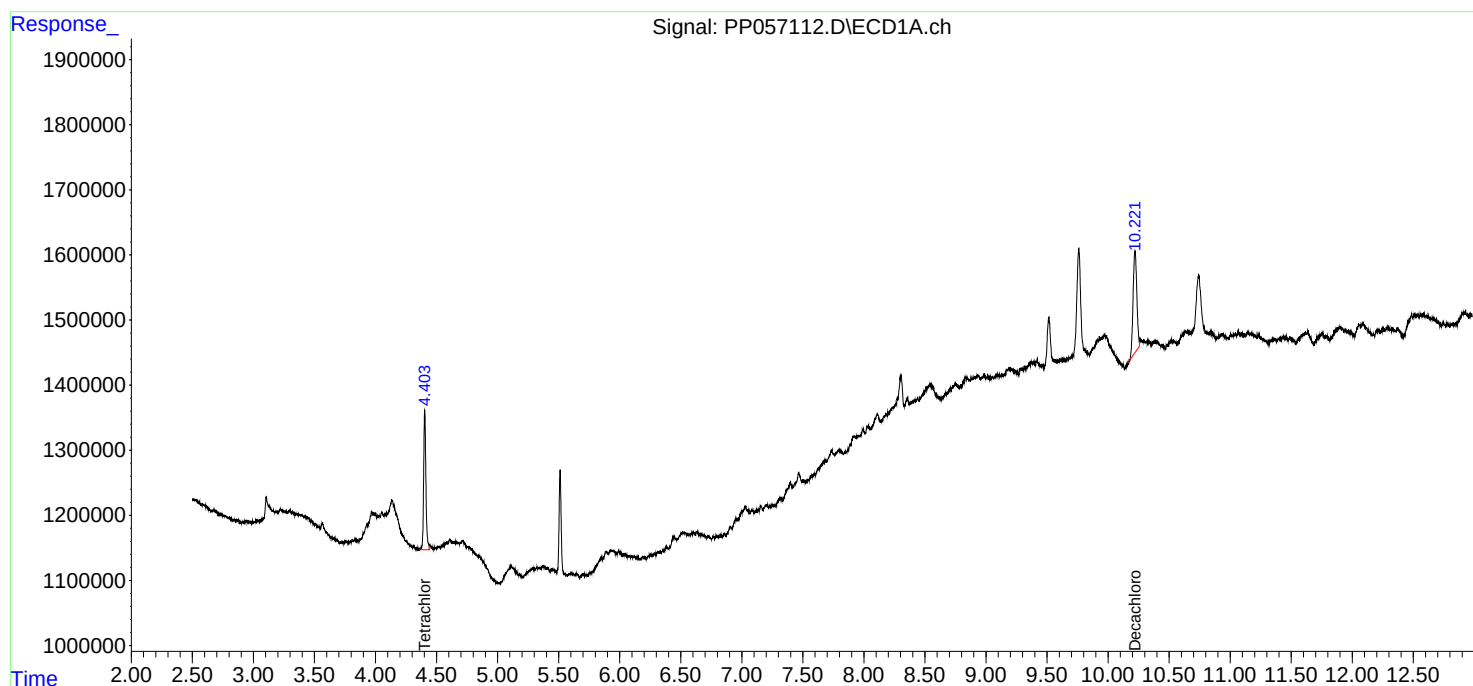


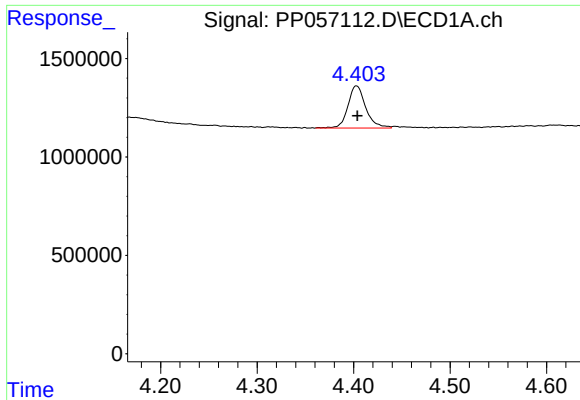

#1 Tetrachloro-m-xylene


R.T.: 4.403 min
Delta R.T.: 0.000 min
Response: 2740656
Conc: 1.24 ng/ml

Instrument :
ECD_P
ClientSampleId :
SOM041923R-END-2-2

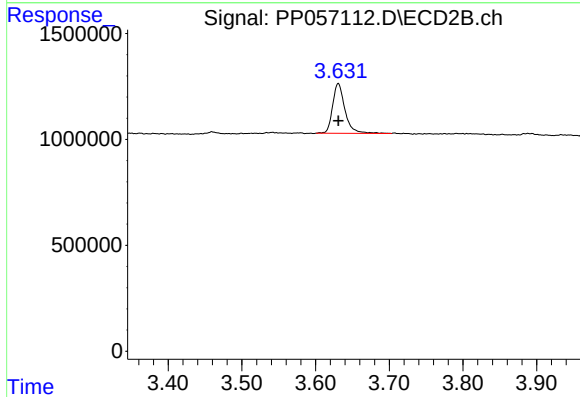


#1 Tetrachloro-m-xylene

R.T.: 3.631 min
Delta R.T.: 0.000 min
Response: 2732624
Conc: 1.62 ng/ml

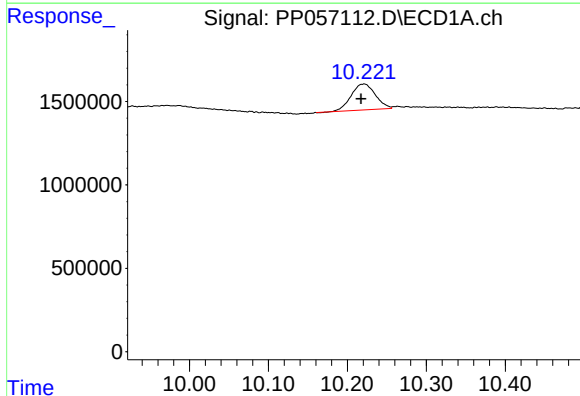

#2 Decachlorobiphenyl

R.T.: 10.221 min
Delta R.T.: 0.004 min
Response: 3292006
Conc: 2.05 ng/ml

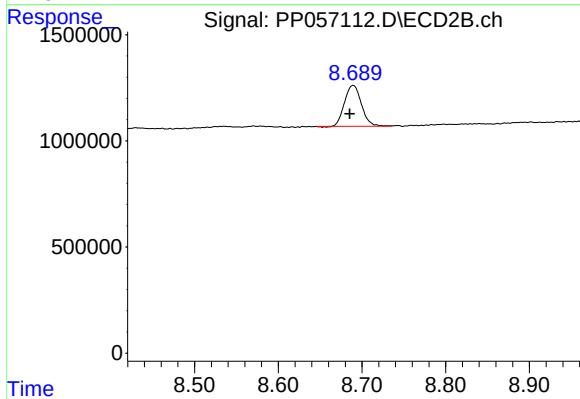

#2 Decachlorobiphenyl

R.T.: 8.689 min
Delta R.T.: 0.004 min
Response: 2693475
Conc: 1.51 ng/ml