

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042121\
 Data File : PP035110.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Apr 2021 23:49
 Operator : DD\AJ
 Sample : M2076-10
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SB-16-0-2.0

Manual Integrations
 APPROVED

Ankita
 4/22/2021 2:45:39 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 22 07:36:57 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 21 17:37:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.835	4.251	1833739	1104918	22.504	21.456
2) SA Decachlor...	10.743	9.541	1310071	476307	20.731	20.047
Target Compounds						
31) L7 AR-1260-1	7.826	7.076	104112	79704	30.915m	45.557 #
32) L7 AR-1260-2	8.090	7.272	230249	72981	67.632	40.940 #
33) L7 AR-1260-3	8.455	7.426	115120	60091	45.864	33.326 #
34) L7 AR-1260-4	8.683	7.904	145617	50999	49.610	40.066
35) L7 AR-1260-5	9.003	8.149	197014	100344	40.046	41.272

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042121\
Data File : PP035110.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Apr 2021 23:49
Operator : DD\AJ
Sample : M2076-10
Misc :
ALS Vial : 38 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
SB-16-0-2.0


Manual Integrations
APPROVED

Ankita
4/22/2021 2:45:39 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 07:36:57 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 21 17:37:28 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

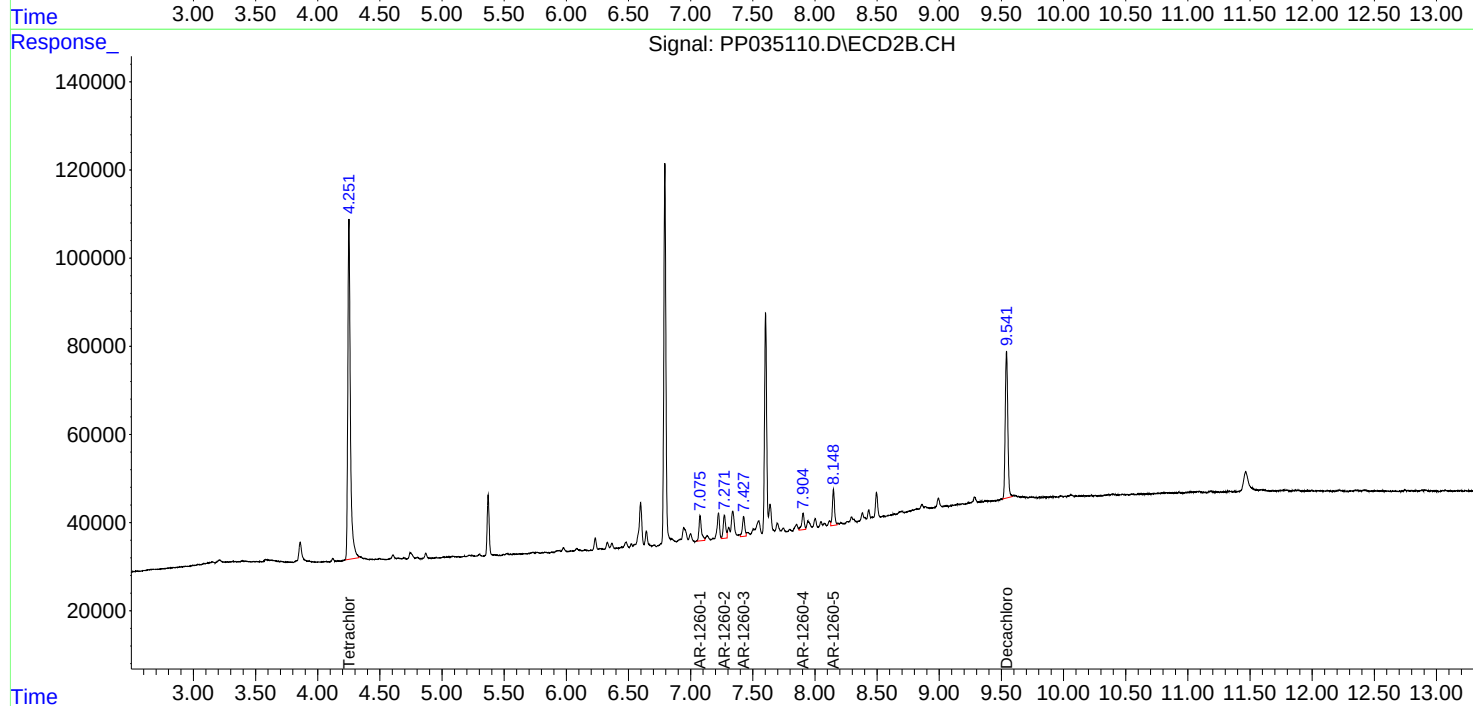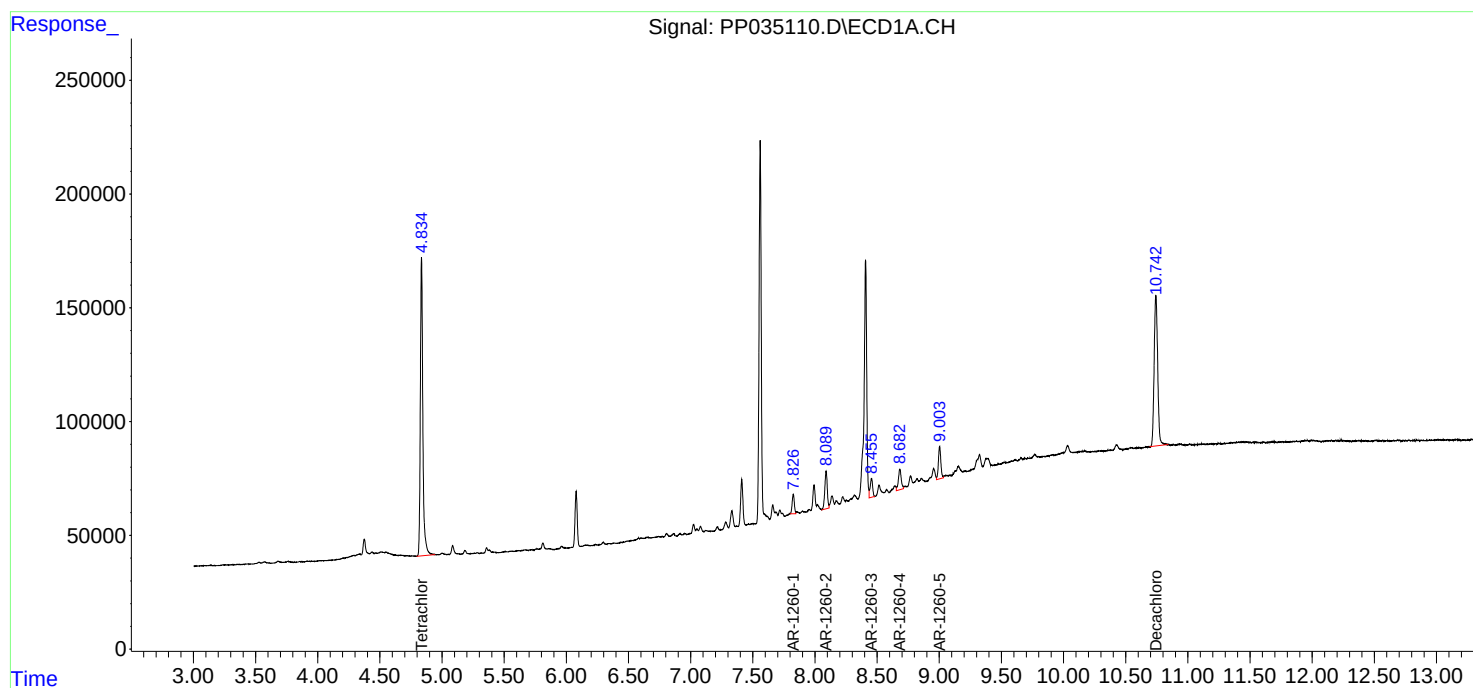

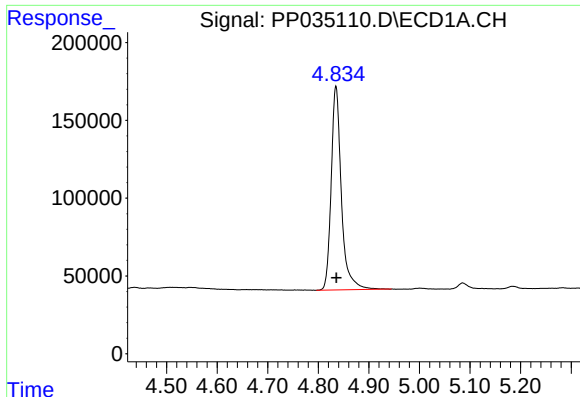


#1 Tetrachloro-m-xylene

R.T.: 4.835 min
Delta R.T.: -0.001 min
Response: 1833739
Conc: 22.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-16-0-2.0


Manual Integrations
APPROVED

Ankita
4/22/2021 2:45:39 PM

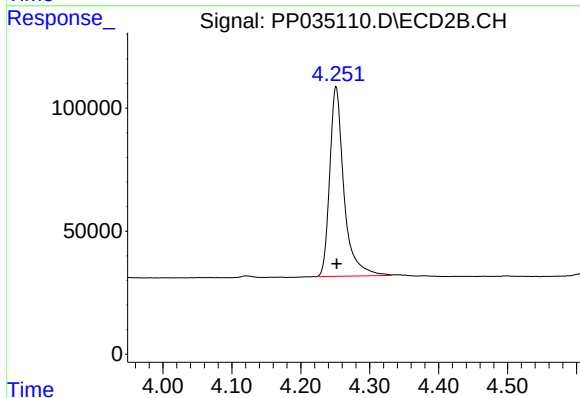


#1 Tetrachloro-m-xylene

R.T.: 4.251 min
Delta R.T.: 0.000 min
Response: 1104918
Conc: 21.46 ng/ml

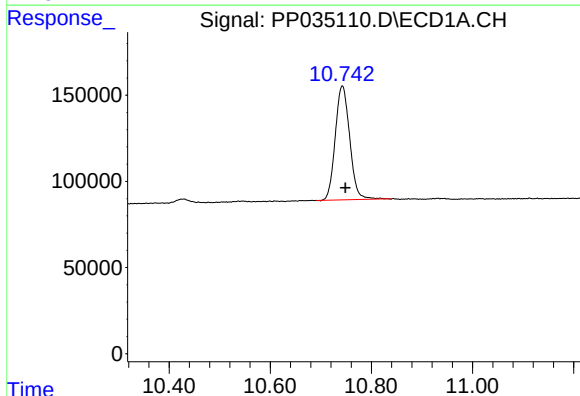


#2 Decachlorobiphenyl

R.T.: 10.743 min
Delta R.T.: -0.006 min
Response: 1310071
Conc: 20.73 ng/ml

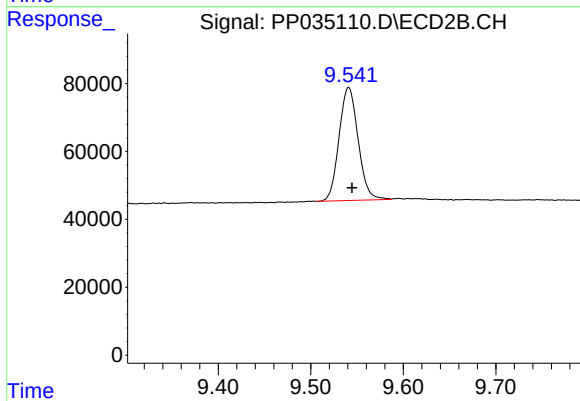

#2 Decachlorobiphenyl

R.T.: 9.541 min
Delta R.T.: -0.004 min
Response: 476307
Conc: 20.05 ng/ml

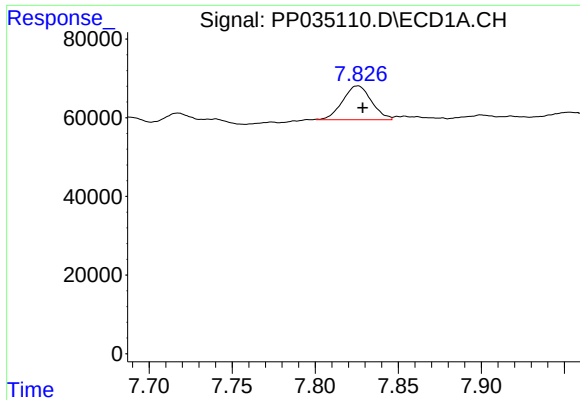


#31 AR-1260-1

R.T.: 7.826 min
Delta R.T.: -0.003 min
Response: 104112
Conc: 30.91 ng/ml m

Instrument :
ECD_P
ClientSampleId :
SB-16-0-2.0


Manual Integrations
APPROVED

Ankita
4/22/2021 2:45:39 PM

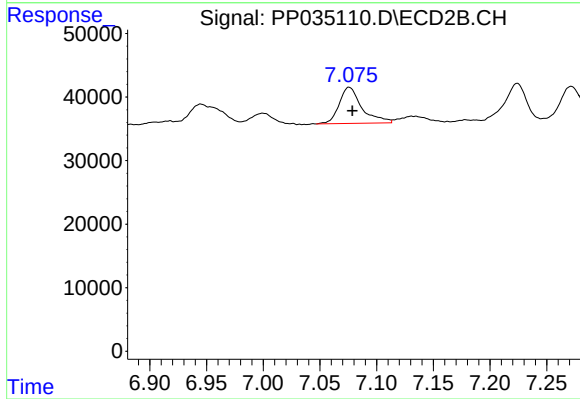


#31 AR-1260-1

R.T.: 7.076 min
Delta R.T.: -0.003 min
Response: 79704
Conc: 45.56 ng/ml

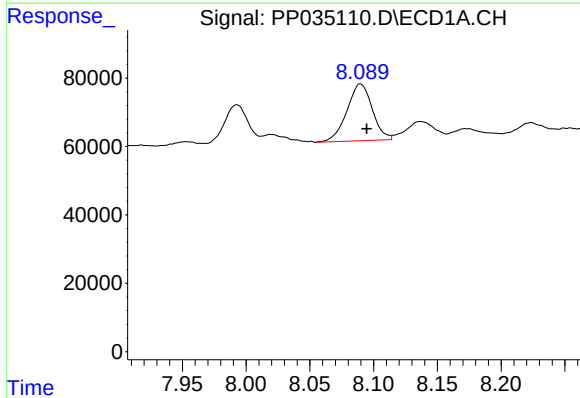


#32 AR-1260-2

R.T.: 8.090 min
Delta R.T.: -0.005 min
Response: 230249
Conc: 67.63 ng/ml

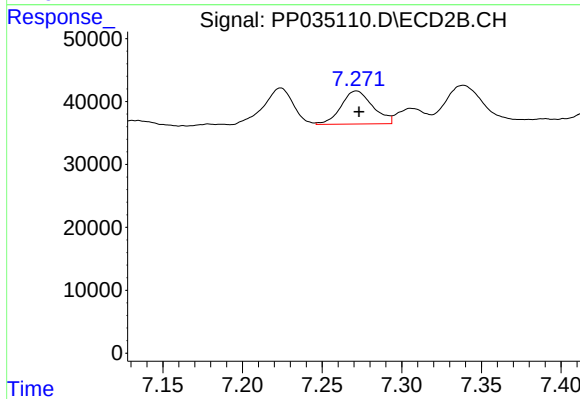

#32 AR-1260-2

R.T.: 7.272 min
Delta R.T.: -0.002 min
Response: 72981
Conc: 40.94 ng/ml

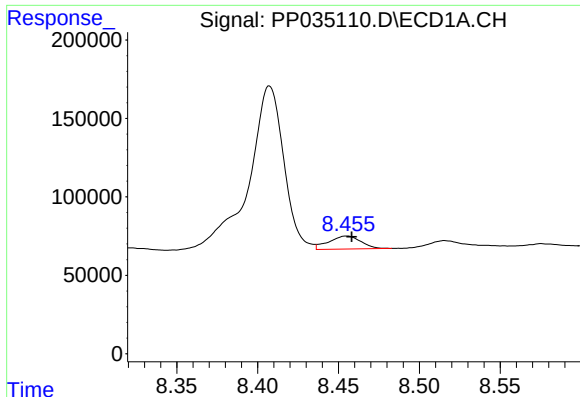


#33 AR-1260-3

R.T.: 8.455 min
Delta R.T.: -0.003 min
Response: 115120
Conc: 45.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-16-0-2.0


Manual Integrations
APPROVED

Ankita
4/22/2021 2:45:39 PM

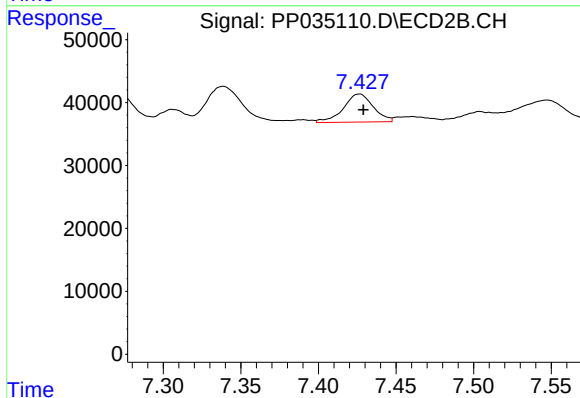


#33 AR-1260-3

R.T.: 7.426 min
Delta R.T.: -0.003 min
Response: 60091
Conc: 33.33 ng/ml

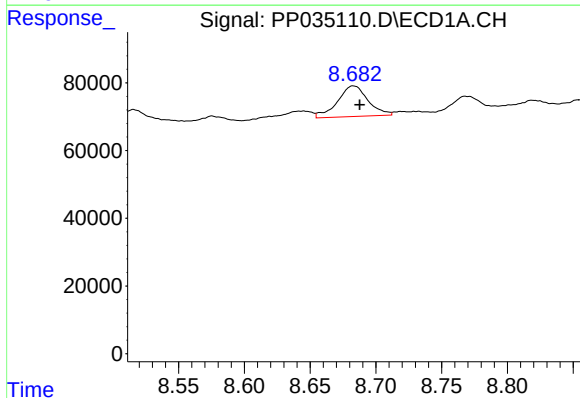


#34 AR-1260-4

R.T.: 8.683 min
Delta R.T.: -0.005 min
Response: 145617
Conc: 49.61 ng/ml

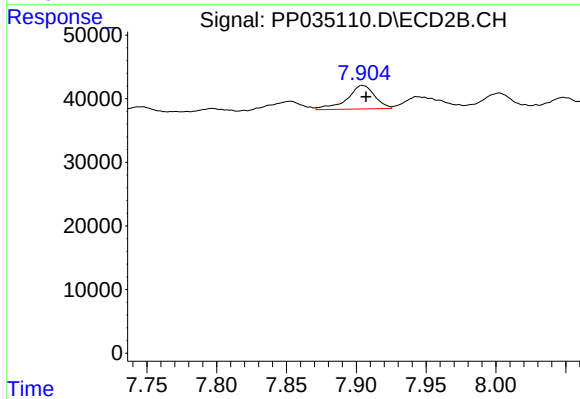

#34 AR-1260-4

R.T.: 7.904 min
Delta R.T.: -0.003 min
Response: 50999
Conc: 40.07 ng/ml

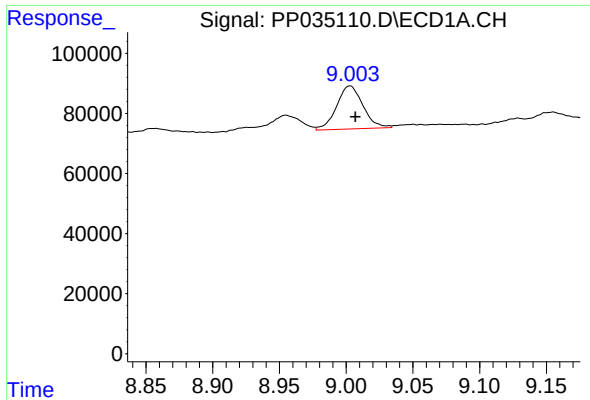


#35 AR-1260-5

R.T.: 9.003 min
Delta R.T.: -0.004 min
Response: 197014
Conc: 40.05 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-16-0-2.0

Manual Integrations
APPROVED

Ankita
4/22/2021 2:45:39 PM

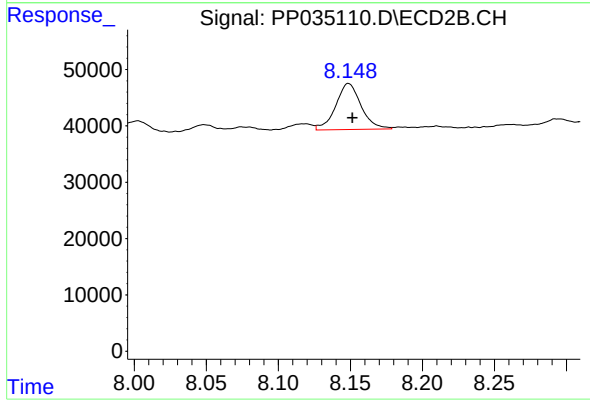

#35 AR-1260-5

R.T.: 8.149 min
Delta R.T.: -0.003 min
Response: 100344
Conc: 41.27 ng/ml