

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042121\
 Data File : PP035112.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Apr 2021 00:23
 Operator : DD\AJ
 Sample : M2076-13
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SB-17-0-2.0

Manual Integrations
 APPROVED

Ankita
 4/22/2021 2:45:42 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 22 07:41:16 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 21 17:37:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.835	4.250	1819933	1123938	22.334	21.825
2) SA Decachlor...	10.743	9.540	1507655	549910	23.858	23.144
Target Compounds						
31) L7 AR-1260-1	7.825	7.073	20380	27091	6.052m	15.485 #
32) L7 AR-1260-2	8.090	7.273	67910	28667	19.948	16.081
33) L7 AR-1260-3	8.455	7.427	33157	12128	13.210	6.726 #
34) L7 AR-1260-4	8.684	7.904	31137	11226	10.608m	8.820
35) L7 AR-1260-5	9.004	8.147	44498	26243	9.045	10.794

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042121\
Data File : PP035112.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Apr 2021 00:23
Operator : DD\AJ
Sample : M2076-13
Misc :
ALS Vial : 40 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
SB-17-0-2.0


Manual Integrations
APPROVED

Ankita
4/22/2021 2:45:42 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 07:41:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 21 17:37:28 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

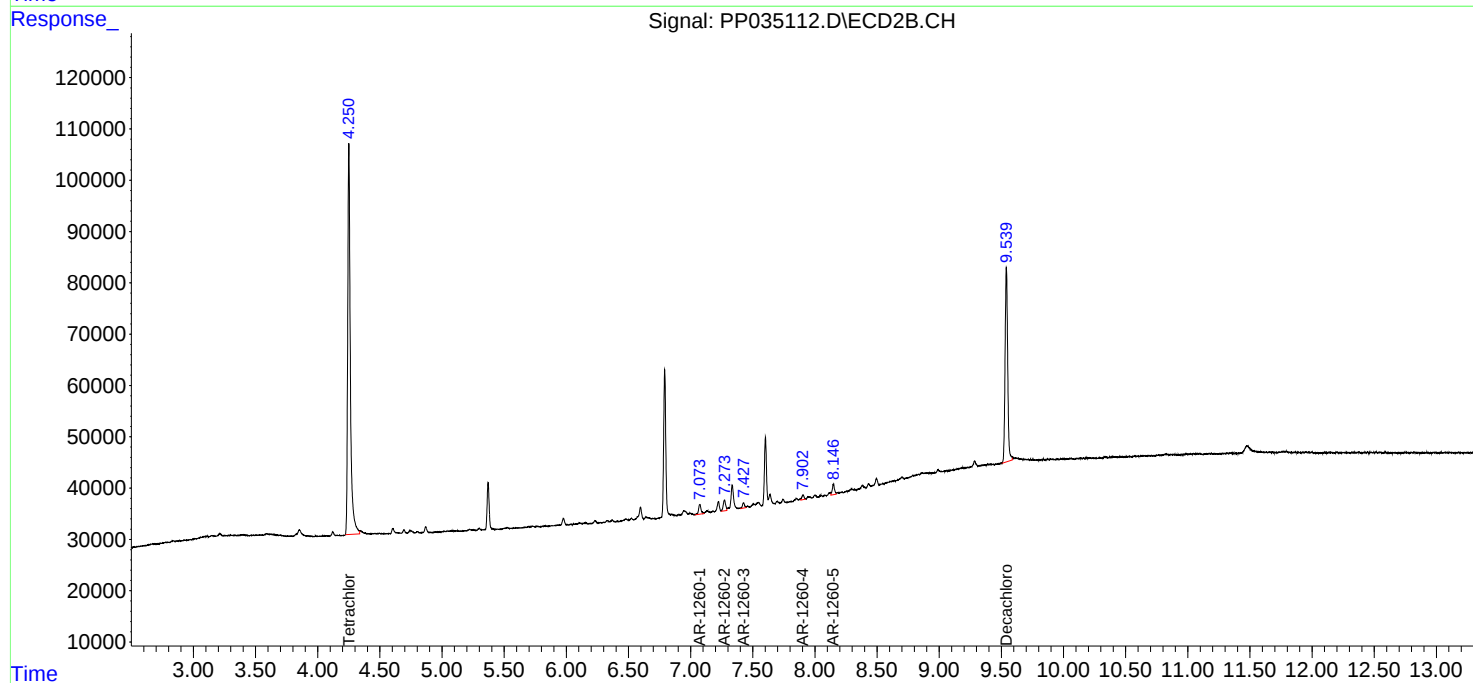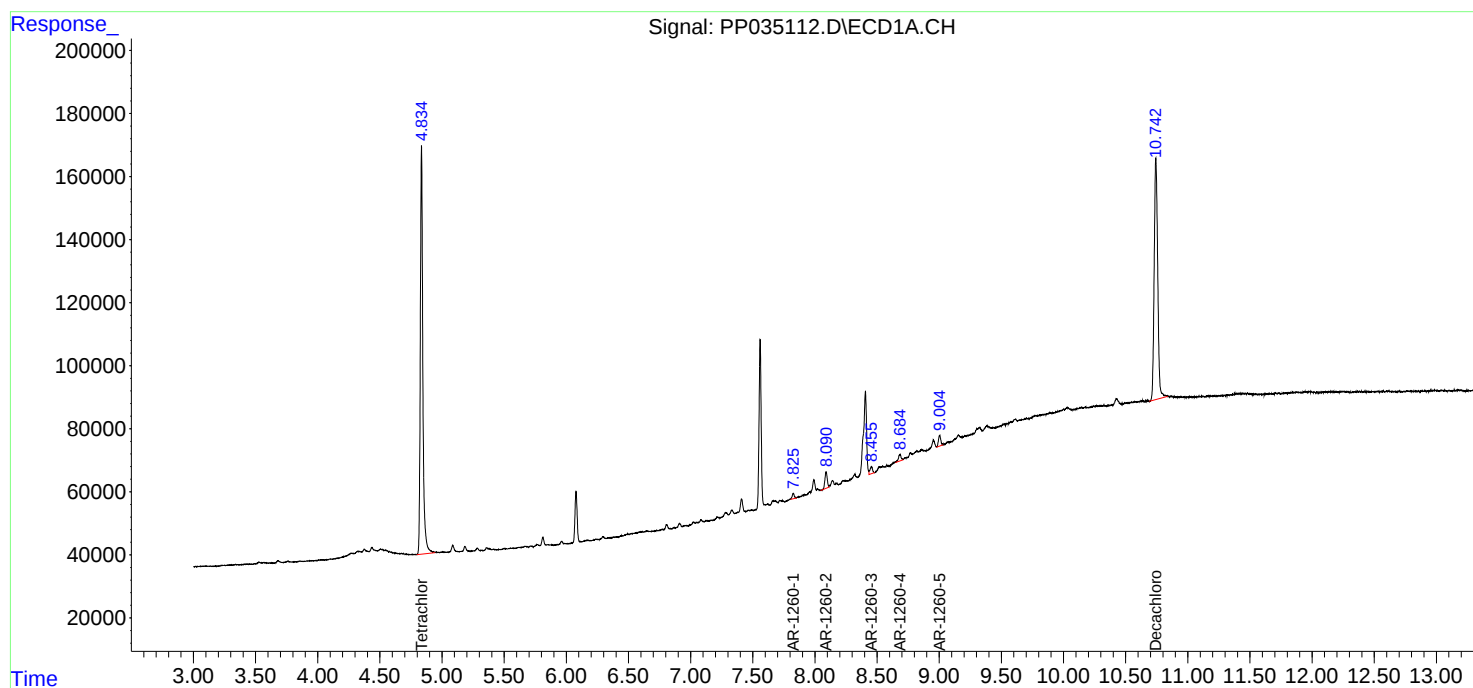

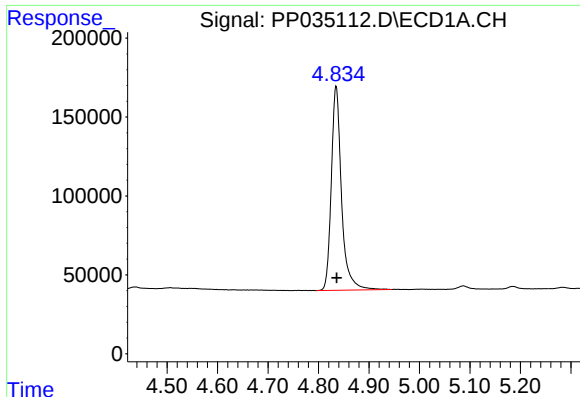


#1 Tetrachloro-m-xylene

R.T.: 4.835 min
Delta R.T.: -0.001 min
Response: 1819933
Conc: 22.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-17-0-2.0


Manual Integrations
APPROVED

Ankita
4/22/2021 2:45:42 PM

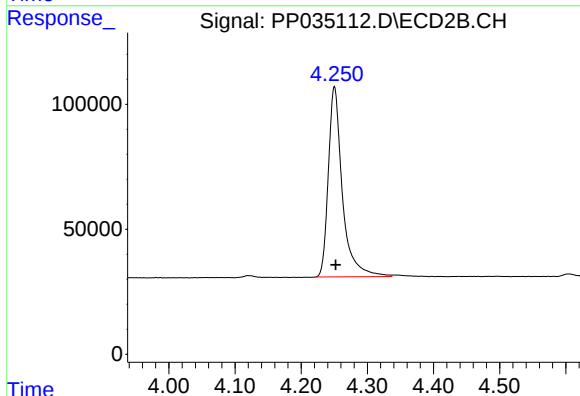


#1 Tetrachloro-m-xylene

R.T.: 4.250 min
Delta R.T.: -0.002 min
Response: 1123938
Conc: 21.83 ng/ml

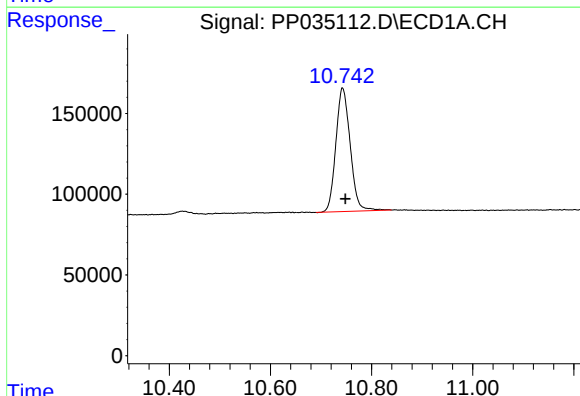


#2 Decachlorobiphenyl

R.T.: 10.743 min
Delta R.T.: -0.006 min
Response: 1507655
Conc: 23.86 ng/ml

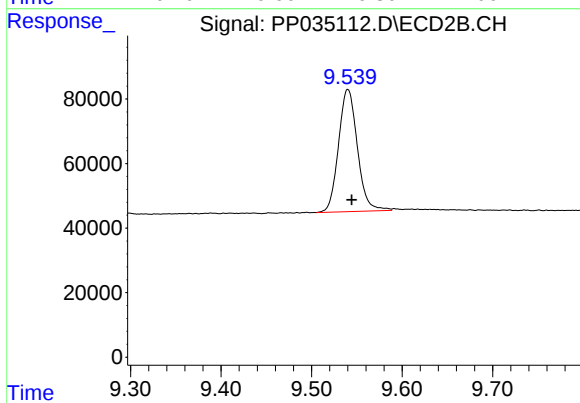

#2 Decachlorobiphenyl

R.T.: 9.540 min
Delta R.T.: -0.004 min
Response: 549910
Conc: 23.14 ng/ml

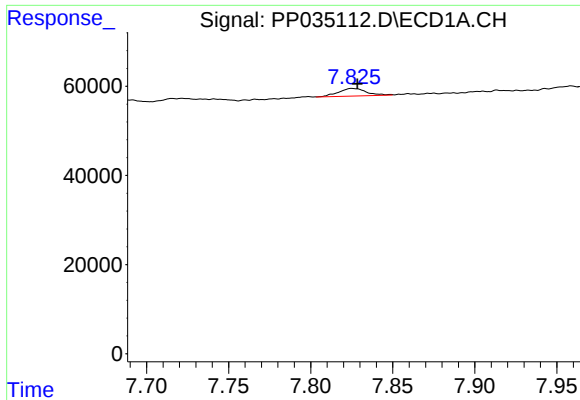


#31 AR-1260-1

R.T.: 7.825 min
Delta R.T.: -0.004 min
Response: 20380
Conc: 6.05 ng/ml m

Instrument :
ECD_P
ClientSampleId :
SB-17-0-2.0


Manual Integrations
APPROVED

Ankita
4/22/2021 2:45:42 PM

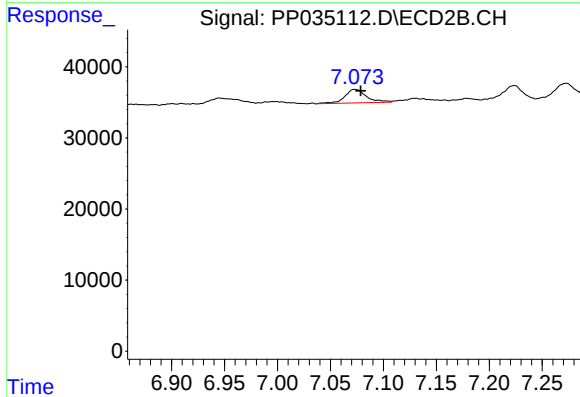


#31 AR-1260-1

R.T.: 7.073 min
Delta R.T.: -0.006 min
Response: 27091
Conc: 15.48 ng/ml

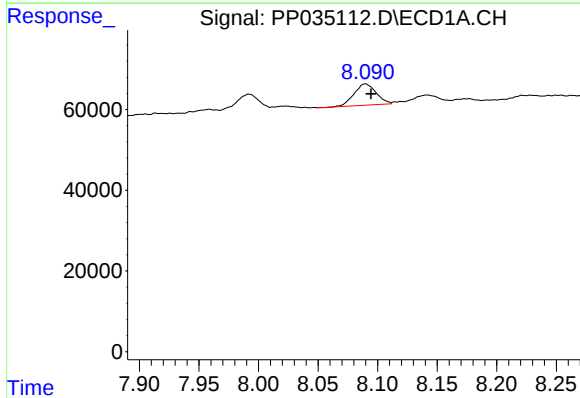


#32 AR-1260-2

R.T.: 8.090 min
Delta R.T.: -0.005 min
Response: 67910
Conc: 19.95 ng/ml

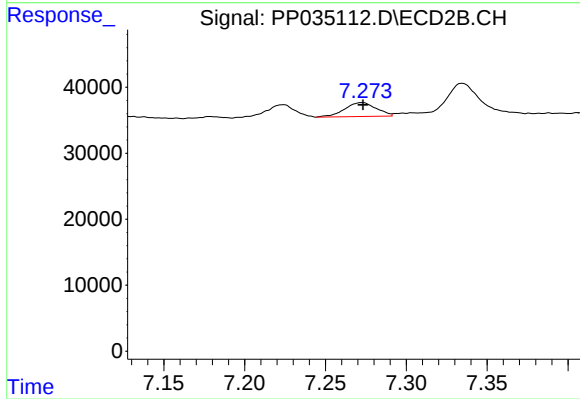

#32 AR-1260-2

R.T.: 7.273 min
Delta R.T.: 0.000 min
Response: 28667
Conc: 16.08 ng/ml

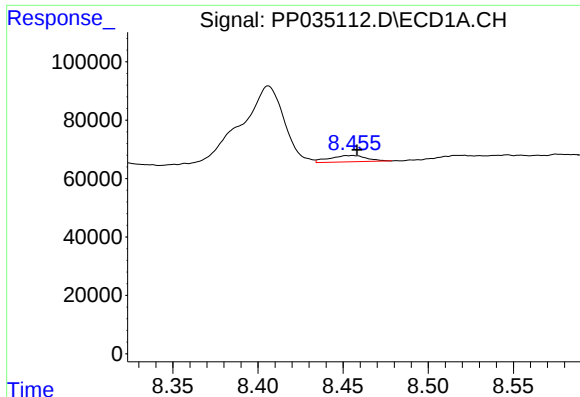


#33 AR-1260-3

R.T.: 8.455 min
Delta R.T.: -0.003 min
Response: 33157
Conc: 13.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-17-0-2.0


Manual Integrations
APPROVED

Ankita
4/22/2021 2:45:42 PM

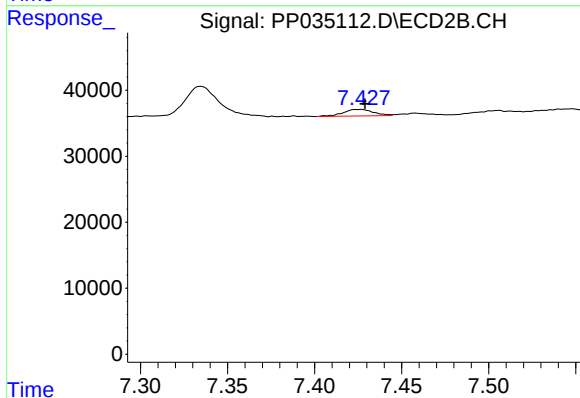


#33 AR-1260-3

R.T.: 7.427 min
Delta R.T.: -0.002 min
Response: 12128
Conc: 6.73 ng/ml

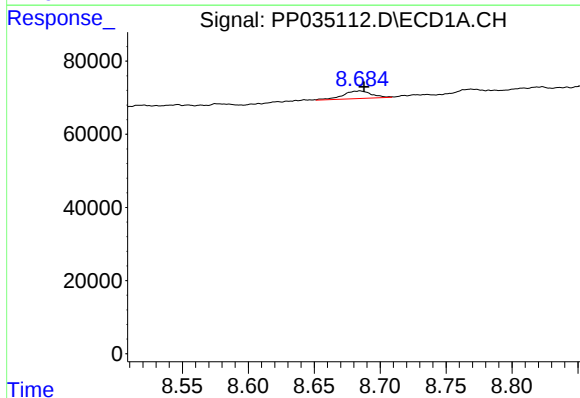


#34 AR-1260-4

R.T.: 8.684 min
Delta R.T.: -0.003 min
Response: 31137
Conc: 10.61 ng/ml m

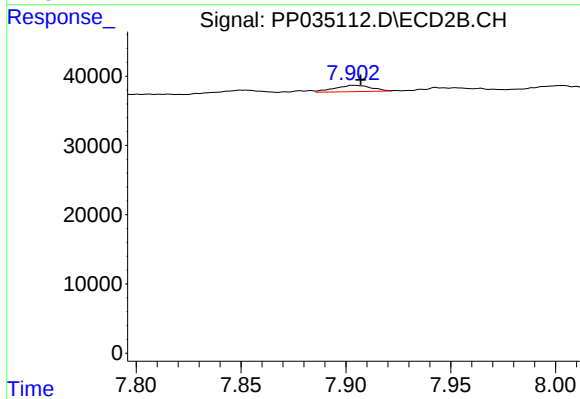

#34 AR-1260-4

R.T.: 7.904 min
Delta R.T.: -0.004 min
Response: 11226
Conc: 8.82 ng/ml

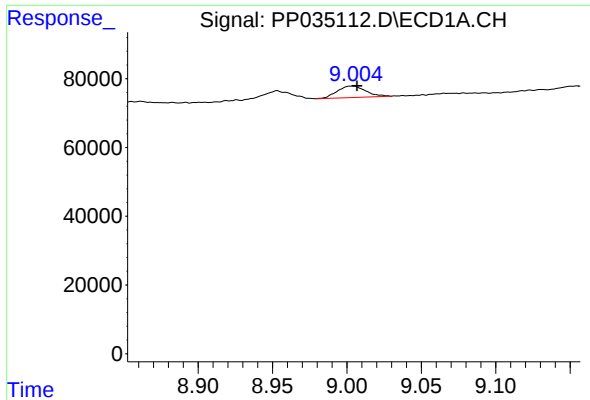


#35 AR-1260-5

R.T.: 9.004 min
Delta R.T.: -0.003 min
Response: 44498
Conc: 9.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-17-0-2.0

Manual Integrations
APPROVED

Ankita
4/22/2021 2:45:42 PM

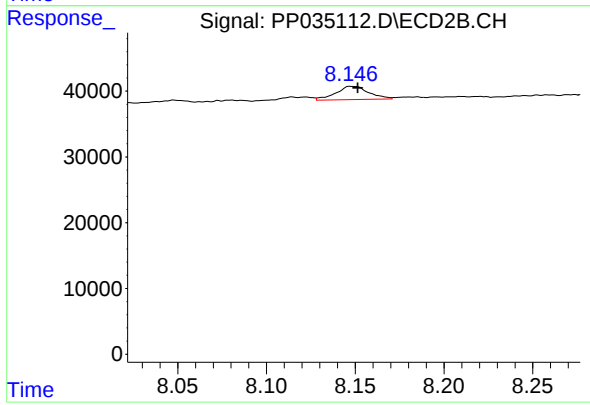

#35 AR-1260-5

R.T.: 8.147 min
Delta R.T.: -0.004 min
Response: 26243
Conc: 10.79 ng/ml