

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042121\
 Data File : PP035113.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Apr 2021 00:40
 Operator : DD\AJ
 Sample : M2076-15
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SB-17-14.5-15.0

Manual Integrations
 APPROVED

Ankita
 4/22/2021 2:45:43 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 22 07:41:52 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 21 17:37:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.834	4.250	1766144	1075128	21.674	20.878
2) SA Decachlor...	10.743	9.540	1867290	659844	29.549	27.771
Target Compounds						
31) L7 AR-1260-1	7.823	7.075	45784	36307	13.595m	20.752 #
32) L7 AR-1260-2	8.090	7.271	201255	45999	59.116	25.804 #
33) L7 AR-1260-3	8.455	7.425	32005	22306	12.751	12.371
34) L7 AR-1260-4	8.682	7.904	65534	15504	22.326	12.180 #
35) L7 AR-1260-5	9.002	8.149	71737	38464	14.582	15.820

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042121\
Data File : PP035113.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Apr 2021 00:40
Operator : DD\AJ
Sample : M2076-15
Misc :
ALS Vial : 41 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
SB-17-14.5-15.0


Manual Integrations
APPROVED

Ankita
4/22/2021 2:45:43 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 07:41:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 21 17:37:28 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

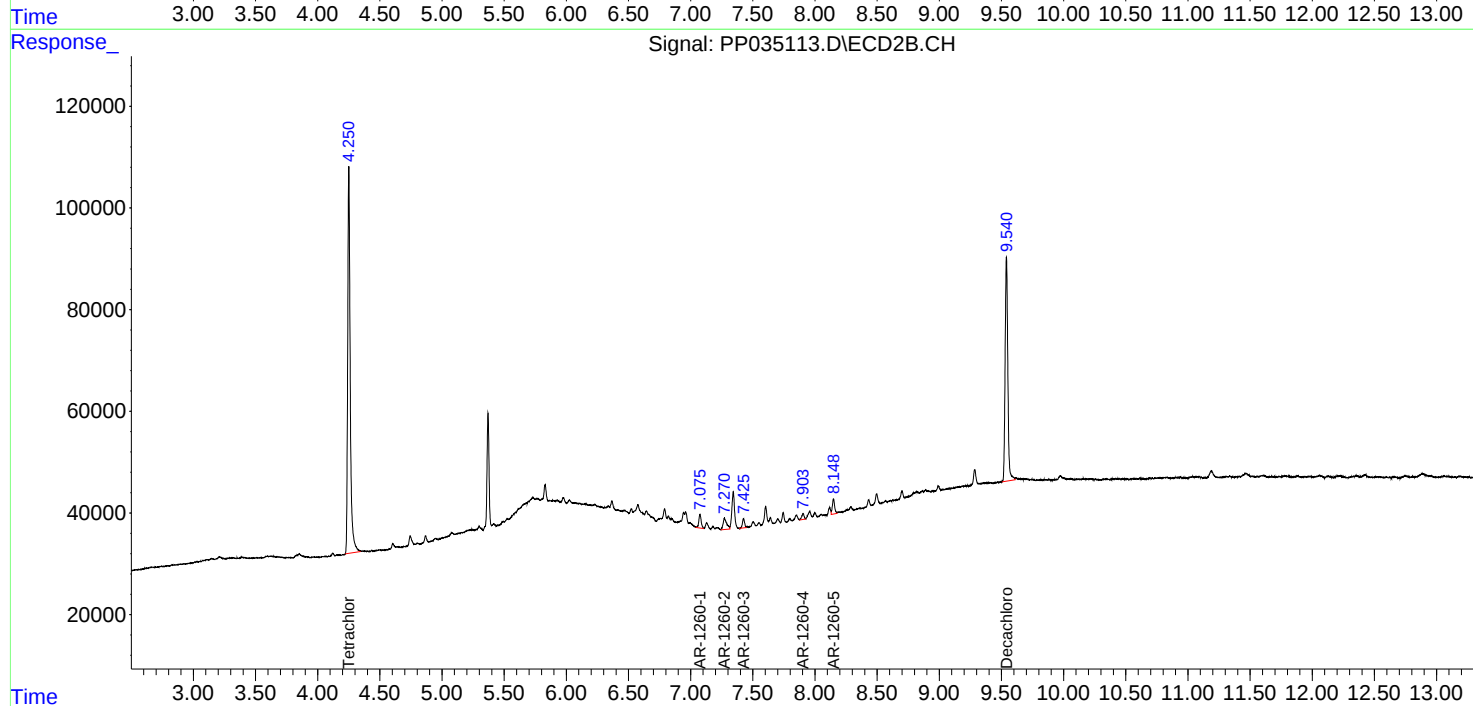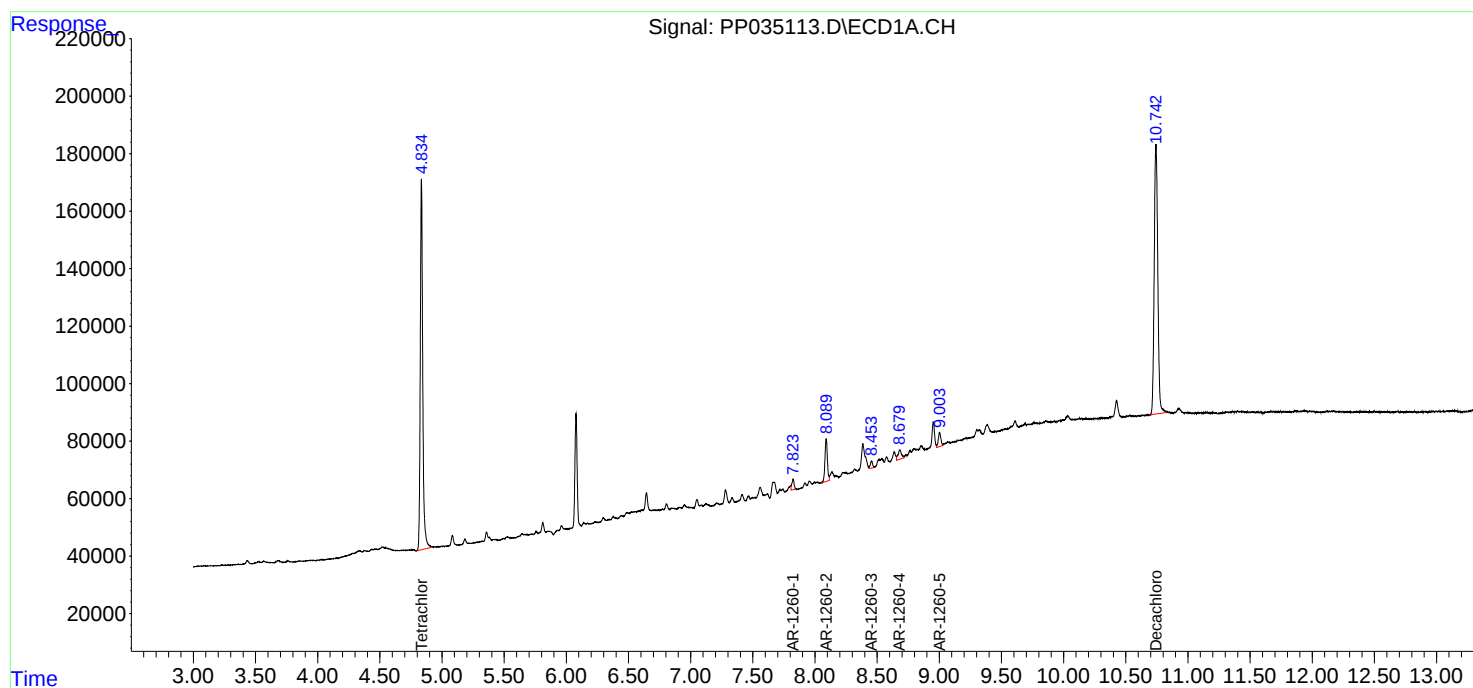

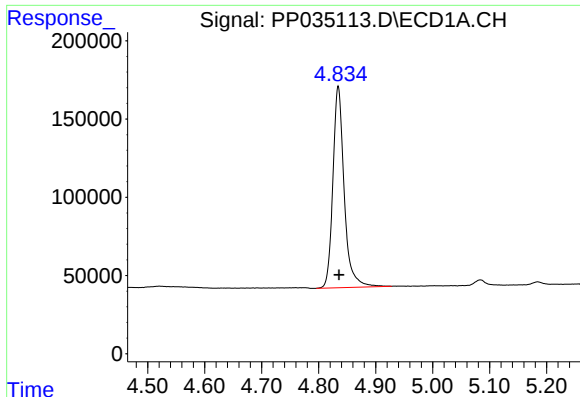


#1 Tetrachloro-m-xylene

R.T.: 4.834 min
Delta R.T.: -0.002 min
Response: 1766144
Conc: 21.67 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-17-14.5-15.0


Manual Integrations
APPROVED

Ankita
4/22/2021 2:45:43 PM

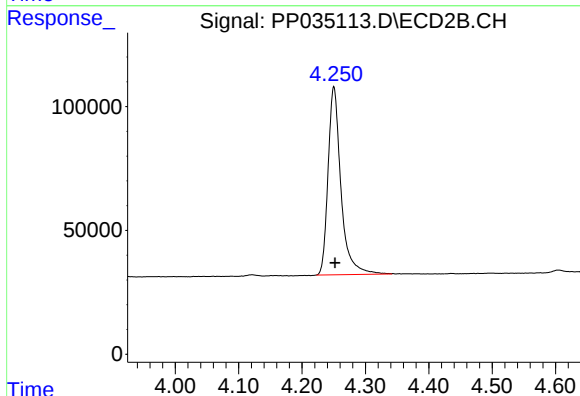


#1 Tetrachloro-m-xylene

R.T.: 4.250 min
Delta R.T.: -0.002 min
Response: 1075128
Conc: 20.88 ng/ml

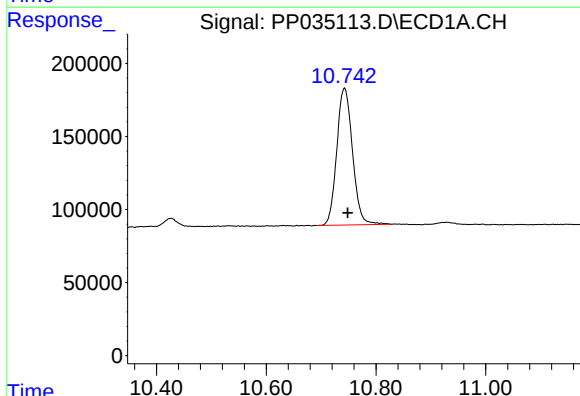


#2 Decachlorobiphenyl

R.T.: 10.743 min
Delta R.T.: -0.006 min
Response: 1867290
Conc: 29.55 ng/ml

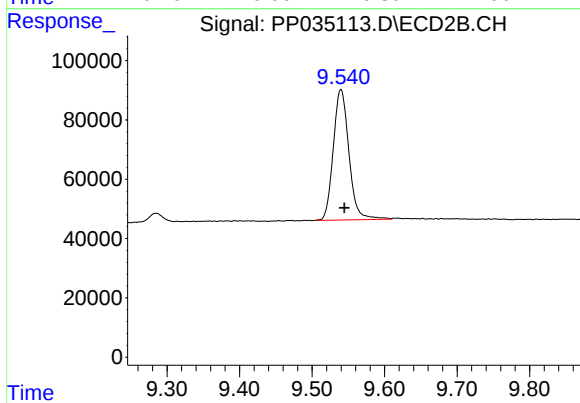

#2 Decachlorobiphenyl

R.T.: 9.540 min
Delta R.T.: -0.005 min
Response: 659844
Conc: 27.77 ng/ml

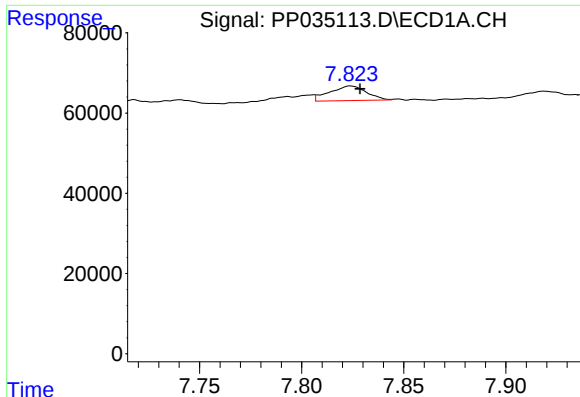


#31 AR-1260-1

R.T.: 7.823 min
Delta R.T.: -0.006 min
Response: 45784
Conc: 13.59 ng/ml m

Instrument :
ECD_P
ClientSampleId :
SB-17-14.5-15.0


Manual Integrations
APPROVED

Ankita
4/22/2021 2:45:43 PM

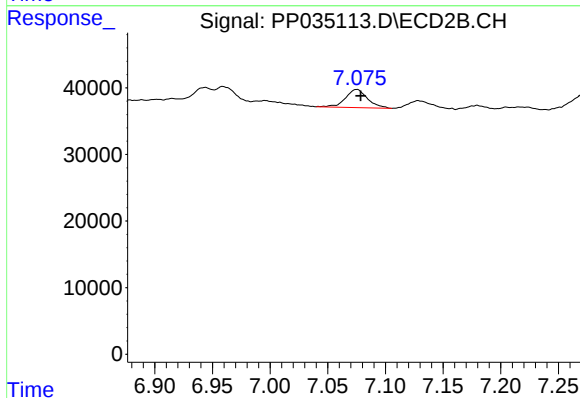


#31 AR-1260-1

R.T.: 7.075 min
Delta R.T.: -0.003 min
Response: 36307
Conc: 20.75 ng/ml

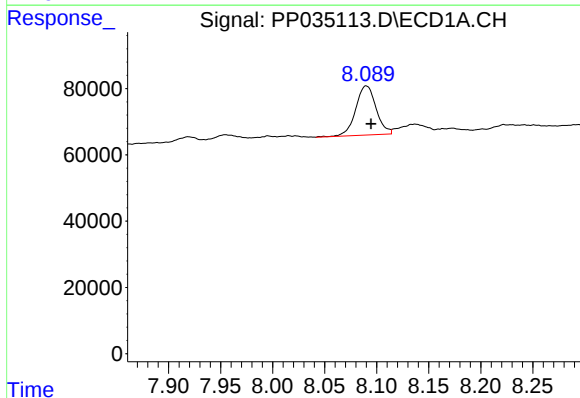


#32 AR-1260-2

R.T.: 8.090 min
Delta R.T.: -0.005 min
Response: 201255
Conc: 59.12 ng/ml

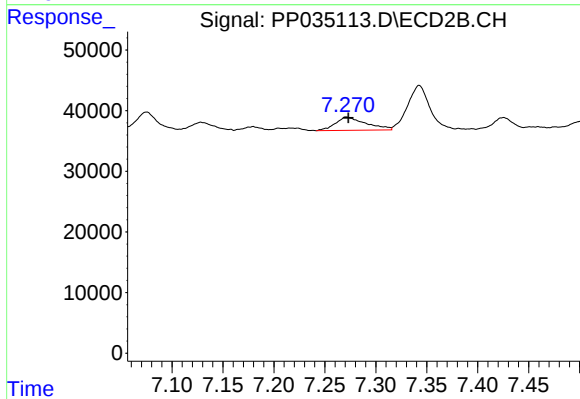

#32 AR-1260-2

R.T.: 7.271 min
Delta R.T.: -0.002 min
Response: 45999
Conc: 25.80 ng/ml

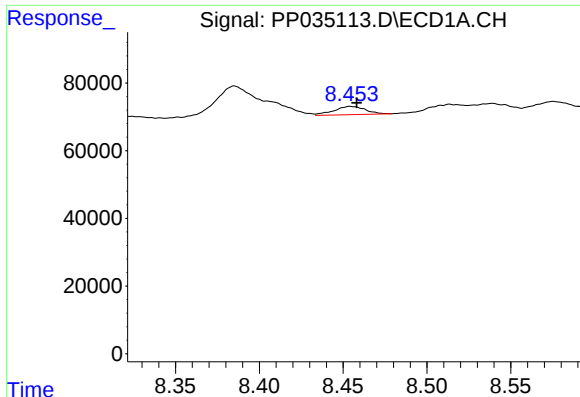


#33 AR-1260-3

R.T.: 8.455 min
Delta R.T.: -0.003 min
Response: 32005
Conc: 12.75 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-17-14.5-15.0


Manual Integrations
APPROVED

Ankita
4/22/2021 2:45:43 PM

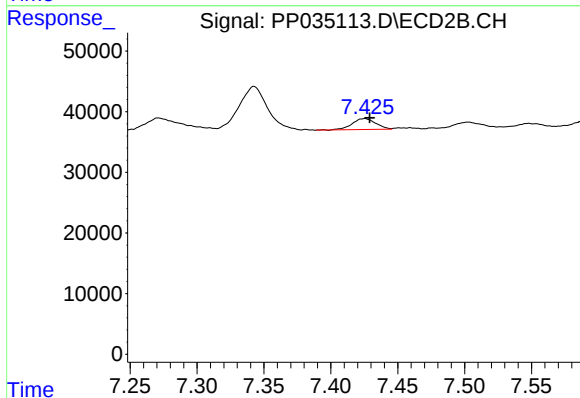


#33 AR-1260-3

R.T.: 7.425 min
Delta R.T.: -0.004 min
Response: 22306
Conc: 12.37 ng/ml

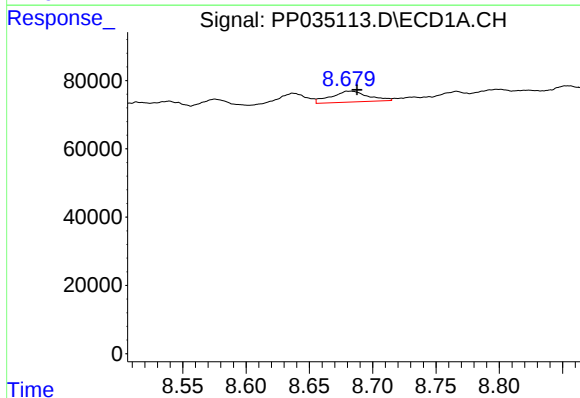


#34 AR-1260-4

R.T.: 8.682 min
Delta R.T.: -0.006 min
Response: 65534
Conc: 22.33 ng/ml

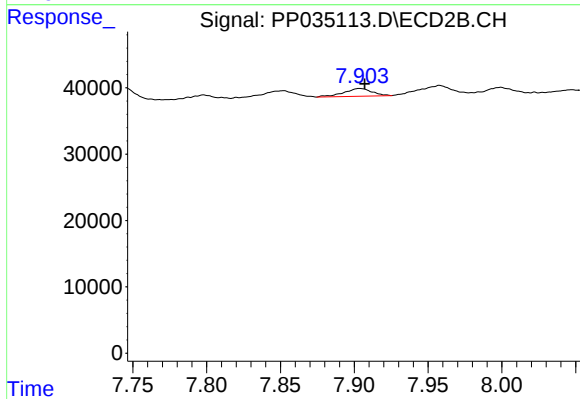

#34 AR-1260-4

R.T.: 7.904 min
Delta R.T.: -0.003 min
Response: 15504
Conc: 12.18 ng/ml

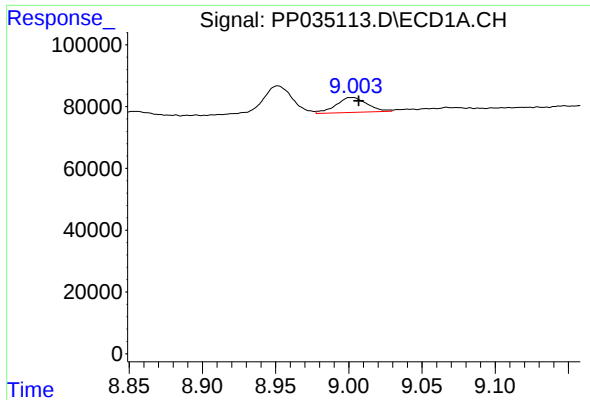


#35 AR-1260-5

R.T.: 9.002 min
Delta R.T.: -0.005 min
Response: 71737
Conc: 14.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-17-14.5-15.0

Manual Integrations
APPROVED

Ankita
4/22/2021 2:45:43 PM

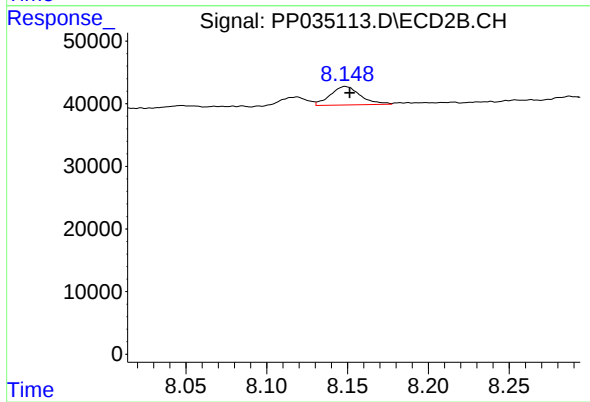

#35 AR-1260-5

R.T.: 8.149 min
Delta R.T.: -0.003 min
Response: 38464
Conc: 15.82 ng/ml