

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042121\
 Data File : PP035115.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Apr 2021 1:14
 Operator : DD\AJ
 Sample : M2076-18
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SB-18-14.5-15.0

Manual Integrations
 APPROVED

Ankita
 4/22/2021 2:45:46 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 22 07:40:11 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 21 17:37:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.834	4.250	1773183	1044695	21.761	20.287
2)	SA Decachlor...	10.743	9.541	4275976	1482402	67.665	62.391
Target Compounds							
31)	L7 AR-1260-1	7.812f	7.076	169147	134665	50.226m	76.971 #
32)	L7 AR-1260-2	8.090	7.279	601150	58870	176.579	33.025m#
33)	L7 AR-1260-3	8.455	7.425	101808	58314	40.561	32.341
34)	L7 AR-1260-4	8.684	7.902	186999	60415	63.708	47.463 #
35)	L7 AR-1260-5	9.002	8.149	212094	117134	43.112	48.178

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042121\
Data File : PP035115.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Apr 2021 1:14
Operator : DD\AJ
Sample : M2076-18
Misc :
ALS Vial : 43 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
SB-18-14.5-15.0


Manual Integrations
APPROVED

Ankita
4/22/2021 2:45:46 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 07:40:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 21 17:37:28 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

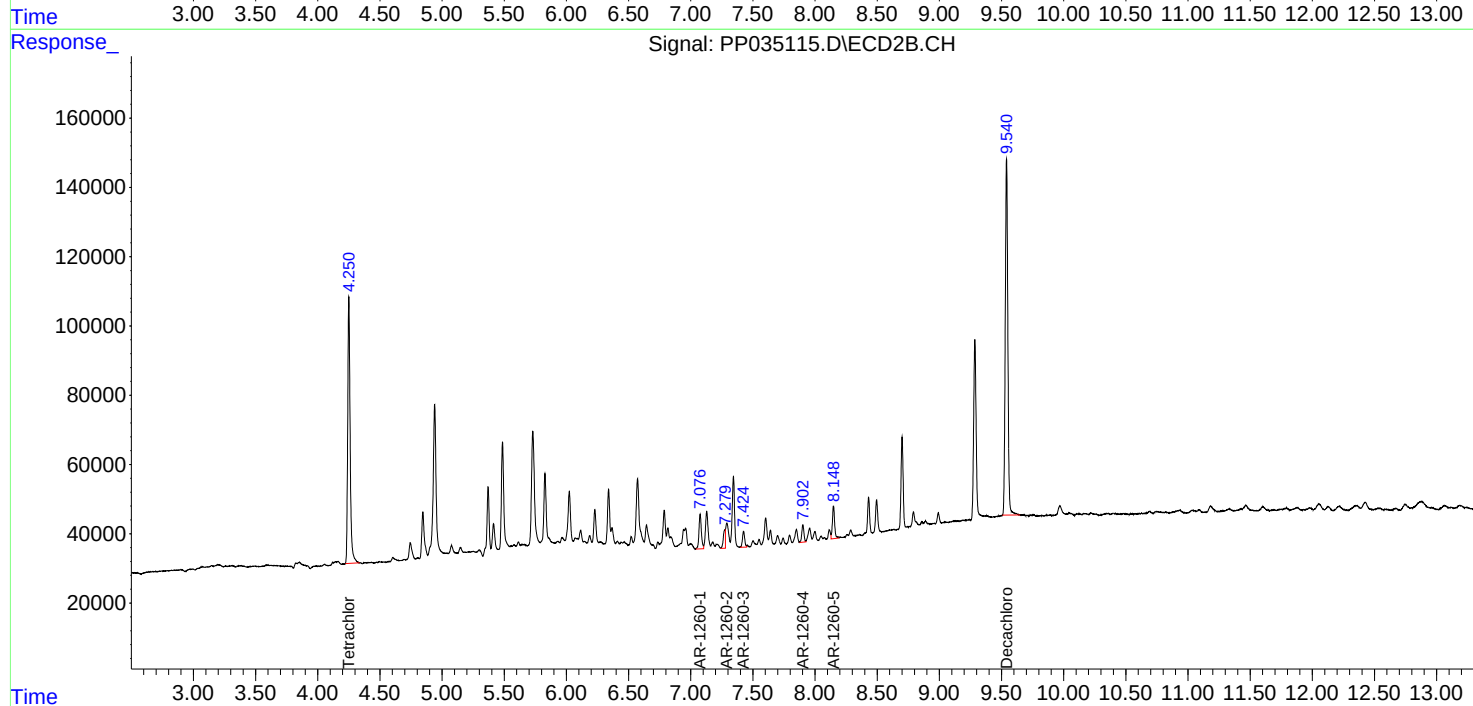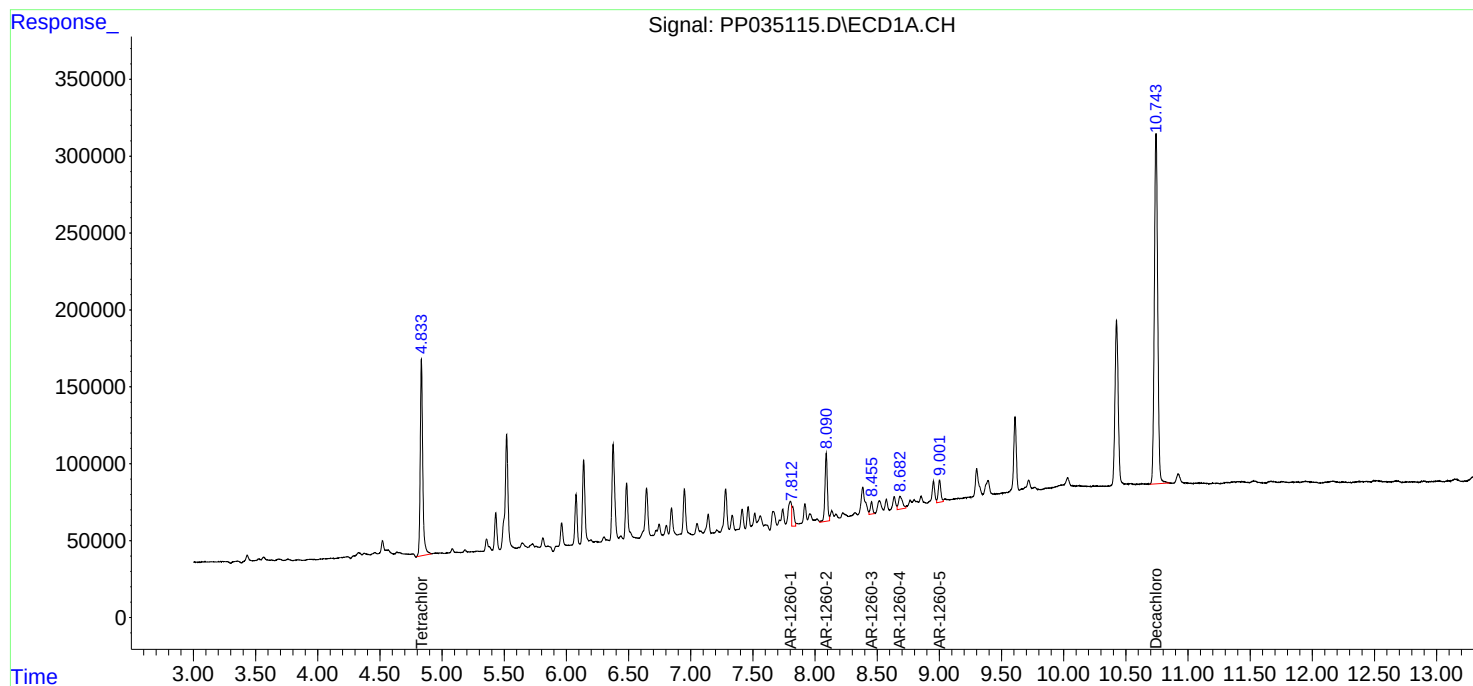

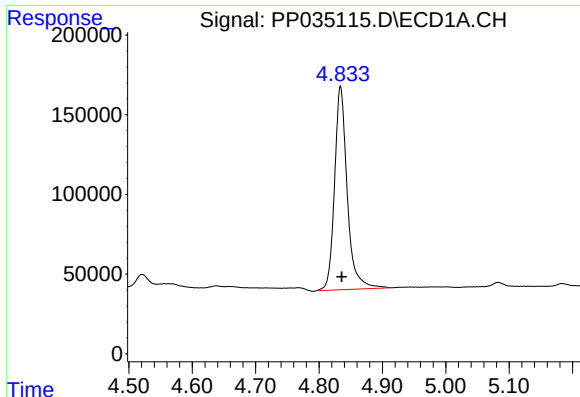


#1 Tetrachloro-m-xylene

R.T.: 4.834 min
Delta R.T.: -0.002 min
Response: 1773183
Conc: 21.76 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-18-14.5-15.0


Manual Integrations
APPROVED

Ankita
4/22/2021 2:45:46 PM

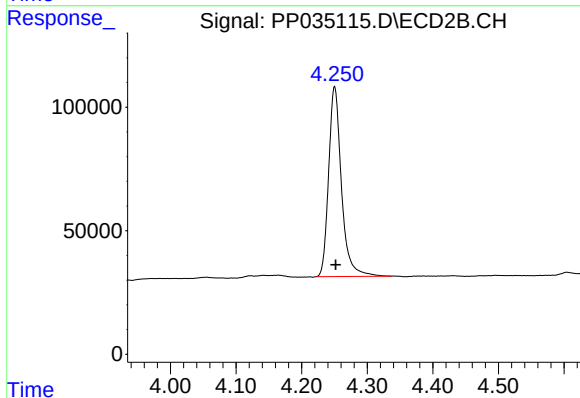


#1 Tetrachloro-m-xylene

R.T.: 4.250 min
Delta R.T.: -0.002 min
Response: 1044695
Conc: 20.29 ng/ml

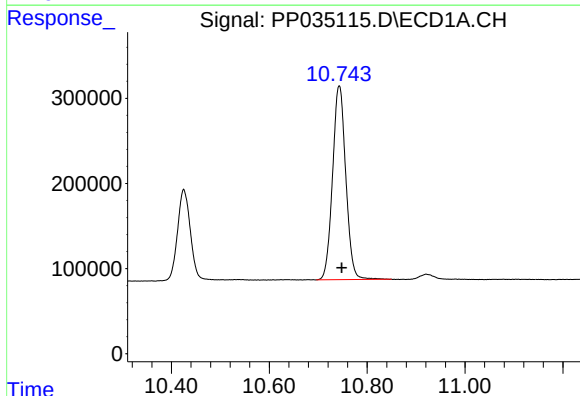


#2 Decachlorobiphenyl

R.T.: 10.743 min
Delta R.T.: -0.005 min
Response: 4275976
Conc: 67.67 ng/ml

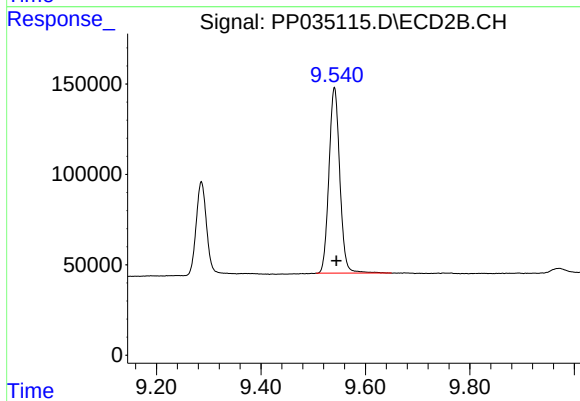

#2 Decachlorobiphenyl

R.T.: 9.541 min
Delta R.T.: -0.004 min
Response: 1482402
Conc: 62.39 ng/ml

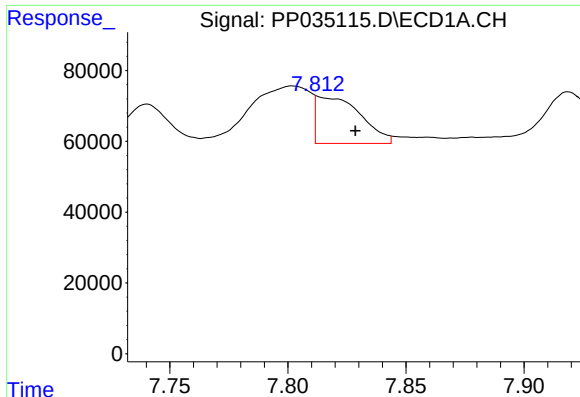


#31 AR-1260-1

R.T.: 7.812 min
Delta R.T.: -0.017 min
Response: 169147
Conc: 50.23 ng/ml m

Instrument :
ECD_P
ClientSampleId :
SB-18-14.5-15.0


Manual Integrations
APPROVED

Ankita
4/22/2021 2:45:46 PM

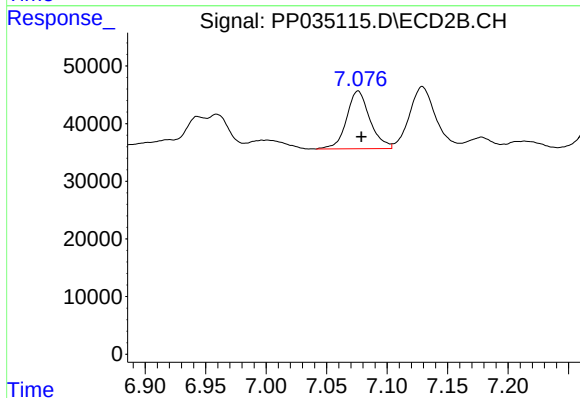


#31 AR-1260-1

R.T.: 7.076 min
Delta R.T.: -0.003 min
Response: 134665
Conc: 76.97 ng/ml

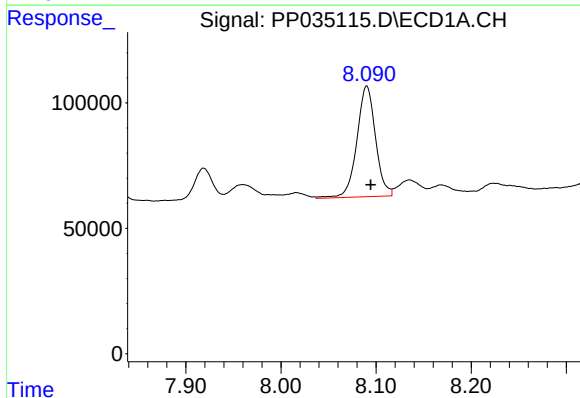


#32 AR-1260-2

R.T.: 8.090 min
Delta R.T.: -0.004 min
Response: 601150
Conc: 176.58 ng/ml

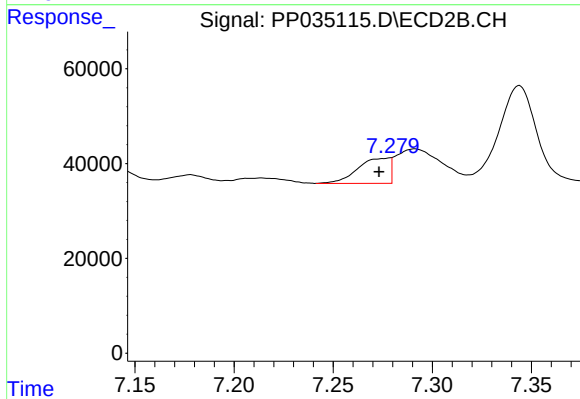

#32 AR-1260-2

R.T.: 7.279 min
Delta R.T.: 0.006 min
Response: 58870
Conc: 33.02 ng/ml m

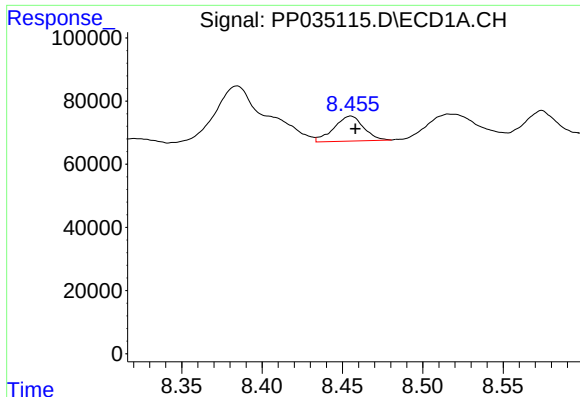


#33 AR-1260-3

R.T.: 8.455 min
Delta R.T.: -0.003 min
Response: 101808
Conc: 40.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-18-14.5-15.0


Manual Integrations
APPROVED

Ankita
4/22/2021 2:45:46 PM

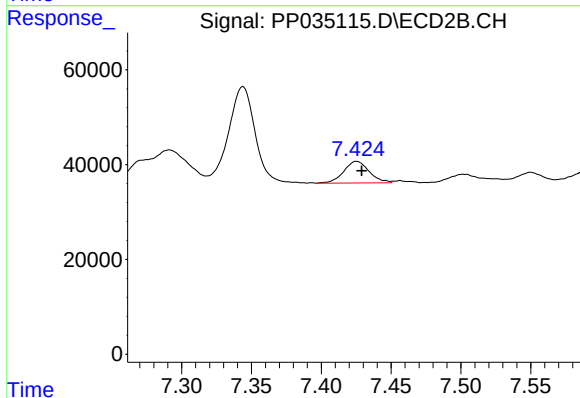


#33 AR-1260-3

R.T.: 7.425 min
Delta R.T.: -0.004 min
Response: 58314
Conc: 32.34 ng/ml

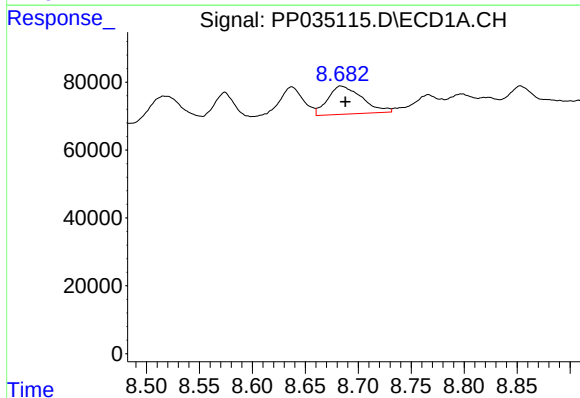


#34 AR-1260-4

R.T.: 8.684 min
Delta R.T.: -0.004 min
Response: 186999
Conc: 63.71 ng/ml

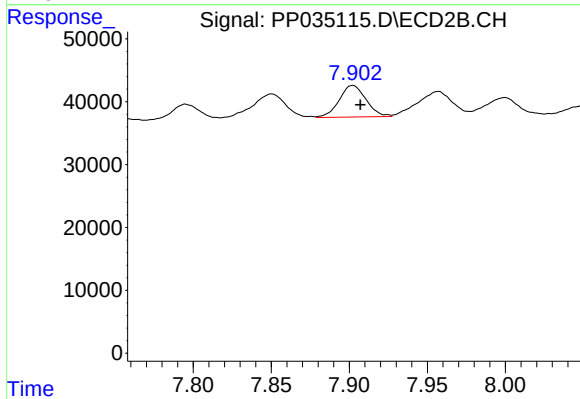

#34 AR-1260-4

R.T.: 7.902 min
Delta R.T.: -0.005 min
Response: 60415
Conc: 47.46 ng/ml

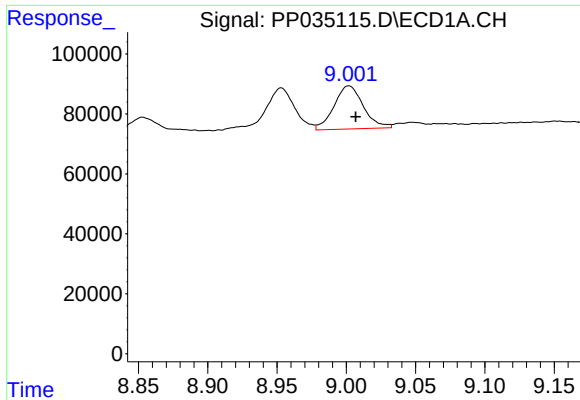


#35 AR-1260-5

R.T.: 9.002 min
Delta R.T.: -0.005 min
Response: 212094
Conc: 43.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-18-14.5-15.0

Manual Integrations
APPROVED

Ankita
4/22/2021 2:45:46 PM

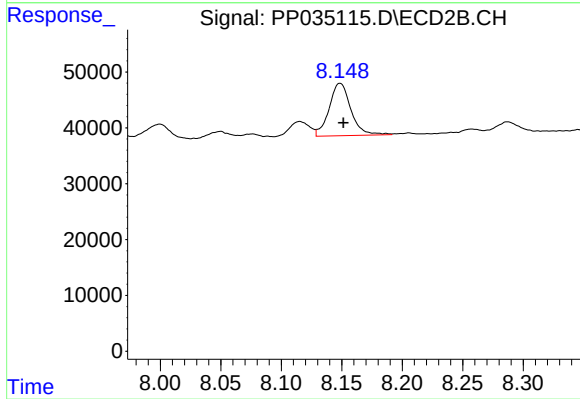

#35 AR-1260-5

R.T.: 8.149 min
Delta R.T.: -0.003 min
Response: 117134
Conc: 48.18 ng/ml