

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042121\
 Data File : PP035116.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Apr 2021 1:31
 Operator : DD\AJ
 Sample : M2076-19
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SB-19-0-2.0

Manual Integrations
 APPROVED

Ankita
 4/22/2021 2:45:48 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 22 02:56:48 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 21 17:37:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.835	4.251	1901788	1170175	23.339	22.723
2) SA Decachlor...	10.744	9.540	1774741	656325	28.084	27.623
Target Compounds						
31) L7 AR-1260-1	7.826	7.076	151462	88120	44.975	50.367
32) L7 AR-1260-2	8.089	7.274	332949	74085	97.799m	41.560 #
33) L7 AR-1260-3	8.455	7.425	116271	68795	46.323	38.153
34) L7 AR-1260-4	8.685	7.904	152515	62189	51.960	48.856
35) L7 AR-1260-5	9.003	8.147	281785	135603	57.278	55.774

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042121\
Data File : PP035116.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Apr 2021 1:31
Operator : DD\AJ
Sample : M2076-19
Misc :
ALS Vial : 44 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
SB-19-0-2.0


Manual Integrations
APPROVED

Ankita
4/22/2021 2:45:48 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 02:56:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 21 17:37:28 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

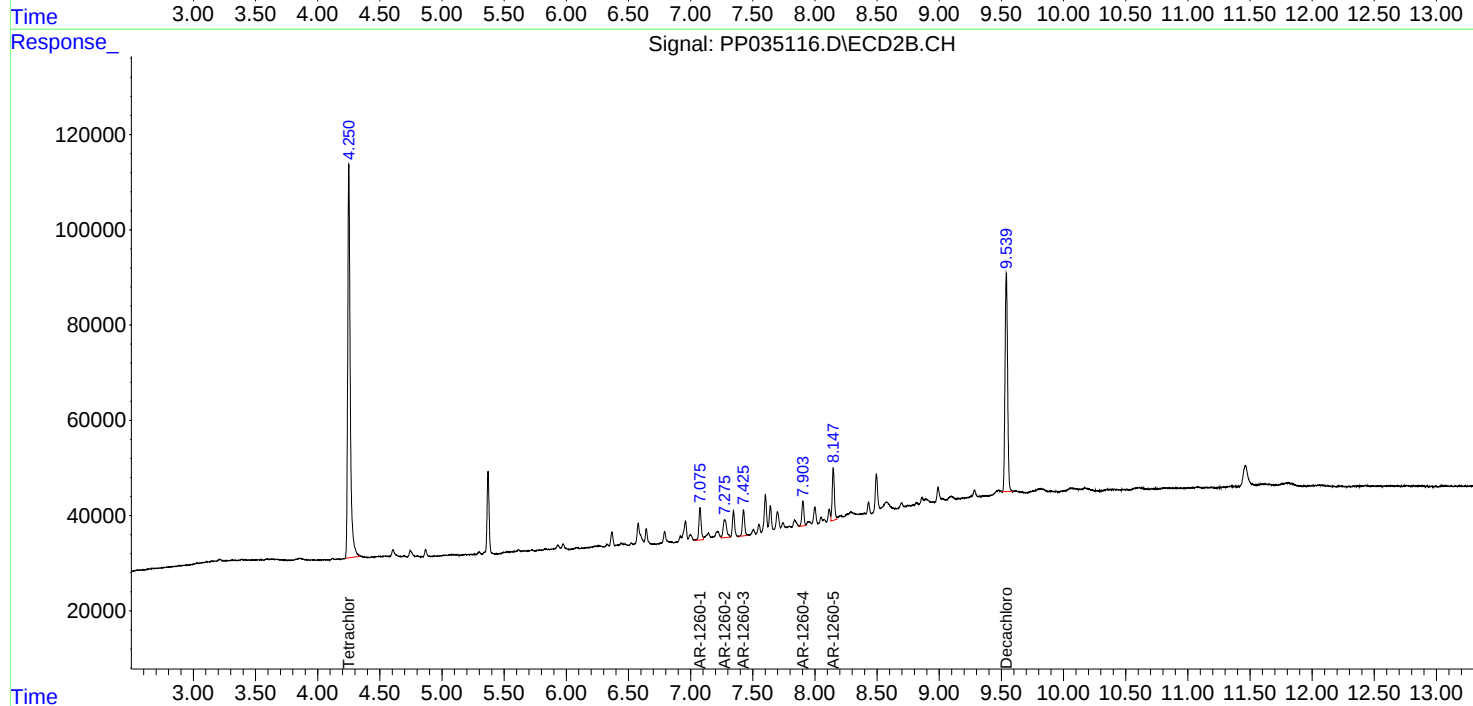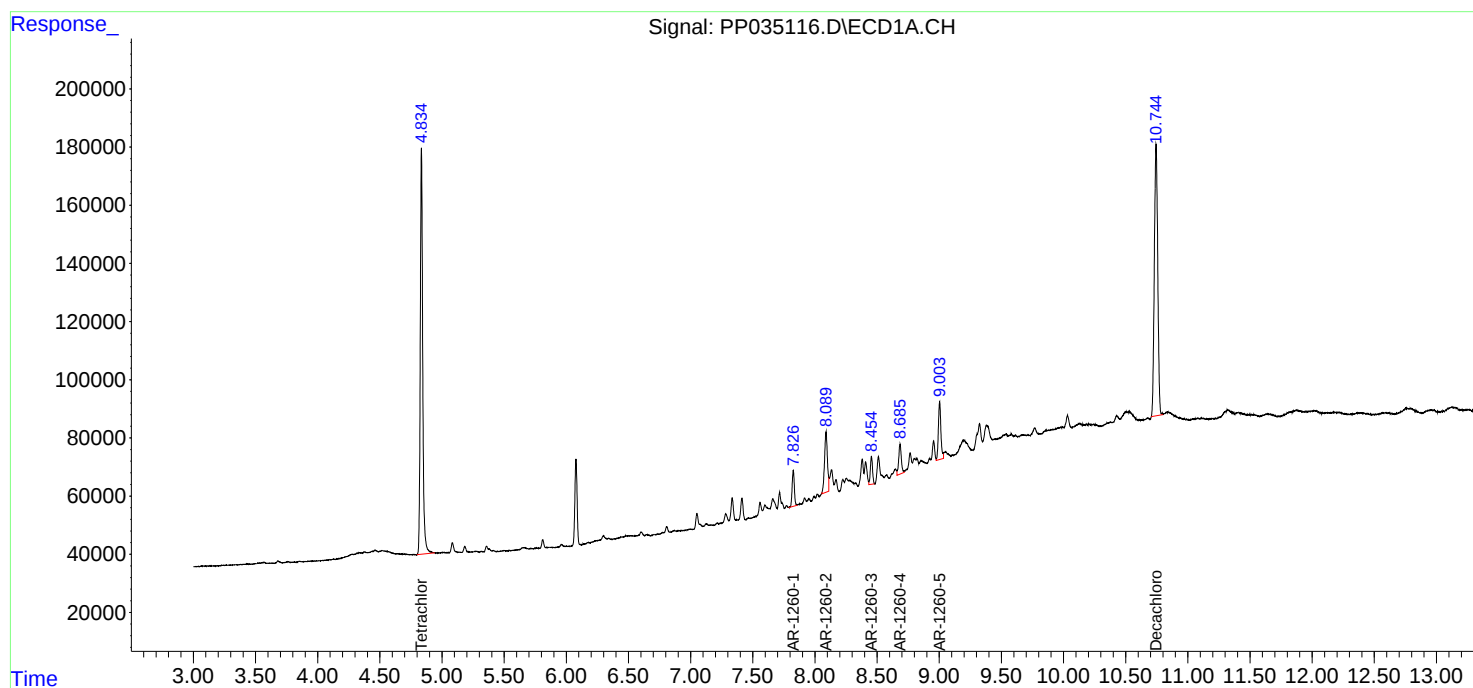

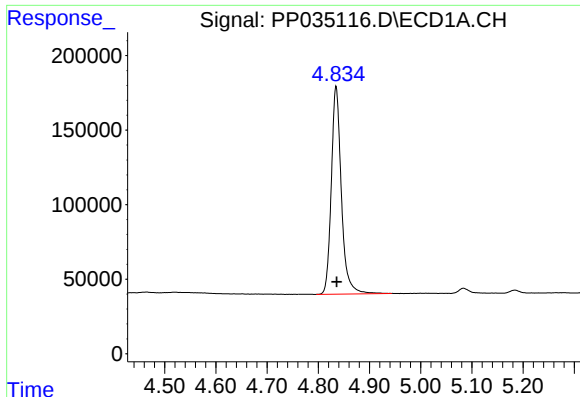


#1 Tetrachloro-m-xylene

R.T.: 4.835 min
Delta R.T.: -0.001 min
Response: 1901788
Conc: 23.34 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-19-0-2.0


Manual Integrations
APPROVED

Ankita
4/22/2021 2:45:48 PM

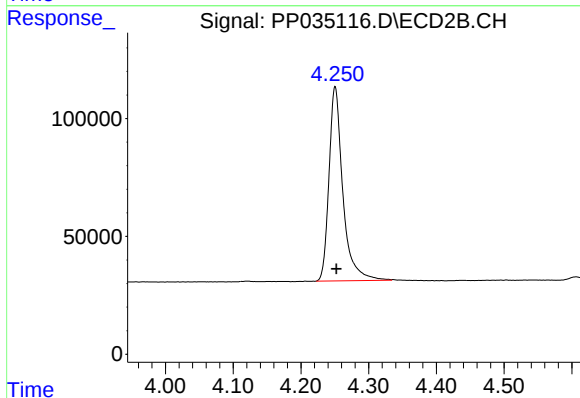


#1 Tetrachloro-m-xylene

R.T.: 4.251 min
Delta R.T.: -0.002 min
Response: 1170175
Conc: 22.72 ng/ml

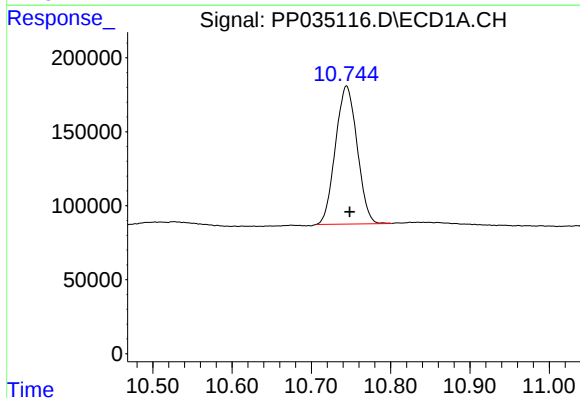


#2 Decachlorobiphenyl

R.T.: 10.744 min
Delta R.T.: -0.004 min
Response: 1774741
Conc: 28.08 ng/ml

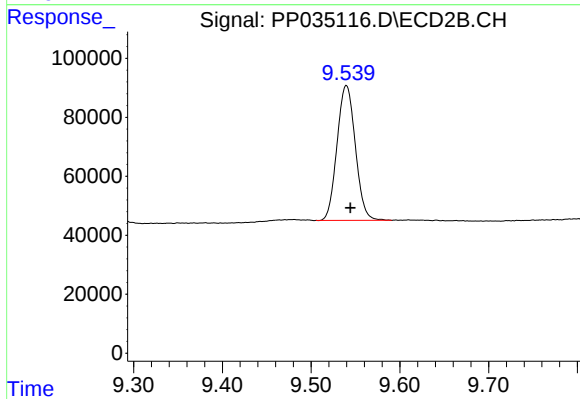

#2 Decachlorobiphenyl

R.T.: 9.540 min
Delta R.T.: -0.005 min
Response: 656325
Conc: 27.62 ng/ml

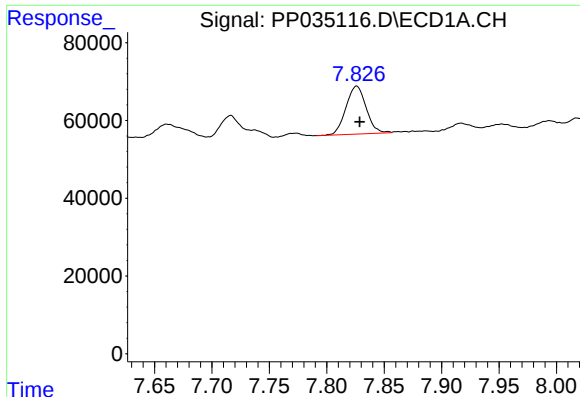


#31 AR-1260-1

R.T.: 7.826 min
Delta R.T.: -0.003 min
Response: 151462
Conc: 44.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-19-0-2.0


Manual Integrations
APPROVED

Ankita
4/22/2021 2:45:48 PM

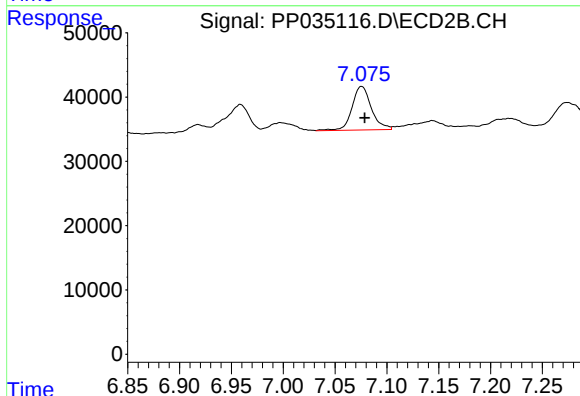


#31 AR-1260-1

R.T.: 7.076 min
Delta R.T.: -0.003 min
Response: 88120
Conc: 50.37 ng/ml

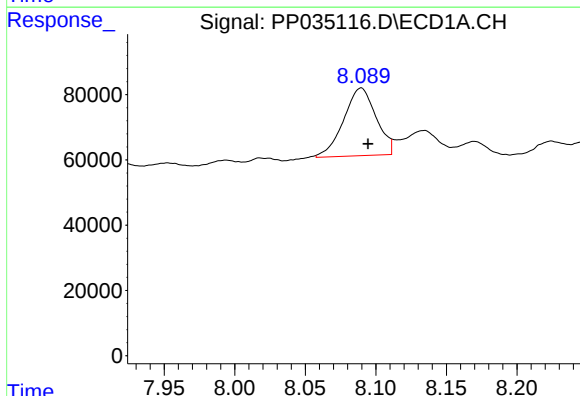


#32 AR-1260-2

R.T.: 8.089 min
Delta R.T.: -0.005 min
Response: 332949
Conc: 97.80 ng/ml m

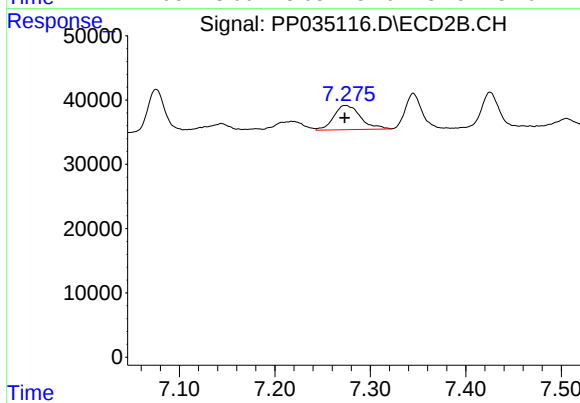

#32 AR-1260-2

R.T.: 7.274 min
Delta R.T.: 0.001 min
Response: 74085
Conc: 41.56 ng/ml

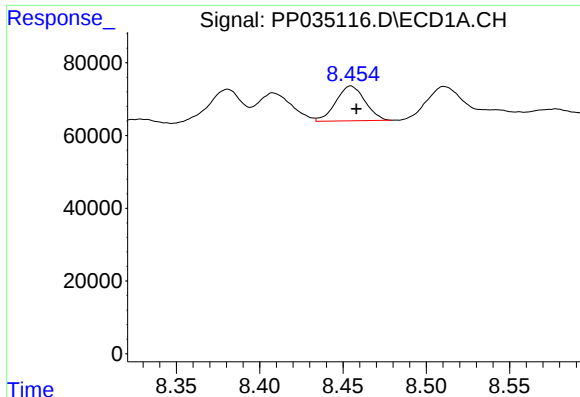


#33 AR-1260-3

R.T.: 8.455 min
Delta R.T.: -0.003 min
Response: 116271
Conc: 46.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-19-0-2.0


Manual Integrations
APPROVED

Ankita
4/22/2021 2:45:48 PM

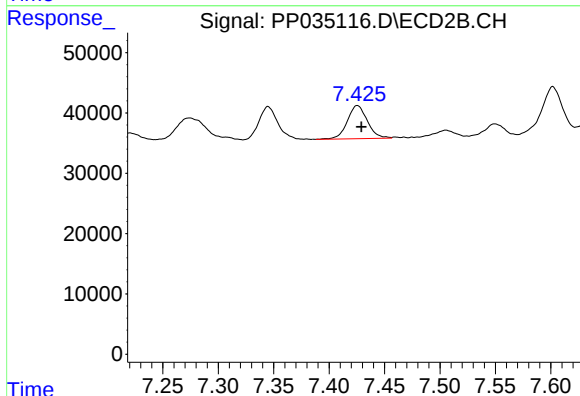


#33 AR-1260-3

R.T.: 7.425 min
Delta R.T.: -0.004 min
Response: 68795
Conc: 38.15 ng/ml

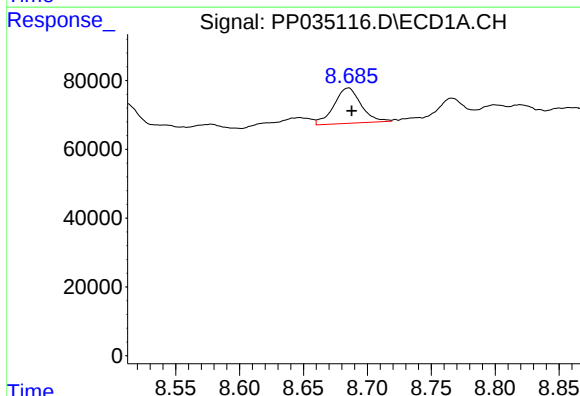


#34 AR-1260-4

R.T.: 8.685 min
Delta R.T.: -0.003 min
Response: 152515
Conc: 51.96 ng/ml

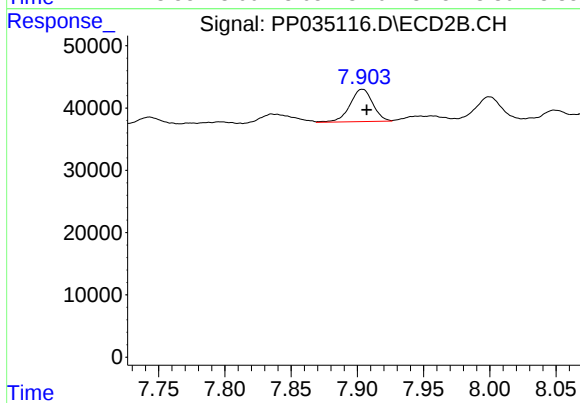

#34 AR-1260-4

R.T.: 7.904 min
Delta R.T.: -0.003 min
Response: 62189
Conc: 48.86 ng/ml

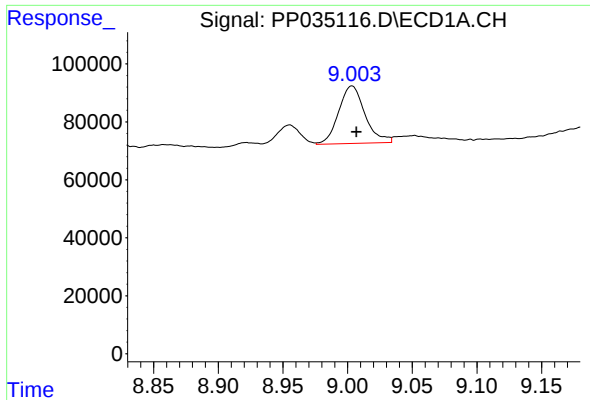


#35 AR-1260-5

R.T.: 9.003 min
Delta R.T.: -0.003 min
Response: 281785
Conc: 57.28 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-19-0-2.0

Manual Integrations
APPROVED

Ankita
4/22/2021 2:45:48 PM

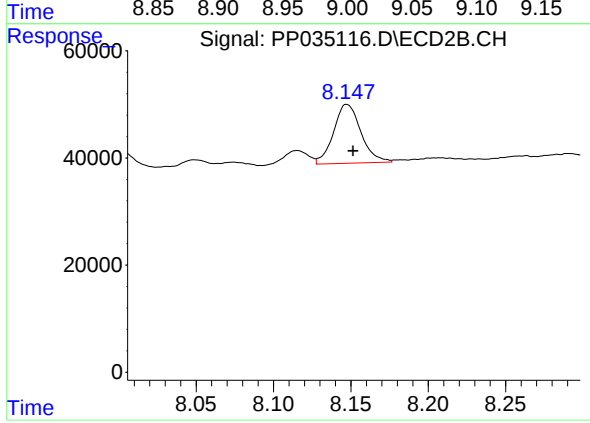

#35 AR-1260-5

R.T.: 8.147 min
Delta R.T.: -0.004 min
Response: 135603
Conc: 55.77 ng/ml