

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042121\
 Data File : PP035117.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Apr 2021 1:48
 Operator : DD\AJ
 Sample : M2077-01
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SB-19-14.5-15.0

Manual Integrations
 APPROVED

Ankita
 4/22/2021 2:45:49 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 22 07:46:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 21 17:37:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.835	4.250	1689197	1020431	20.730	19.815
2) SA Decachlor...	10.742	9.540	2901506	1041166	45.915	43.820
Target Compounds						
31) L7 AR-1260-1	7.812f	7.077	34308	58939	10.187m	33.688 #
32) L7 AR-1260-2	8.091	7.271	310495	89064	91.203	49.962m#
33) L7 AR-1260-3	8.455	7.426	65703	44742	26.176	24.814m
34) L7 AR-1260-4	8.683	7.903	110571	39389	37.670	30.944
35) L7 AR-1260-5	9.002	8.148	129053	86278	26.232	35.487 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042121\
Data File : PP035117.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Apr 2021 1:48
Operator : DD\AJ
Sample : M2077-01
Misc :
ALS Vial : 45 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
SB-19-14.5-15.0


Manual Integrations
APPROVED

Ankita
4/22/2021 2:45:49 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 07:46:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 21 17:37:28 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

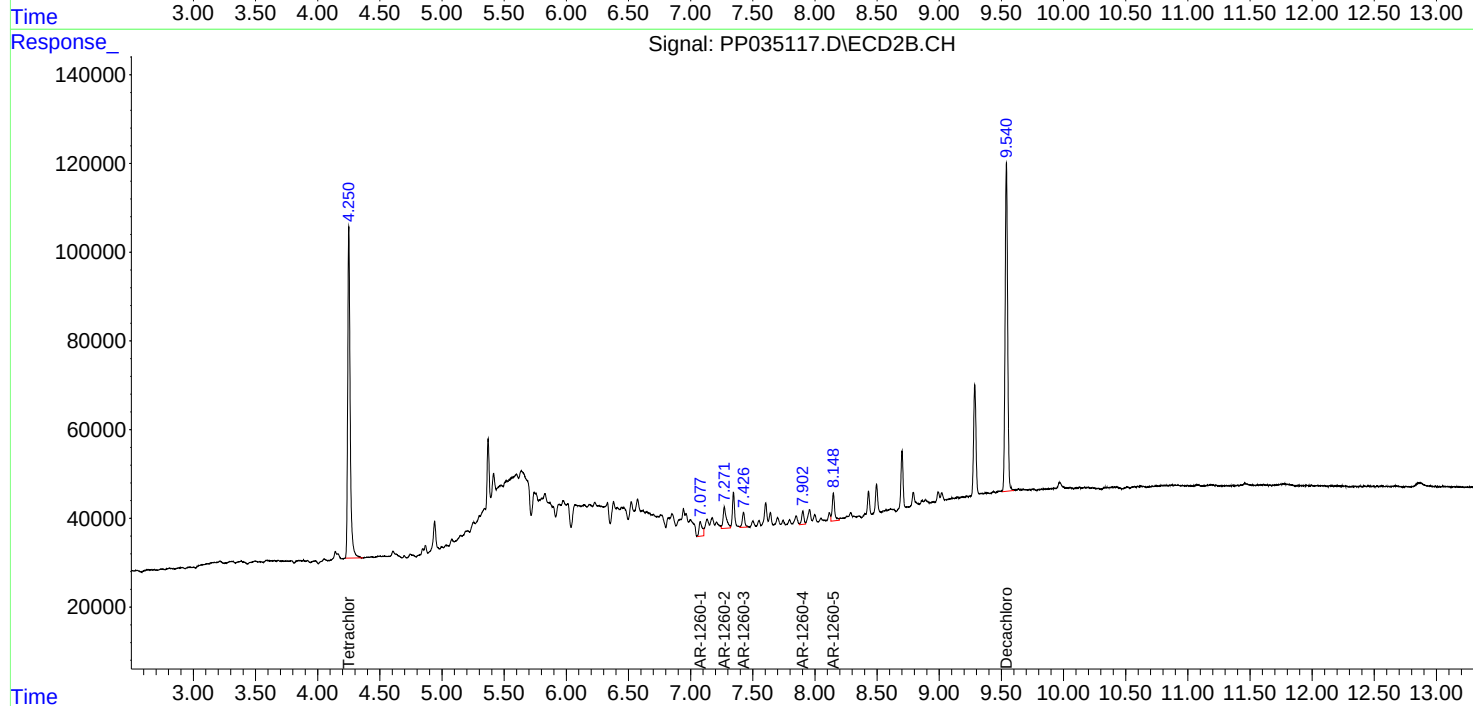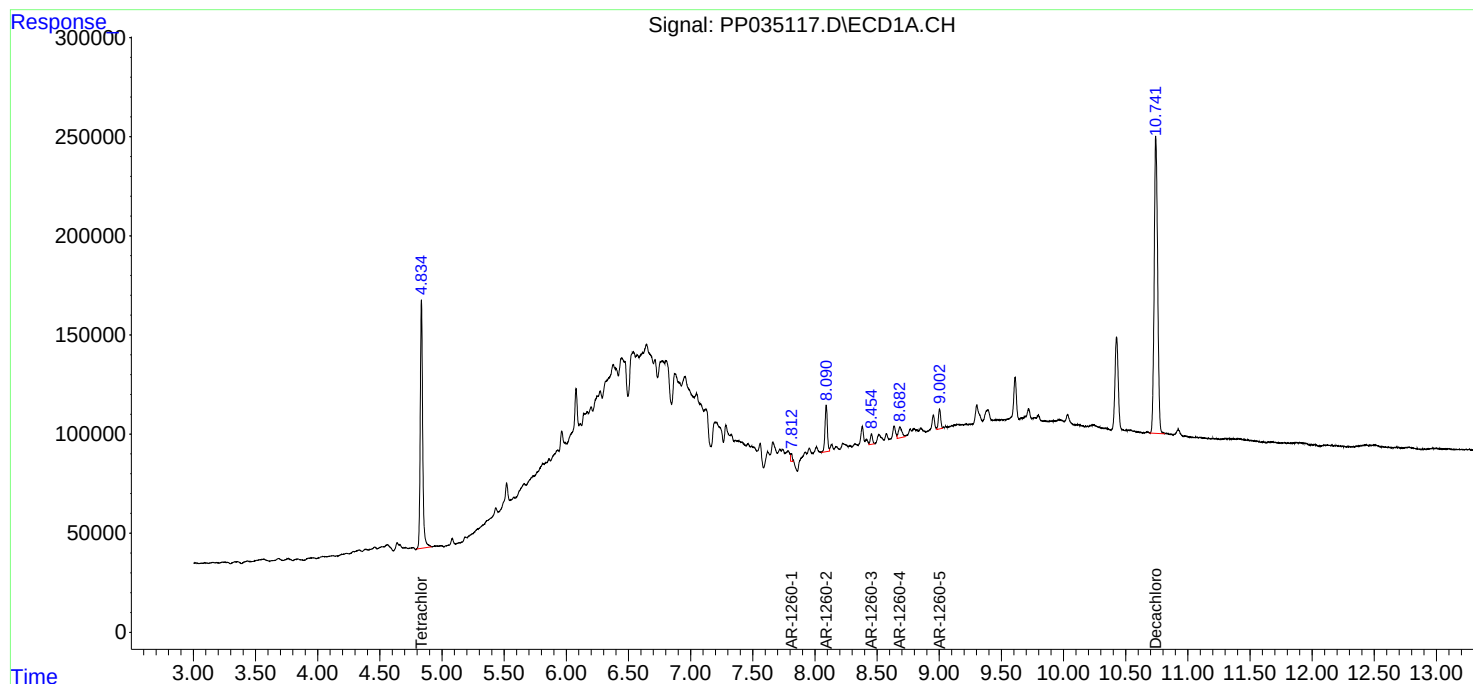

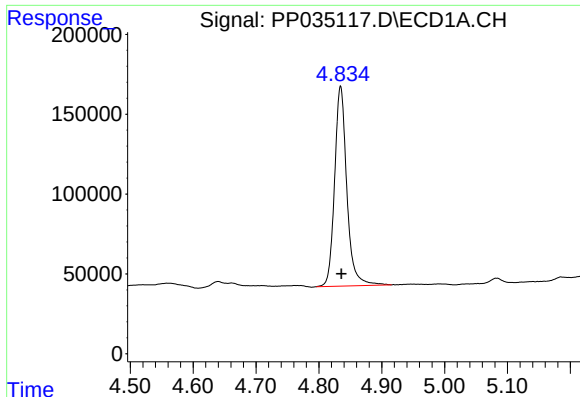


#1 Tetrachloro-m-xylene

R.T.: 4.835 min
Delta R.T.: -0.001 min
Response: 1689197
Conc: 20.73 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-19-14.5-15.0


Manual Integrations
APPROVED

Ankita
4/22/2021 2:45:49 PM

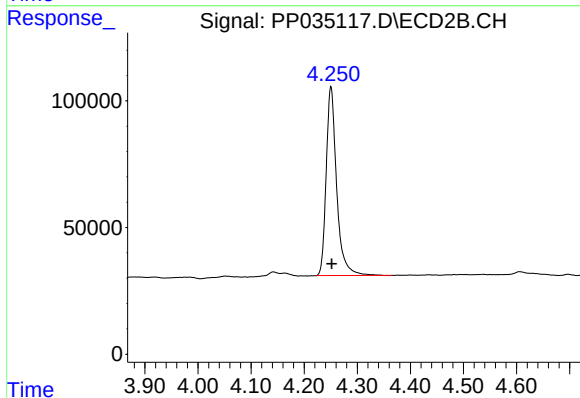


#1 Tetrachloro-m-xylene

R.T.: 4.250 min
Delta R.T.: -0.002 min
Response: 1020431
Conc: 19.82 ng/ml

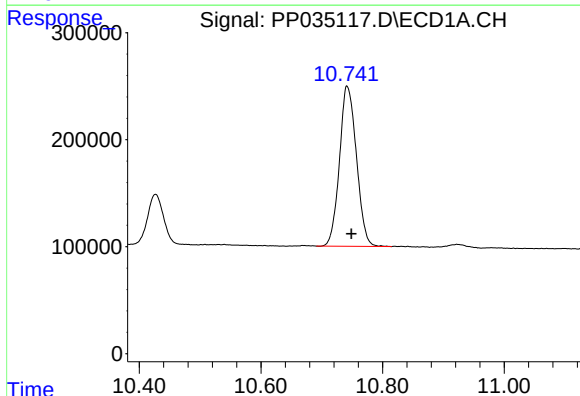


#2 Decachlorobiphenyl

R.T.: 10.742 min
Delta R.T.: -0.007 min
Response: 2901506
Conc: 45.91 ng/ml

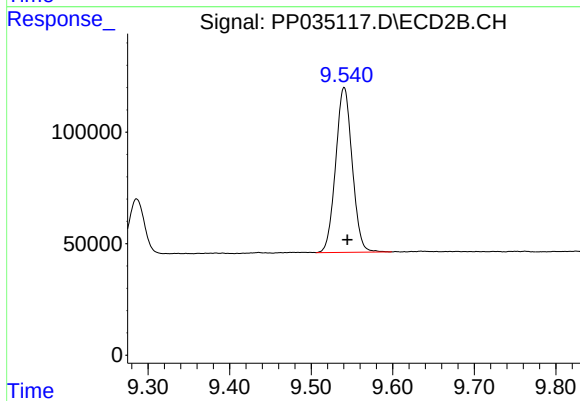

#2 Decachlorobiphenyl

R.T.: 9.540 min
Delta R.T.: -0.004 min
Response: 1041166
Conc: 43.82 ng/ml

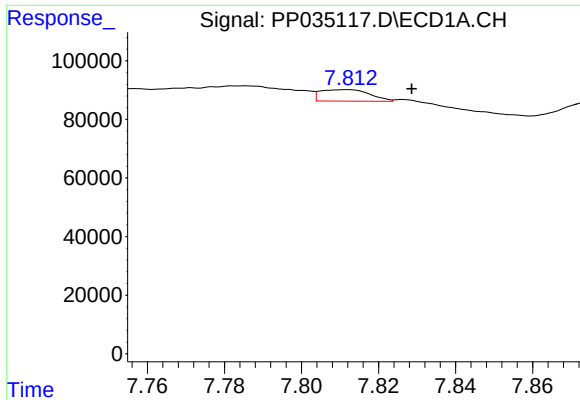


#31 AR-1260-1

R.T.: 7.812 min
Delta R.T.: -0.016 min
Response: 34308
Conc: 10.19 ng/ml m

Instrument :
ECD_P
ClientSampleId :
SB-19-14.5-15.0


Manual Integrations
APPROVED

Ankita
4/22/2021 2:45:49 PM

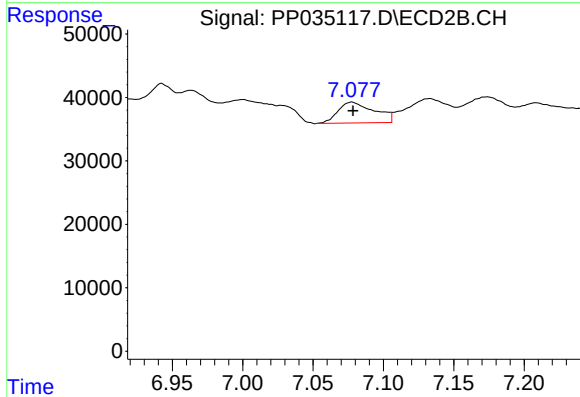


#31 AR-1260-1

R.T.: 7.077 min
Delta R.T.: -0.001 min
Response: 58939
Conc: 33.69 ng/ml

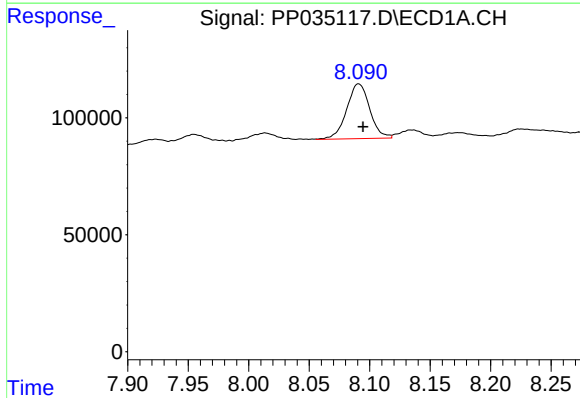


#32 AR-1260-2

R.T.: 8.091 min
Delta R.T.: -0.004 min
Response: 310495
Conc: 91.20 ng/ml

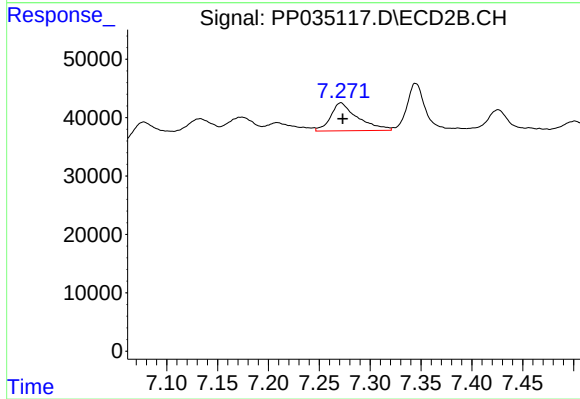

#32 AR-1260-2

R.T.: 7.271 min
Delta R.T.: -0.002 min
Response: 89064
Conc: 49.96 ng/ml m

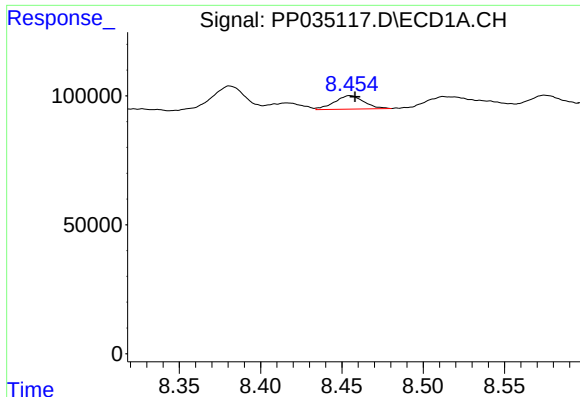


#33 AR-1260-3

R.T.: 8.455 min
Delta R.T.: -0.003 min
Response: 65703
Conc: 26.18 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-19-14.5-15.0


Manual Integrations
APPROVED

Ankita
4/22/2021 2:45:49 PM

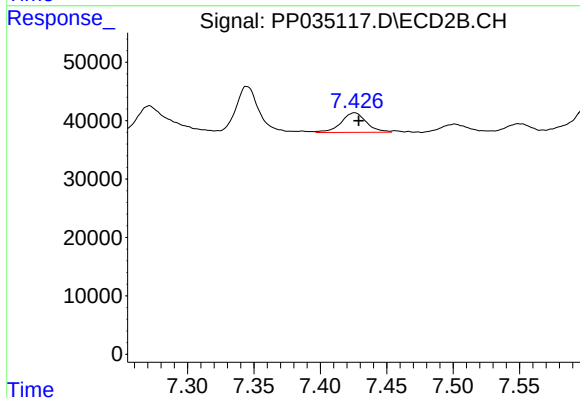


#33 AR-1260-3

R.T.: 7.426 min
Delta R.T.: -0.003 min
Response: 44742
Conc: 24.81 ng/ml m

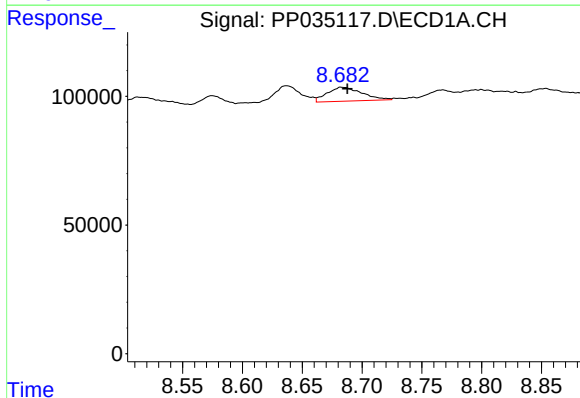


#34 AR-1260-4

R.T.: 8.683 min
Delta R.T.: -0.005 min
Response: 110571
Conc: 37.67 ng/ml

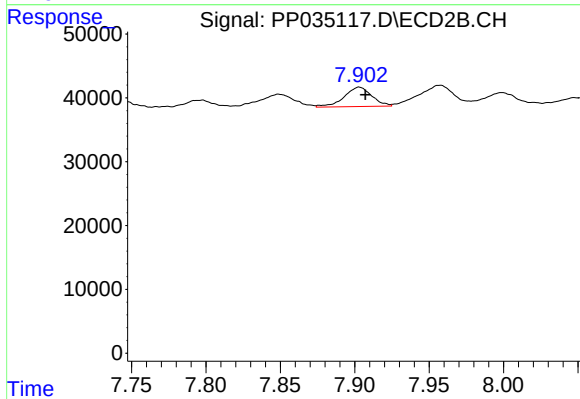

#34 AR-1260-4

R.T.: 7.903 min
Delta R.T.: -0.004 min
Response: 39389
Conc: 30.94 ng/ml

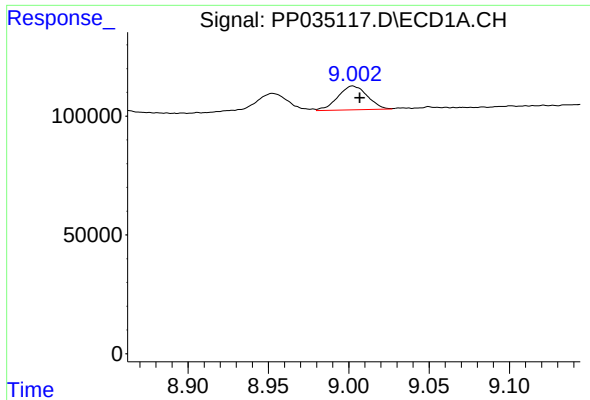


#35 AR-1260-5

R.T.: 9.002 min
Delta R.T.: -0.004 min
Response: 129053
Conc: 26.23 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-19-14.5-15.0

Manual Integrations
APPROVED

Ankita
4/22/2021 2:45:49 PM

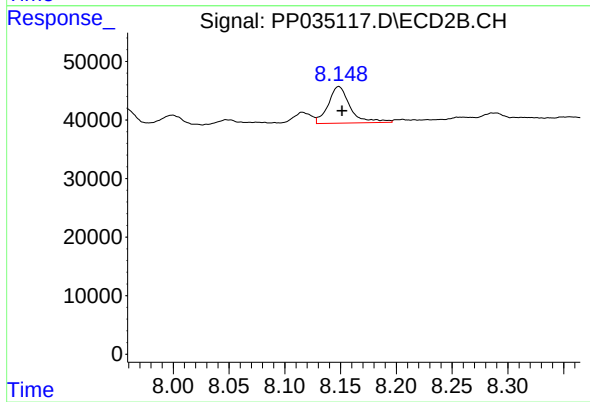

#35 AR-1260-5

R.T.: 8.148 min
Delta R.T.: -0.003 min
Response: 86278
Conc: 35.49 ng/ml