

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042121\
 Data File : PP035127.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Apr 2021 4:54
 Operator : DD\AJ
 Sample : M2090-13
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SEDGWICK-COMP-3

Manual Integrations
 APPROVED

Ankita
 4/22/2021 2:45:58 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 22 07:09:48 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 21 17:37:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.835	4.249	1686349	1007511	20.695	19.565
2)	SA Decachlor...	10.746	9.541	1798559	619026	28.461	26.053
Target Compounds							
26)	L6 AR-1254-1	7.053	6.367	155376	105157	60.271m	62.122
27)	L6 AR-1254-2	7.281	6.522	292524	66523	77.303m	44.523 #
28)	L6 AR-1254-3	7.661	6.942	304629	120747	81.651	56.783m#
29)	L6 AR-1254-4	7.956	7.178	127502	54855	60.877	61.211
30)	L6 AR-1254-5	8.382	7.602	356414	284151	122.514	159.867 #
31)	L7 AR-1260-1	7.826	7.074	192979	91752	57.303	52.443m
32)	L7 AR-1260-2	8.091	7.270	713113	120830	209.466	67.782 #
33)	L7 AR-1260-3	8.456	7.424	124872	95189	49.750	52.791m
34)	L7 AR-1260-4	8.682	7.903	255734	54665	87.125	42.946 #
35)	L7 AR-1260-5	9.003	8.147	273939	146773	55.683	60.369m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042121\
Data File : PP035127.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Apr 2021 4:54
Operator : DD\AJ
Sample : M2090-13
Misc :
ALS Vial : 53 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
SEDGWICK-COMP-3


Manual Integrations
APPROVED

Ankita
4/22/2021 2:45:58 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 07:09:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 21 17:37:28 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

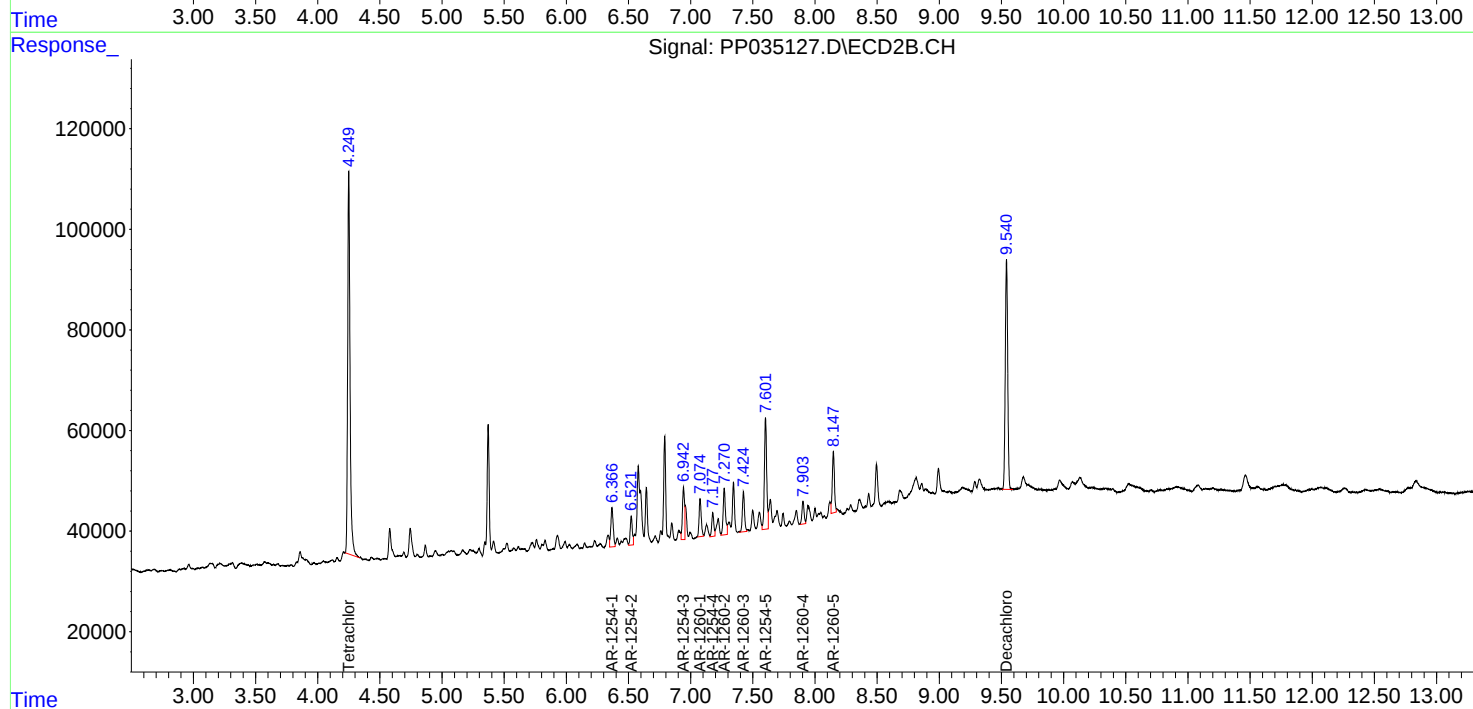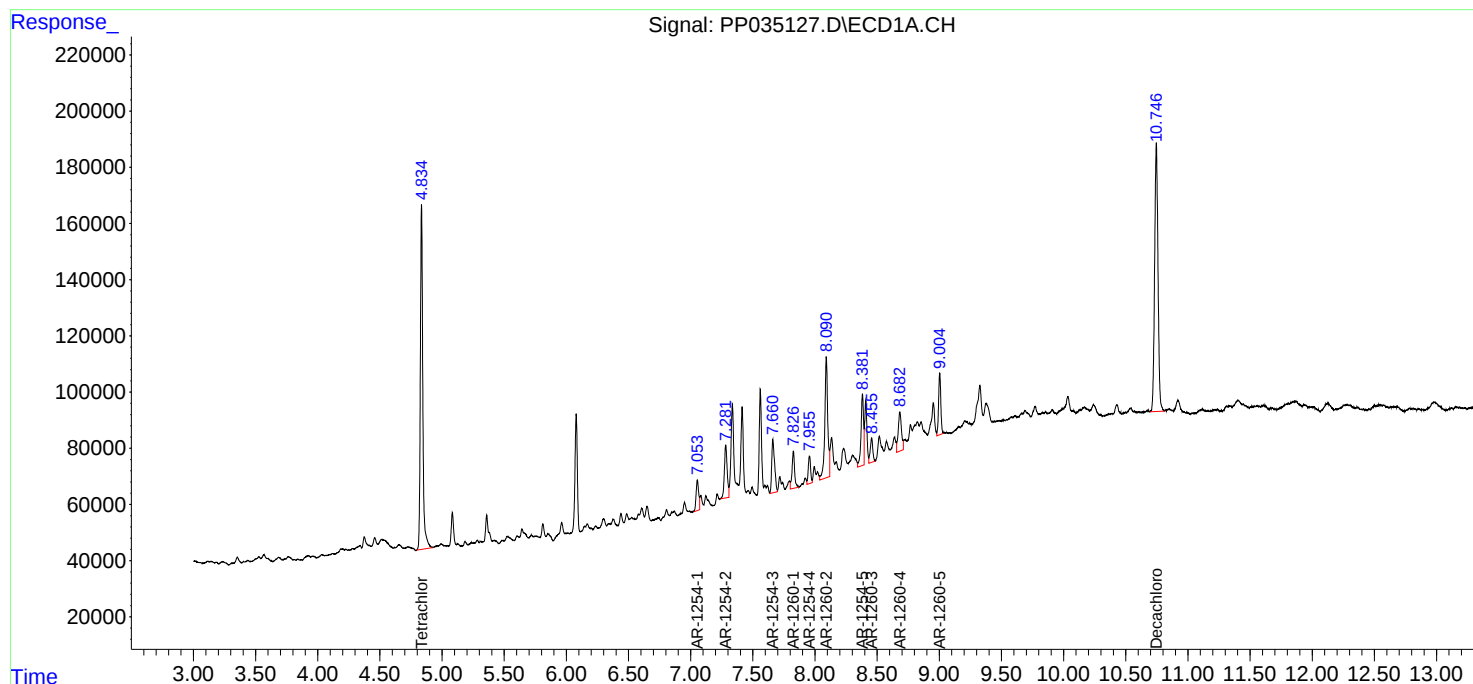

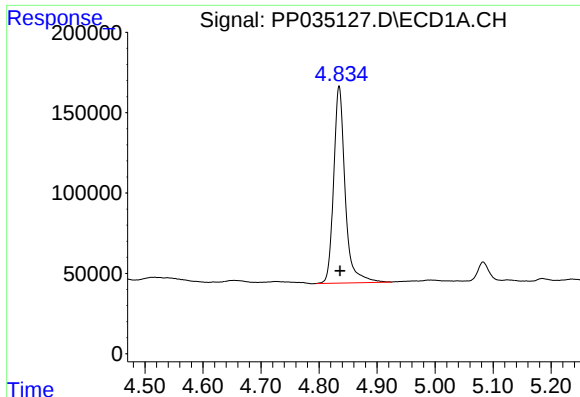


#1 Tetrachloro-m-xylene

R.T.: 4.835 min
Delta R.T.: -0.001 min
Response: 1686349
Conc: 20.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
SEDGWICK-COMP-3


Manual Integrations
APPROVED

Ankita
4/22/2021 2:45:58 PM

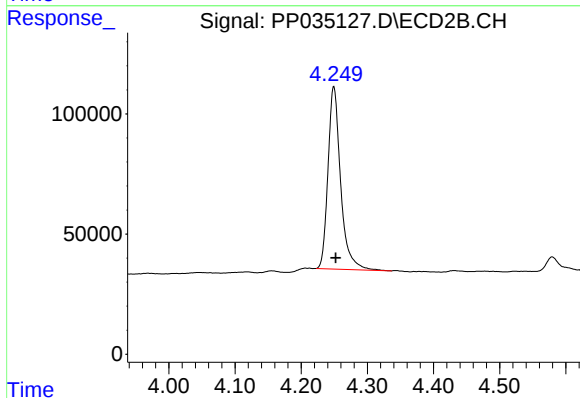


#1 Tetrachloro-m-xylene

R.T.: 4.249 min
Delta R.T.: -0.003 min
Response: 1007511
Conc: 19.56 ng/ml

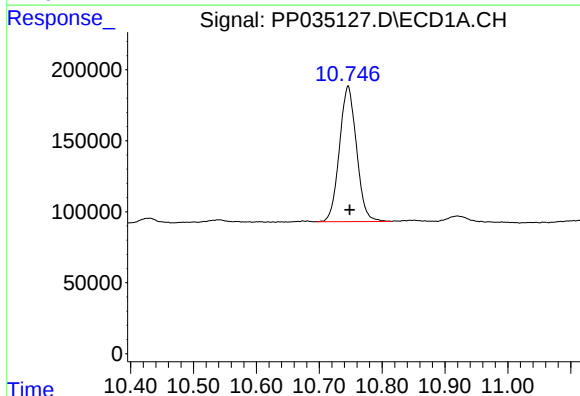


#2 Decachlorobiphenyl

R.T.: 10.746 min
Delta R.T.: -0.003 min
Response: 1798559
Conc: 28.46 ng/ml

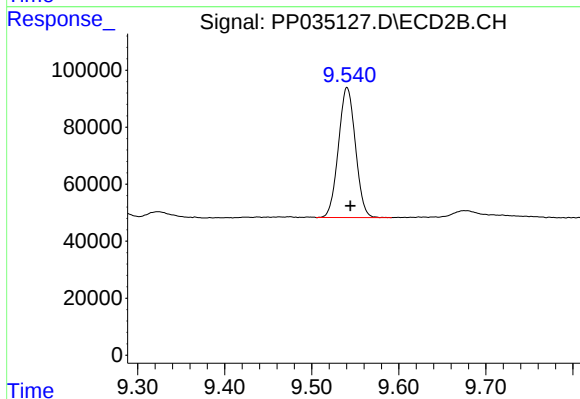

#2 Decachlorobiphenyl

R.T.: 9.541 min
Delta R.T.: -0.004 min
Response: 619026
Conc: 26.05 ng/ml

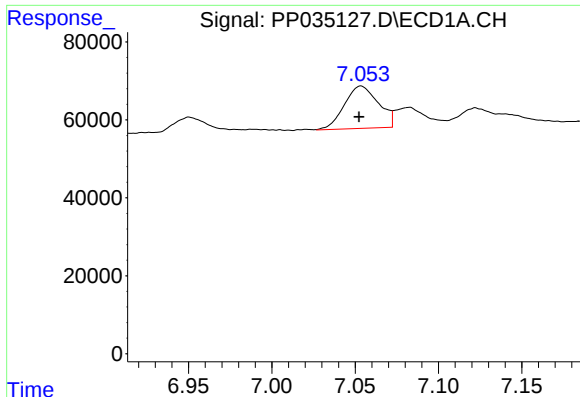


#26 AR-1254-1

R.T.: 7.053 min
Delta R.T.: 0.000 min
Response: 155376
Conc: 60.27 ng/ml m

Instrument :
ECD_P
ClientSampleId :
SEDGWICK-COMP-3


Manual Integrations
APPROVED

Ankita
4/22/2021 2:45:58 PM

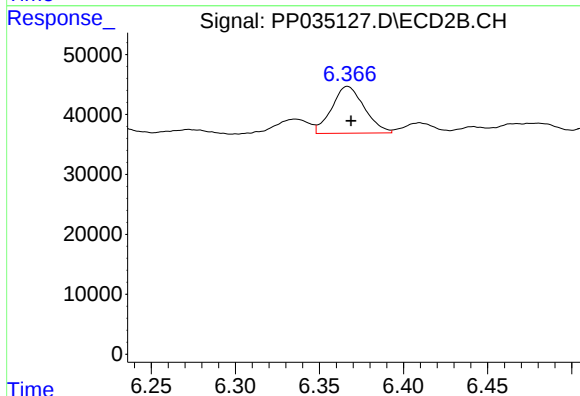


#26 AR-1254-1

R.T.: 6.367 min
Delta R.T.: -0.002 min
Response: 105157
Conc: 62.12 ng/ml

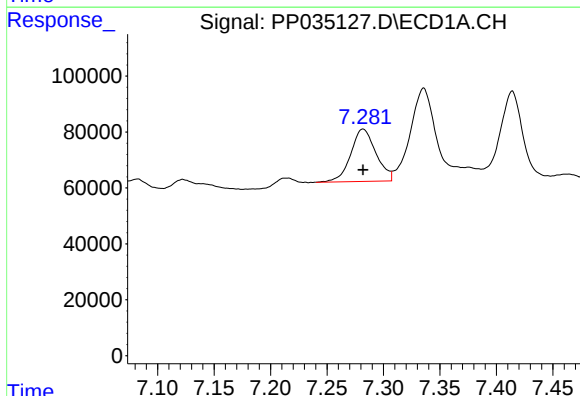


#27 AR-1254-2

R.T.: 7.281 min
Delta R.T.: 0.000 min
Response: 292524
Conc: 77.30 ng/ml m

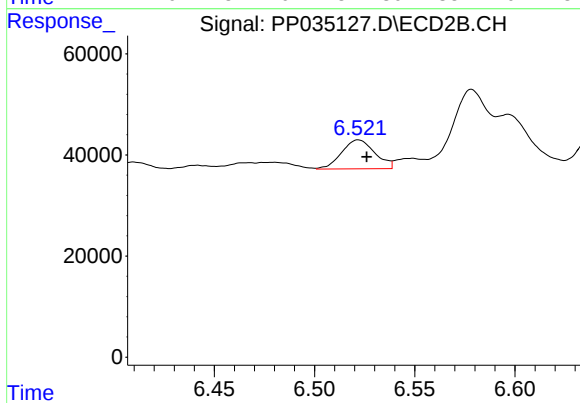

#27 AR-1254-2

R.T.: 6.522 min
Delta R.T.: -0.004 min
Response: 66523
Conc: 44.52 ng/ml

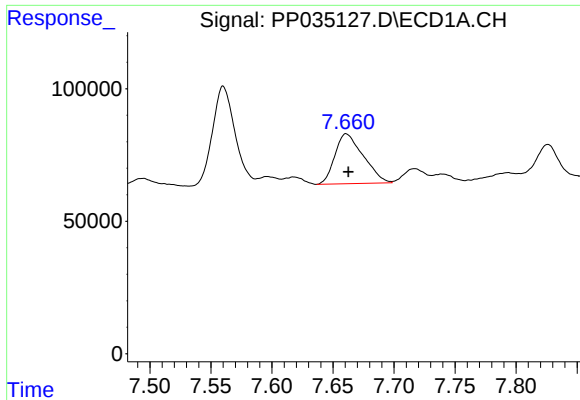


#28 AR-1254-3

R.T.: 7.661 min
Delta R.T.: -0.002 min
Response: 304629
Conc: 81.65 ng/ml

Instrument :
ECD_P
ClientSampleId :
SEDGWICK-COMP-3


Manual Integrations
APPROVED

Ankita
4/22/2021 2:45:58 PM

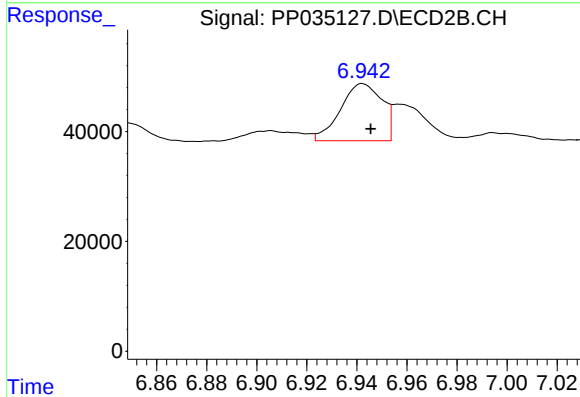


#28 AR-1254-3

R.T.: 6.942 min
Delta R.T.: -0.004 min
Response: 120747
Conc: 56.78 ng/ml m

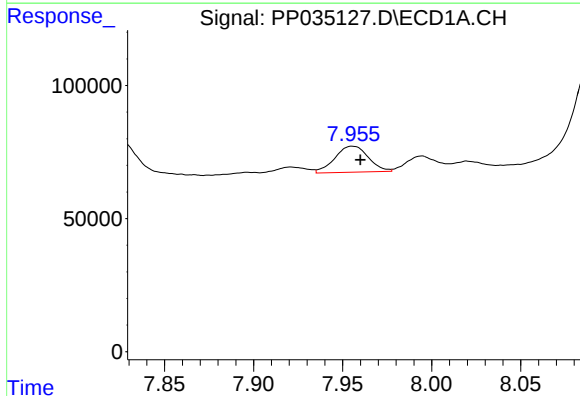


#29 AR-1254-4

R.T.: 7.956 min
Delta R.T.: -0.004 min
Response: 127502
Conc: 60.88 ng/ml

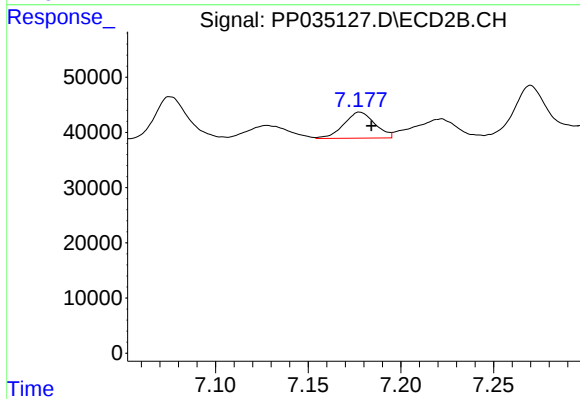

#29 AR-1254-4

R.T.: 7.178 min
Delta R.T.: -0.006 min
Response: 54855
Conc: 61.21 ng/ml

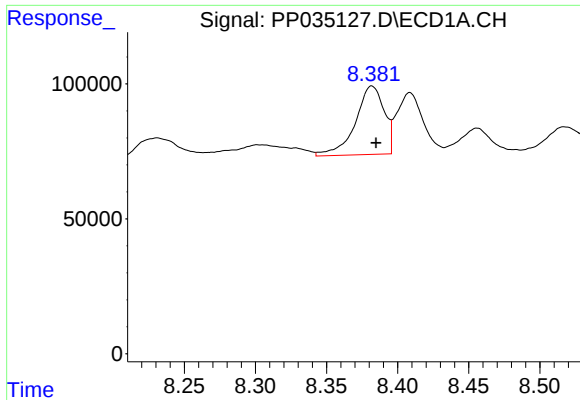


#30 AR-1254-5

R.T.: 8.382 min
Delta R.T.: -0.003 min
Response: 356414
Conc: 122.51 ng/ml

Instrument :
ECD_P
ClientSampleId :
SEDGWICK-COMP-3


Manual Integrations
APPROVED

Ankita
4/22/2021 2:45:58 PM

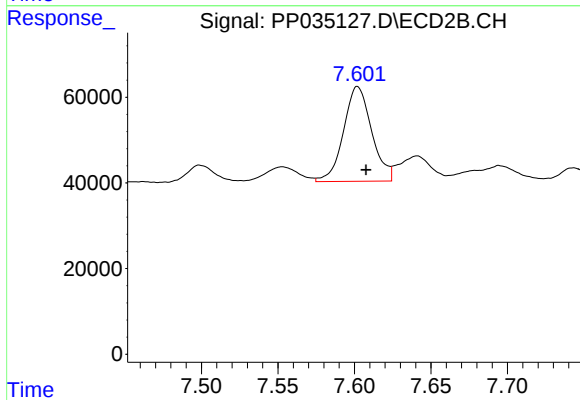


#30 AR-1254-5

R.T.: 7.602 min
Delta R.T.: -0.005 min
Response: 284151
Conc: 159.87 ng/ml

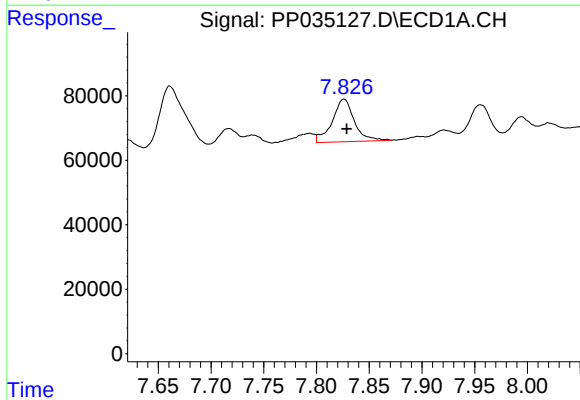


#31 AR-1260-1

R.T.: 7.826 min
Delta R.T.: -0.002 min
Response: 192979
Conc: 57.30 ng/ml

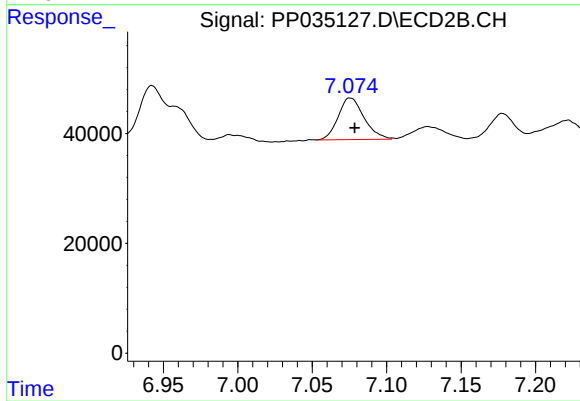

#31 AR-1260-1

R.T.: 7.074 min
Delta R.T.: -0.004 min
Response: 91752
Conc: 52.44 ng/ml m

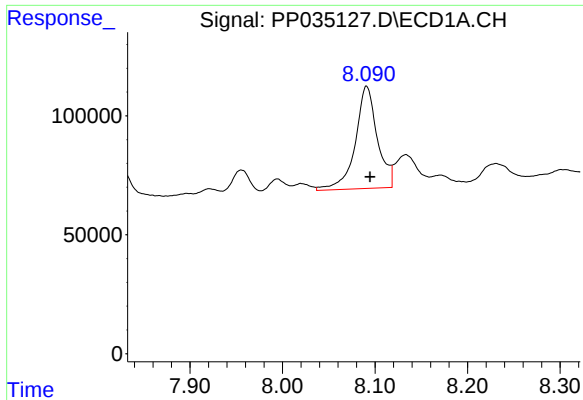


#32 AR-1260-2

R.T.: 8.091 min
Delta R.T.: -0.004 min
Response: 713113
Conc: 209.47 ng/ml

Instrument :
ECD_P
ClientSampleId :
SEDGWICK-COMP-3


Manual Integrations
APPROVED

Ankita
4/22/2021 2:45:58 PM

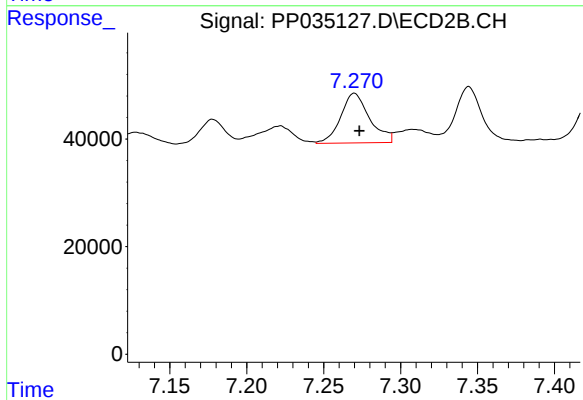


#32 AR-1260-2

R.T.: 7.270 min
Delta R.T.: -0.003 min
Response: 120830
Conc: 67.78 ng/ml

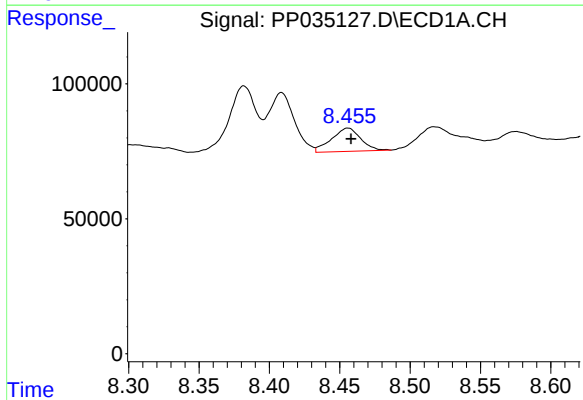


#33 AR-1260-3

R.T.: 8.456 min
Delta R.T.: -0.002 min
Response: 124872
Conc: 49.75 ng/ml

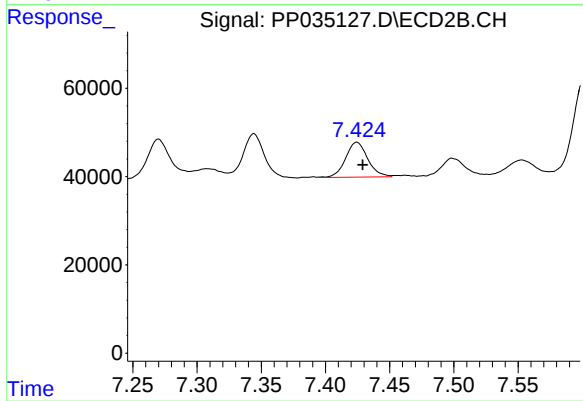

#33 AR-1260-3

R.T.: 7.424 min
Delta R.T.: -0.005 min
Response: 95189
Conc: 52.79 ng/ml m

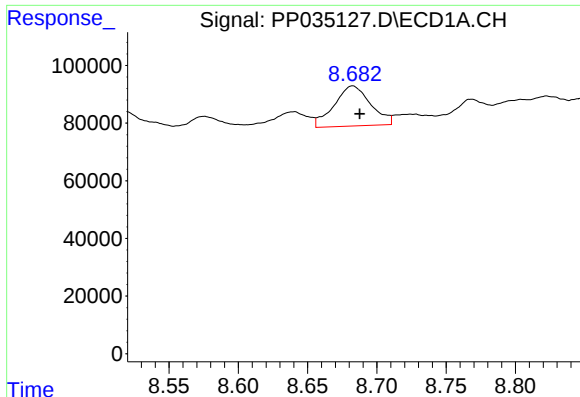


#34 AR-1260-4

R.T.: 8.682 min
Delta R.T.: -0.005 min
Response: 255734
Conc: 87.12 ng/ml

Instrument :
ECD_P
ClientSampleId :
SEDGWICK-COMP-3


Manual Integrations
APPROVED

Ankita
4/22/2021 2:45:58 PM

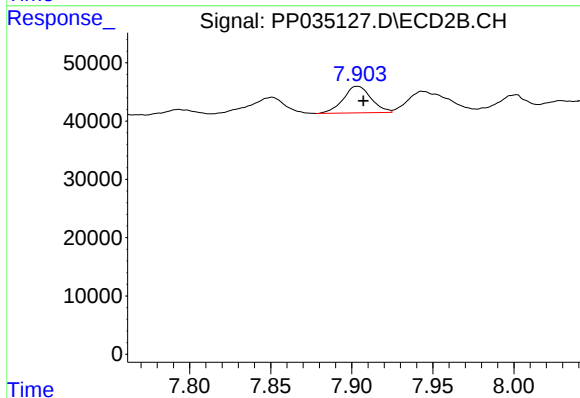


#34 AR-1260-4

R.T.: 7.903 min
Delta R.T.: -0.004 min
Response: 54665
Conc: 42.95 ng/ml

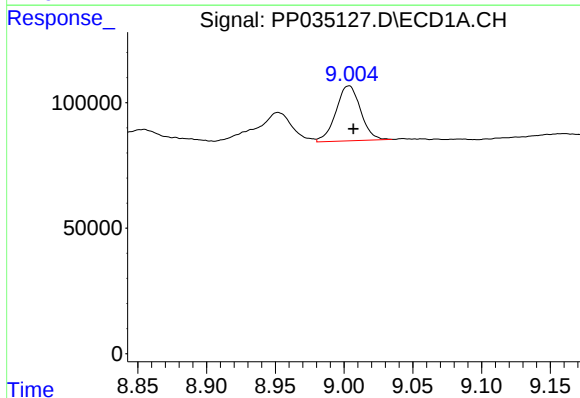

#35 AR-1260-5

R.T.: 9.003 min
Delta R.T.: -0.003 min
Response: 273939
Conc: 55.68 ng/ml

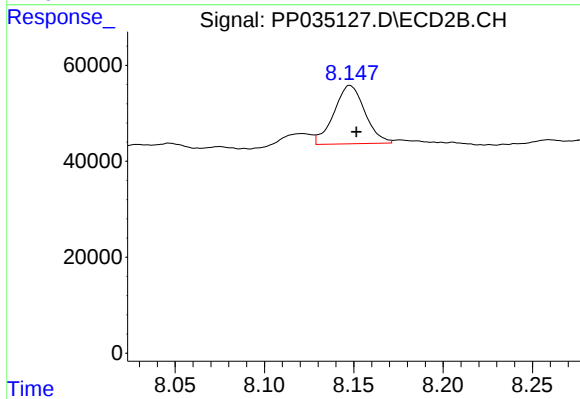

#35 AR-1260-5

R.T.: 8.147 min
Delta R.T.: -0.004 min
Response: 146773
Conc: 60.37 ng/ml m