

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042121\
 Data File : PP035140.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Apr 2021 10:53
 Operator : DD\AJ
 Sample : M2078-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TWP-01

Manual Integrations
 APPROVED

Ankita
 4/22/2021 2:46:04 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 22 13:48:15 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 21 17:37:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.838	4.250	1193170	720610	14.643m	13.993
2) SA Decachlor...	10.749	9.539	1290417	462324	20.420	19.458

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042121\
Data File : PP035140.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Apr 2021 10:53
Operator : DD\AJ
Sample : M2078-01
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
TWP-01


Manual Integrations
APPROVED

Ankita
4/22/2021 2:46:04 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 13:48:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 21 17:37:28 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

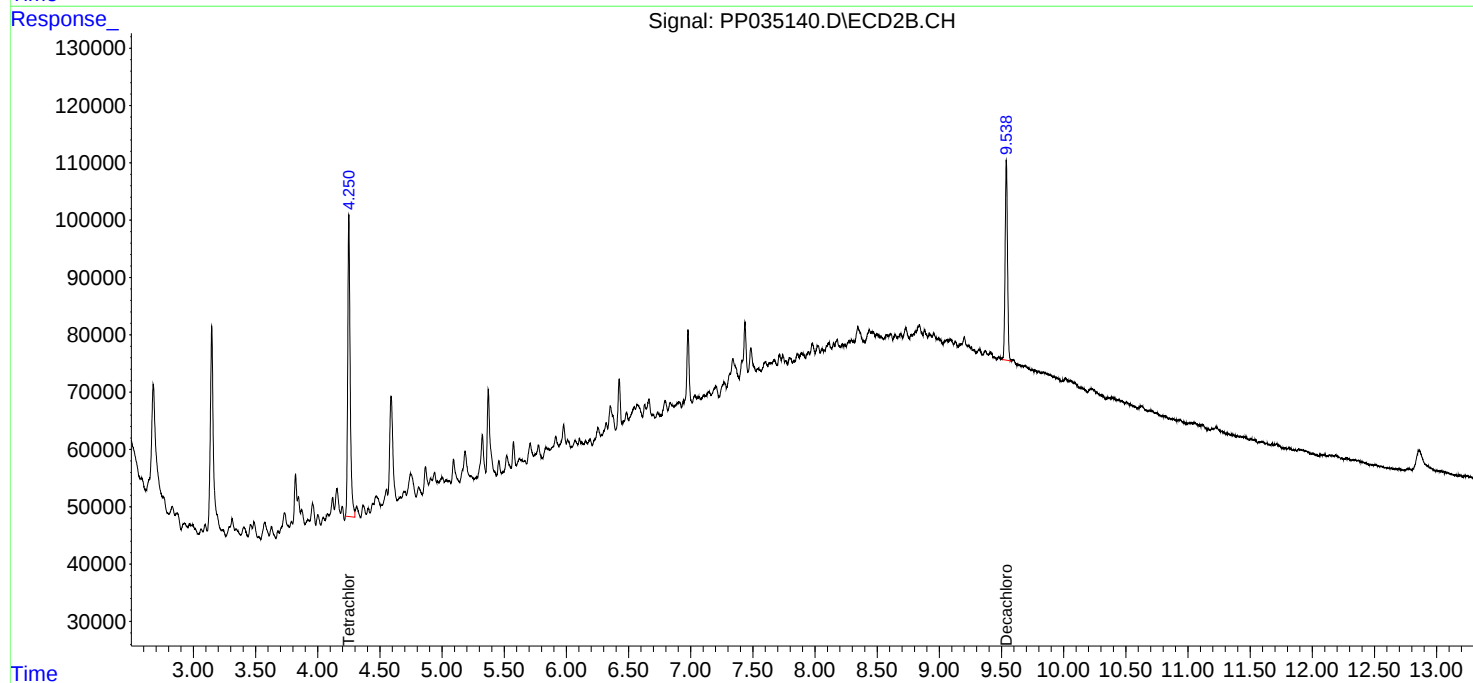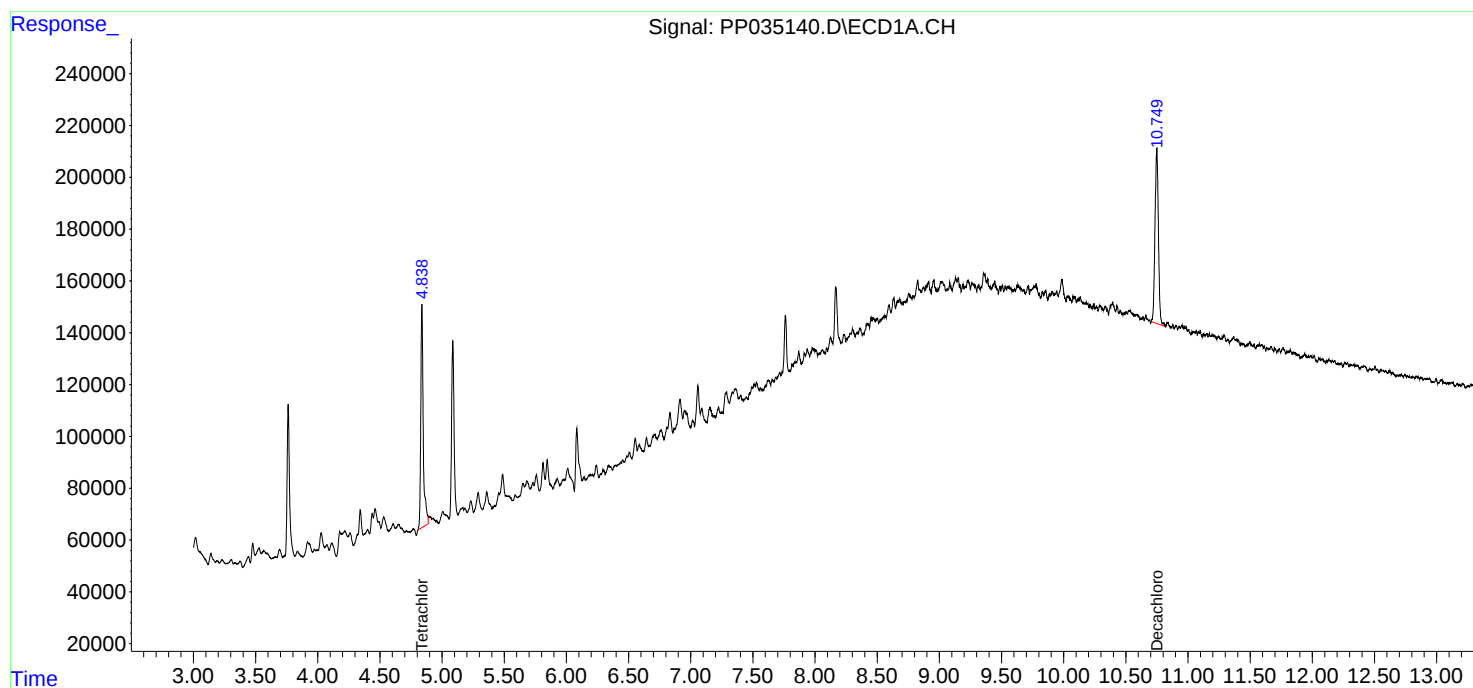

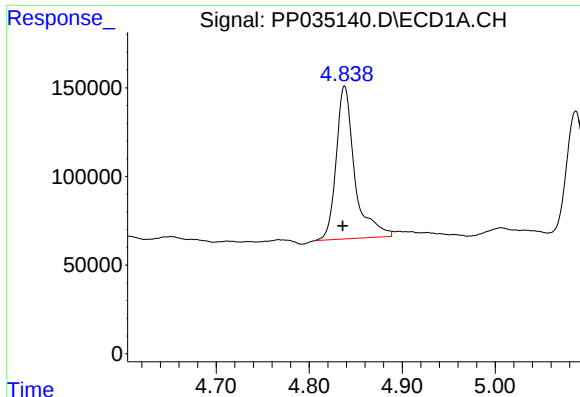


#1 Tetrachloro-m-xylene

R.T.: 4.838 min
Delta R.T.: 0.002 min
Response: 1193170
Conc: 14.64 ng/ml m

Instrument :
ECD_P
ClientSampleId :
TWP-01


Manual Integrations
APPROVED

Ankita
4/22/2021 2:46:04 PM

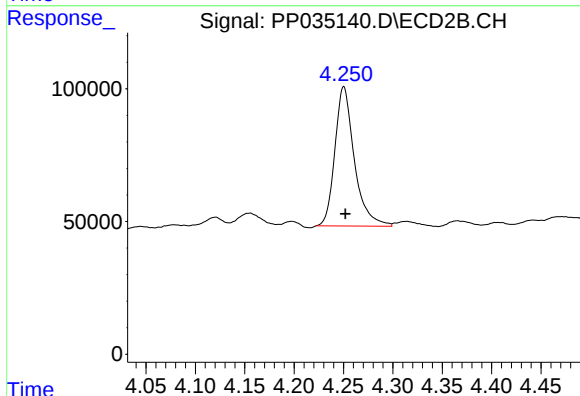


#1 Tetrachloro-m-xylene

R.T.: 4.250 min
Delta R.T.: -0.002 min
Response: 720610
Conc: 13.99 ng/ml

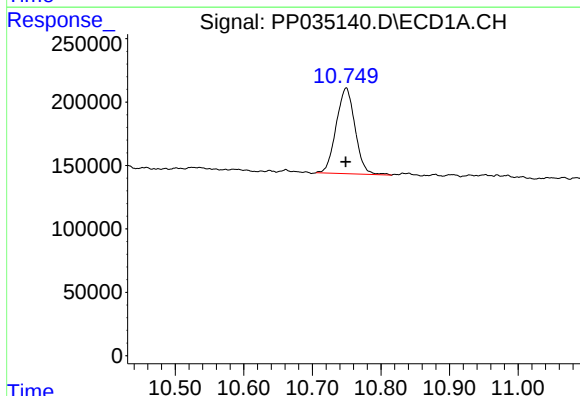

#2 Decachlorobiphenyl

R.T.: 10.749 min
Delta R.T.: 0.000 min
Response: 1290417
Conc: 20.42 ng/ml

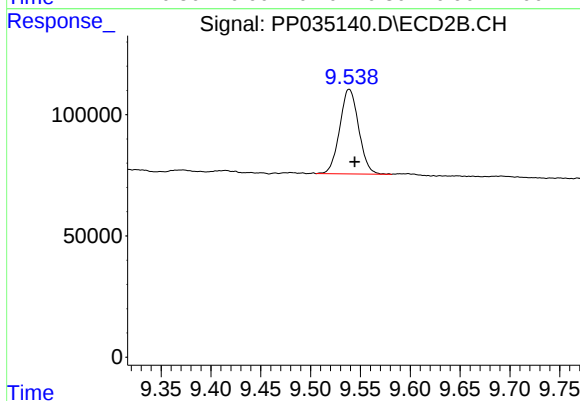

#2 Decachlorobiphenyl

R.T.: 9.539 min
Delta R.T.: -0.006 min
Response: 462324
Conc: 19.46 ng/ml