

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042123\
 Data File : PP057142.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Apr 2023 16:34
 Operator : YP\AJ
 Sample : 02427-11
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 20230352-COMP-30

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 21 22:01:49 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042023.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Apr 20 16:59:40 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.404	3.632	41417167	31467109	18.724	18.627
2) SA Decachlor...	10.219	8.687	20842775	21858817	12.988	12.219

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042123\
Data File : PP057142.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Apr 2023 16:34
Operator : YP\AJ
Sample : 02427-11
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
20230352-COMP-30

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 21 22:01:49 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042023.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Apr 20 16:59:40 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

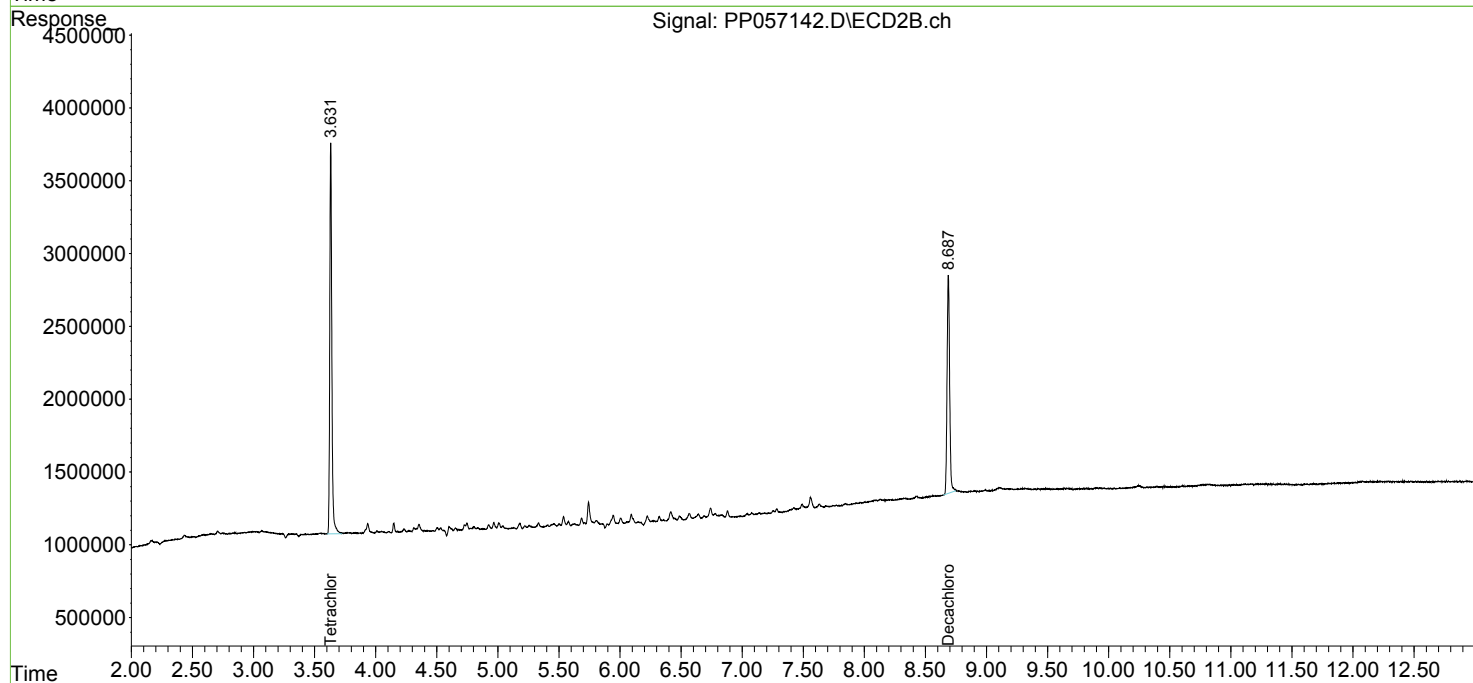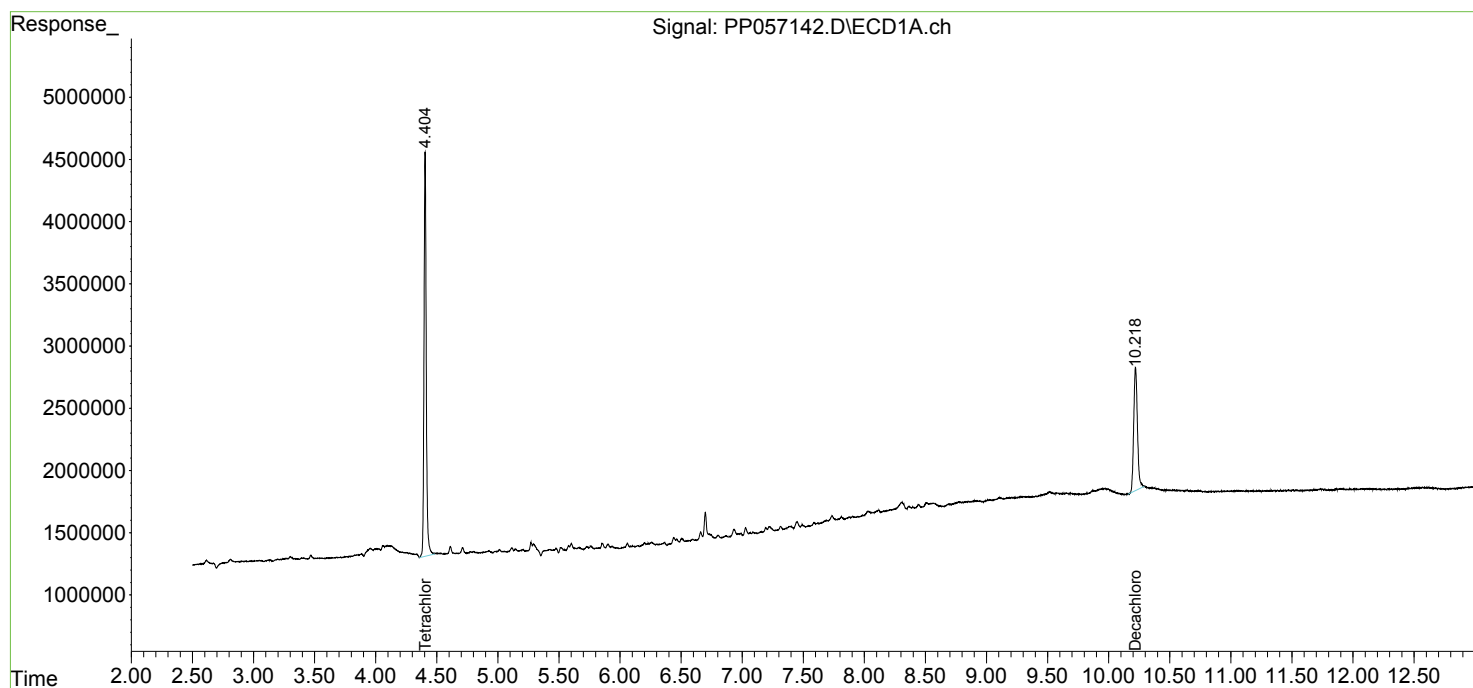


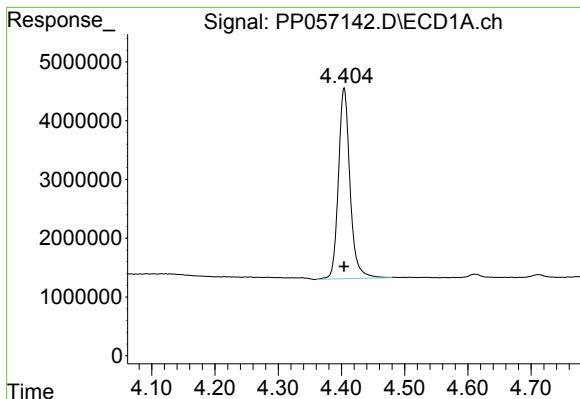

#1 Tetrachloro-m-xylene


R.T.: 4.404 min
Delta R.T.: 0.000 min
Response: 41417167
Conc: 18.72 ng/ml

Instrument :
ECD_P
ClientSampleId :
20230352-COMP-30

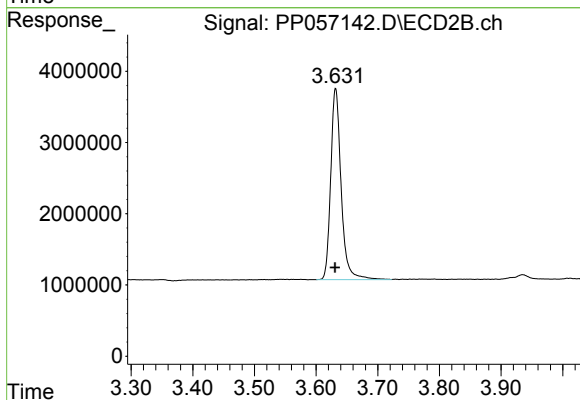


#1 Tetrachloro-m-xylene

R.T.: 3.632 min
Delta R.T.: 0.000 min
Response: 31467109
Conc: 18.63 ng/ml

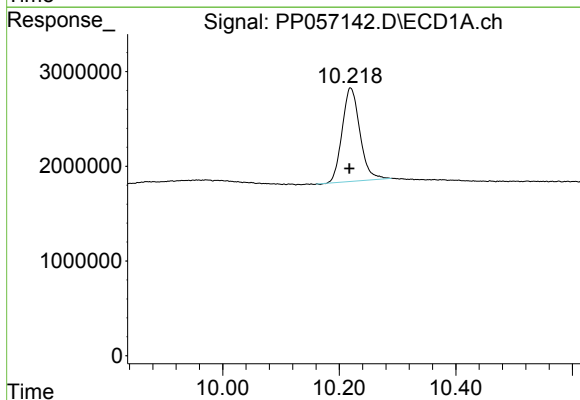

#2 Decachlorobiphenyl

R.T.: 10.219 min
Delta R.T.: 0.002 min
Response: 20842775
Conc: 12.99 ng/ml

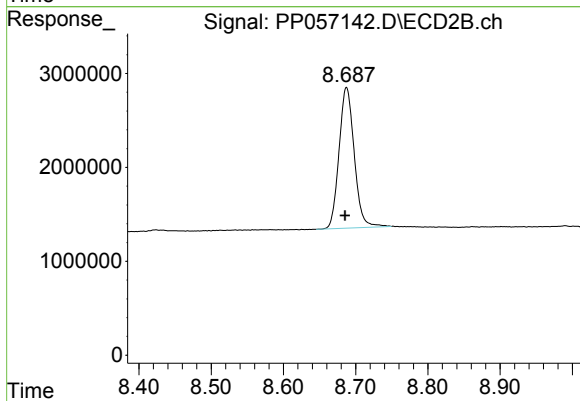

#2 Decachlorobiphenyl

R.T.: 8.687 min
Delta R.T.: 0.002 min
Response: 21858817
Conc: 12.22 ng/ml