

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042221\
 Data File : PP035171.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Apr 2021 21:26
 Operator : DD\AJ
 Sample : M2106-18
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 03:00:38 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 21 17:37:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.837	4.249	1713065	1101702	21.023	21.394
2)	SA Decachlor...	10.744	9.537	1433330	565836	22.682	23.815
Target Compounds							
8)	L2 AR-1221-1	5.091	0.000	62263	0	75.703	N.D. #
27)	L6 AR-1254-2	7.296	0.000	16537	0	4.370	N.D. #
30)	L6 AR-1254-5	8.384	0.000	16041	0	5.514	N.D. #
32)	L7 AR-1260-2	8.097	0.000	9756	0	2.866	N.D. #
34)	L7 AR-1260-4	8.696	0.000	5502	0	1.874	N.D. #
35)	L7 AR-1260-5	9.006	0.000	1710	0	0.348	N.D. #
37)	L8 AR-1262-2	9.006	0.000	1710	0	0.294	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042221\
Data File : PP035171.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Apr 2021 21:26
Operator : DD\AJ
Sample : M2106-18
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 03:00:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 21 17:37:28 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

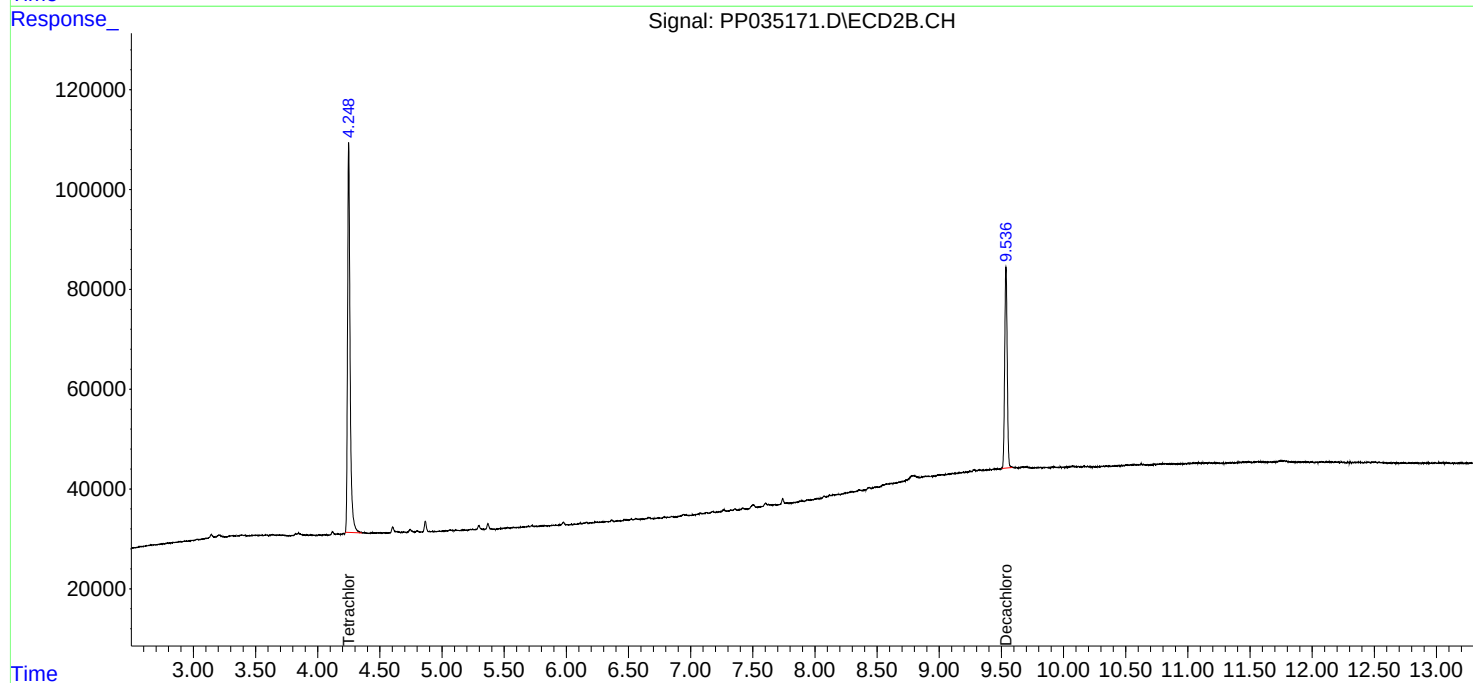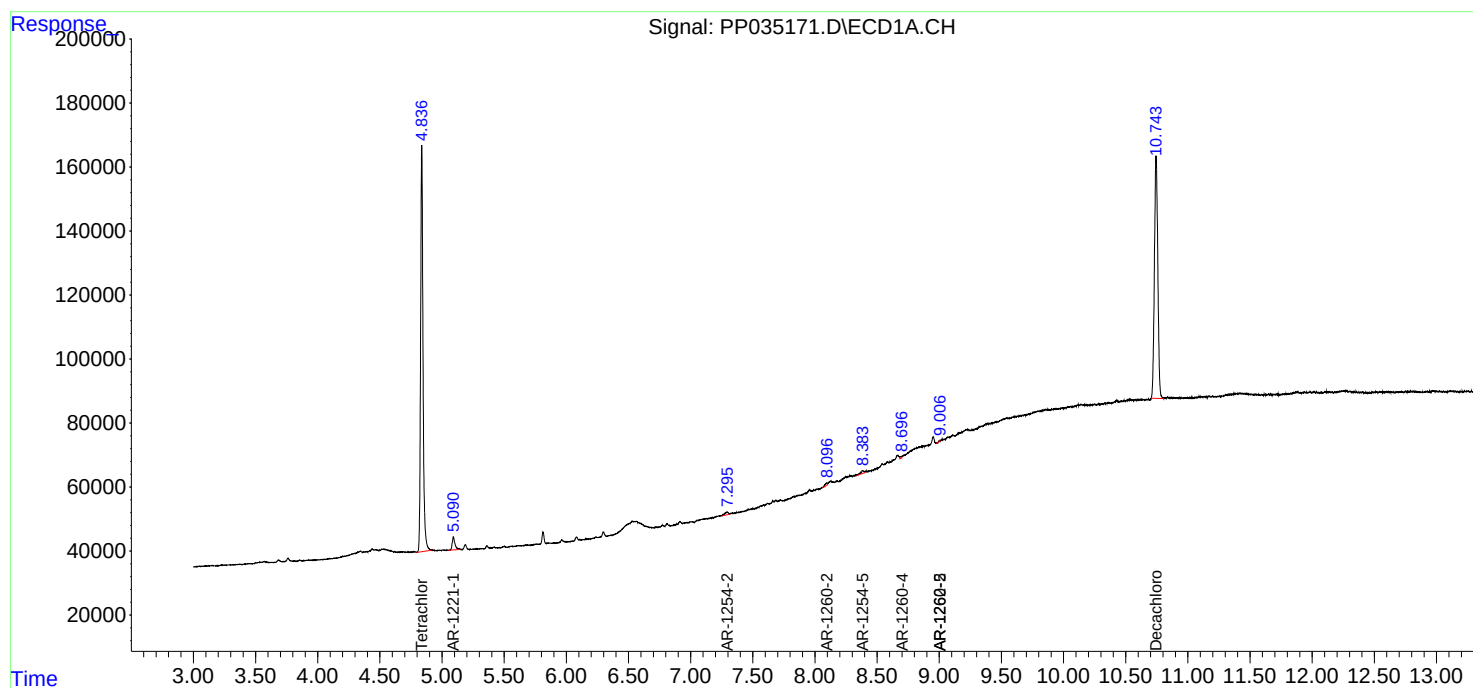


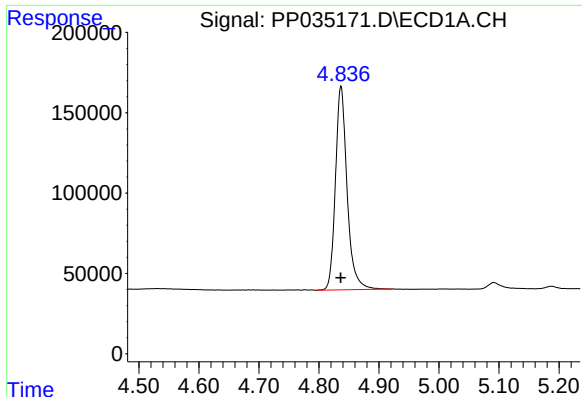

#1 Tetrachloro-m-xylene


R.T.: 4.837 min
Delta R.T.: 0.000 min
Response: 1713065
Conc: 21.02 ng/ml

Instrument :
ECD_P
ClientSampleId :

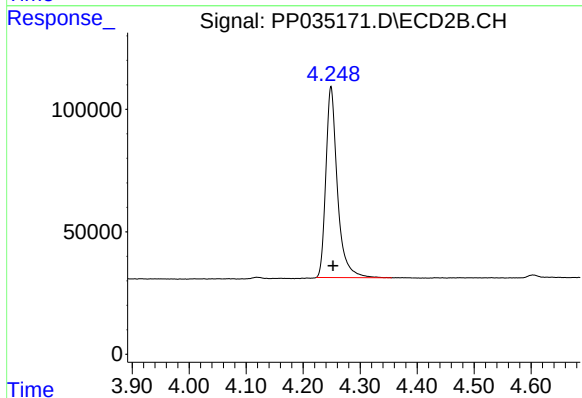


#1 Tetrachloro-m-xylene

R.T.: 4.249 min
Delta R.T.: -0.003 min
Response: 1101702
Conc: 21.39 ng/ml

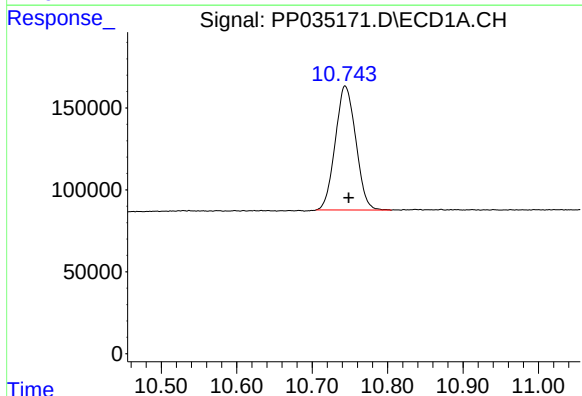


#2 Decachlorobiphenyl

R.T.: 10.744 min
Delta R.T.: -0.005 min
Response: 1433330
Conc: 22.68 ng/ml

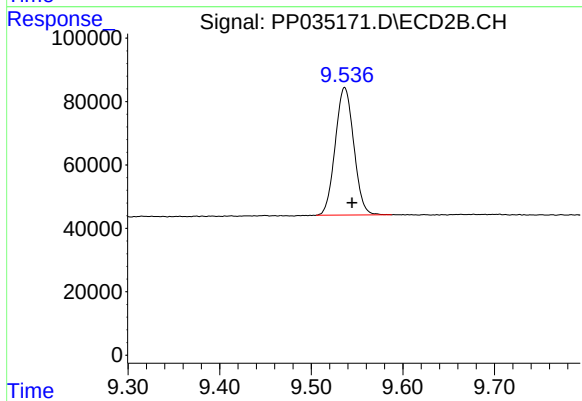

#2 Decachlorobiphenyl


R.T.: 9.537 min
Delta R.T.: -0.008 min
Response: 565836
Conc: 23.81 ng/ml

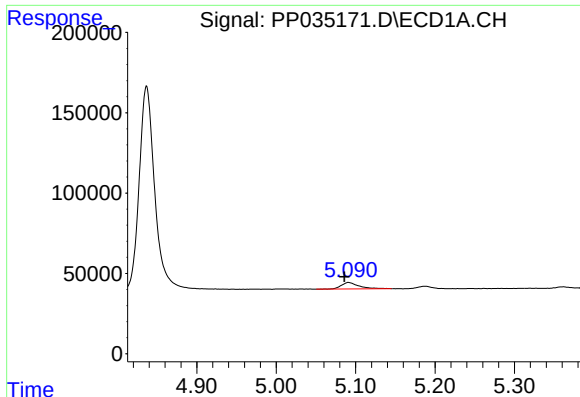

#8 AR-1221-1


R.T.: 5.091 min
Delta R.T.: 0.005 min
Response: 62263
Conc: 75.70 ng/ml

Instrument :
ECD_P
ClientSampleId :

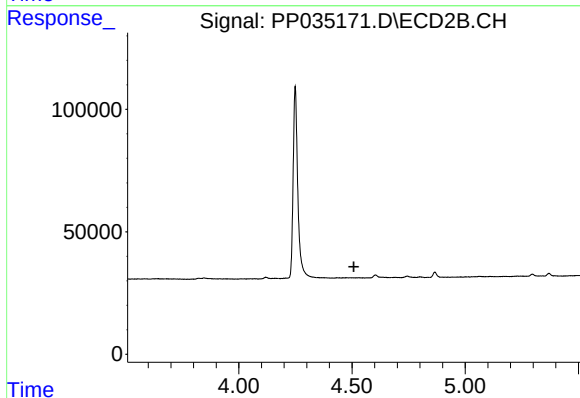


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.508 min
Response: 0
Conc: N.D.

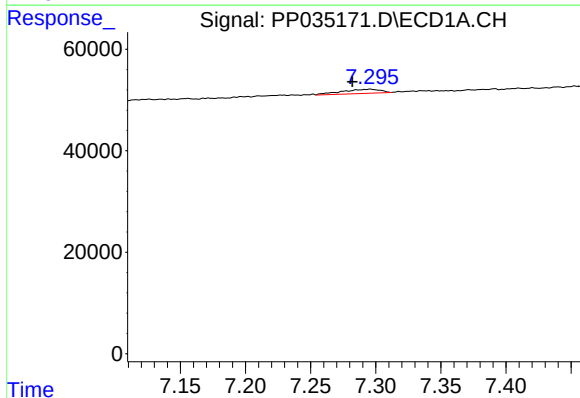


#27 AR-1254-2

R.T.: 7.296 min
Delta R.T.: 0.014 min
Response: 16537
Conc: 4.37 ng/ml

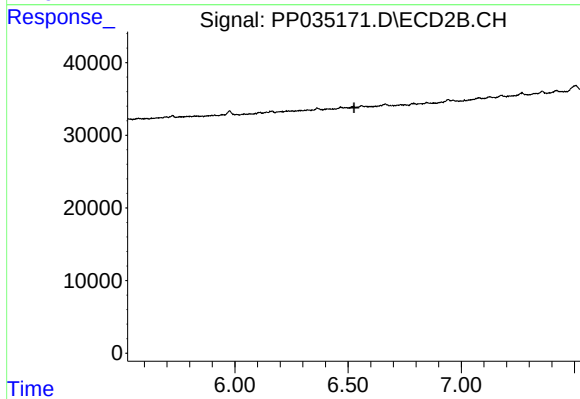

#27 AR-1254-2


R.T.: 0.000 min
Exp R.T. : 6.526 min
Response: 0
Conc: N.D.

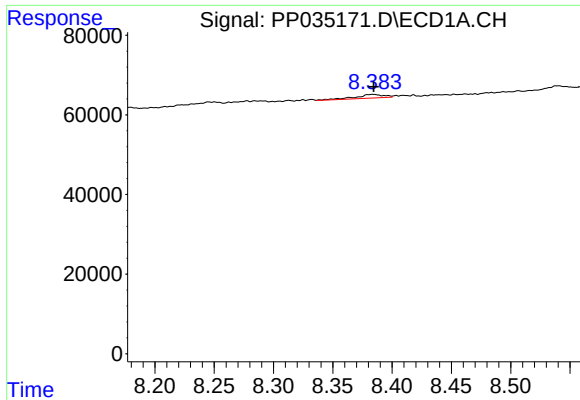

#30 AR-1254-5


R.T.: 8.384 min
Delta R.T.: 0.000 min
Response: 16041
Conc: 5.51 ng/ml

Instrument :
ECD_P
ClientSampleId :

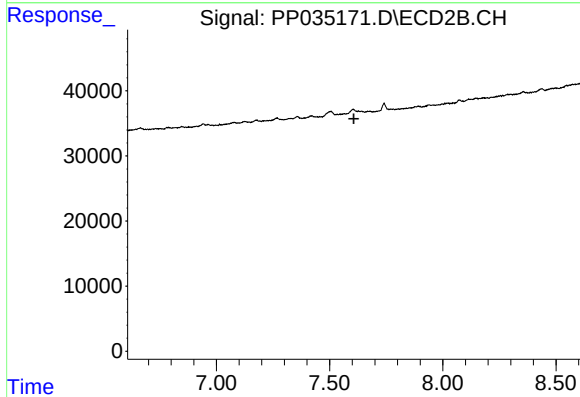


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.608 min
Response: 0
Conc: N.D.

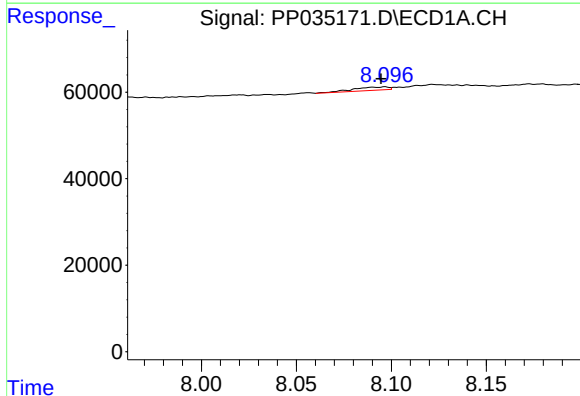


#32 AR-1260-2

R.T.: 8.097 min
Delta R.T.: 0.002 min
Response: 9756
Conc: 2.87 ng/ml

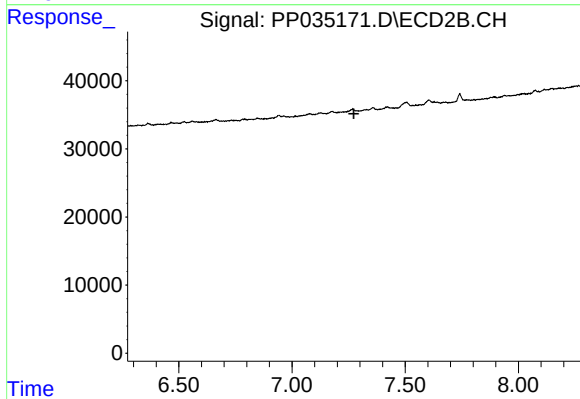

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 7.273 min
Response: 0
Conc: N.D.

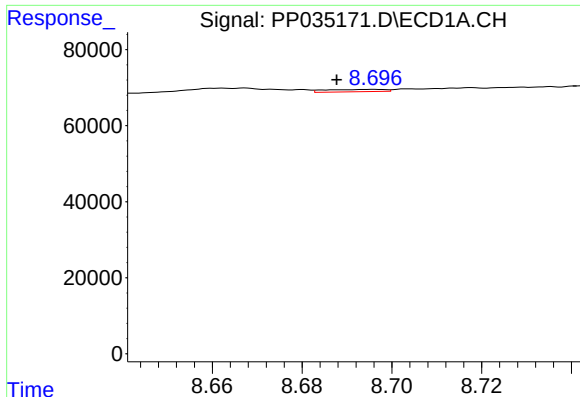

#34 AR-1260-4


R.T.: 8.696 min
Delta R.T.: 0.008 min
Response: 5502
Conc: 1.87 ng/ml

Instrument :
ECD_P
ClientSampleId :

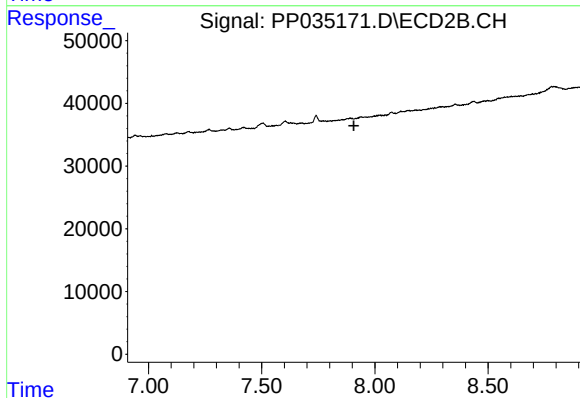


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.907 min
Response: 0
Conc: N.D.

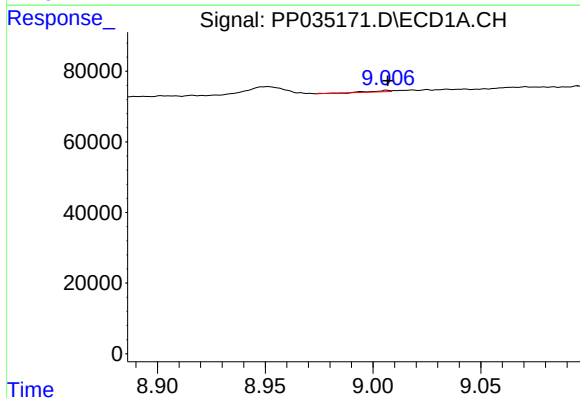


#35 AR-1260-5

R.T.: 9.006 min
Delta R.T.: 0.000 min
Response: 1710
Conc: 0.35 ng/ml

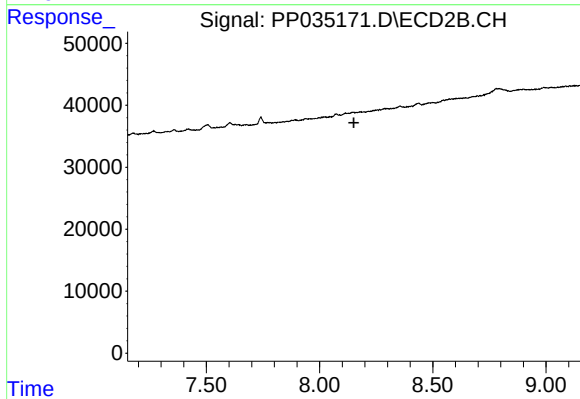

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 8.151 min
Response: 0
Conc: N.D.

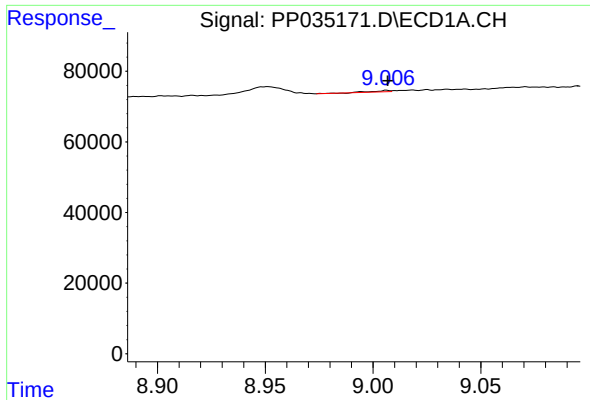

#37 AR-1262-2

R.T.: 9.006 min
Delta R.T.: 0.000 min
Response: 1710
Conc: 0.29 ng/ml

Instrument :
ECD_P
ClientSampleId :

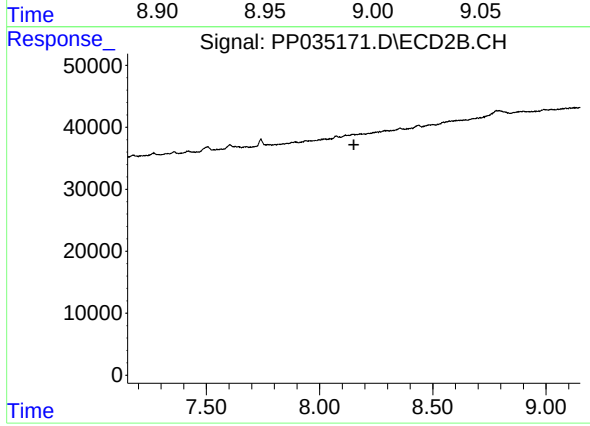

#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 8.151 min
Response: 0
Conc: N.D.