

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042221\
 Data File : PP035173.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Apr 2021 22:00
 Operator : DD\AJ
 Sample : M2106-21
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 03:01:19 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 21 17:37:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.837	4.249	1682792	1080969	20.651	20.991
2)	SA Decachlor...	10.745	9.537	1232744	492387	19.508	20.723
Target Compounds							
9)	L2 AR-1221-2	5.188	0.000	21482	0	34.083	N.D. #
27)	L6 AR-1254-2	7.300f	0.000	22007	0	5.816	N.D. #
28)	L6 AR-1254-3	7.688f	0.000	32428	0	8.692	N.D. #
30)	L6 AR-1254-5	8.386	0.000	14841	0	5.102	N.D. #
39)	L8 AR-1262-4	9.408	0.000	20693	0	5.747	N.D. #
42)	L9 AR-1268-2	9.408	0.000	20693	0	2.590	N.D. #
43)	L9 AR-1268-3	9.612	0.000	18884	0	2.476	N.D. #
45)	L9 AR-1268-5	10.429	0.000	49899	0	2.250	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042221\
Data File : PP035173.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Apr 2021 22:00
Operator : DD\AJ
Sample : M2106-21
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 03:01:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 21 17:37:28 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

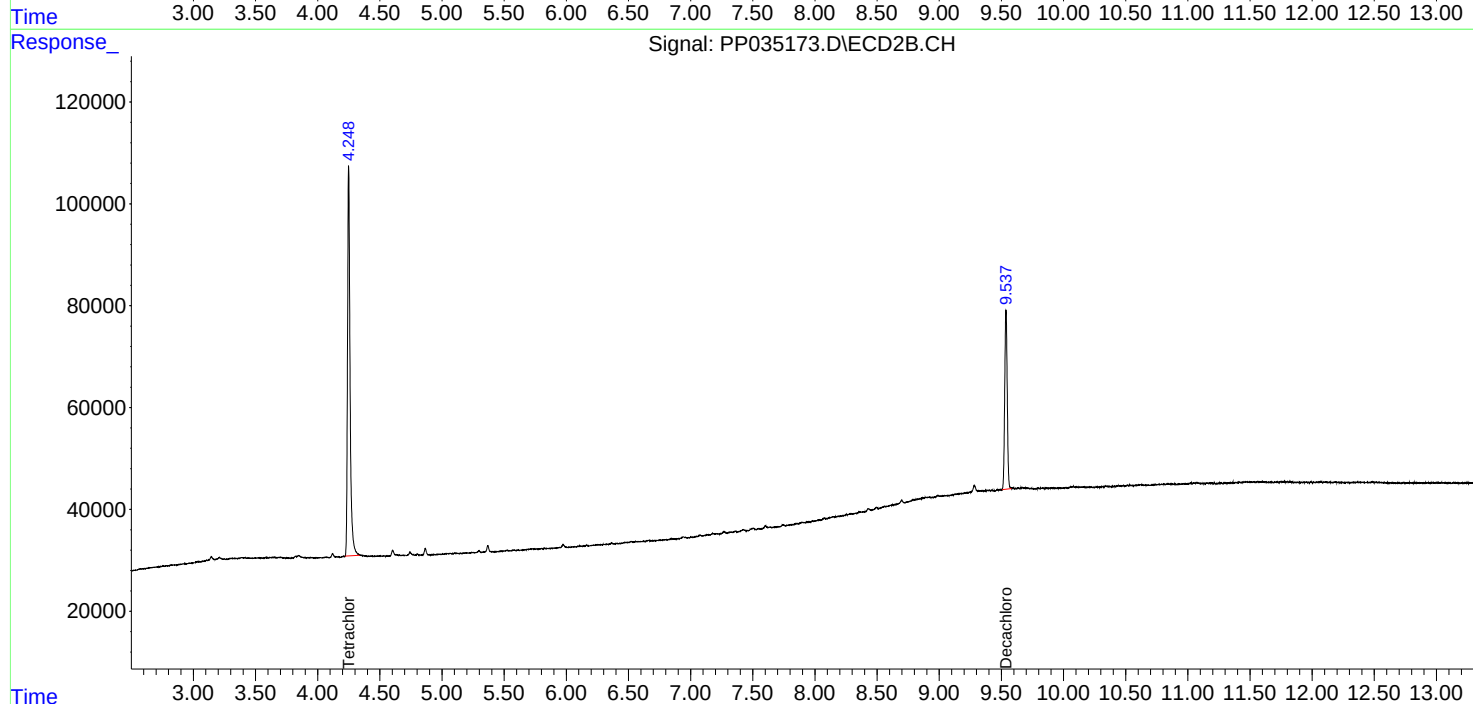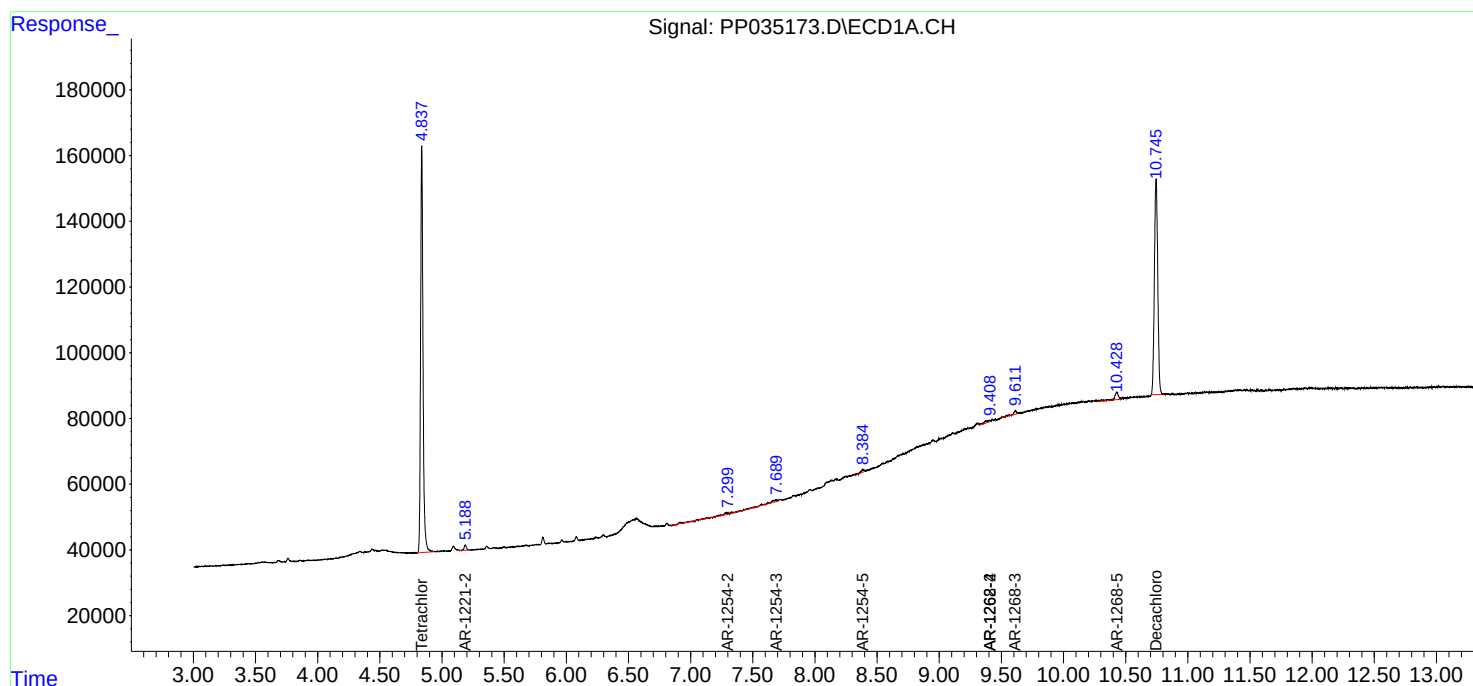


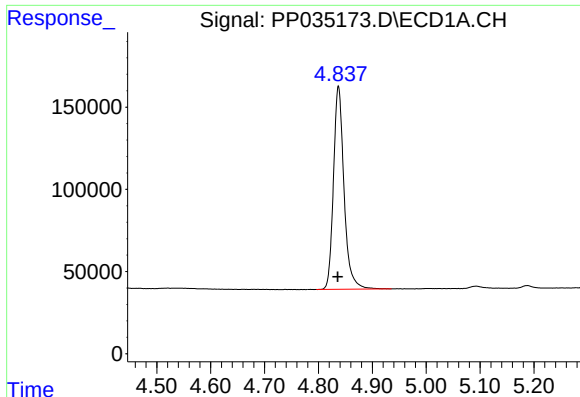

#1 Tetrachloro-m-xylene


R.T.: 4.837 min
Delta R.T.: 0.001 min
Response: 1682792
Conc: 20.65 ng/ml

Instrument :
ECD_P
ClientSampleId :

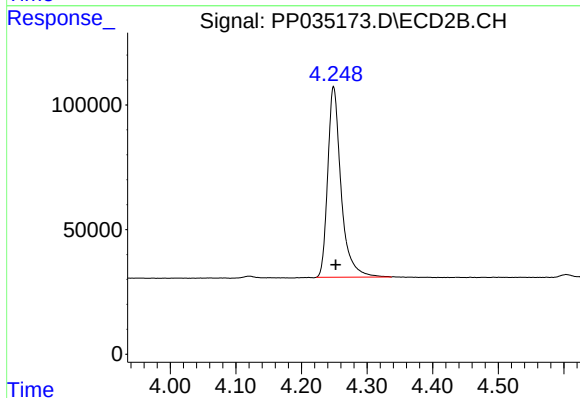


#1 Tetrachloro-m-xylene

R.T.: 4.249 min
Delta R.T.: -0.003 min
Response: 1080969
Conc: 20.99 ng/ml

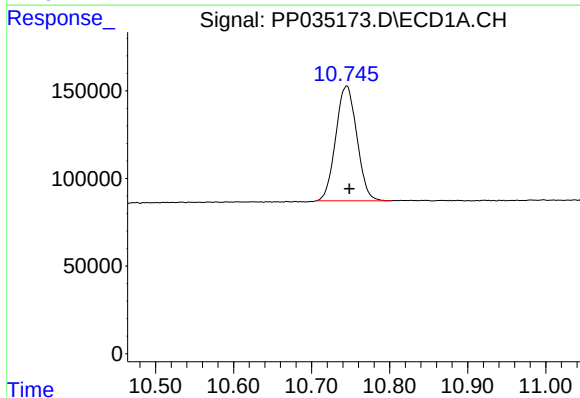


#2 Decachlorobiphenyl

R.T.: 10.745 min
Delta R.T.: -0.004 min
Response: 1232744
Conc: 19.51 ng/ml

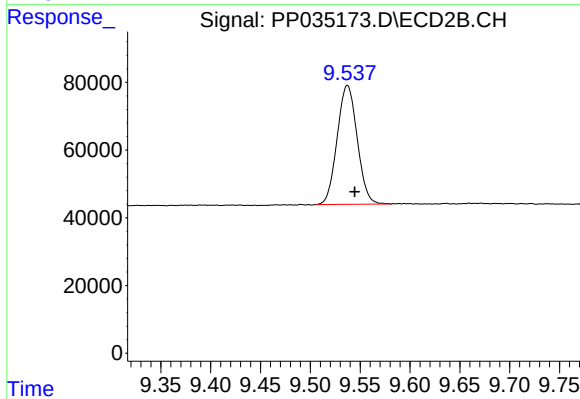

#2 Decachlorobiphenyl


R.T.: 9.537 min
Delta R.T.: -0.007 min
Response: 492387
Conc: 20.72 ng/ml

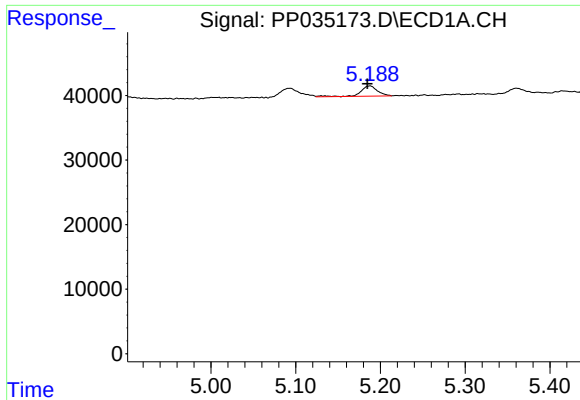

#9 AR-1221-2


R.T.: 5.188 min
Delta R.T.: 0.003 min
Response: 21482
Conc: 34.08 ng/ml

Instrument :
ECD_P
ClientSampleId :

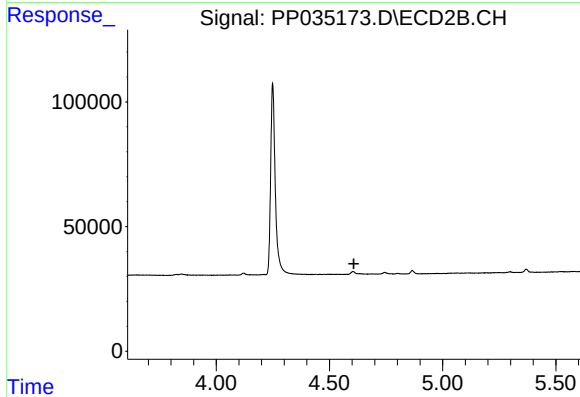


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.608 min
Response: 0
Conc: N.D.

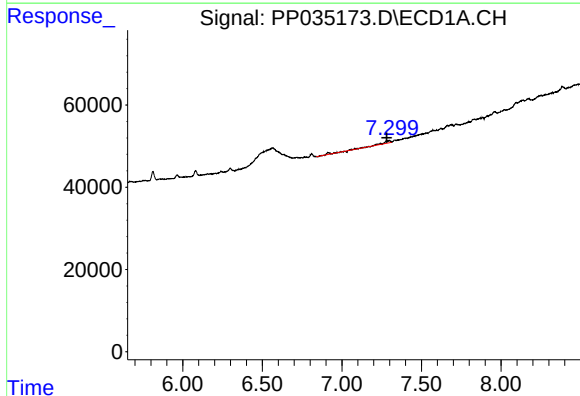


#27 AR-1254-2

R.T.: 7.300 min
Delta R.T.: 0.018 min
Response: 22007
Conc: 5.82 ng/ml

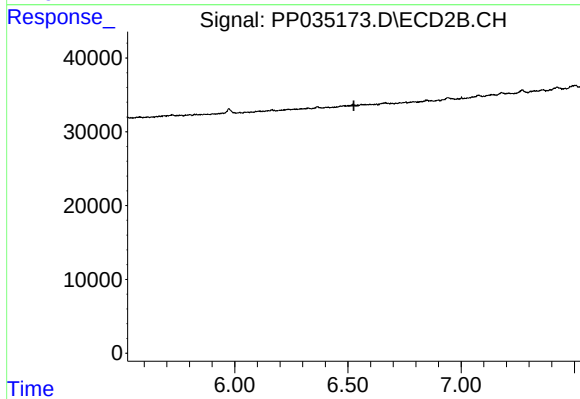

#27 AR-1254-2


R.T.: 0.000 min
Exp R.T. : 6.526 min
Response: 0
Conc: N.D.

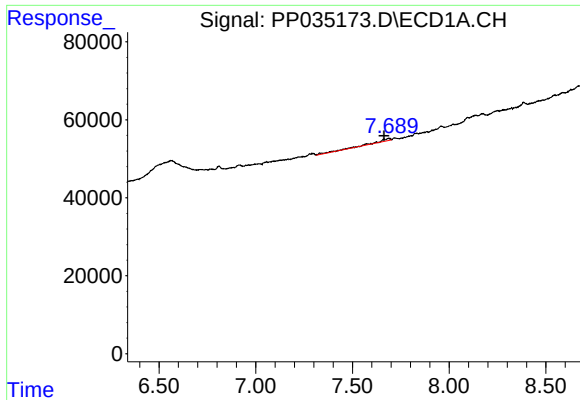

#28 AR-1254-3


R.T.: 7.688 min
Delta R.T.: 0.026 min
Response: 32428
Conc: 8.69 ng/ml

Instrument :
ECD_P
ClientSampleId :

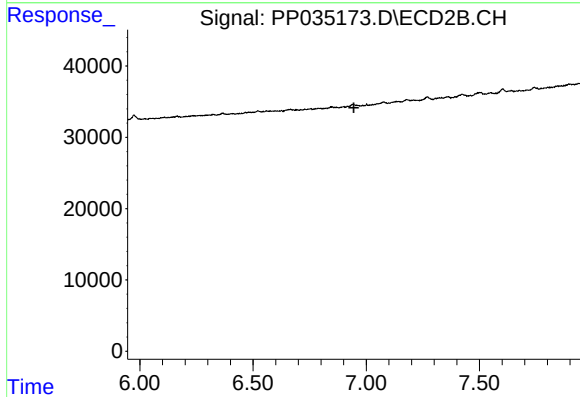


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.946 min
Response: 0
Conc: N.D.

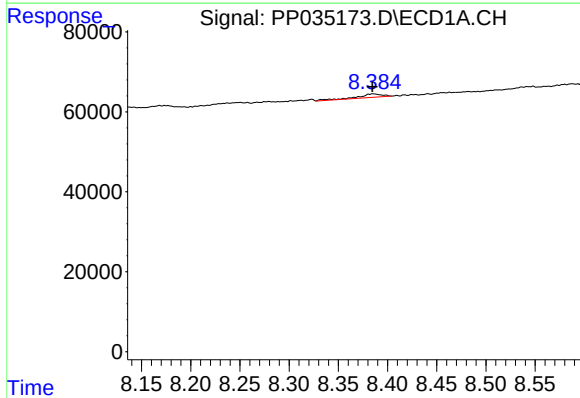


#30 AR-1254-5

R.T.: 8.386 min
Delta R.T.: 0.000 min
Response: 14841
Conc: 5.10 ng/ml

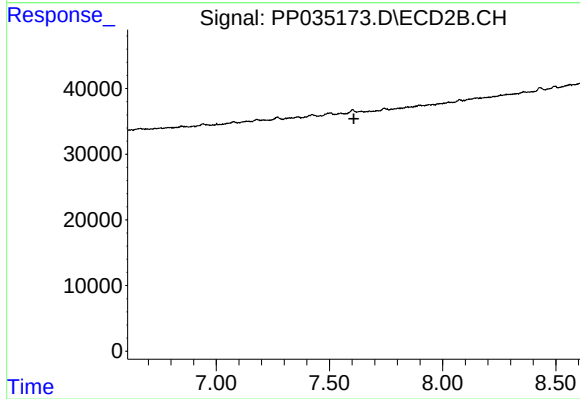

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 7.608 min
Response: 0
Conc: N.D.

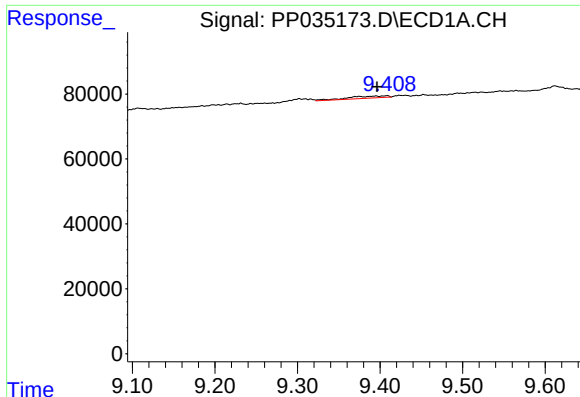

#39 AR-1262-4


R.T.: 9.408 min
Delta R.T.: 0.012 min
Response: 20693
Conc: 5.75 ng/ml

Instrument :
ECD_P
ClientSampleId :

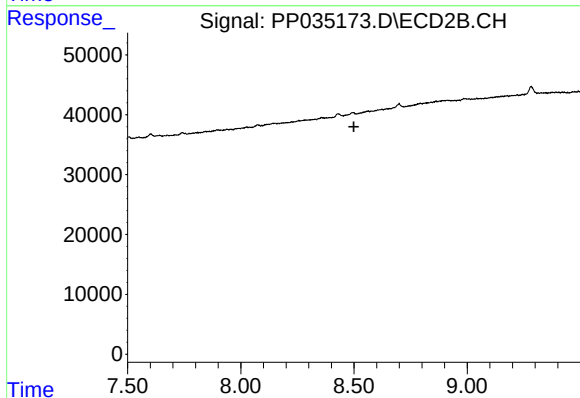


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 8.499 min
Response: 0
Conc: N.D.

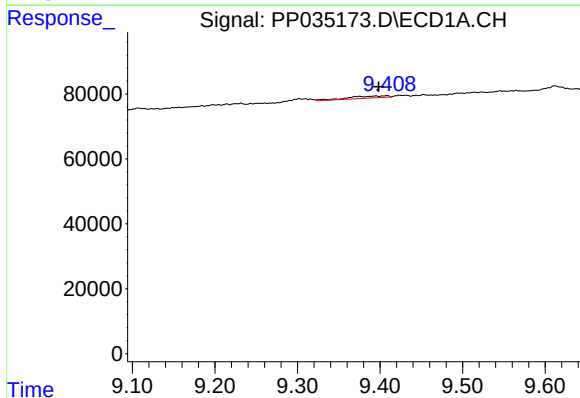


#42 AR-1268-2

R.T.: 9.408 min
Delta R.T.: 0.010 min
Response: 20693
Conc: 2.59 ng/ml

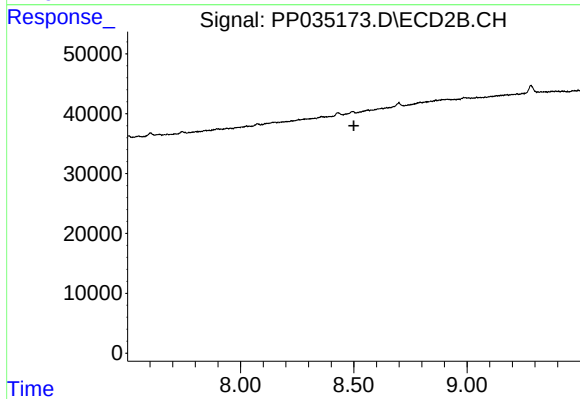

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T. : 8.500 min
Response: 0
Conc: N.D.

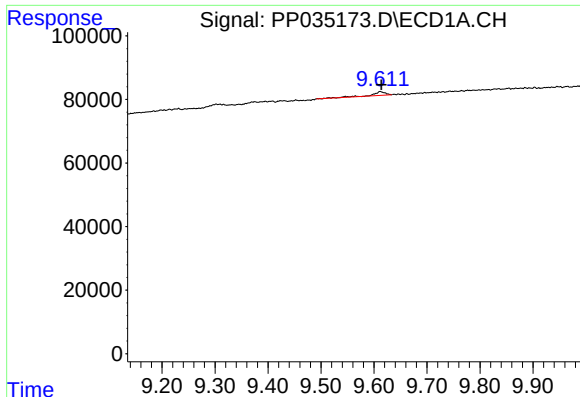

#43 AR-1268-3


R.T.: 9.612 min
Delta R.T.: -0.002 min
Response: 18884
Conc: 2.48 ng/ml

Instrument :
ECD_P
ClientSampleId :

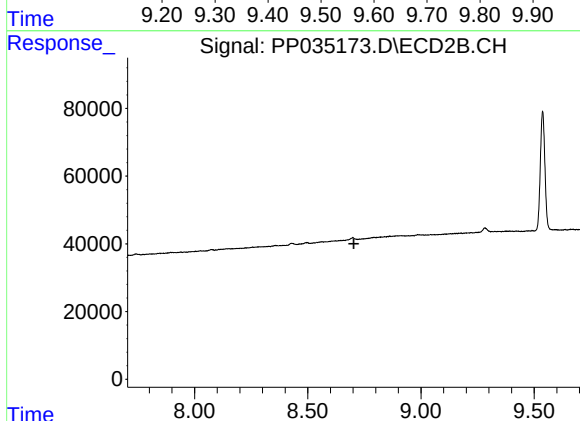


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 8.704 min
Response: 0
Conc: N.D.

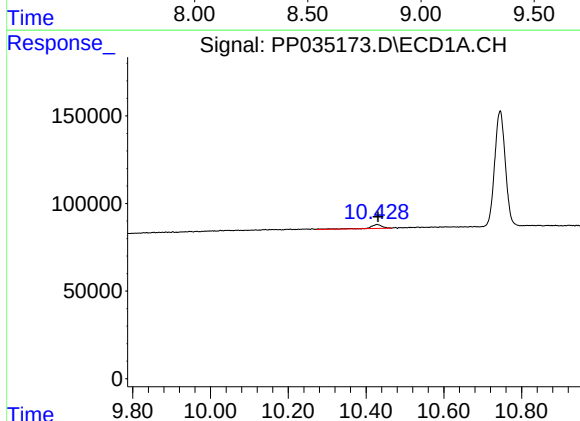

#45 AR-1268-5

R.T.: 10.429 min
Delta R.T.: -0.002 min
Response: 49899
Conc: 2.25 ng/ml

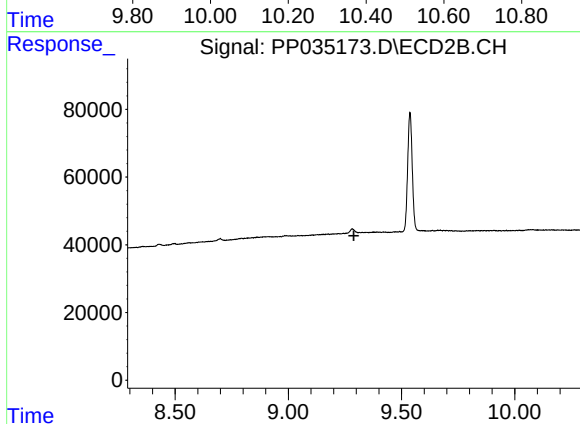

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 9.290 min
Response: 0
Conc: N.D.