

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042221\
 Data File : PP035177.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Apr 2021 23:41
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 03:02:58 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 21 17:37:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.836	4.249	1758148	1149371	21.576	22.319
2)	SA Decachlor...	10.743	9.537	1744991	693181	27.614	29.174
Target Compounds							
9)	L2 AR-1221-2	5.186	0.000	20217	0	32.076	N.D. #
20)	L4 AR-1242-5	7.132	0.000	91883	0	84.597	N.D. #
24)	L5 AR-1248-4	7.079	0.000	92255	0	48.742	N.D. #
25)	L5 AR-1248-5	7.132	0.000	91883	0	47.645	N.D. #
26)	L6 AR-1254-1	7.079f	0.000	92255	0	35.786	N.D. #
28)	L6 AR-1254-3	7.683f	0.000	431712	0	115.713	N.D. #
29)	L6 AR-1254-4	7.955	0.000	107889	0	51.513	N.D. #
45)	L9 AR-1268-5	10.429	0.000	22722	0	1.025	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042221\
Data File : PP035177.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Apr 2021 23:41
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 03:02:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 21 17:37:28 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

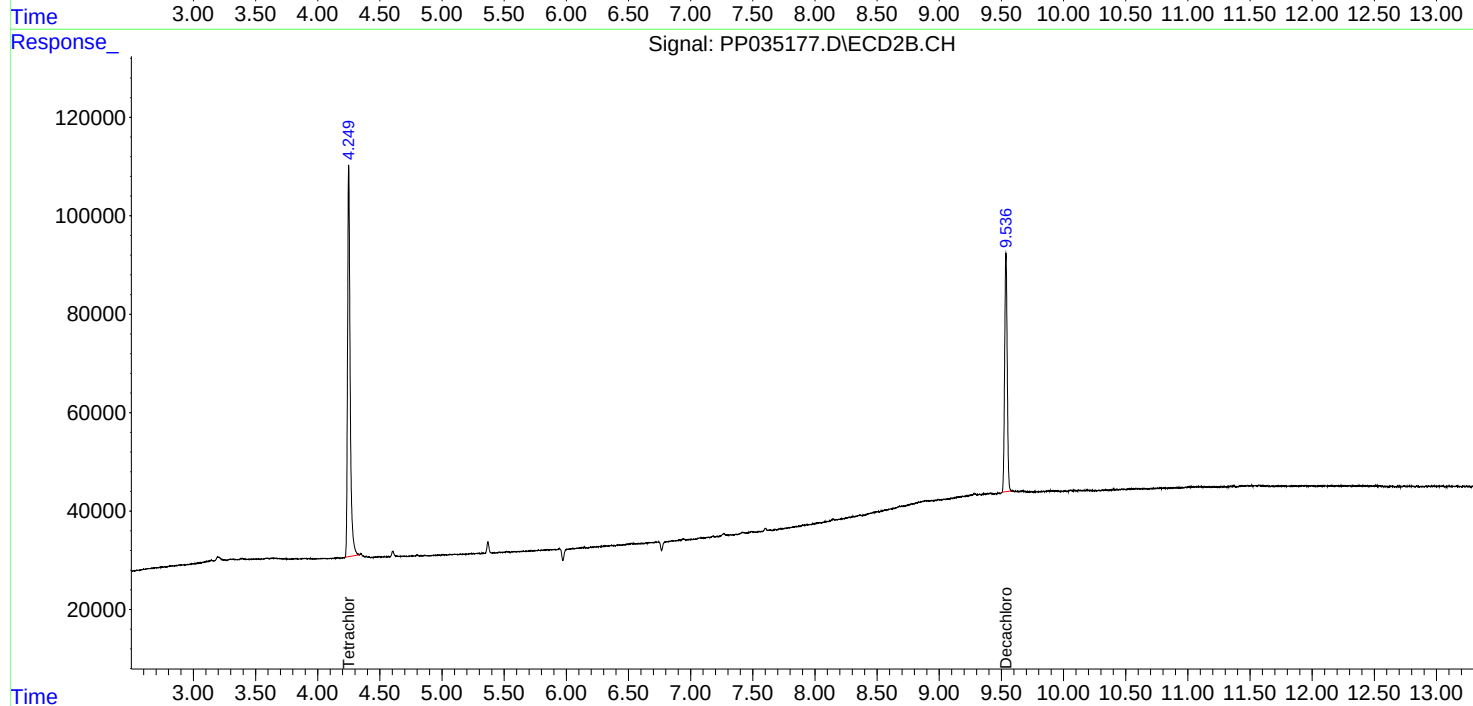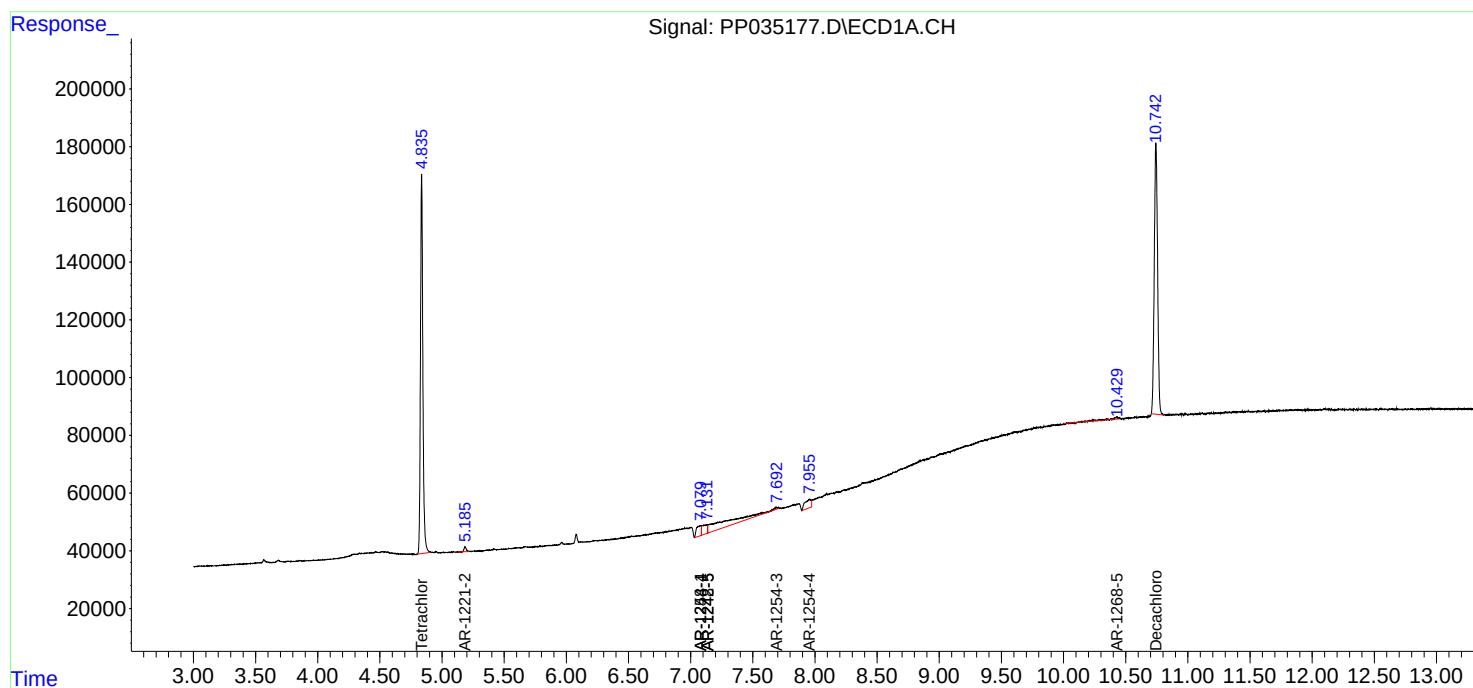


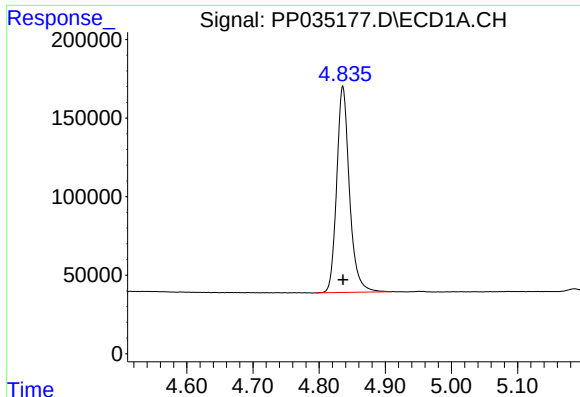

#1 Tetrachloro-m-xylene


R.T.: 4.836 min
Delta R.T.: 0.000 min
Response: 1758148
Conc: 21.58 ng/ml

Instrument :
ECD_P
ClientSampleId :

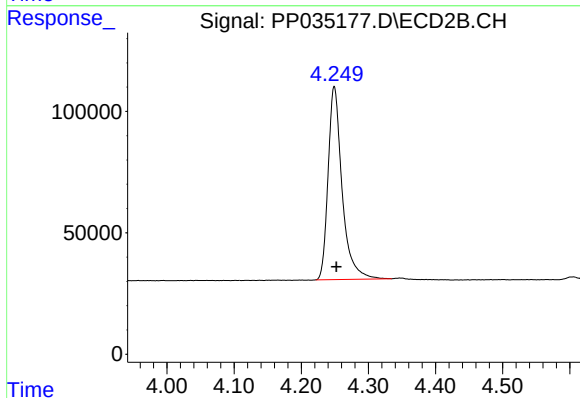


#1 Tetrachloro-m-xylene

R.T.: 4.249 min
Delta R.T.: -0.003 min
Response: 1149371
Conc: 22.32 ng/ml

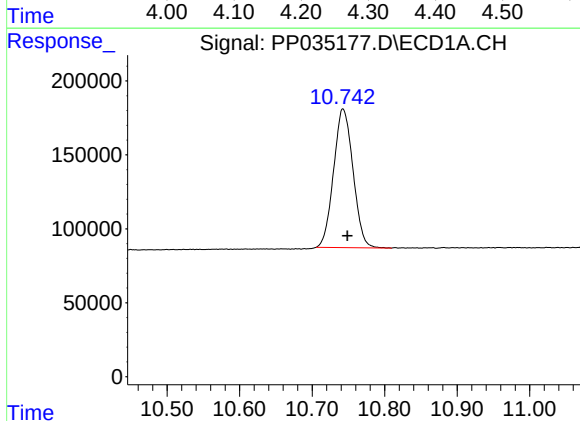


#2 Decachlorobiphenyl

R.T.: 10.743 min
Delta R.T.: -0.006 min
Response: 1744991
Conc: 27.61 ng/ml

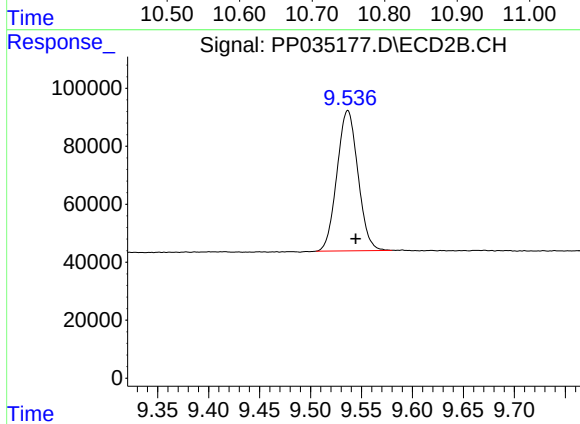

#2 Decachlorobiphenyl


R.T.: 9.537 min
Delta R.T.: -0.008 min
Response: 693181
Conc: 29.17 ng/ml

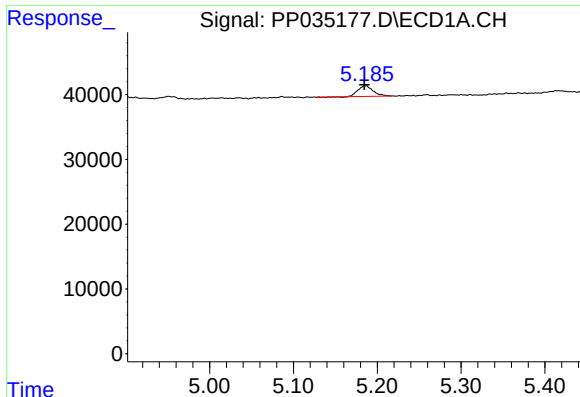

#9 AR-1221-2


R.T.: 5.186 min
Delta R.T.: 0.001 min
Response: 20217
Conc: 32.08 ng/ml

Instrument :
ECD_P
ClientSampleId :

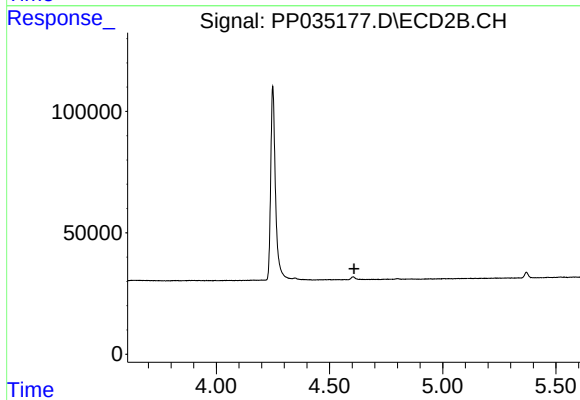


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.608 min
Response: 0
Conc: N.D.

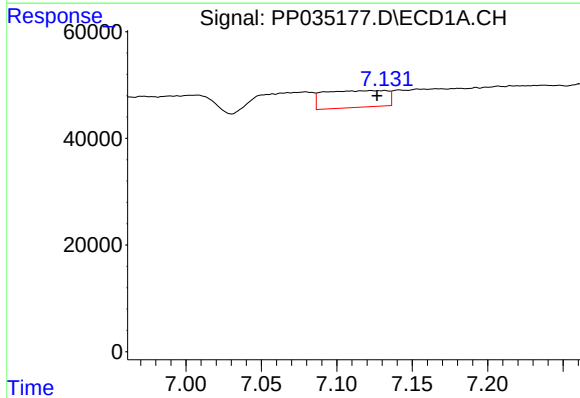


#20 AR-1242-5

R.T.: 7.132 min
Delta R.T.: 0.005 min
Response: 91883
Conc: 84.60 ng/ml

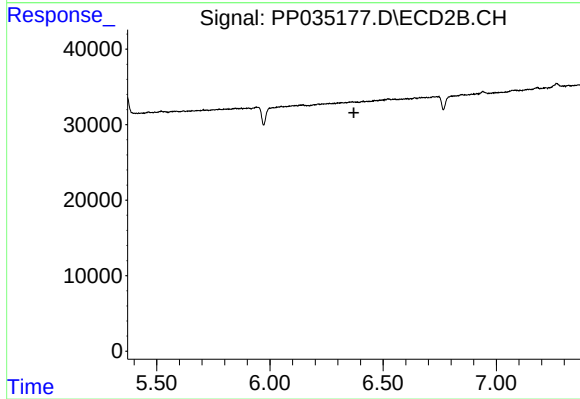

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T. : 6.371 min
Response: 0
Conc: N.D.

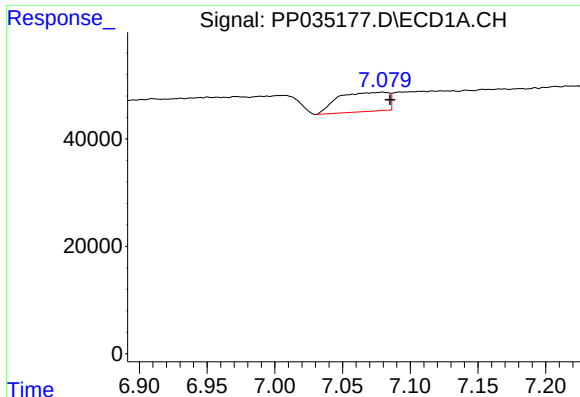

#24 AR-1248-4


R.T.: 7.079 min
Delta R.T.: -0.006 min
Response: 92255
Conc: 48.74 ng/ml

Instrument :
ECD_P
ClientSampleId :

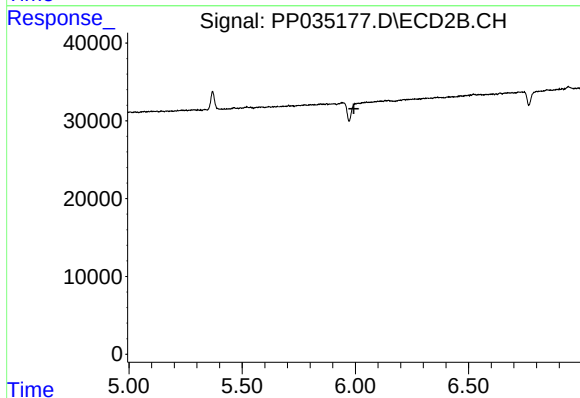


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.993 min
Response: 0
Conc: N.D.

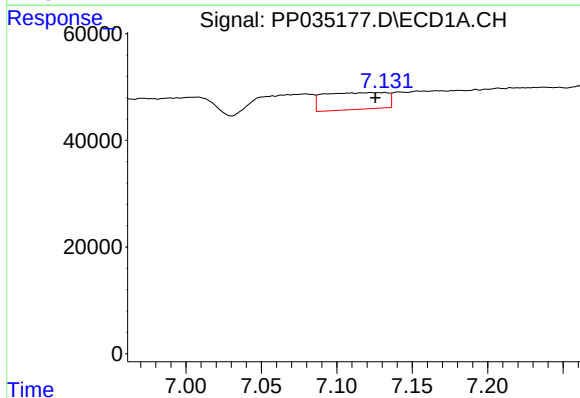


#25 AR-1248-5

R.T.: 7.132 min
Delta R.T.: 0.006 min
Response: 91883
Conc: 47.65 ng/ml

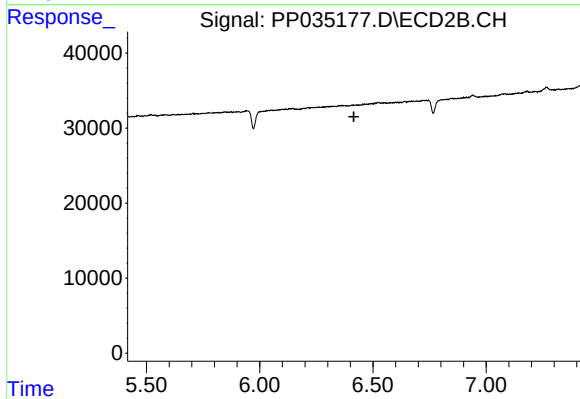

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T. : 6.416 min
Response: 0
Conc: N.D.

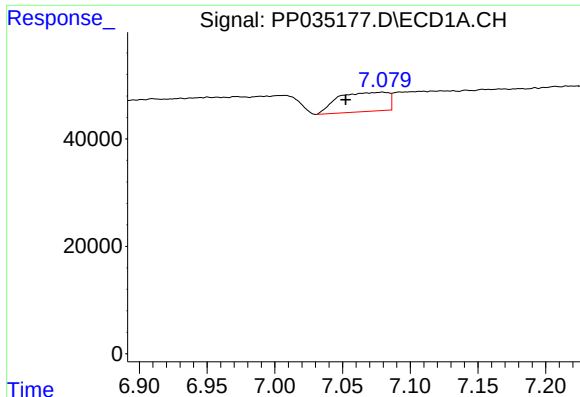

#26 AR-1254-1


R.T.: 7.079 min
Delta R.T.: 0.027 min
Response: 92255
Conc: 35.79 ng/ml

Instrument :
ECD_P
ClientSampleId :

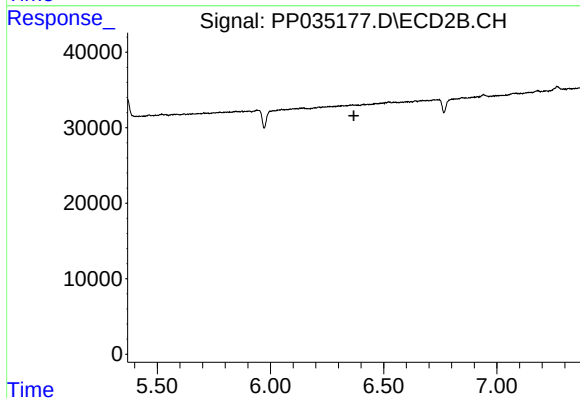


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 6.369 min
Response: 0
Conc: N.D.

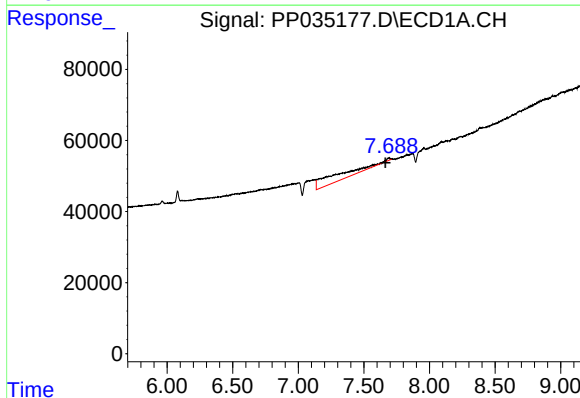


#28 AR-1254-3

R.T.: 7.683 min
Delta R.T.: 0.020 min
Response: 431712
Conc: 115.71 ng/ml

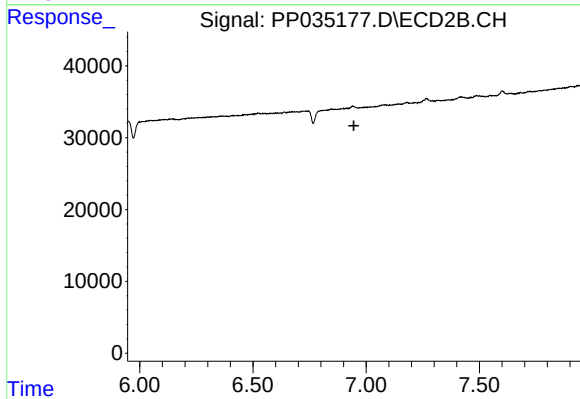

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.946 min
Response: 0
Conc: N.D.

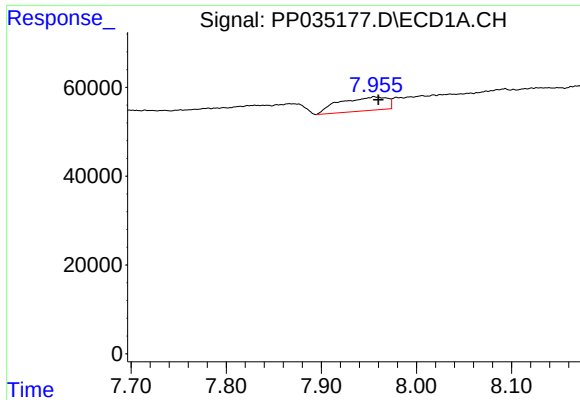

#29 AR-1254-4


R.T.: 7.955 min
Delta R.T.: -0.004 min
Response: 107889
Conc: 51.51 ng/ml

Instrument :
ECD_P
ClientSampleId :

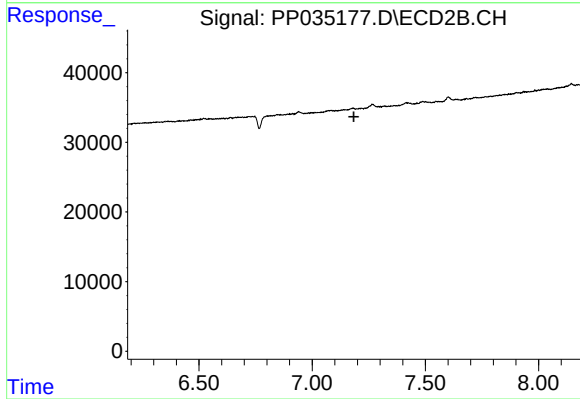


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 7.184 min
Response: 0
Conc: N.D.

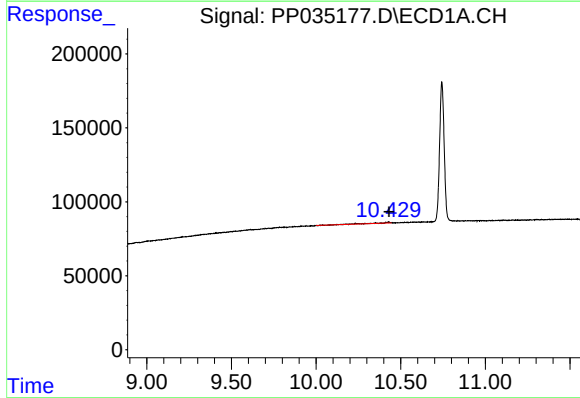

#45 AR-1268-5

R.T.: 10.429 min
Delta R.T.: -0.002 min
Response: 22722
Conc: 1.02 ng/ml

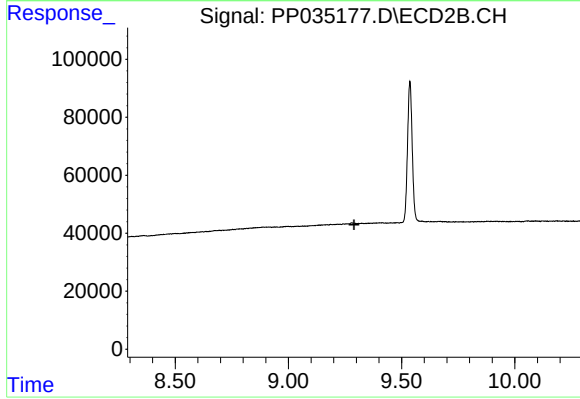

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 9.290 min
Response: 0
Conc: N.D.