

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042221\
 Data File : PP035189.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Apr 2021 3:38
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 04:53:18 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 21 17:37:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.837	4.248	1795864	1150555	22.039	22.342
2)	SA Decachlor...	10.743	9.535	1753638	702199	27.750	29.554
Target Compounds							
9)	L2 AR-1221-2	5.188	0.000	22308	0	35.393	N.D. #
20)	L4 AR-1242-5	7.124	0.000	69090	0	63.611	N.D. #
24)	L5 AR-1248-4	7.092	0.000	114767	0	60.636	N.D. #
25)	L5 AR-1248-5	7.124	0.000	69090	0	35.826	N.D. #
27)	L6 AR-1254-2	7.277	0.000	92854	0	24.538	N.D. #
28)	L6 AR-1254-3	7.664	0.000	4213	0	1.129	N.D. #
29)	L6 AR-1254-4	7.942f	0.000	58570	0	27.965	N.D. #
30)	L6 AR-1254-5	8.382	0.000	316858	0	108.917	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042221\
Data File : PP035189.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Apr 2021 3:38
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 04:53:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 21 17:37:28 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

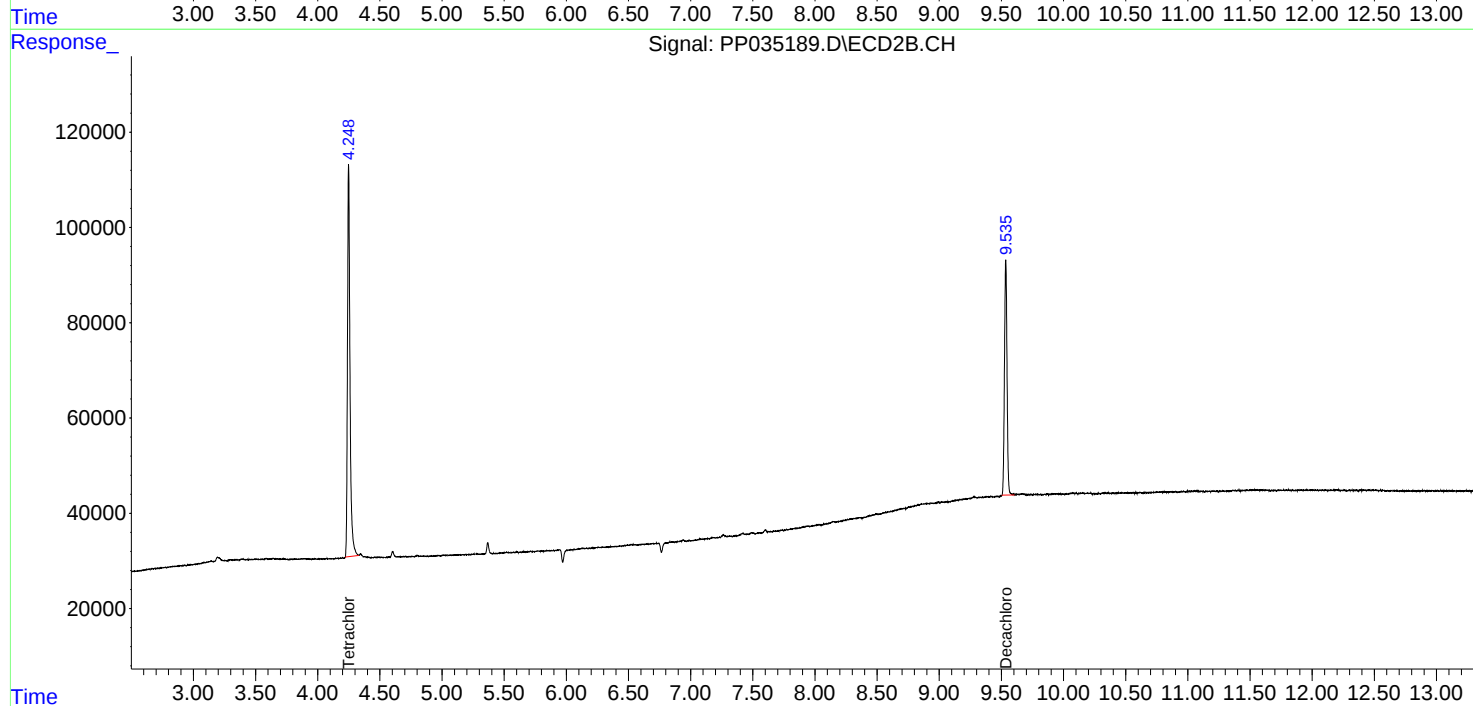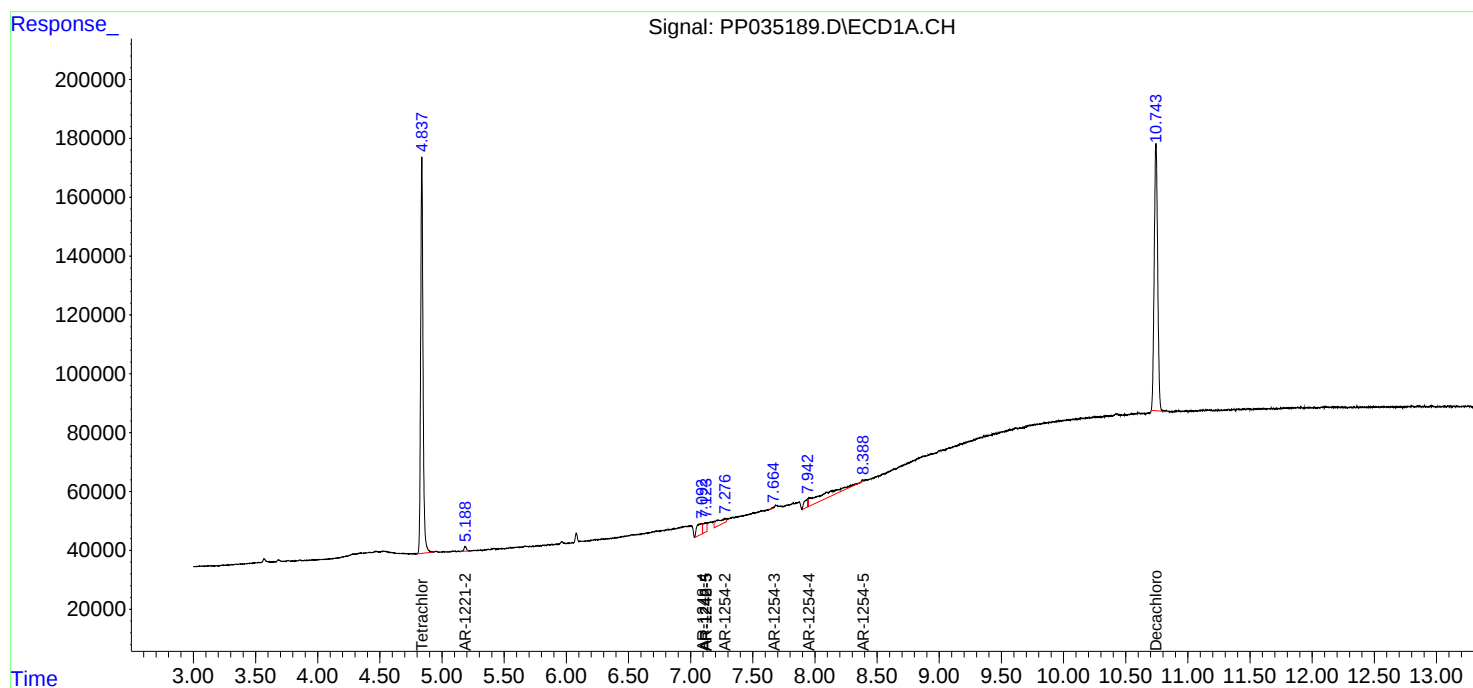


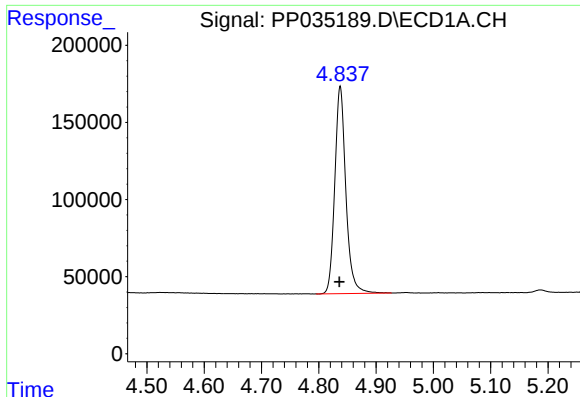

#1 Tetrachloro-m-xylene


R.T.: 4.837 min
Delta R.T.: 0.001 min
Response: 1795864
Conc: 22.04 ng/ml

Instrument :
ECD_P
ClientSampleId :

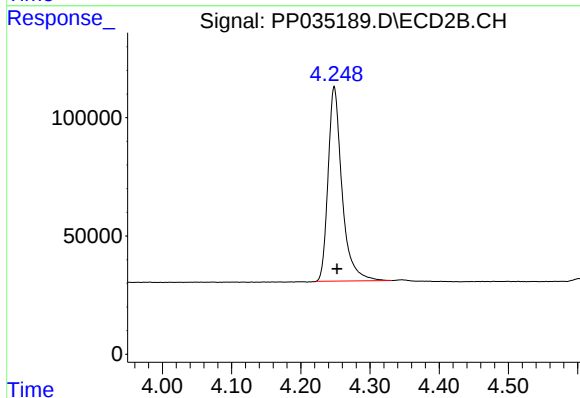


#1 Tetrachloro-m-xylene

R.T.: 4.248 min
Delta R.T.: -0.004 min
Response: 1150555
Conc: 22.34 ng/ml

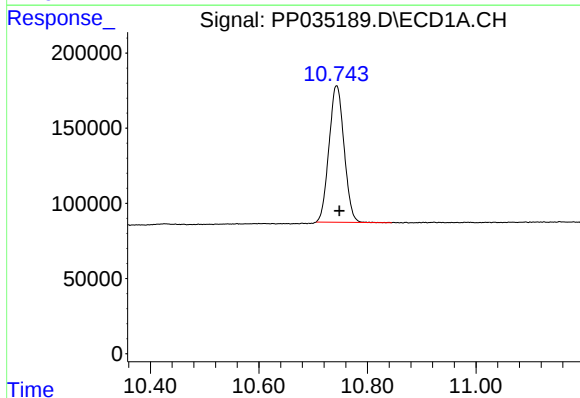


#2 Decachlorobiphenyl

R.T.: 10.743 min
Delta R.T.: -0.005 min
Response: 1753638
Conc: 27.75 ng/ml

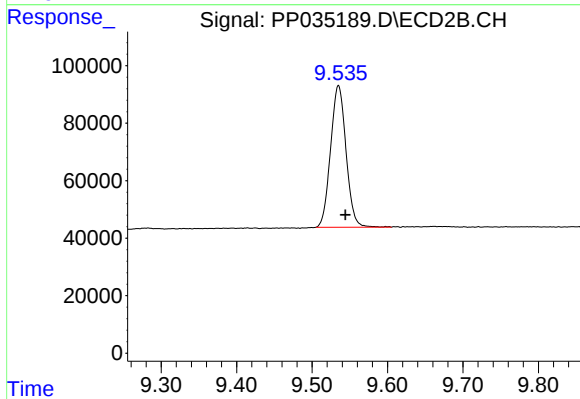

#2 Decachlorobiphenyl


R.T.: 9.535 min
Delta R.T.: -0.009 min
Response: 702199
Conc: 29.55 ng/ml

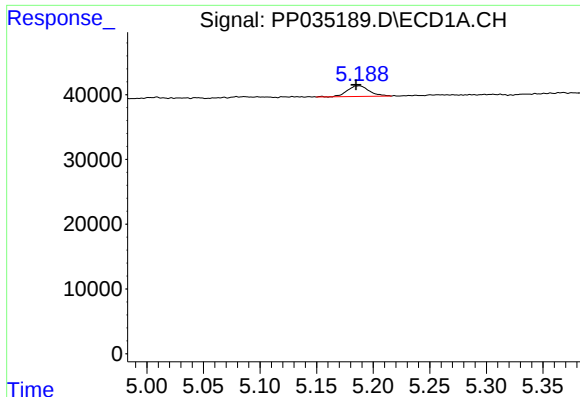

#9 AR-1221-2


R.T.: 5.188 min
Delta R.T.: 0.003 min
Response: 22308
Conc: 35.39 ng/ml

Instrument :
ECD_P
ClientSampleId :

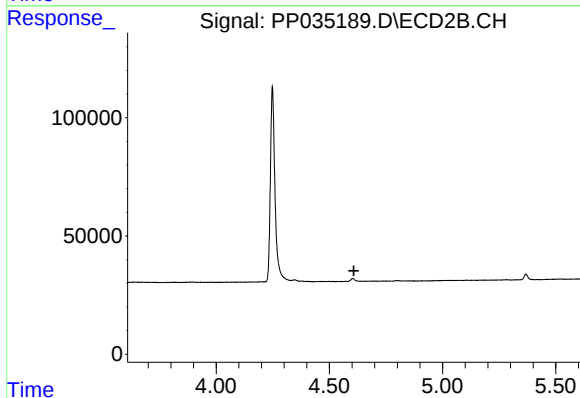


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.608 min
Response: 0
Conc: N.D.

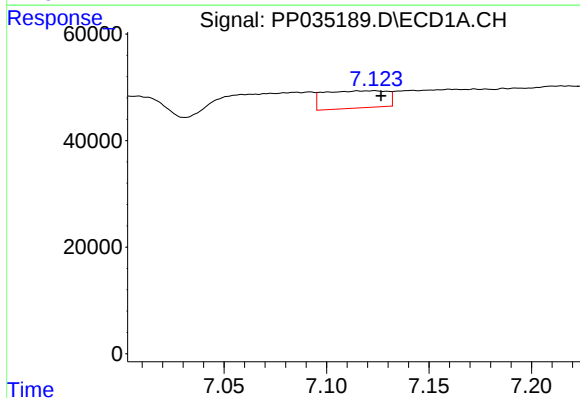


#20 AR-1242-5

R.T.: 7.124 min
Delta R.T.: -0.003 min
Response: 69090
Conc: 63.61 ng/ml

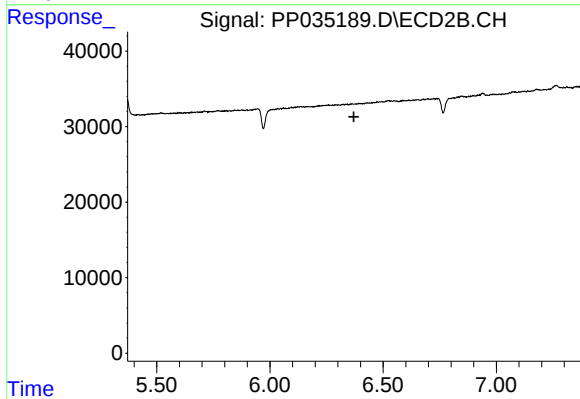

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T. : 6.371 min
Response: 0
Conc: N.D.

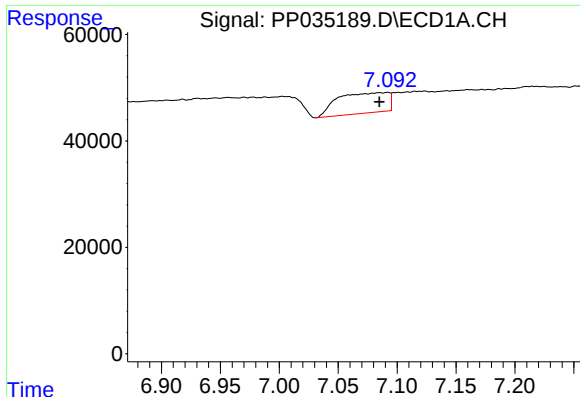

#24 AR-1248-4


R.T.: 7.092 min
Delta R.T.: 0.007 min
Response: 114767
Conc: 60.64 ng/ml

Instrument :
ECD_P
ClientSampleId :

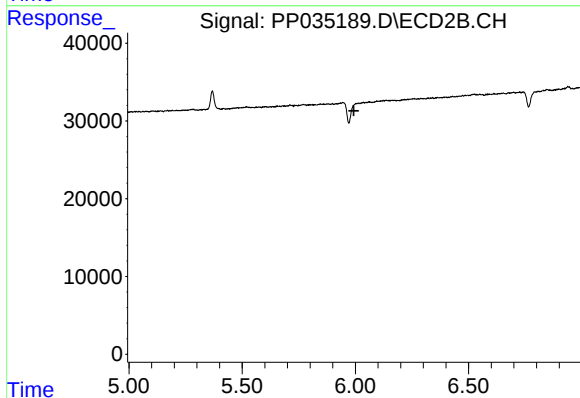


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.993 min
Response: 0
Conc: N.D.

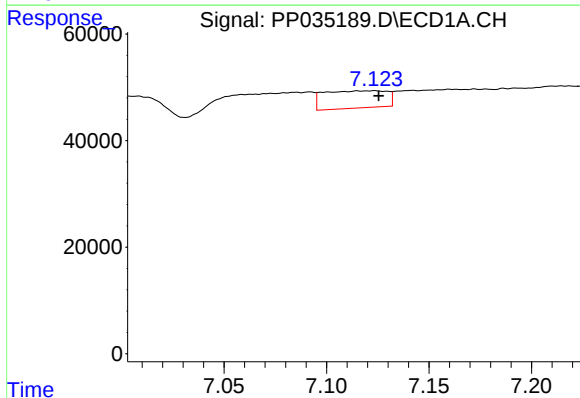


#25 AR-1248-5

R.T.: 7.124 min
Delta R.T.: -0.002 min
Response: 69090
Conc: 35.83 ng/ml

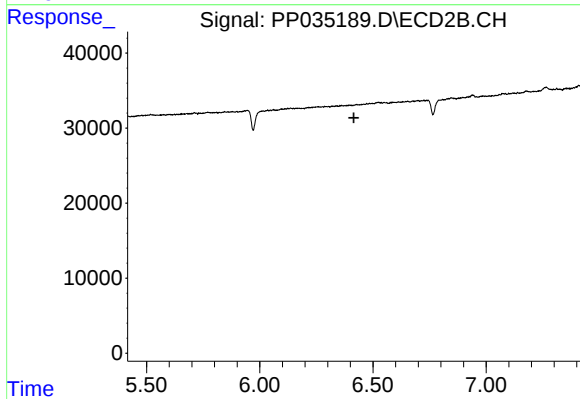

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T. : 6.416 min
Response: 0
Conc: N.D.

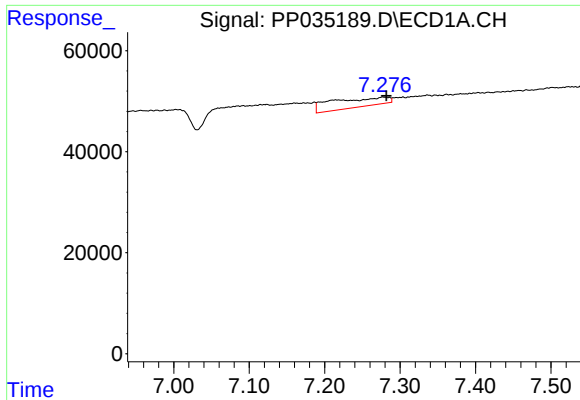

#27 AR-1254-2


R.T.: 7.277 min
Delta R.T.: -0.005 min
Response: 92854
Conc: 24.54 ng/ml

Instrument :
ECD_P
ClientSampleId :

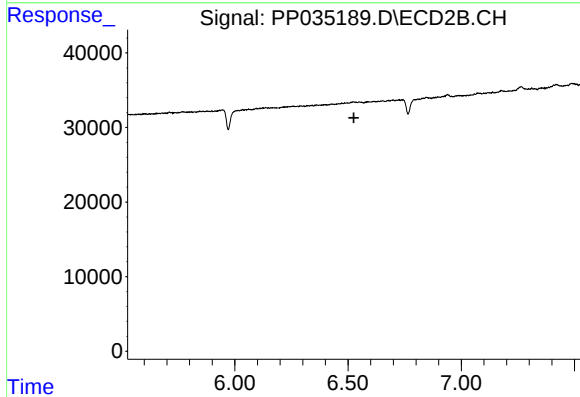


#27 AR-1254-2

R.T.: 0.000 min
Exp R.T. : 6.526 min
Response: 0
Conc: N.D.

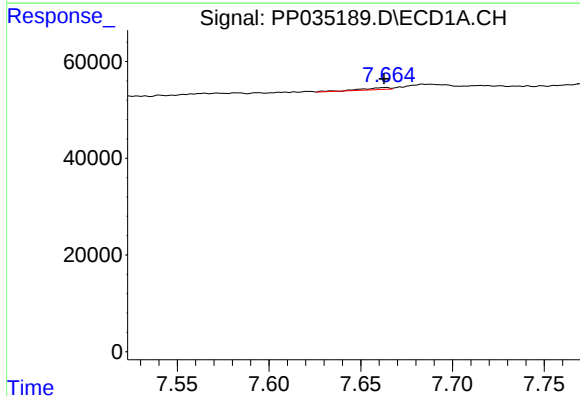


#28 AR-1254-3

R.T.: 7.664 min
Delta R.T.: 0.001 min
Response: 4213
Conc: 1.13 ng/ml

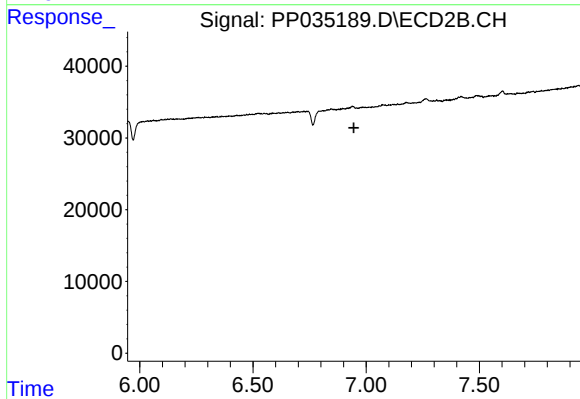

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.946 min
Response: 0
Conc: N.D.

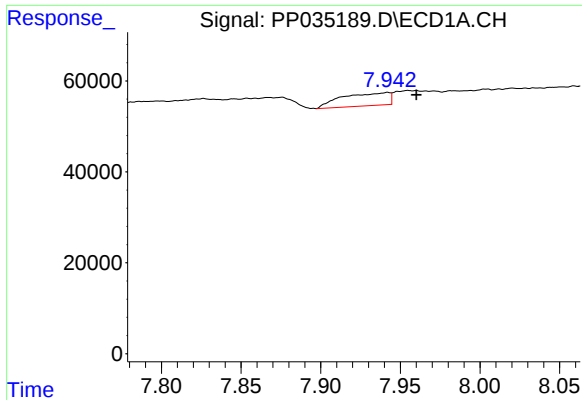

#29 AR-1254-4


R.T.: 7.942 min
Delta R.T.: -0.018 min
Response: 58570
Conc: 27.96 ng/ml

Instrument :
ECD_P
ClientSampleId :

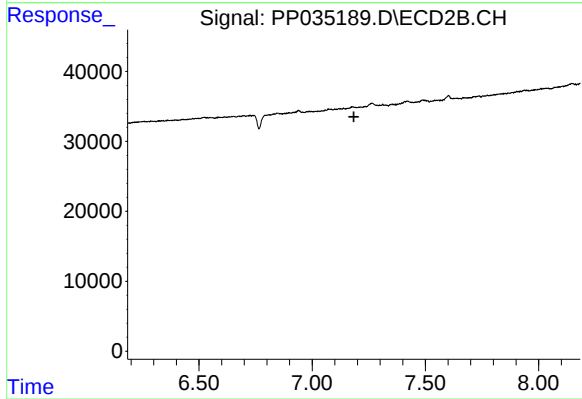


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 7.184 min
Response: 0
Conc: N.D.

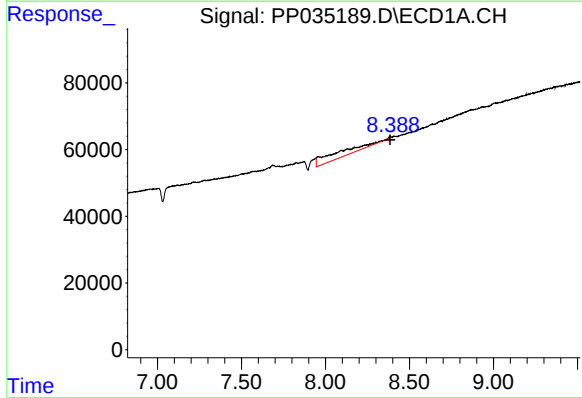

#30 AR-1254-5

R.T.: 8.382 min
Delta R.T.: -0.003 min
Response: 316858
Conc: 108.92 ng/ml

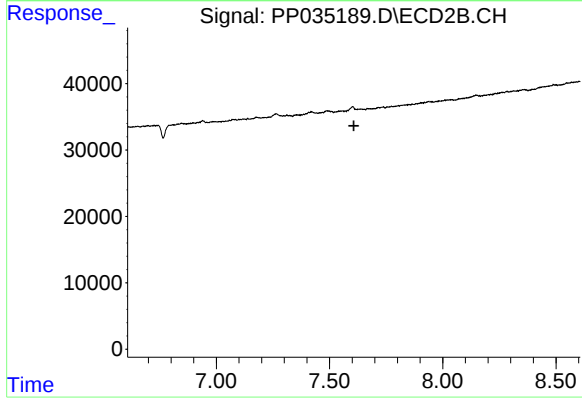

#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.608 min
Response: 0
Conc: N.D.