

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042221\
 Data File : PP035147.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Apr 2021 14:23
 Operator : DD\AJ
 Sample : M2076-18RE
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SB-18-14.5-15.0RE

Manual Integrations
 APPROVED

Ankita
 4/23/2021 4:44:23 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 22 16:18:08 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 21 17:37:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.838	4.250	1764234	1097313	21.651	21.308
2) SA Decachlor...	10.748	9.540	4256494	1526277	67.357	64.237
Target Compounds						
31) L7 AR-1260-1	7.816	7.076	161625	164157	47.992m	93.828 #
32) L7 AR-1260-2	8.094	7.271	600078	99217	176.264m	55.658 #
33) L7 AR-1260-3	8.458	7.425	110172	73756	43.893m	40.904
34) L7 AR-1260-4	8.688	7.903	139895	63164	47.660m	49.622
35) L7 AR-1260-5	9.006	8.148	262165	135137	53.289	55.583

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042221\
Data File : PP035147.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Apr 2021 14:23
Operator : DD\AJ
Sample : M2076-18RE
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
SB-18-14.5-15.0RE


Manual Integrations
APPROVED

Ankita
4/23/2021 4:44:23 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 16:18:08 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 21 17:37:28 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

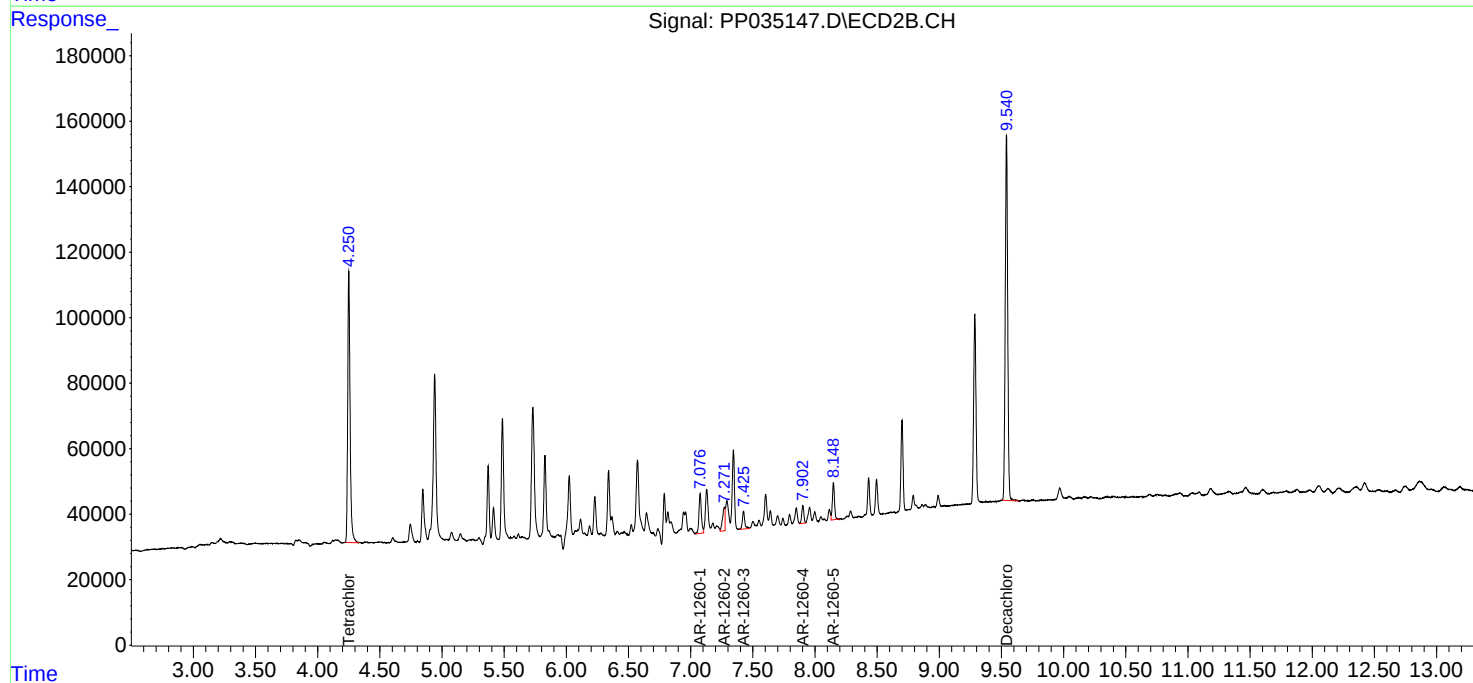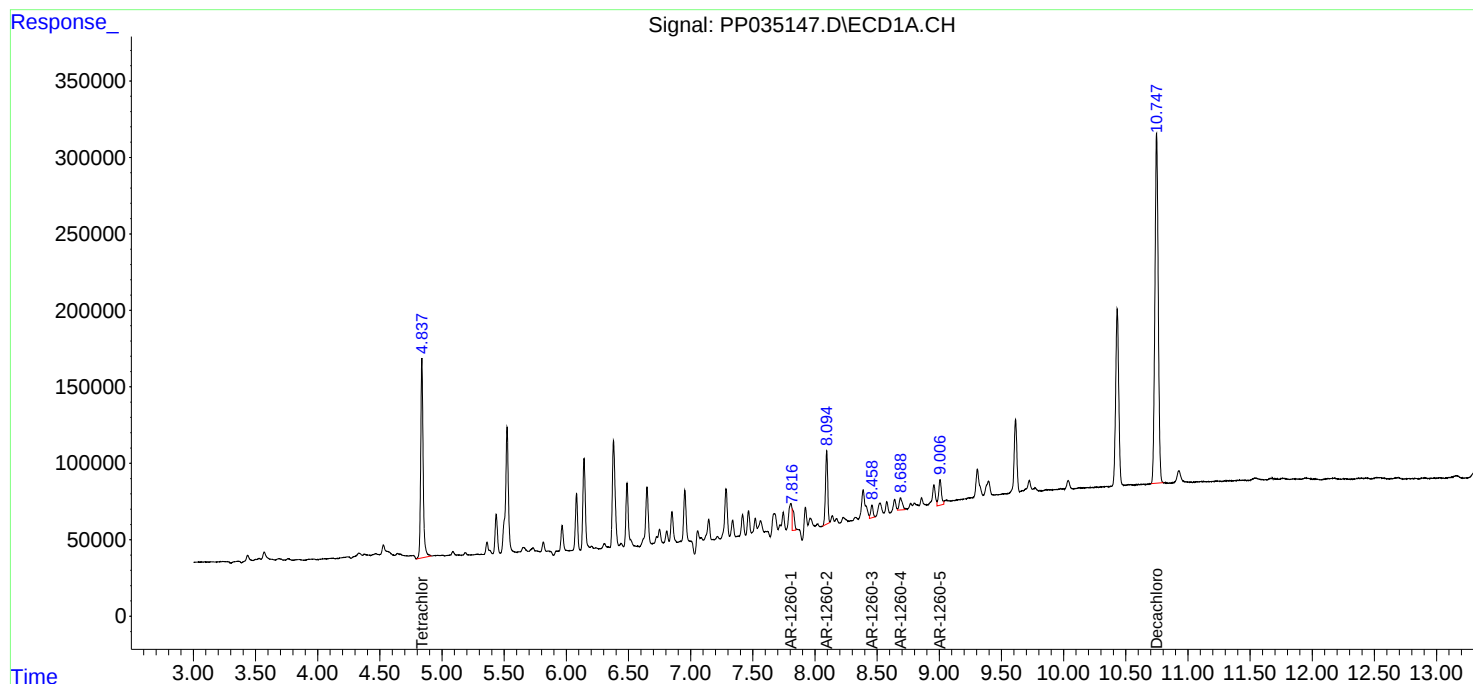

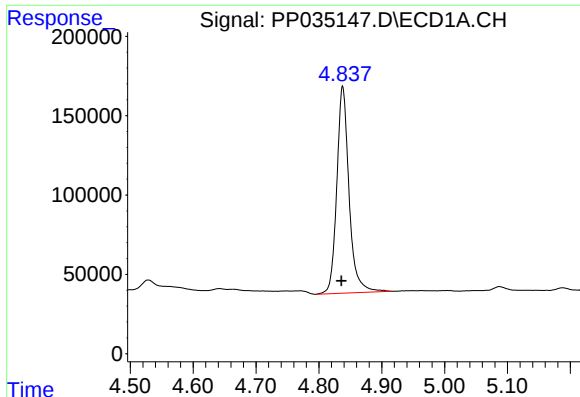


#1 Tetrachloro-m-xylene

R.T.: 4.838 min
Delta R.T.: 0.002 min
Response: 1764234
Conc: 21.65 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-18-14.5-15.0RE


Manual Integrations
APPROVED

Ankita
4/23/2021 4:44:23 PM

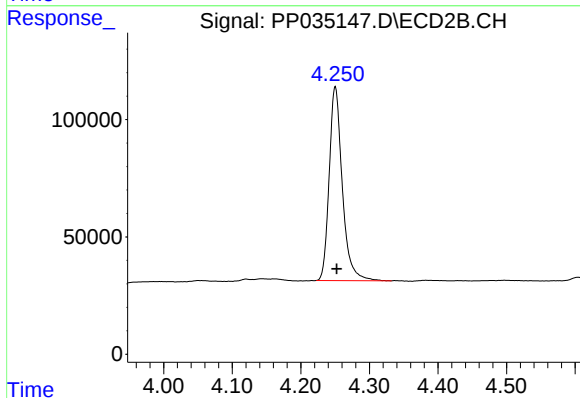


#1 Tetrachloro-m-xylene

R.T.: 4.250 min
Delta R.T.: -0.002 min
Response: 1097313
Conc: 21.31 ng/ml

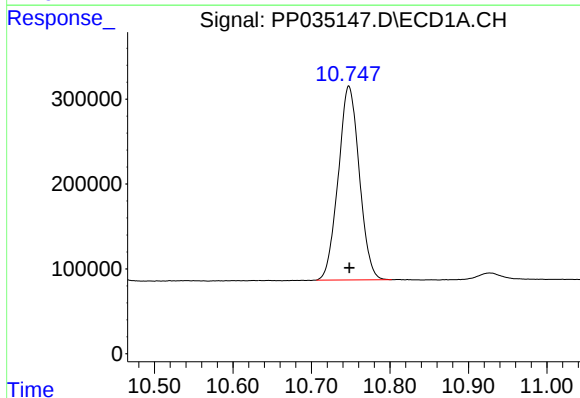


#2 Decachlorobiphenyl

R.T.: 10.748 min
Delta R.T.: 0.000 min
Response: 4256494
Conc: 67.36 ng/ml

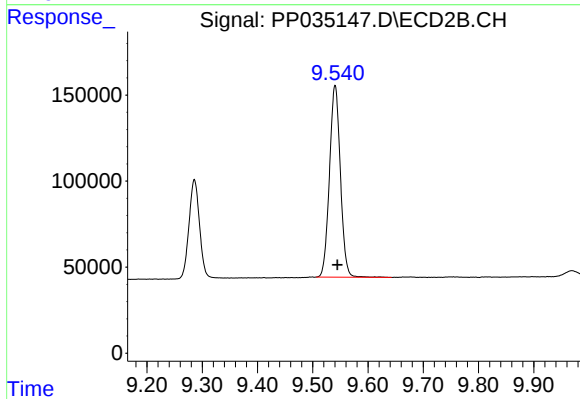

#2 Decachlorobiphenyl

R.T.: 9.540 min
Delta R.T.: -0.004 min
Response: 1526277
Conc: 64.24 ng/ml

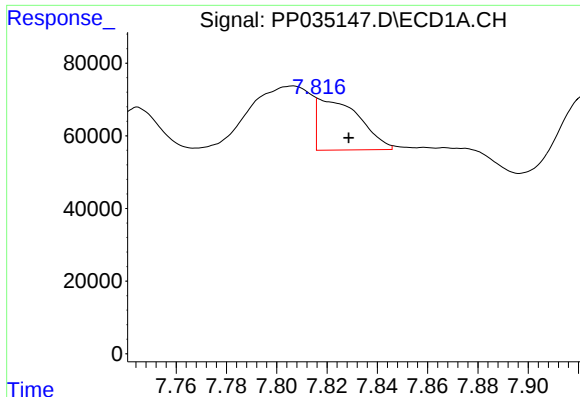


#31 AR-1260-1

R.T.: 7.816 min
Delta R.T.: -0.013 min
Response: 161625
Conc: 47.99 ng/ml m

Instrument :
ECD_P
ClientSampleId :
SB-18-14.5-15.0RE


Manual Integrations
APPROVED

Ankita
4/23/2021 4:44:23 PM

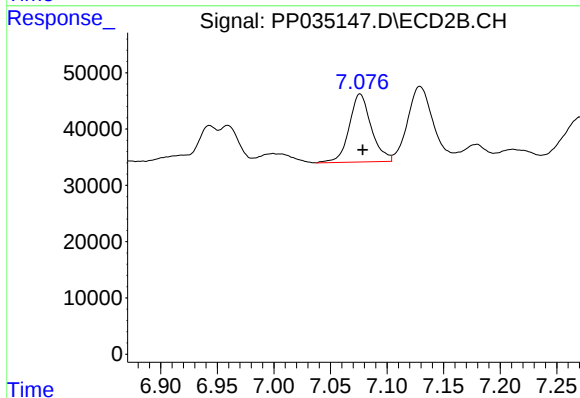


#31 AR-1260-1

R.T.: 7.076 min
Delta R.T.: -0.002 min
Response: 164157
Conc: 93.83 ng/ml

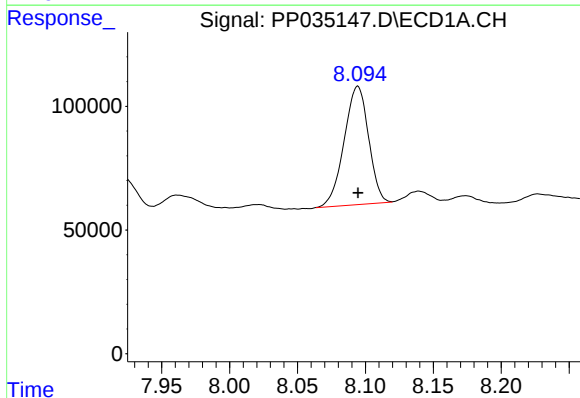


#32 AR-1260-2

R.T.: 8.094 min
Delta R.T.: 0.000 min
Response: 600078
Conc: 176.26 ng/ml m

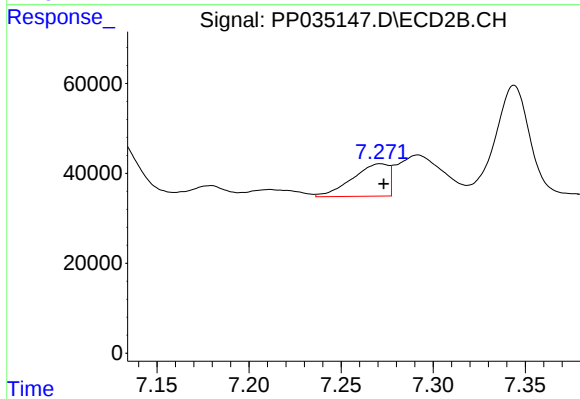

#32 AR-1260-2

R.T.: 7.271 min
Delta R.T.: -0.002 min
Response: 99217
Conc: 55.66 ng/ml

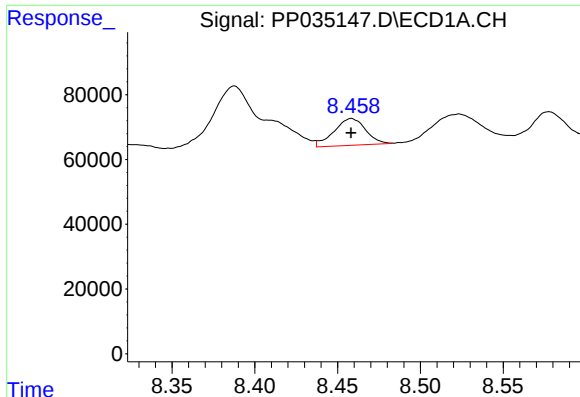


#33 AR-1260-3

R.T.: 8.458 min
Delta R.T.: 0.000 min
Response: 110172
Conc: 43.89 ng/ml m

Instrument :
ECD_P
ClientSampleId :
SB-18-14.5-15.0RE


Manual Integrations
APPROVED

Ankita
4/23/2021 4:44:23 PM

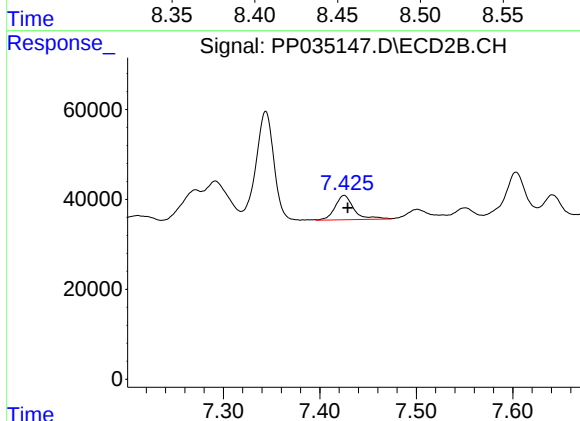


#33 AR-1260-3

R.T.: 7.425 min
Delta R.T.: -0.004 min
Response: 73756
Conc: 40.90 ng/ml

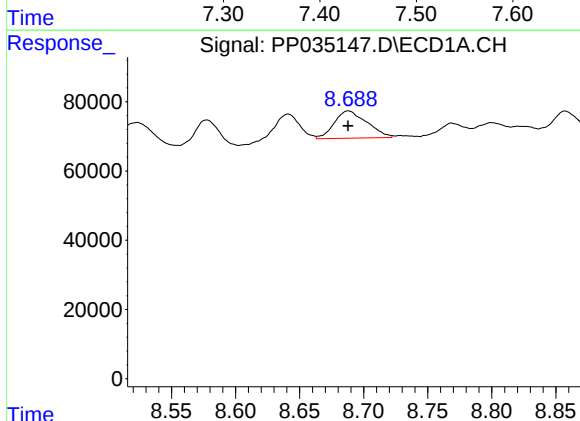


#34 AR-1260-4

R.T.: 8.688 min
Delta R.T.: 0.000 min
Response: 139895
Conc: 47.66 ng/ml m

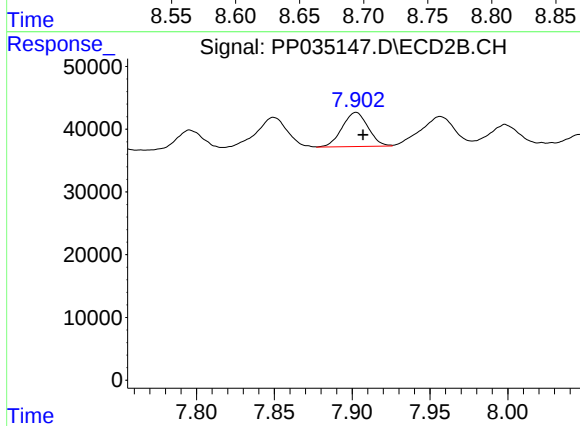

#34 AR-1260-4

R.T.: 7.903 min
Delta R.T.: -0.005 min
Response: 63164
Conc: 49.62 ng/ml

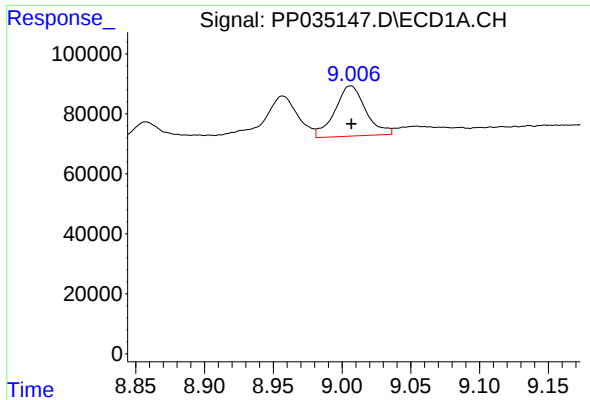


#35 AR-1260-5

R.T.: 9.006 min
Delta R.T.: 0.000 min
Response: 262165
Conc: 53.29 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-18-14.5-15.0RE

Manual Integrations
APPROVED

Ankita
4/23/2021 4:44:23 PM

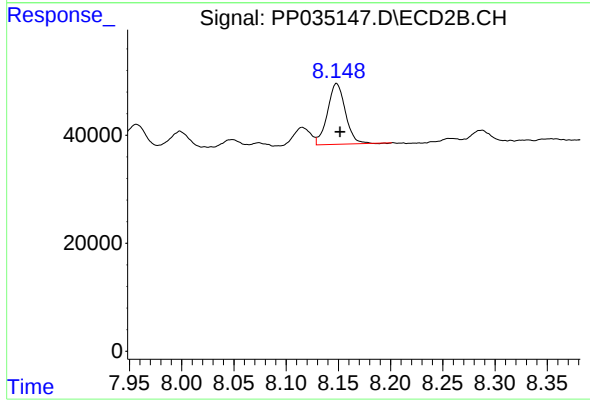

#35 AR-1260-5

R.T.: 8.148 min
Delta R.T.: -0.003 min
Response: 135137
Conc: 55.58 ng/ml