

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042221\
 Data File : PP035149.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Apr 2021 14:57
 Operator : DD\AJ
 Sample : M2077-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SB-19-14.5-15.0

Manual Integrations
 APPROVED

Ankita
 4/23/2021 4:44:25 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 22 16:19:02 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 21 17:37:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.837	4.250	1649584	1034141	20.244	20.082
2) SA Decachlor...	10.748	9.539	2794919	1000498	44.228	42.109
Target Compounds						
26) L6 AR-1254-1	7.052	6.377	65947	63971	25.581m	37.791 #
27) L6 AR-1254-2	7.284	6.522	121441	48676	32.092m	32.579
28) L6 AR-1254-3	7.663	6.941	163237	43555	43.753m	20.482m#
29) L6 AR-1254-4	7.957	7.174	65417	62847	31.234m	70.129 #
30) L6 AR-1254-5	8.384	7.603	146089	112163	50.217m	63.104 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042221\
Data File : PP035149.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Apr 2021 14:57
Operator : DD\AJ
Sample : M2077-01
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
SB-19-14.5-15.0


Manual Integrations
APPROVED

Ankita
4/23/2021 4:44:25 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 16:19:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 21 17:37:28 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

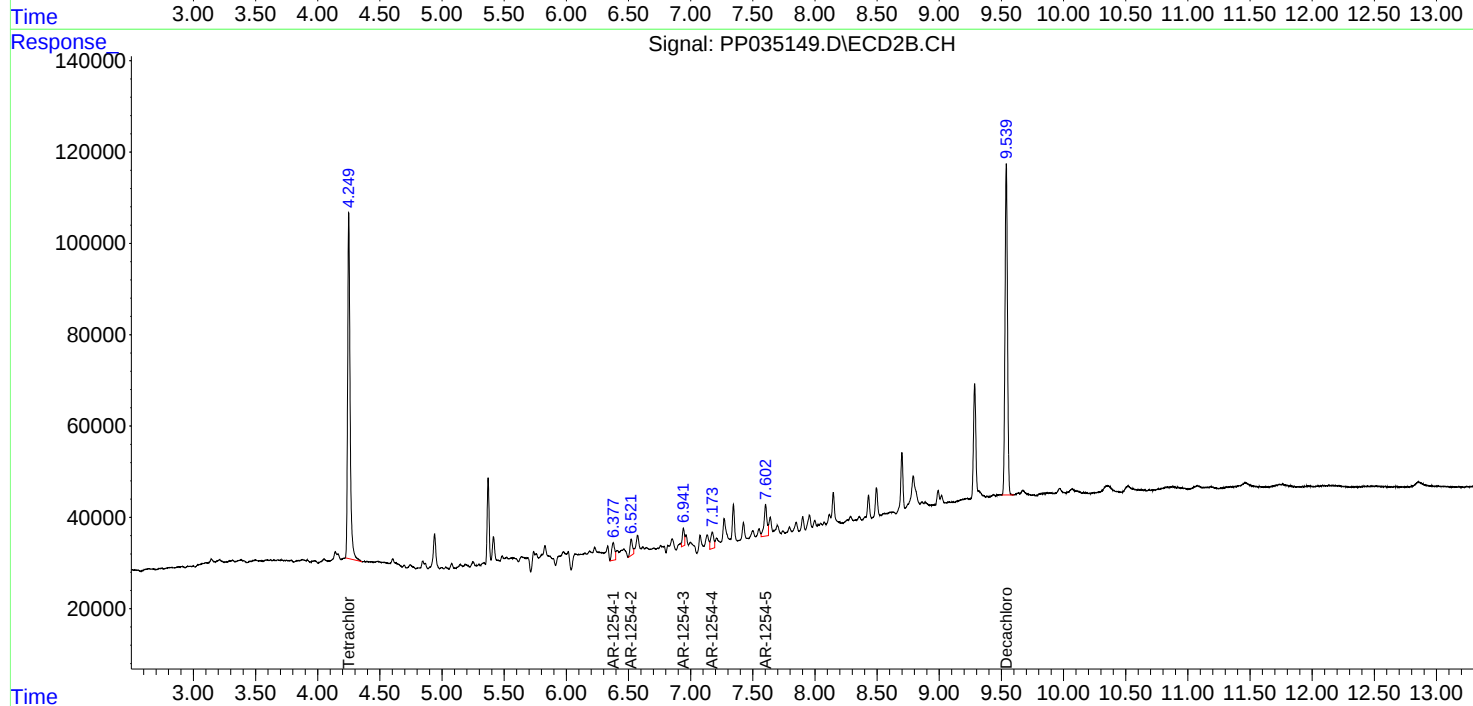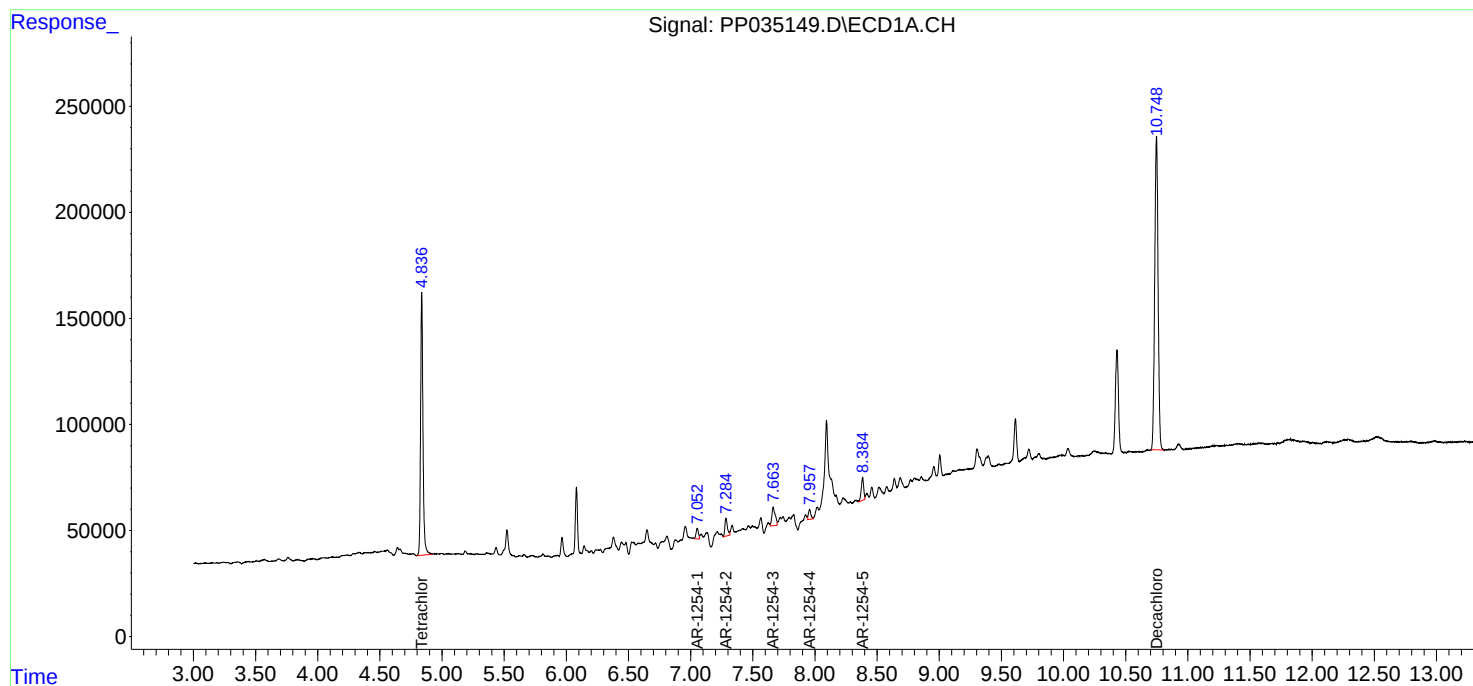

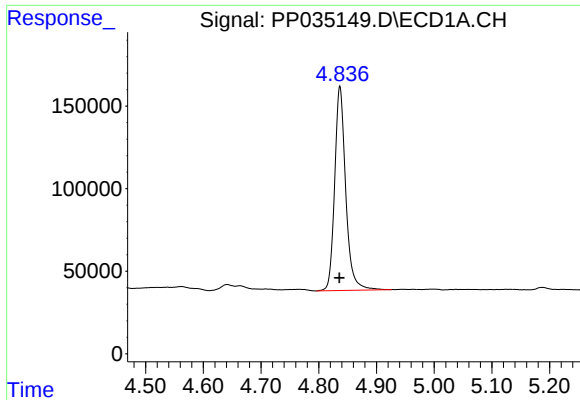


#1 Tetrachloro-m-xylene

R.T.: 4.837 min
Delta R.T.: 0.000 min
Response: 1649584
Conc: 20.24 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-19-14.5-15.0


Manual Integrations
APPROVED

Ankita
4/23/2021 4:44:25 PM

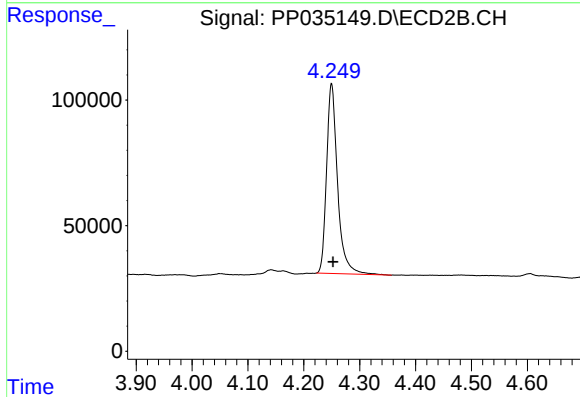


#1 Tetrachloro-m-xylene

R.T.: 4.250 min
Delta R.T.: -0.003 min
Response: 1034141
Conc: 20.08 ng/ml

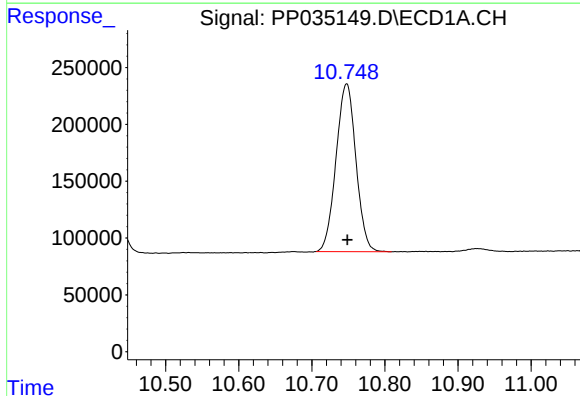


#2 Decachlorobiphenyl

R.T.: 10.748 min
Delta R.T.: 0.000 min
Response: 2794919
Conc: 44.23 ng/ml

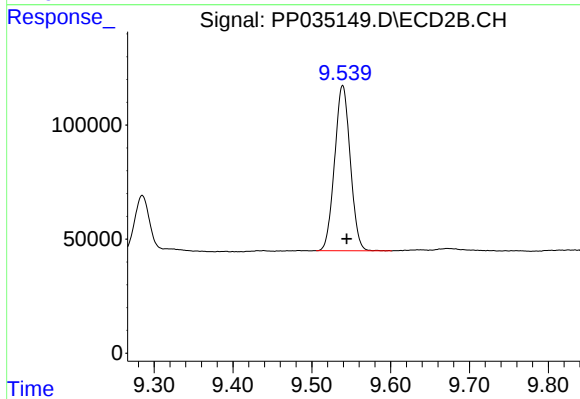

#2 Decachlorobiphenyl

R.T.: 9.539 min
Delta R.T.: -0.005 min
Response: 1000498
Conc: 42.11 ng/ml

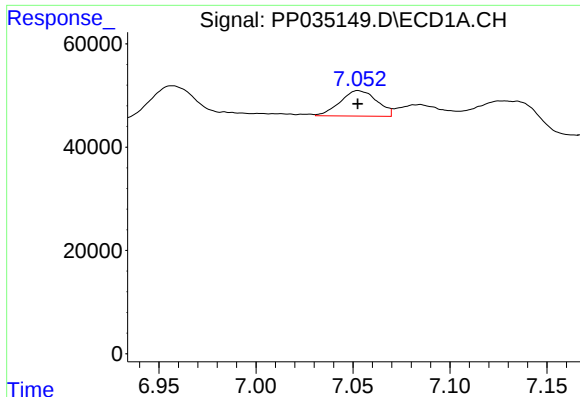


#26 AR-1254-1

R.T.: 7.052 min
Delta R.T.: 0.000 min
Response: 65947
Conc: 25.58 ng/ml m

Instrument :
ECD_P
ClientSampleId :
SB-19-14.5-15.0


Manual Integrations
APPROVED

Ankita
4/23/2021 4:44:25 PM

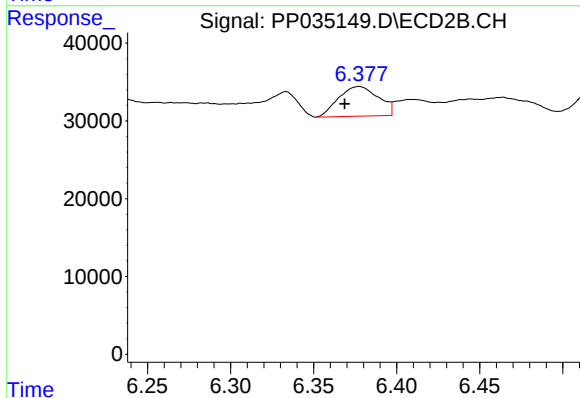


#26 AR-1254-1

R.T.: 6.377 min
Delta R.T.: 0.009 min
Response: 63971
Conc: 37.79 ng/ml

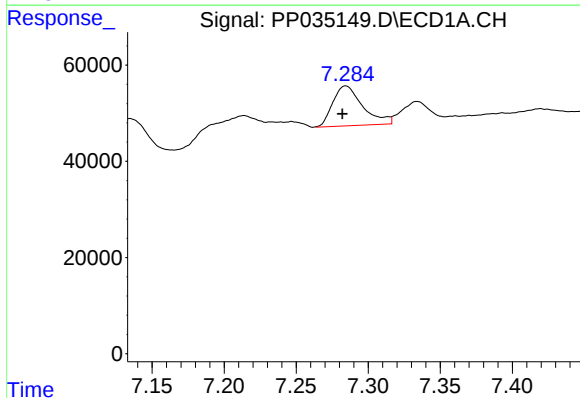


#27 AR-1254-2

R.T.: 7.284 min
Delta R.T.: 0.002 min
Response: 121441
Conc: 32.09 ng/ml m

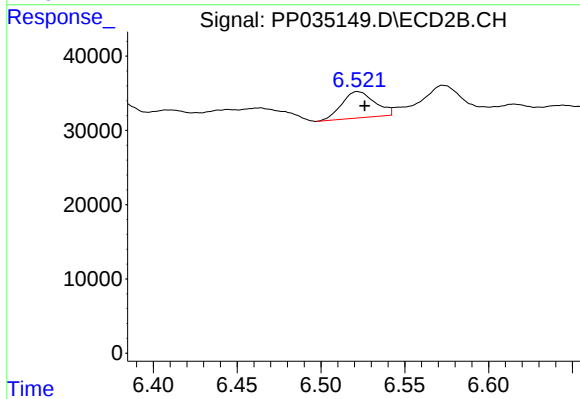

#27 AR-1254-2

R.T.: 6.522 min
Delta R.T.: -0.004 min
Response: 48676
Conc: 32.58 ng/ml

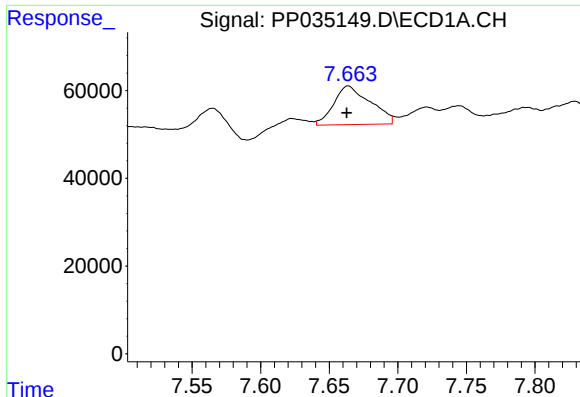


#28 AR-1254-3

R.T.: 7.663 min
Delta R.T.: 0.000 min
Response: 163237
Conc: 43.75 ng/ml m

Instrument :
ECD_P
ClientSampleId :
SB-19-14.5-15.0


Manual Integrations
APPROVED

Ankita
4/23/2021 4:44:25 PM

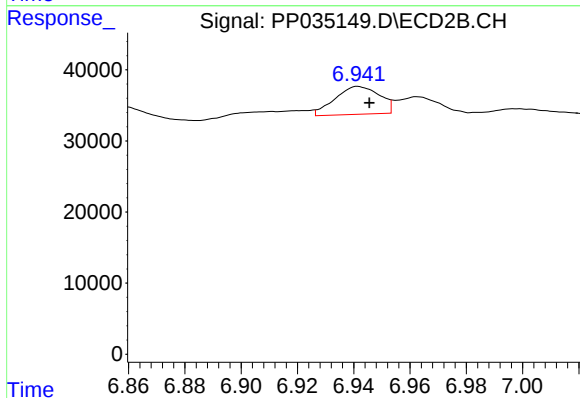


#28 AR-1254-3

R.T.: 6.941 min
Delta R.T.: -0.005 min
Response: 43555
Conc: 20.48 ng/ml m

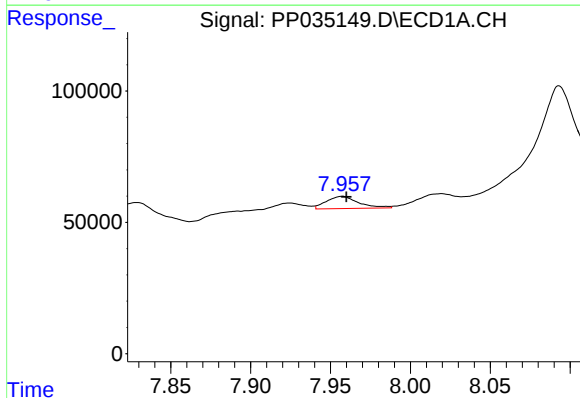


#29 AR-1254-4

R.T.: 7.957 min
Delta R.T.: -0.003 min
Response: 65417
Conc: 31.23 ng/ml m

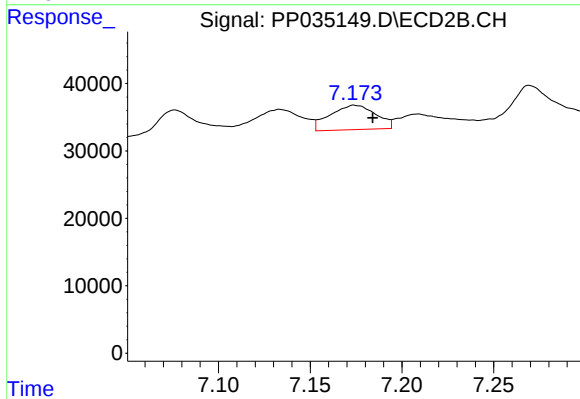

#29 AR-1254-4

R.T.: 7.174 min
Delta R.T.: -0.010 min
Response: 62847
Conc: 70.13 ng/ml

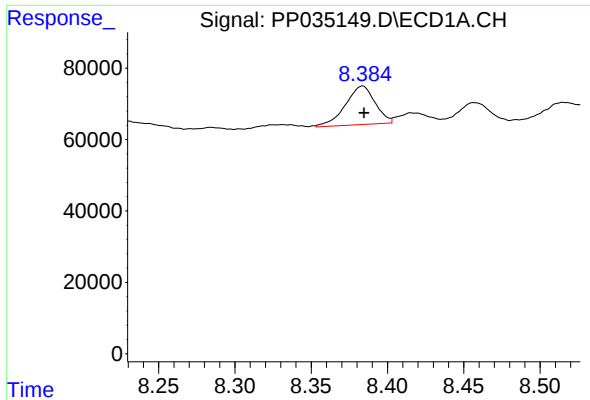


#30 AR-1254-5

R.T.: 8.384 min
Delta R.T.: -0.001 min
Response: 146089
Conc: 50.22 ng/ml m

Instrument :
ECD_P
ClientSampleId :
SB-19-14.5-15.0

Manual Integrations
APPROVED

Ankita
4/23/2021 4:44:25 PM

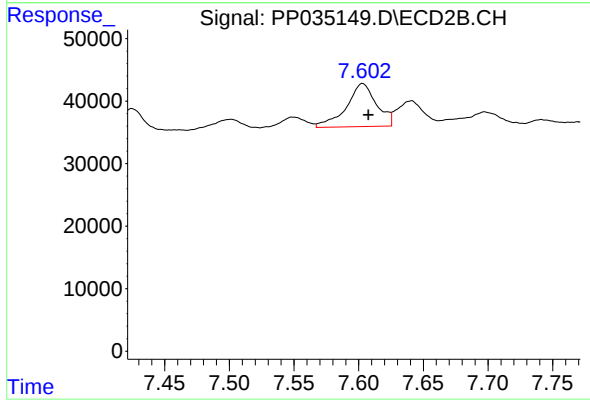

#30 AR-1254-5

R.T.: 7.603 min
Delta R.T.: -0.004 min
Response: 112163
Conc: 63.10 ng/ml