

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042221\
 Data File : PP035150.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Apr 2021 15:14
 Operator : DD\AJ
 Sample : M2077-01RE
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SB-19-14.5-15.0RE

Manual Integrations
 APPROVED

Ankita
 4/23/2021 4:44:27 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 22 16:19:28 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 21 17:37:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.837	4.250	1660462	1059469	20.377	20.573
2) SA Decachlor...	10.748	9.539	2790361	1021044	44.156	42.973
Target Compounds						
26) L6 AR-1254-1	7.053	6.377	78626	66982	30.499	39.570 #
27) L6 AR-1254-2	7.284	6.522	148364	53666	39.207m	35.918
28) L6 AR-1254-3	7.663	6.941	166624	32766	44.661m	15.409m#
29) L6 AR-1254-4	7.956	7.175	87411	40987	41.735m	45.736
30) L6 AR-1254-5	8.383	7.603	154999	84814	53.280m	47.717

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042221\
Data File : PP035150.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Apr 2021 15:14
Operator : DD\AJ
Sample : M2077-01RE
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
SB-19-14.5-15.0RE


Manual Integrations
APPROVED

Ankita
4/23/2021 4:44:27 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 16:19:28 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 21 17:37:28 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

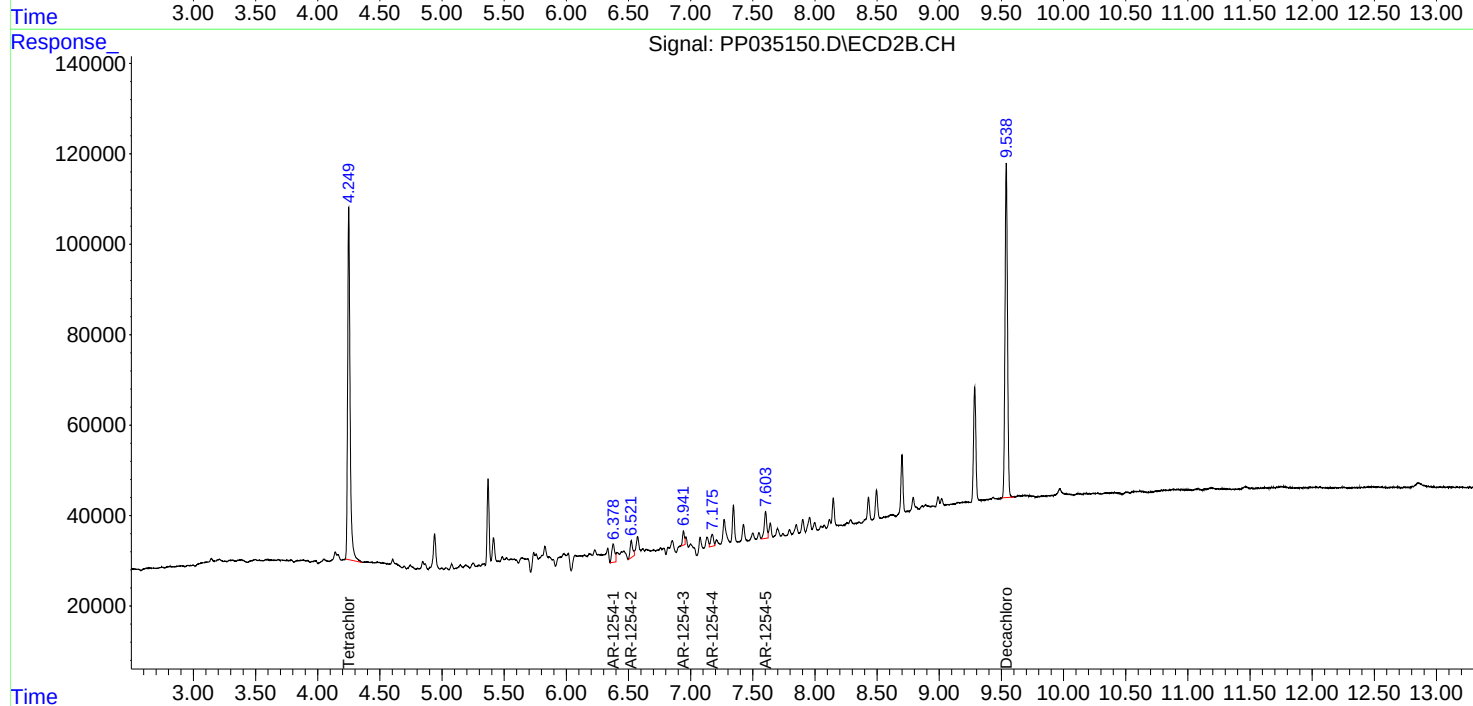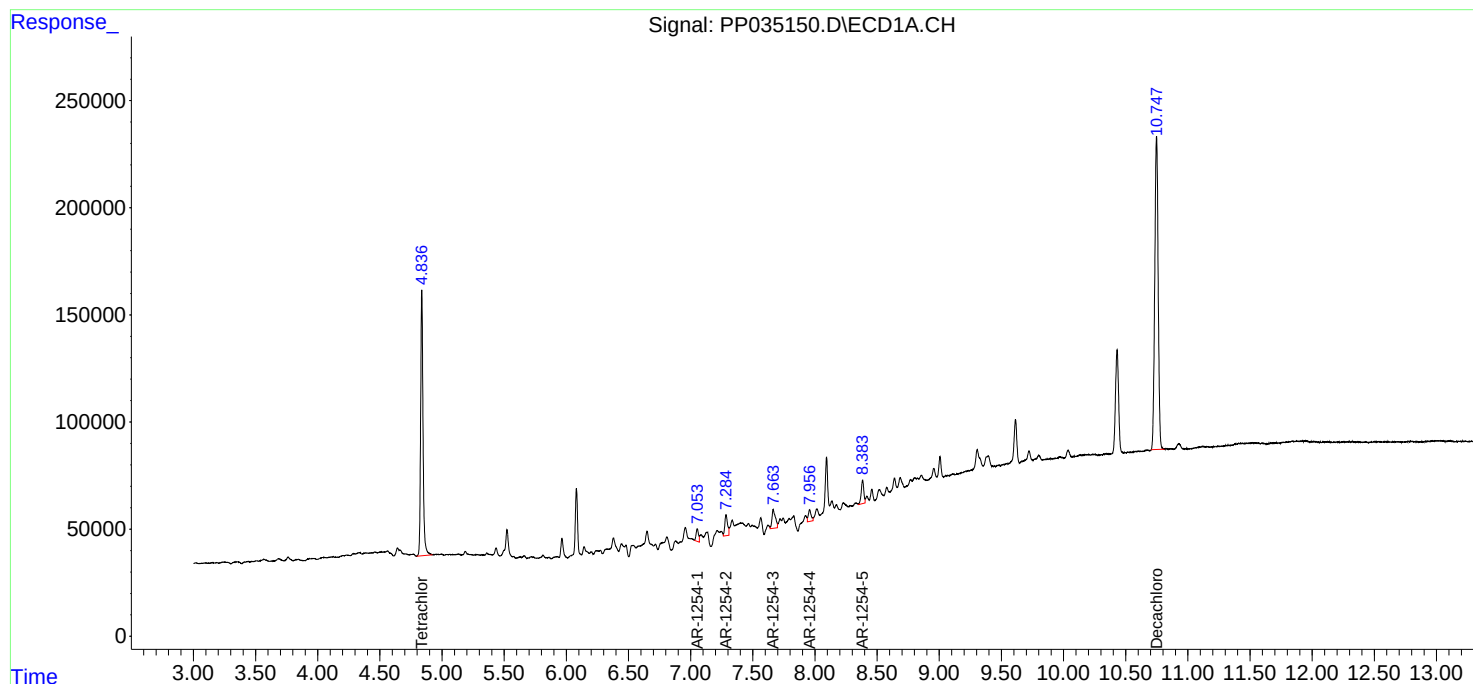

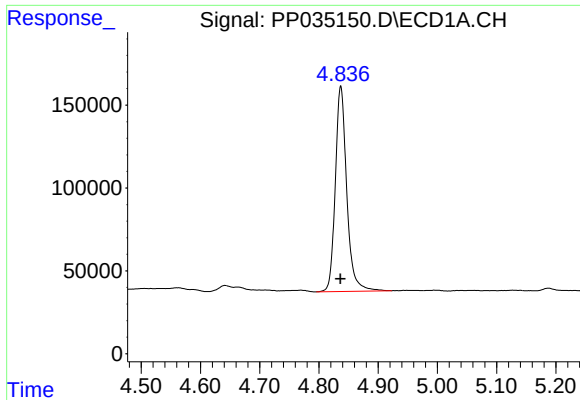


#1 Tetrachloro-m-xylene

R.T.: 4.837 min
Delta R.T.: 0.000 min
Response: 1660462
Conc: 20.38 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-19-14.5-15.0RE


Manual Integrations
APPROVED

Ankita
4/23/2021 4:44:27 PM

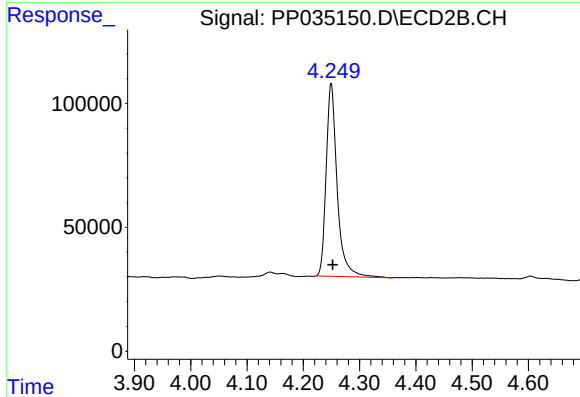


#1 Tetrachloro-m-xylene

R.T.: 4.250 min
Delta R.T.: -0.003 min
Response: 1059469
Conc: 20.57 ng/ml

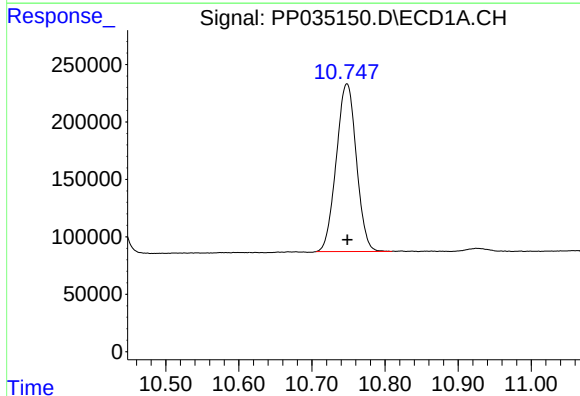


#2 Decachlorobiphenyl

R.T.: 10.748 min
Delta R.T.: 0.000 min
Response: 2790361
Conc: 44.16 ng/ml

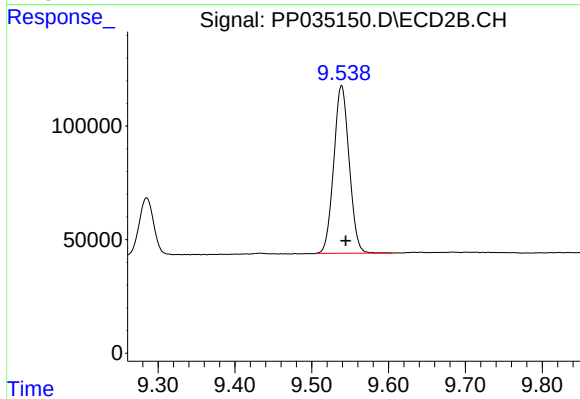

#2 Decachlorobiphenyl

R.T.: 9.539 min
Delta R.T.: -0.006 min
Response: 1021044
Conc: 42.97 ng/ml

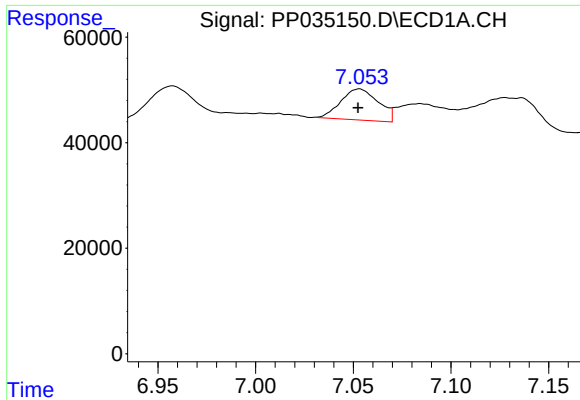


#26 AR-1254-1

R.T.: 7.053 min
Delta R.T.: 0.000 min
Response: 78626
Conc: 30.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-19-14.5-15.0RE


Manual Integrations
APPROVED

Ankita
4/23/2021 4:44:27 PM

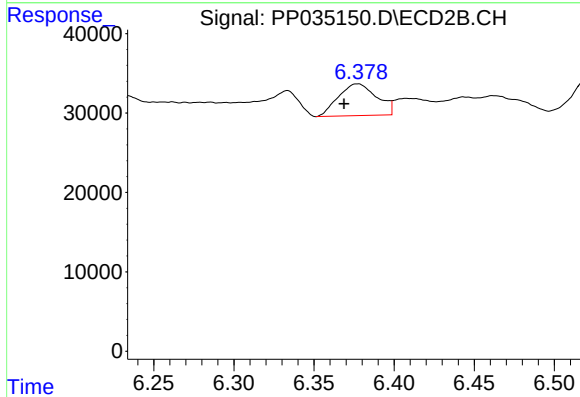


#26 AR-1254-1

R.T.: 6.377 min
Delta R.T.: 0.008 min
Response: 66982
Conc: 39.57 ng/ml

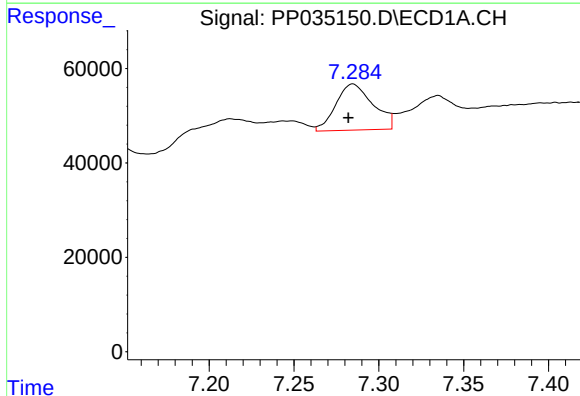


#27 AR-1254-2

R.T.: 7.284 min
Delta R.T.: 0.002 min
Response: 148364
Conc: 39.21 ng/ml m

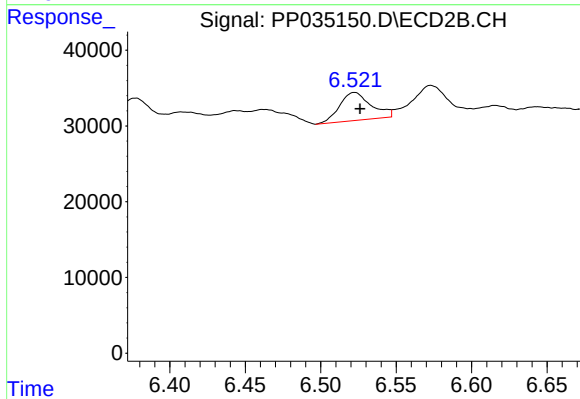

#27 AR-1254-2

R.T.: 6.522 min
Delta R.T.: -0.004 min
Response: 53666
Conc: 35.92 ng/ml

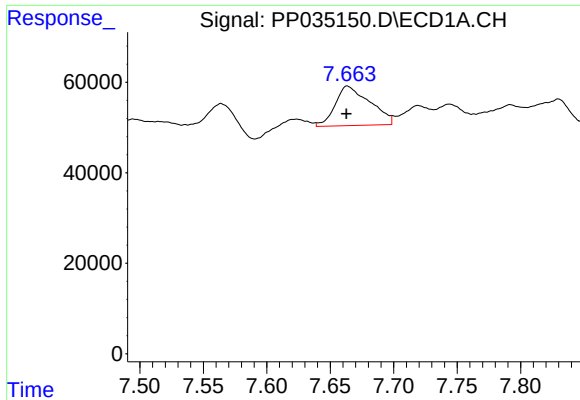


#28 AR-1254-3

R.T.: 7.663 min
Delta R.T.: 0.000 min
Response: 166624
Conc: 44.66 ng/ml m

Instrument :
ECD_P
ClientSampleId :
SB-19-14.5-15.0RE


Manual Integrations
APPROVED

Ankita
4/23/2021 4:44:27 PM

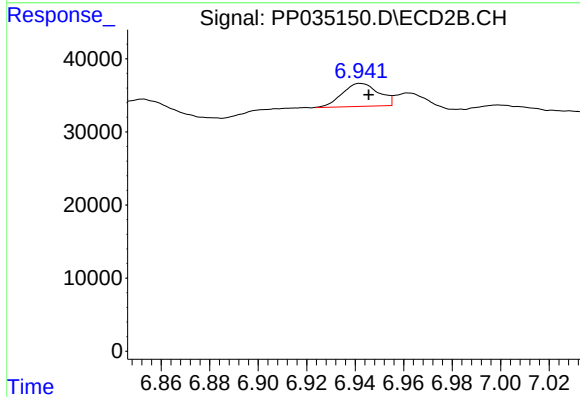


#28 AR-1254-3

R.T.: 6.941 min
Delta R.T.: -0.004 min
Response: 32766
Conc: 15.41 ng/ml m

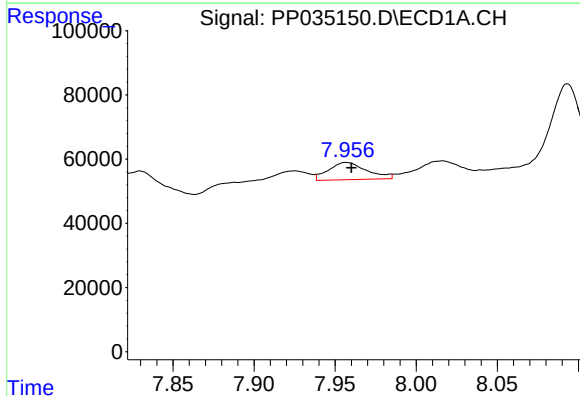


#29 AR-1254-4

R.T.: 7.956 min
Delta R.T.: -0.004 min
Response: 87411
Conc: 41.74 ng/ml m

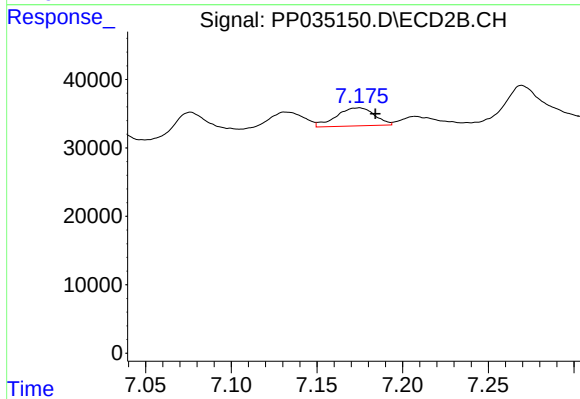

#29 AR-1254-4

R.T.: 7.175 min
Delta R.T.: -0.010 min
Response: 40987
Conc: 45.74 ng/ml

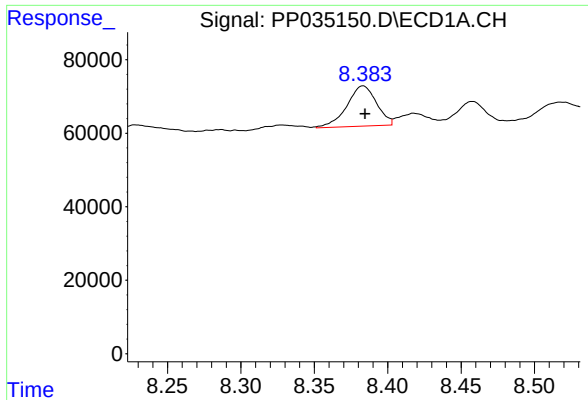


#30 AR-1254-5

R.T.: 8.383 min
Delta R.T.: -0.002 min
Response: 154999
Conc: 53.28 ng/ml m

Instrument :
ECD_P
ClientSampleId :
SB-19-14.5-15.0RE

Manual Integrations
APPROVED

Ankita
4/23/2021 4:44:27 PM

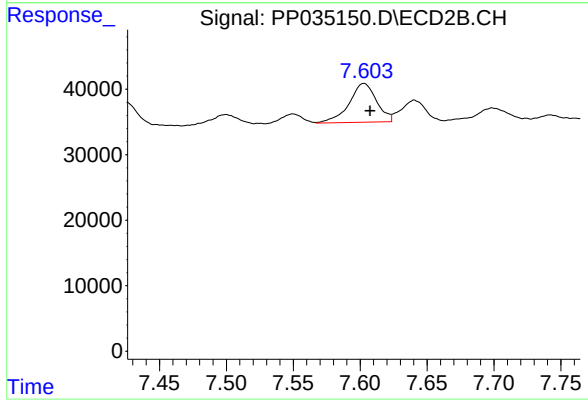

#30 AR-1254-5

R.T.: 7.603 min
Delta R.T.: -0.005 min
Response: 84814
Conc: 47.72 ng/ml