

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042221\
 Data File : PP035152.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Apr 2021 15:48
 Operator : DD\AJ
 Sample : M2077-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SB-20-14.5-15.0-DUP

Manual Integrations
 APPROVED

Ankita
 4/23/2021 4:44:32 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 22 18:12:39 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 21 17:37:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.837	4.250	1685362	1040547	20.683	20.206
2) SA Decachlor...	10.747	9.539	1888893	705763	29.891	29.704

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042221\
Data File : PP035152.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Apr 2021 15:48
Operator : DD\AJ
Sample : M2077-05
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
SB-20-14.5-15.0-DUP


Manual Integrations
APPROVED

Ankita
4/23/2021 4:44:32 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 18:12:39 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 21 17:37:28 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

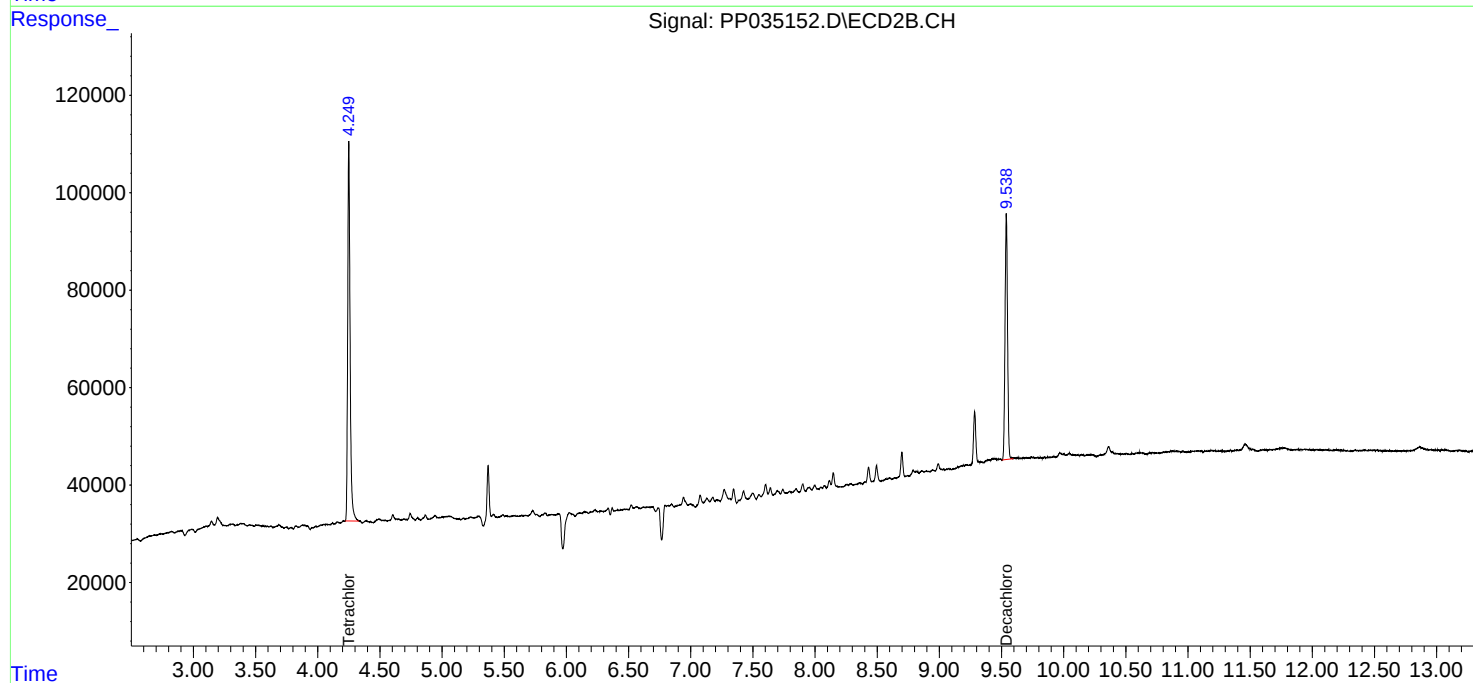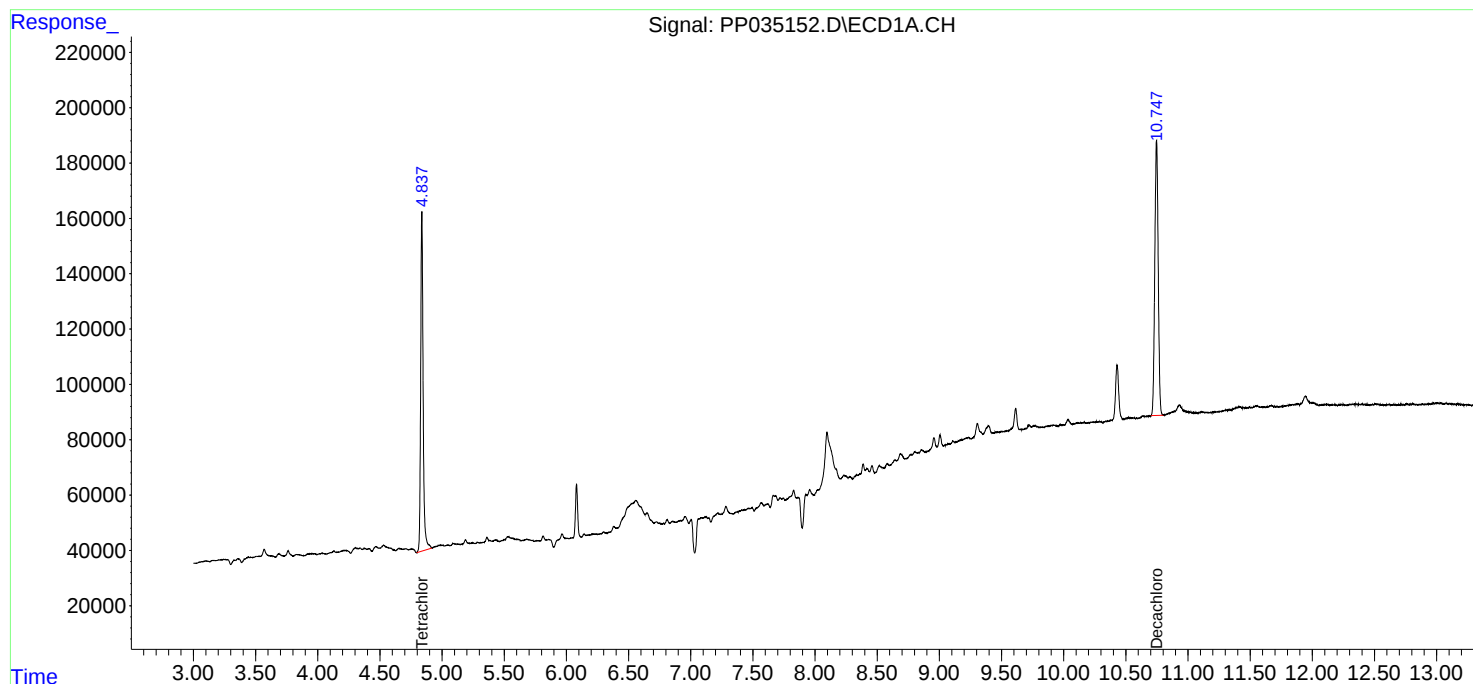

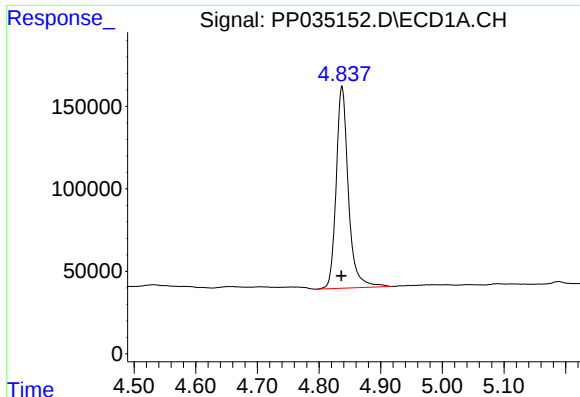


#1 Tetrachloro-m-xylene

R.T.: 4.837 min
Delta R.T.: 0.001 min
Response: 1685362
Conc: 20.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-20-14.5-15.0-DUP


Manual Integrations
APPROVED

Ankita
4/23/2021 4:44:32 PM

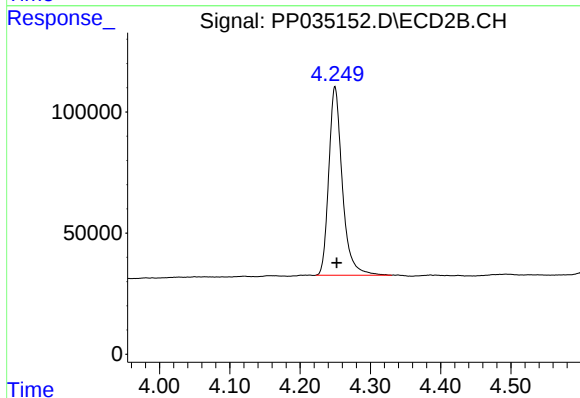


#1 Tetrachloro-m-xylene

R.T.: 4.250 min
Delta R.T.: -0.002 min
Response: 1040547
Conc: 20.21 ng/ml

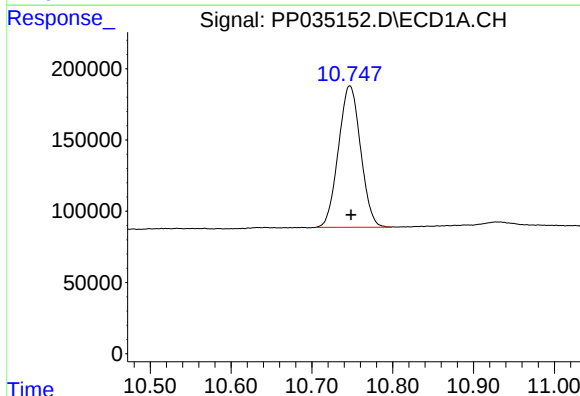

#2 Decachlorobiphenyl

R.T.: 10.747 min
Delta R.T.: -0.002 min
Response: 1888893
Conc: 29.89 ng/ml

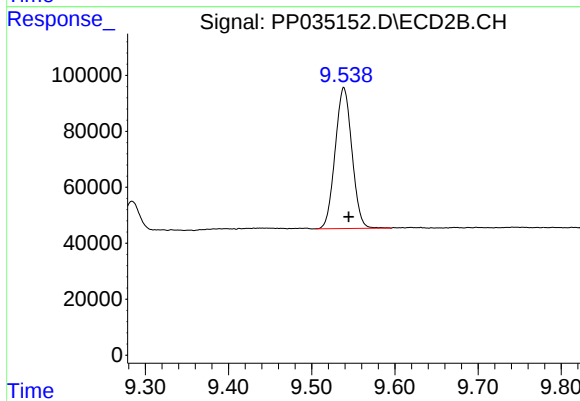

#2 Decachlorobiphenyl

R.T.: 9.539 min
Delta R.T.: -0.006 min
Response: 705763
Conc: 29.70 ng/ml