

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042221\
 Data File : PP035161.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Apr 2021 18:20
 Operator : DD\AJ
 Sample : M2106-09
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SB-24-14.5-15.0

Manual Integrations
 APPROVED

Ankita
 4/23/2021 4:44:36 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 22 18:47:40 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 21 17:37:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.838	4.249	1132093	719603	13.893	13.974
2) SA Decachlor...	10.747	9.539	1484812	566155	23.496	23.828
Target Compounds						
31) L7 AR-1260-1	7.826	7.075	63644	40648	18.898m	23.233
32) L7 AR-1260-2	8.094	7.269	307607	73265	90.355	41.099 #
33) L7 AR-1260-3	8.458	7.425	77760	38789	30.980	21.512 #
34) L7 AR-1260-4	8.688	7.902	83651	30630	28.499m	24.063
35) L7 AR-1260-5	9.005	8.147	119668	64860	24.325	26.677

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042221\
Data File : PP035161.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Apr 2021 18:20
Operator : DD\AJ
Sample : M2106-09
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
SB-24-14.5-15.0


Manual Integrations
APPROVED

Ankita
4/23/2021 4:44:36 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 18:47:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 21 17:37:28 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

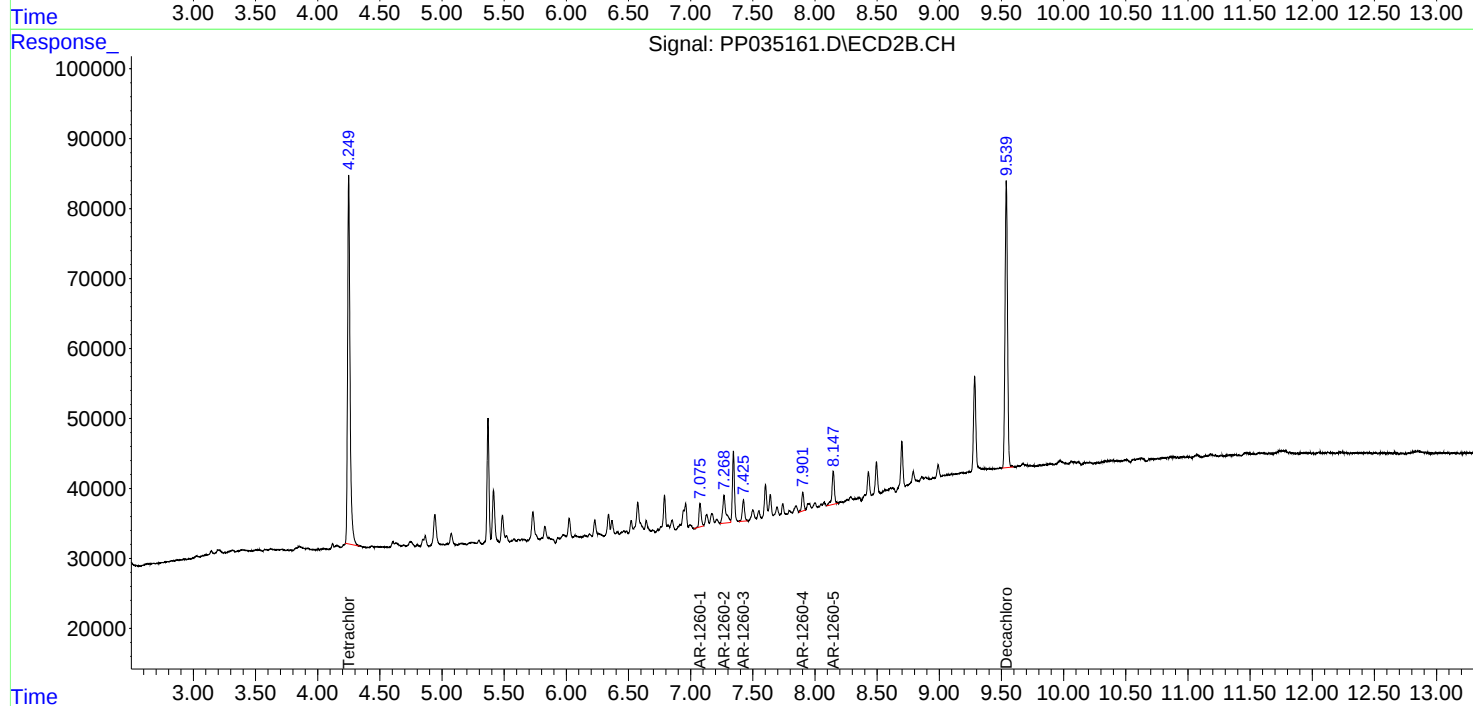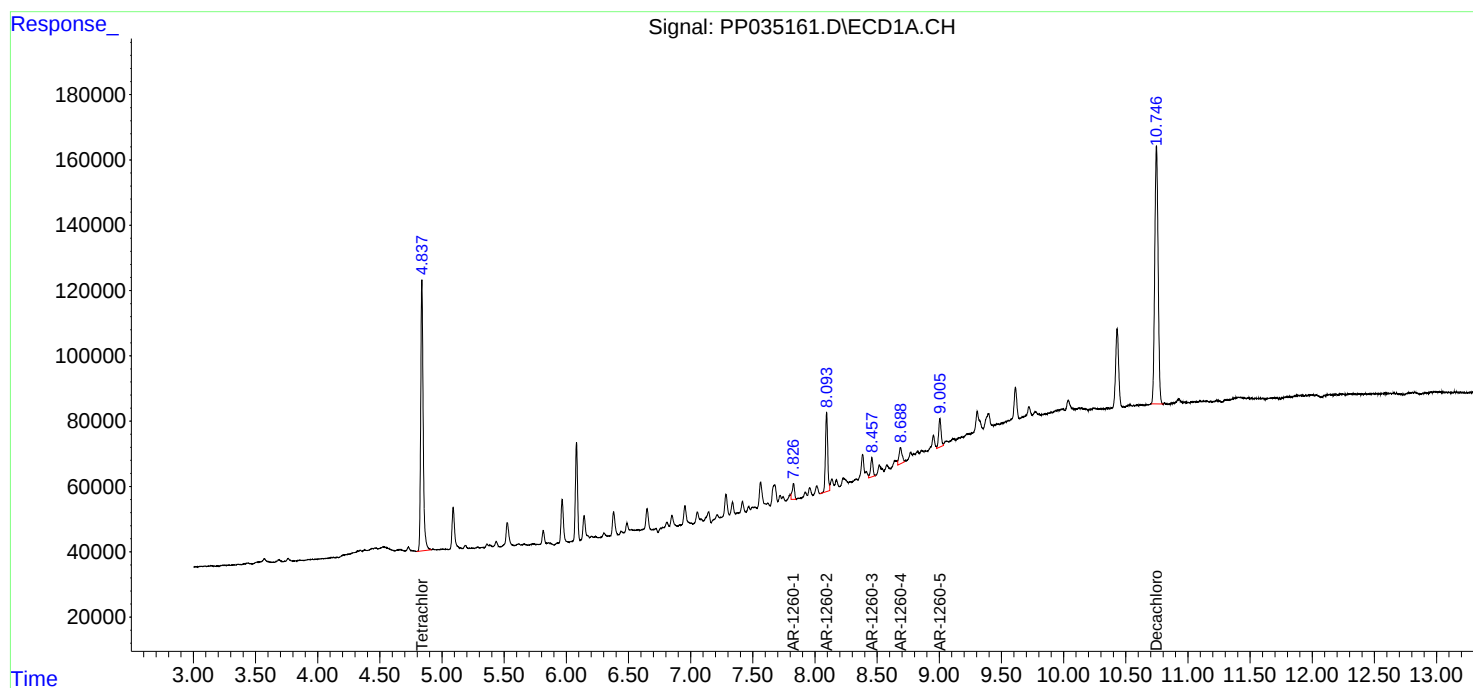

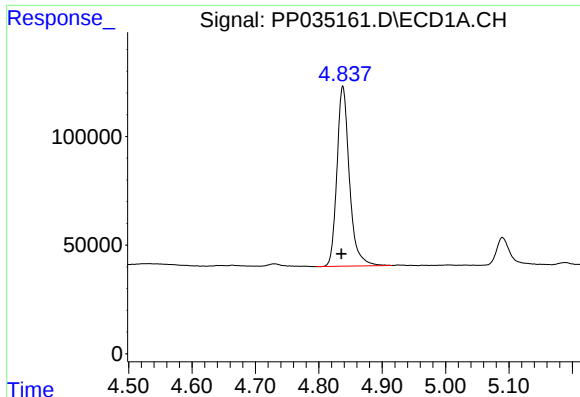


#1 Tetrachloro-m-xylene

R.T.: 4.838 min
Delta R.T.: 0.002 min
Response: 1132093
Conc: 13.89 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-24-14.5-15.0


Manual Integrations
APPROVED

Ankita
4/23/2021 4:44:36 PM

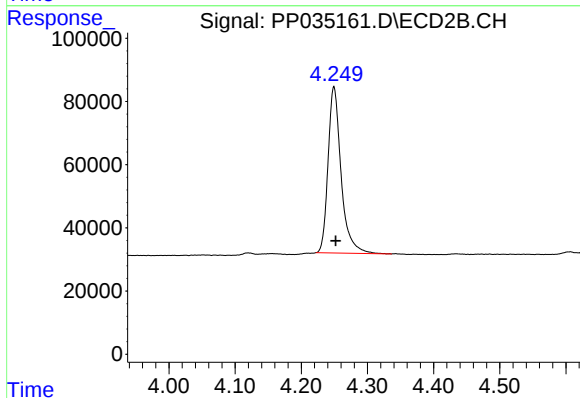


#1 Tetrachloro-m-xylene

R.T.: 4.249 min
Delta R.T.: -0.003 min
Response: 719603
Conc: 13.97 ng/ml

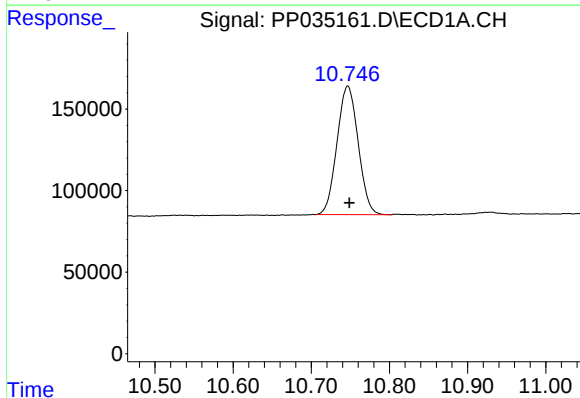


#2 Decachlorobiphenyl

R.T.: 10.747 min
Delta R.T.: -0.002 min
Response: 1484812
Conc: 23.50 ng/ml

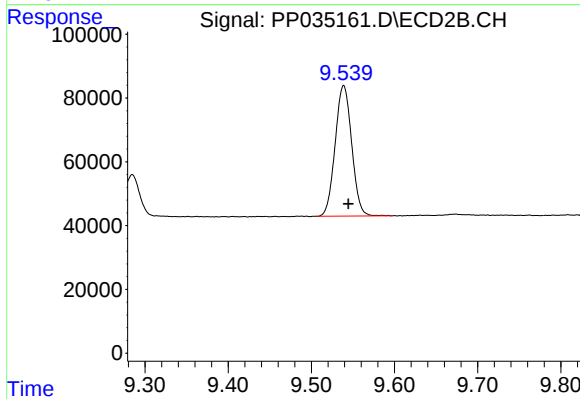

#2 Decachlorobiphenyl

R.T.: 9.539 min
Delta R.T.: -0.006 min
Response: 566155
Conc: 23.83 ng/ml

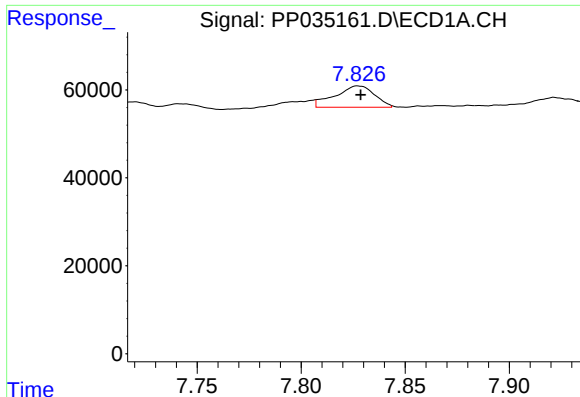


#31 AR-1260-1

R.T.: 7.826 min
Delta R.T.: -0.002 min
Response: 63644
Conc: 18.90 ng/ml m

Instrument :
ECD_P
ClientSampleId :
SB-24-14.5-15.0


Manual Integrations
APPROVED

Ankita
4/23/2021 4:44:36 PM

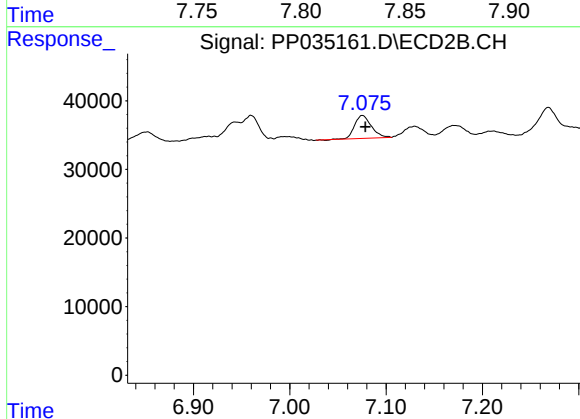


#31 AR-1260-1

R.T.: 7.075 min
Delta R.T.: -0.003 min
Response: 40648
Conc: 23.23 ng/ml

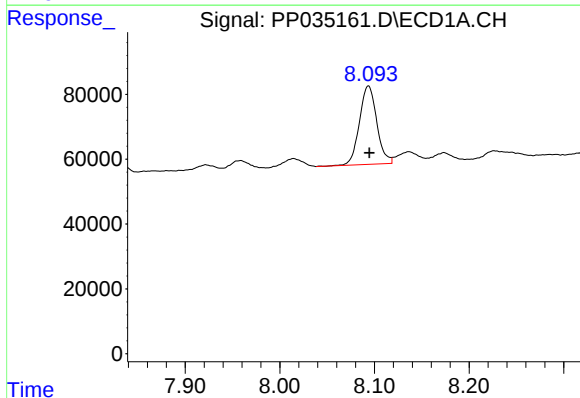


#32 AR-1260-2

R.T.: 8.094 min
Delta R.T.: 0.000 min
Response: 307607
Conc: 90.35 ng/ml

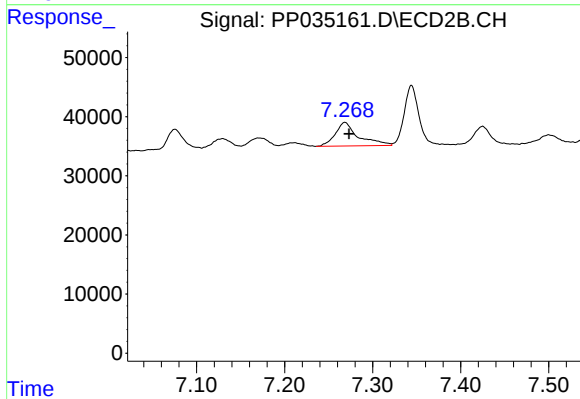

#32 AR-1260-2

R.T.: 7.269 min
Delta R.T.: -0.005 min
Response: 73265
Conc: 41.10 ng/ml

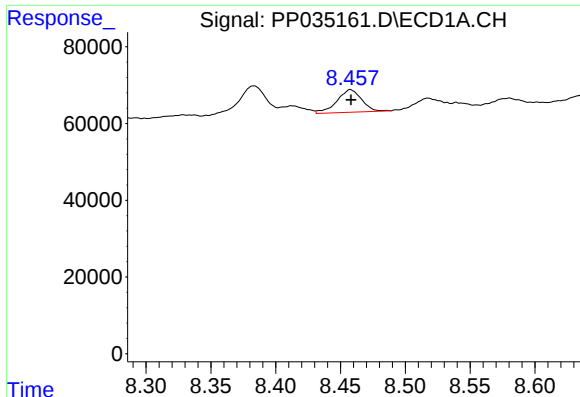


#33 AR-1260-3

R.T.: 8.458 min
Delta R.T.: 0.000 min
Response: 77760
Conc: 30.98 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-24-14.5-15.0


Manual Integrations
APPROVED

Ankita
4/23/2021 4:44:36 PM

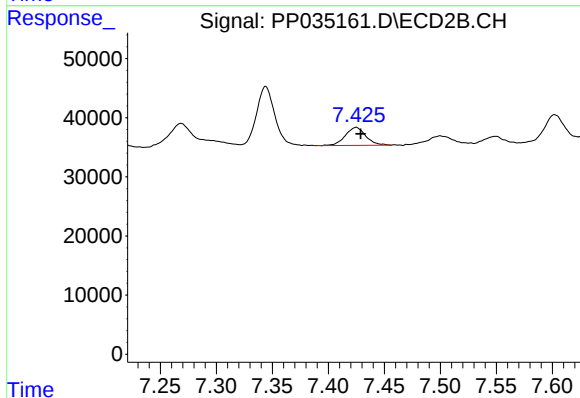


#33 AR-1260-3

R.T.: 7.425 min
Delta R.T.: -0.004 min
Response: 38789
Conc: 21.51 ng/ml

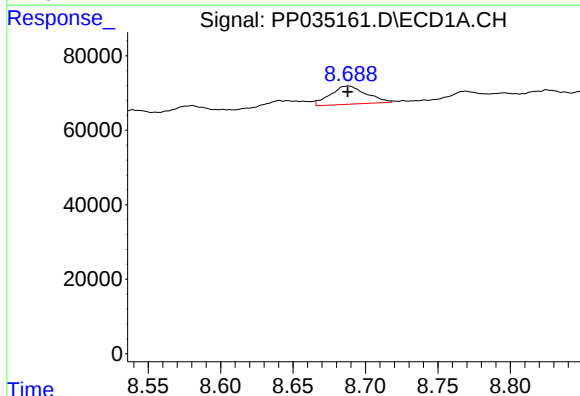


#34 AR-1260-4

R.T.: 8.688 min
Delta R.T.: 0.000 min
Response: 83651
Conc: 28.50 ng/ml m

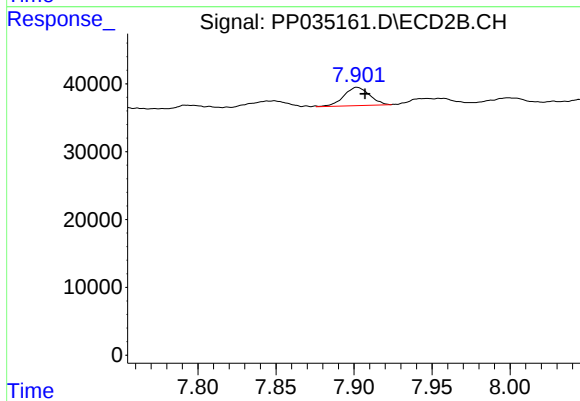

#34 AR-1260-4

R.T.: 7.902 min
Delta R.T.: -0.005 min
Response: 30630
Conc: 24.06 ng/ml

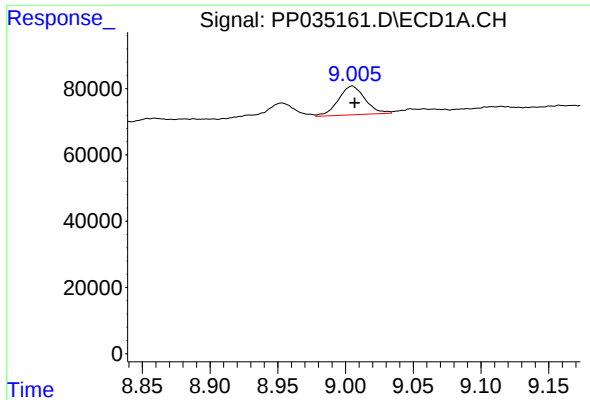


#35 AR-1260-5

R.T.: 9.005 min
Delta R.T.: -0.002 min
Response: 119668
Conc: 24.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-24-14.5-15.0

Manual Integrations
APPROVED

Ankita
4/23/2021 4:44:36 PM

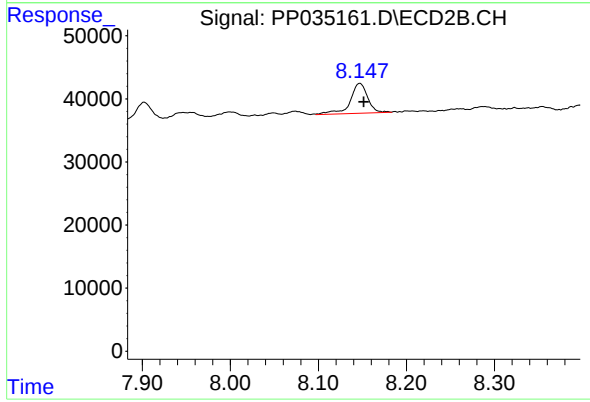

#35 AR-1260-5

R.T.: 8.147 min
Delta R.T.: -0.005 min
Response: 64860
Conc: 26.68 ng/ml