

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042221\
 Data File : PP035163.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Apr 2021 18:54
 Operator : DD\AJ
 Sample : M2106-12
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SB-25-9.5-10.0

Manual Integrations
 APPROVED

Ankita
 4/23/2021 4:44:39 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 22 19:09:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 21 17:37:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.838	4.249	1699890	1095910	20.861	21.281
2) SA Decachlor...	10.747	9.538	1603620	619762	25.376	26.084
Target Compounds						
31) L7 AR-1260-1	7.828	7.074	53590	29741	15.913	16.999
32) L7 AR-1260-2	8.093	7.270	156512	37626	45.973	21.107 #
33) L7 AR-1260-3	8.457	7.425	40379	31498	16.087	17.469
34) L7 AR-1260-4	8.686	7.902	94826	15806	32.306	12.417m#
35) L7 AR-1260-5	9.006	8.147	97840	42221	19.888	17.366

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042221\
Data File : PP035163.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Apr 2021 18:54
Operator : DD\AJ
Sample : M2106-12
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
SB-25-9.5-10.0


Manual Integrations
APPROVED

Ankita
4/23/2021 4:44:39 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 19:09:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 21 17:37:28 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

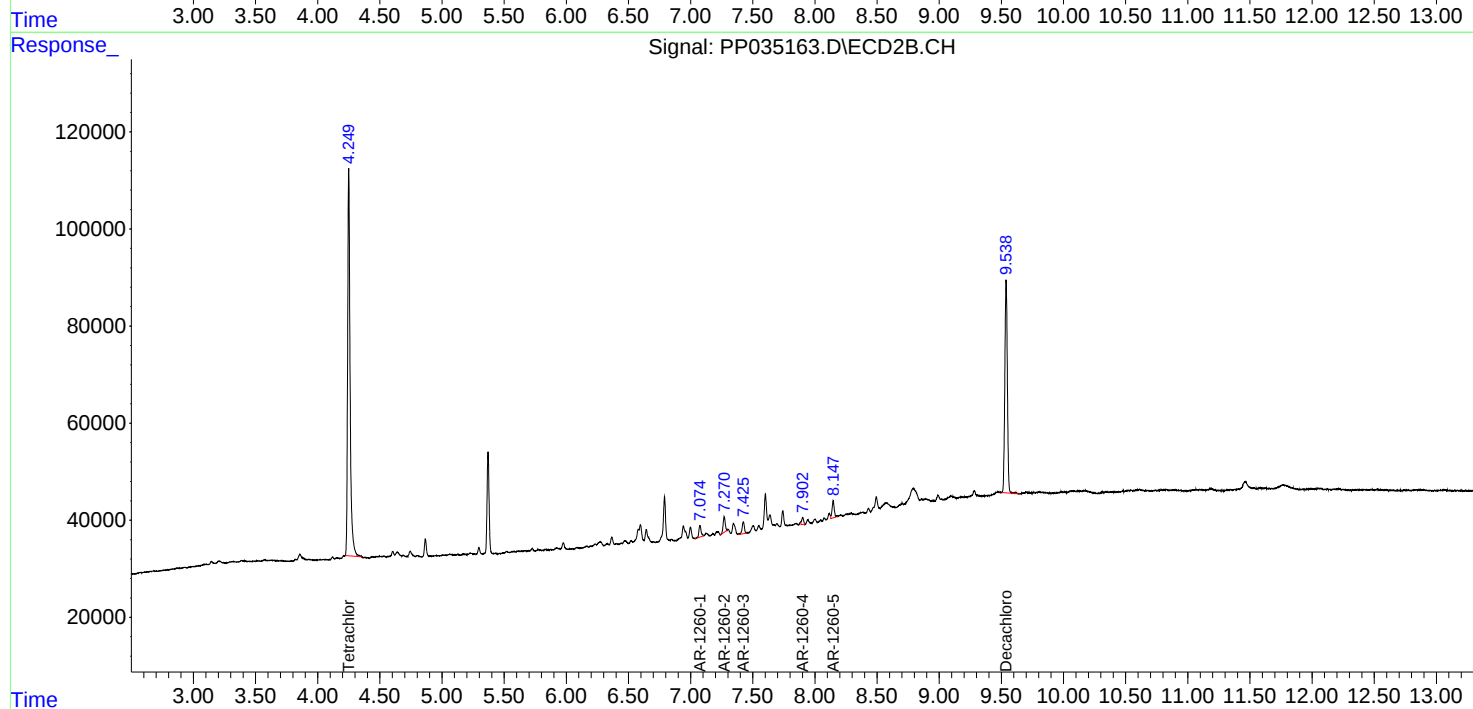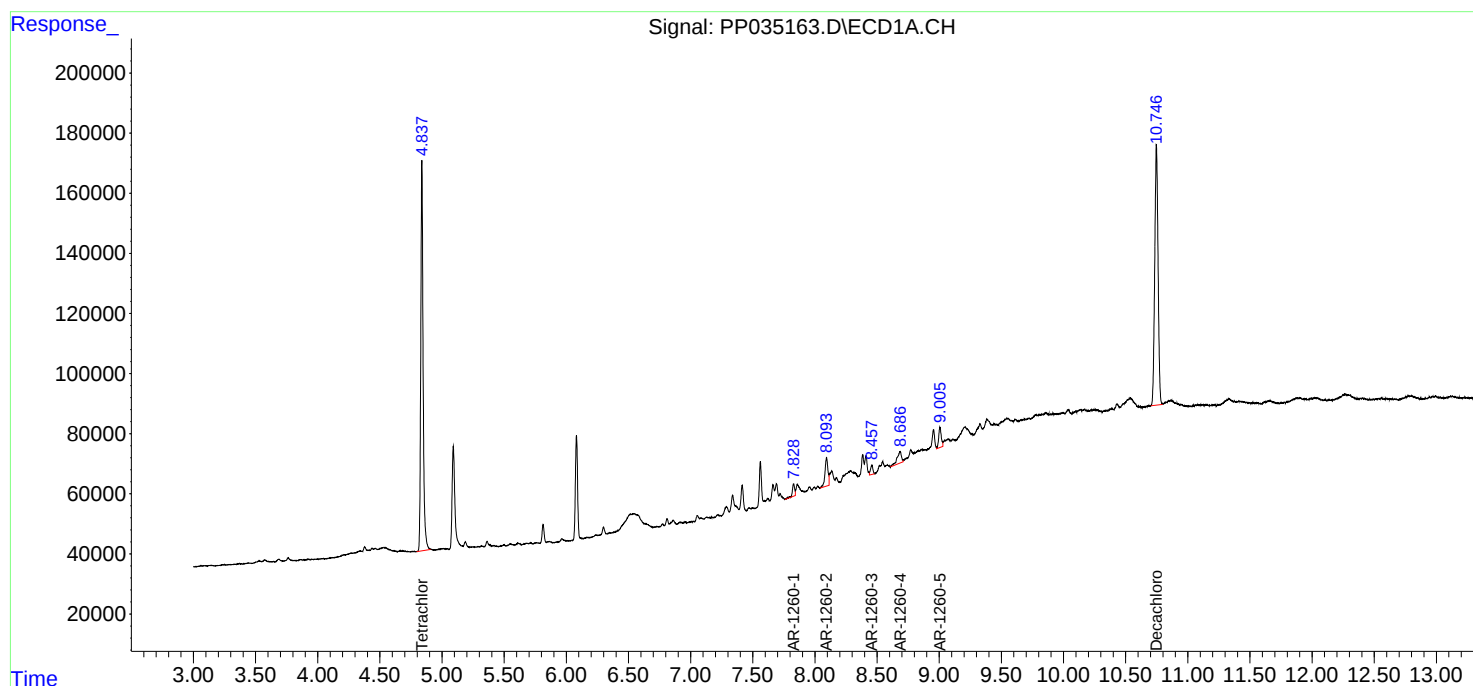

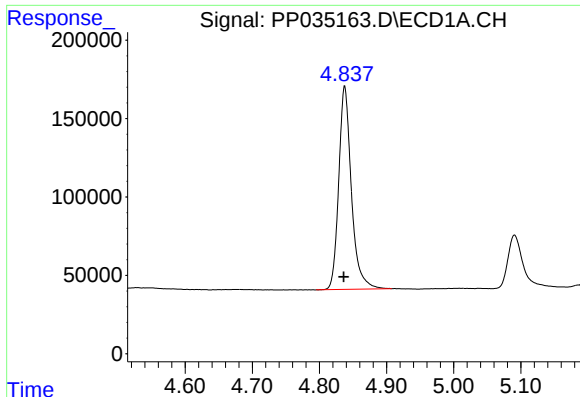


#1 Tetrachloro-m-xylene

R.T.: 4.838 min
Delta R.T.: 0.002 min
Response: 1699890
Conc: 20.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-25-9.5-10.0


Manual Integrations
APPROVED

Ankita
4/23/2021 4:44:39 PM

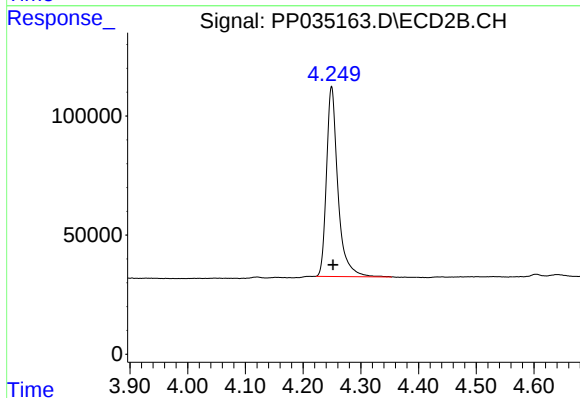


#1 Tetrachloro-m-xylene

R.T.: 4.249 min
Delta R.T.: -0.003 min
Response: 1095910
Conc: 21.28 ng/ml

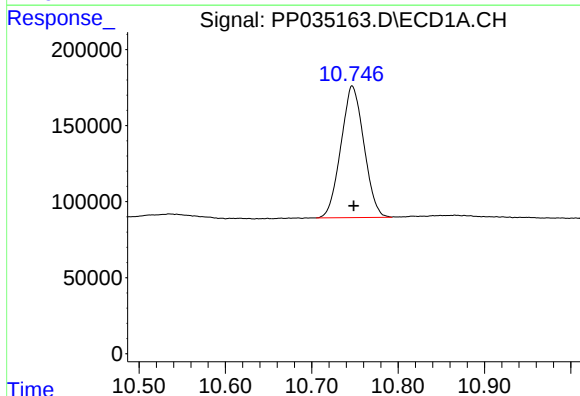


#2 Decachlorobiphenyl

R.T.: 10.747 min
Delta R.T.: -0.002 min
Response: 1603620
Conc: 25.38 ng/ml

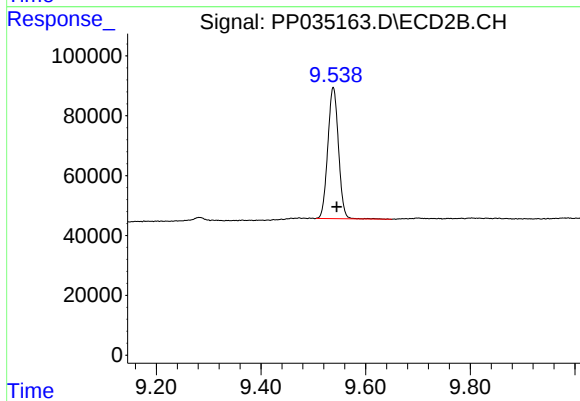

#2 Decachlorobiphenyl

R.T.: 9.538 min
Delta R.T.: -0.006 min
Response: 619762
Conc: 26.08 ng/ml

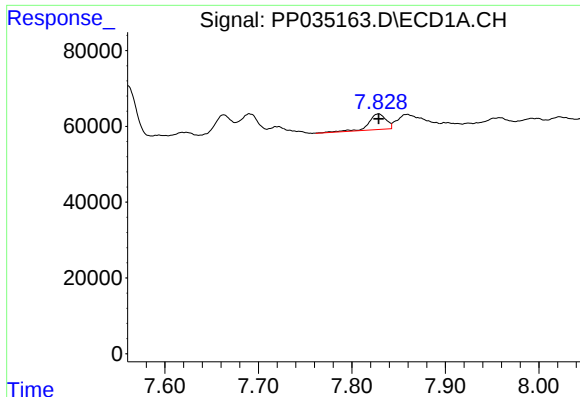


#31 AR-1260-1

R.T.: 7.828 min
Delta R.T.: 0.000 min
Response: 53590
Conc: 15.91 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-25-9.5-10.0


Manual Integrations
APPROVED

Ankita
4/23/2021 4:44:39 PM

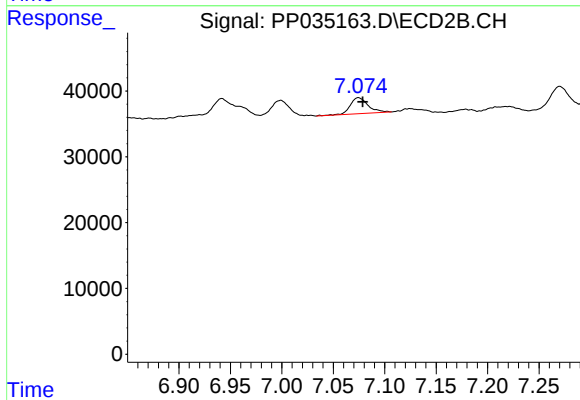


#31 AR-1260-1

R.T.: 7.074 min
Delta R.T.: -0.004 min
Response: 29741
Conc: 17.00 ng/ml

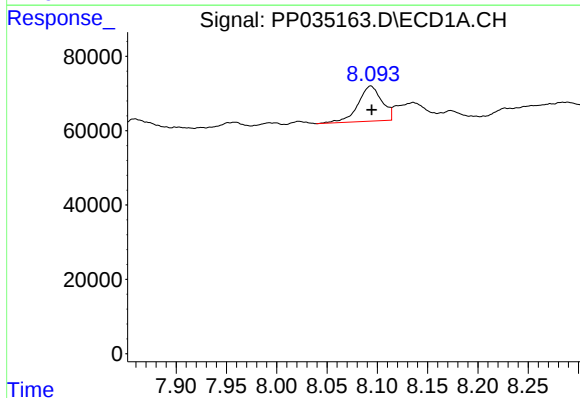


#32 AR-1260-2

R.T.: 8.093 min
Delta R.T.: -0.001 min
Response: 156512
Conc: 45.97 ng/ml

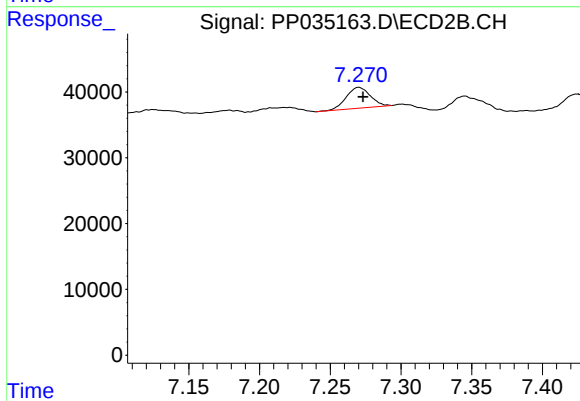

#32 AR-1260-2

R.T.: 7.270 min
Delta R.T.: -0.003 min
Response: 37626
Conc: 21.11 ng/ml

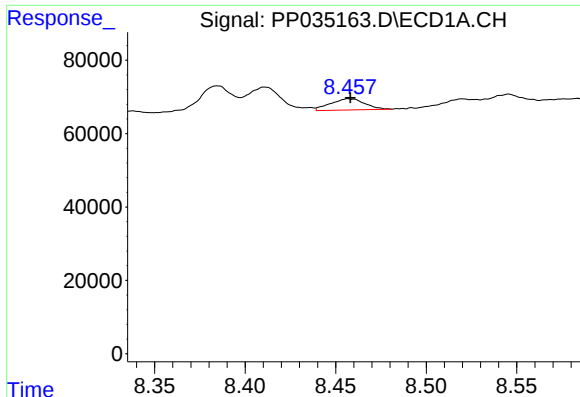


#33 AR-1260-3

R.T.: 8.457 min
Delta R.T.: -0.001 min
Response: 40379
Conc: 16.09 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-25-9.5-10.0


Manual Integrations
APPROVED

Ankita
4/23/2021 4:44:39 PM

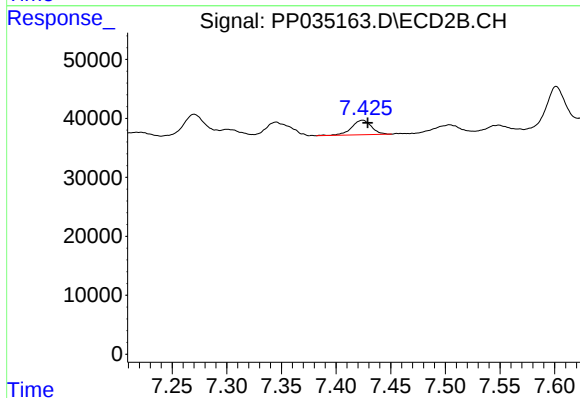


#33 AR-1260-3

R.T.: 7.425 min
Delta R.T.: -0.004 min
Response: 31498
Conc: 17.47 ng/ml

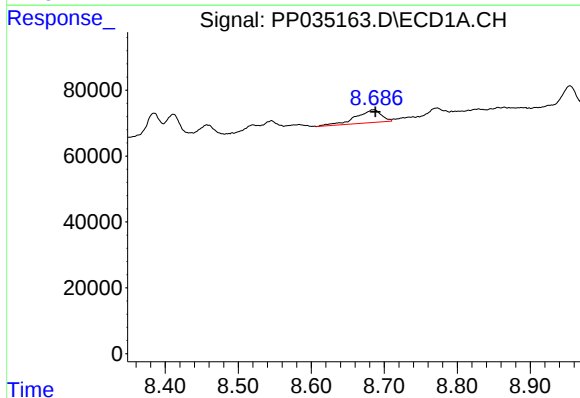


#34 AR-1260-4

R.T.: 8.686 min
Delta R.T.: -0.002 min
Response: 94826
Conc: 32.31 ng/ml

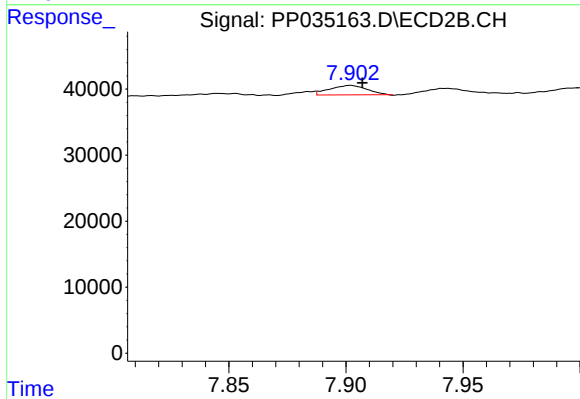

#34 AR-1260-4

R.T.: 7.902 min
Delta R.T.: -0.005 min
Response: 15806
Conc: 12.42 ng/ml m

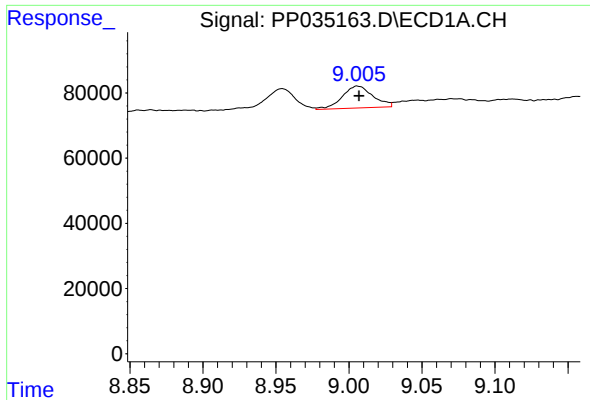


#35 AR-1260-5

R.T.: 9.006 min
Delta R.T.: 0.000 min
Response: 97840
Conc: 19.89 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-25-9.5-10.0

Manual Integrations
APPROVED

Ankita
4/23/2021 4:44:39 PM

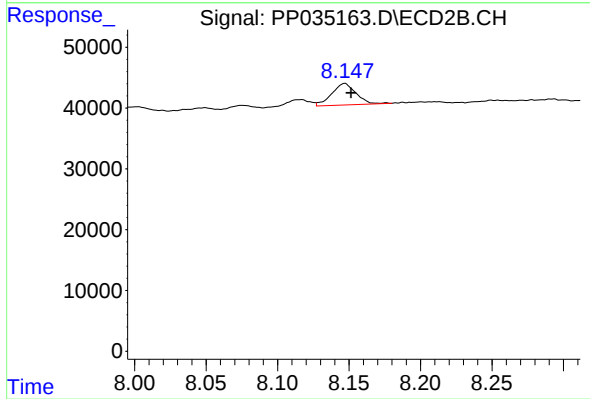

#35 AR-1260-5

R.T.: 8.147 min
Delta R.T.: -0.005 min
Response: 42221
Conc: 17.37 ng/ml