

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042221\
 Data File : PP035168.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Apr 2021 20:35
 Operator : DD\AJ
 Sample : M2106-13
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SB-26-0-2.0

Manual Integrations
 APPROVED

Ankita
 4/23/2021 4:44:41 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 02:59:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 21 17:37:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.837	4.250	1724243	1093199	21.160	21.228
2)	SA Decachlor...	10.746	9.537	1541600	597947	24.395	25.166
Target Compounds							
31)	L7 AR-1260-1	7.826	7.074	92719	58726	27.532m	33.566
32)	L7 AR-1260-2	8.091	7.268	281734	74112	82.755	41.575 #
33)	L7 AR-1260-3	8.457	7.424	111477	64651	44.413	35.855
34)	L7 AR-1260-4	8.684	7.902	122628	47025	41.777m	36.943
35)	L7 AR-1260-5	9.005	8.146	181230	116765	36.838	48.026 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042221\
Data File : PP035168.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Apr 2021 20:35
Operator : DD\AJ
Sample : M2106-13
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
SB-26-0-2.0


Manual Integrations
APPROVED

Ankita
4/23/2021 4:44:41 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 02:59:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 21 17:37:28 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

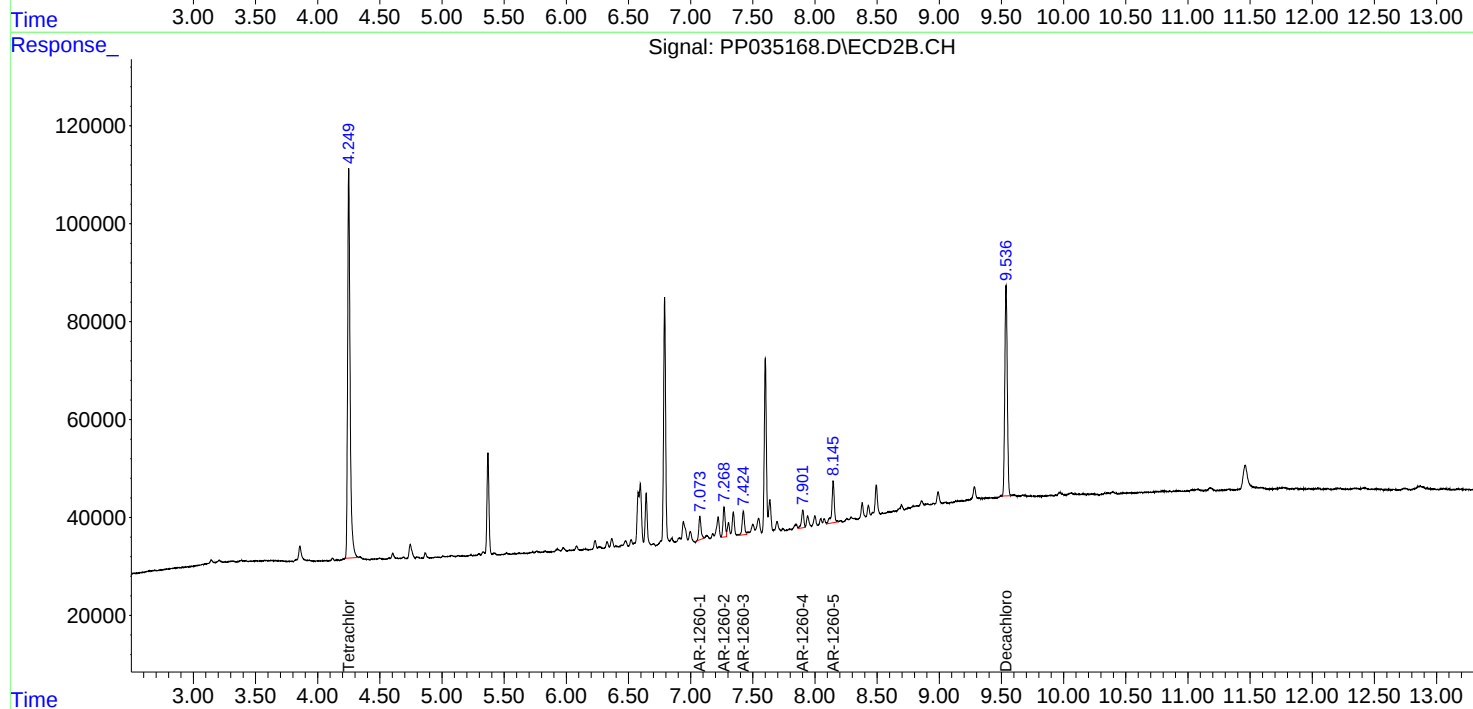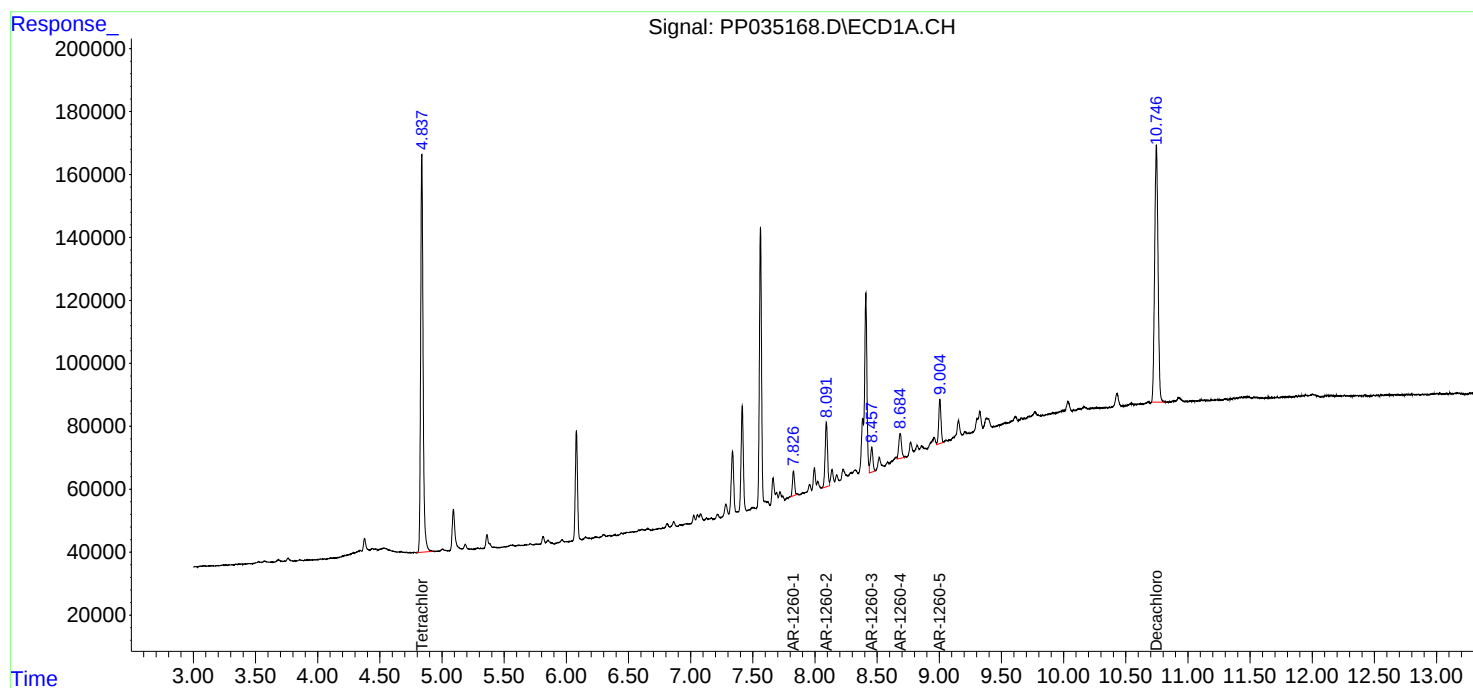

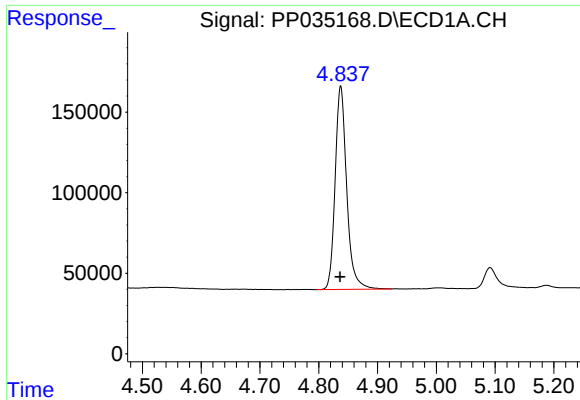


#1 Tetrachloro-m-xylene

R.T.: 4.837 min
Delta R.T.: 0.001 min
Response: 1724243
Conc: 21.16 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-26-0-2.0


Manual Integrations
APPROVED

Ankita
4/23/2021 4:44:41 PM

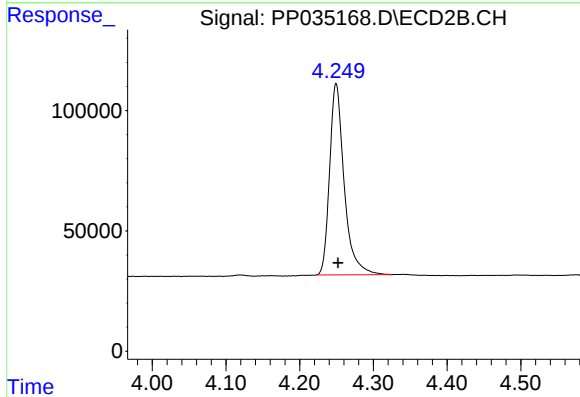


#1 Tetrachloro-m-xylene

R.T.: 4.250 min
Delta R.T.: -0.003 min
Response: 1093199
Conc: 21.23 ng/ml

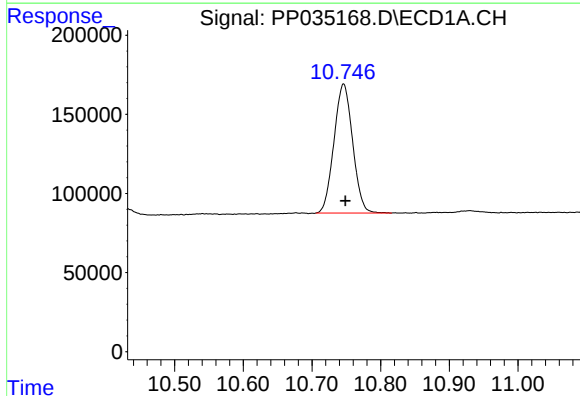


#2 Decachlorobiphenyl

R.T.: 10.746 min
Delta R.T.: -0.002 min
Response: 1541600
Conc: 24.40 ng/ml

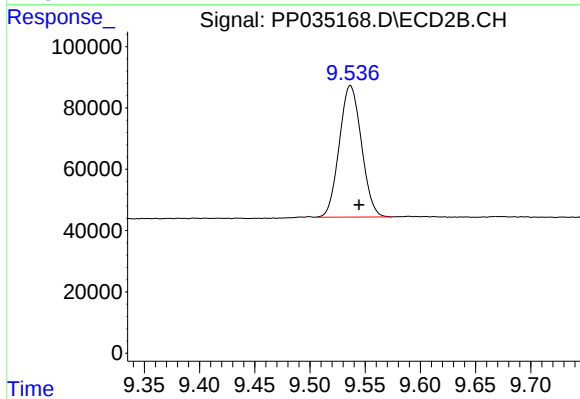

#2 Decachlorobiphenyl

R.T.: 9.537 min
Delta R.T.: -0.008 min
Response: 597947
Conc: 25.17 ng/ml

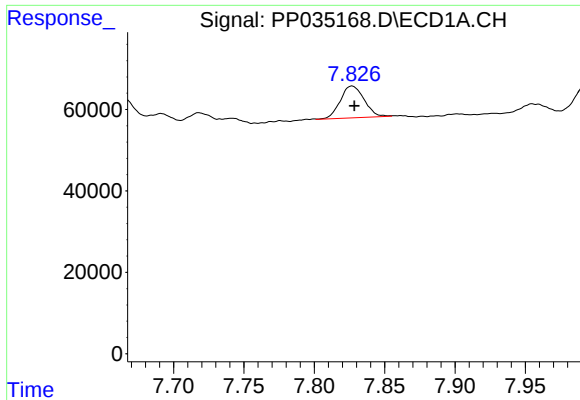


#31 AR-1260-1

R.T.: 7.826 min
Delta R.T.: -0.002 min
Response: 92719
Conc: 27.53 ng/ml m

Instrument :
ECD_P
ClientSampleId :
SB-26-0-2.0


Manual Integrations
APPROVED

Ankita
4/23/2021 4:44:41 PM

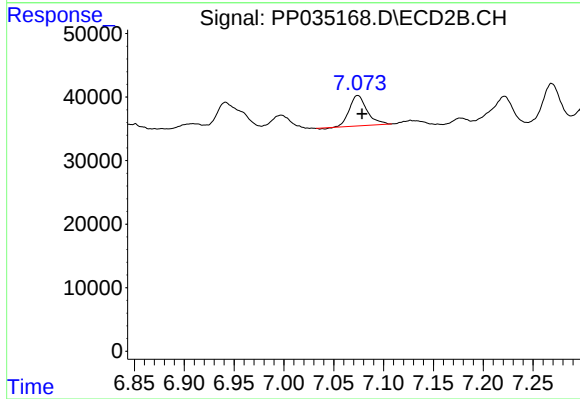


#31 AR-1260-1

R.T.: 7.074 min
Delta R.T.: -0.005 min
Response: 58726
Conc: 33.57 ng/ml

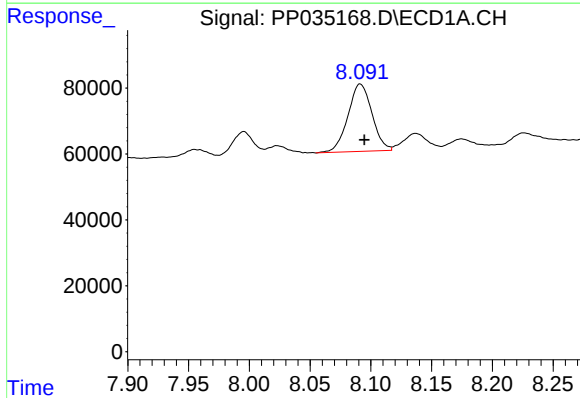


#32 AR-1260-2

R.T.: 8.091 min
Delta R.T.: -0.003 min
Response: 281734
Conc: 82.76 ng/ml

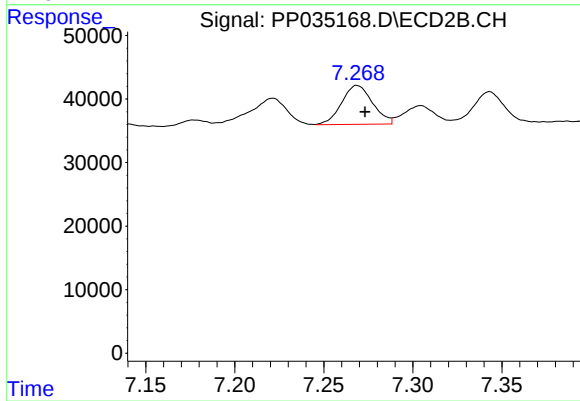

#32 AR-1260-2

R.T.: 7.268 min
Delta R.T.: -0.005 min
Response: 74112
Conc: 41.57 ng/ml

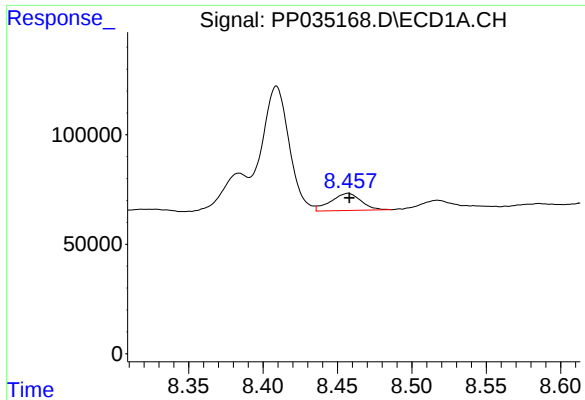


#33 AR-1260-3

R.T.: 8.457 min
Delta R.T.: 0.000 min
Response: 111477
Conc: 44.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-26-0-2.0


Manual Integrations
APPROVED

Ankita
4/23/2021 4:44:41 PM

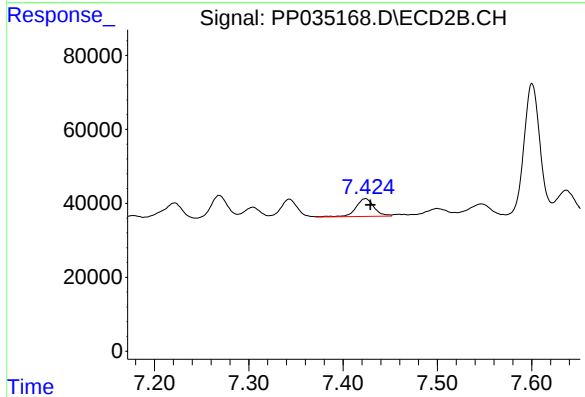


#33 AR-1260-3

R.T.: 7.424 min
Delta R.T.: -0.005 min
Response: 64651
Conc: 35.86 ng/ml

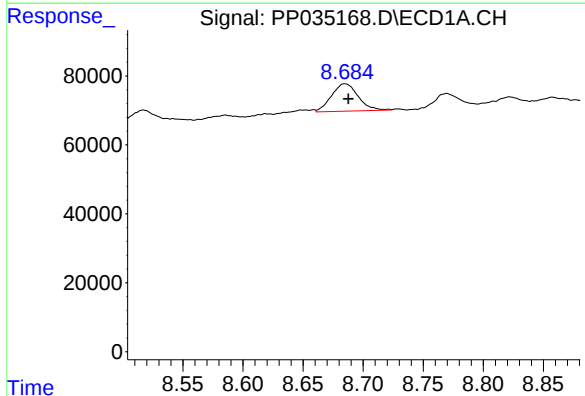


#34 AR-1260-4

R.T.: 8.684 min
Delta R.T.: -0.003 min
Response: 122628
Conc: 41.78 ng/ml m

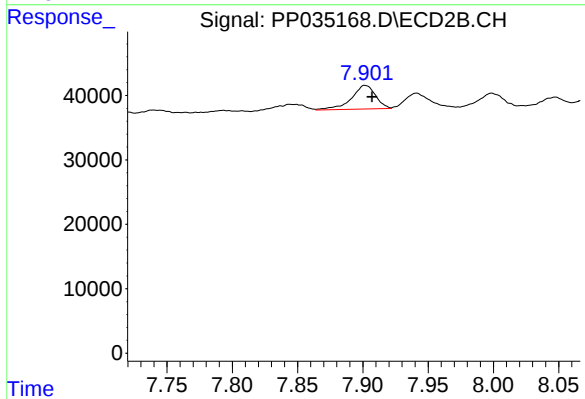

#34 AR-1260-4

R.T.: 7.902 min
Delta R.T.: -0.005 min
Response: 47025
Conc: 36.94 ng/ml

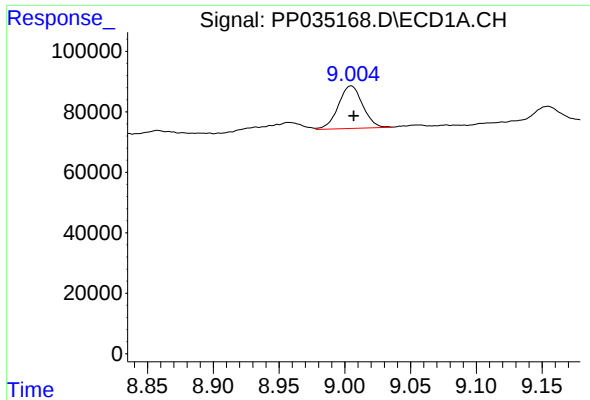


#35 AR-1260-5

R.T.: 9.005 min
Delta R.T.: -0.002 min
Response: 181230
Conc: 36.84 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-26-0-2.0

Manual Integrations
APPROVED

Ankita
4/23/2021 4:44:41 PM

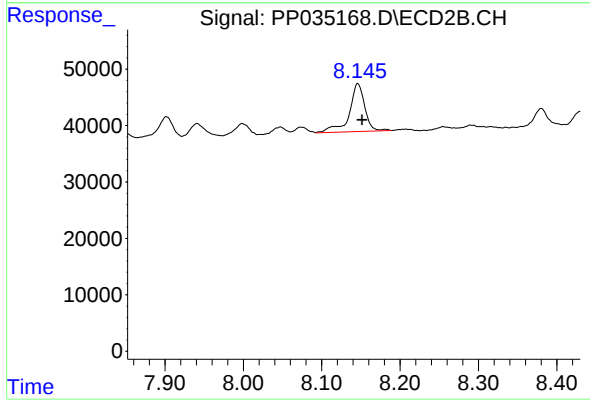

#35 AR-1260-5

R.T.: 8.146 min
Delta R.T.: -0.005 min
Response: 116765
Conc: 48.03 ng/ml