

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042221\
 Data File : PP035172.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Apr 2021 21:43
 Operator : DD\AJ
 Sample : M2106-19
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SB-28-0-2.0

Manual Integrations
 APPROVED

Ankita
 4/23/2021 4:44:43 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 03:00:57 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 21 17:37:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.837	4.249	1686945	1063468	20.702	20.651
2) SA Decachlor...	10.744	9.537	1355536	520931	21.451	21.925
Target Compounds						
31) L7 AR-1260-1	7.826	7.074	28996	16225	8.610m	9.274
32) L7 AR-1260-2	8.093	7.267	103419	21469	30.378	12.044 #
33) L7 AR-1260-3	8.457	7.417	32849	32836	13.087	18.211 #
34) L7 AR-1260-4	8.684	7.900	45550	17102	15.518m	13.435m
35) L7 AR-1260-5	9.005	8.146	60225	33193	12.242	13.653m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042221\
Data File : PP035172.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Apr 2021 21:43
Operator : DD\AJ
Sample : M2106-19
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
SB-28-0-2.0


Manual Integrations
APPROVED

Ankita
4/23/2021 4:44:43 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 03:00:57 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 21 17:37:28 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

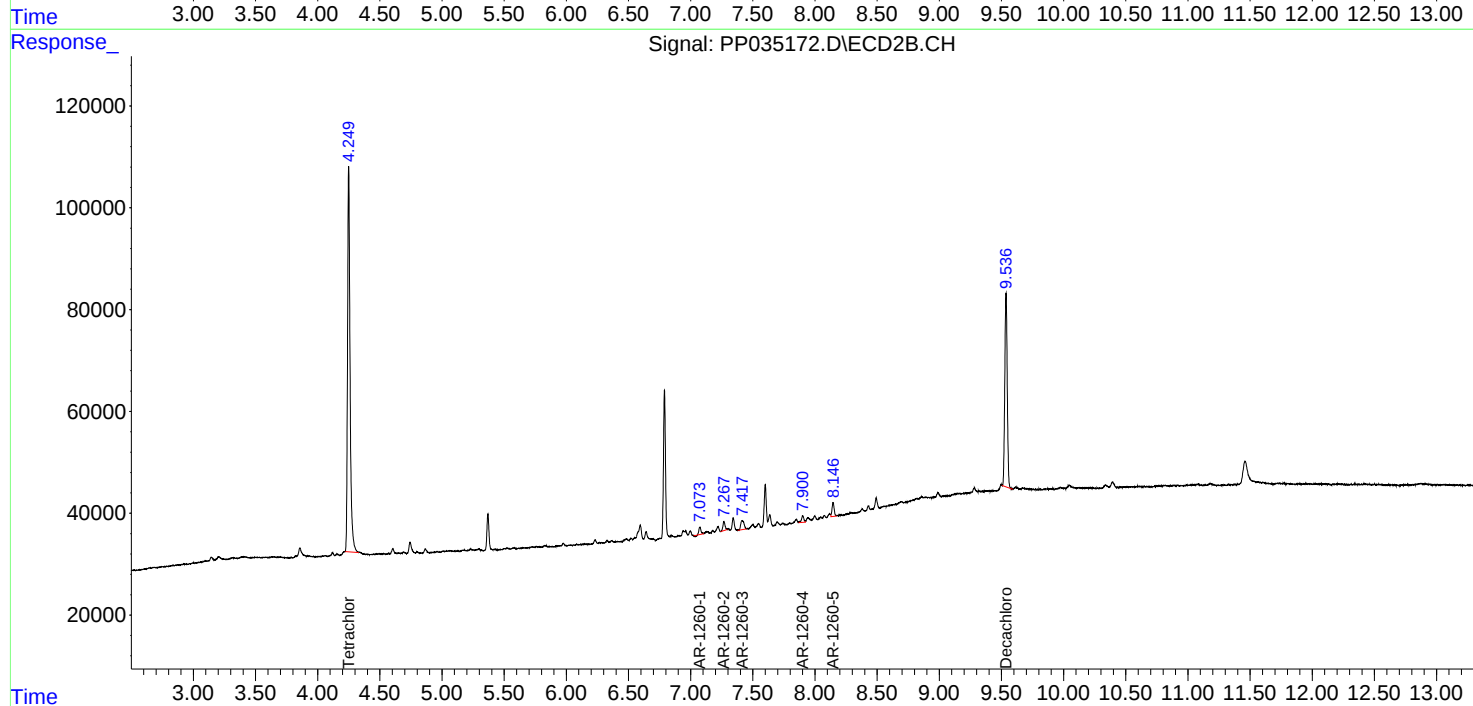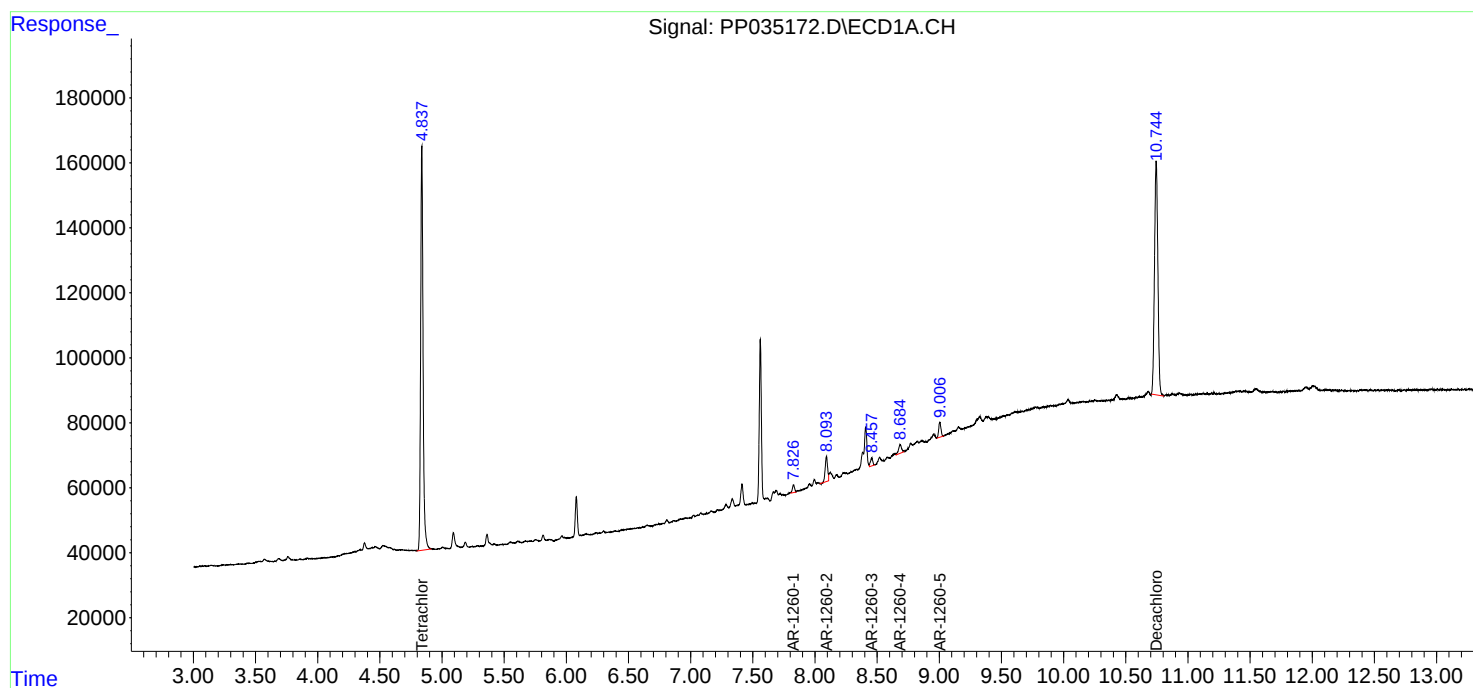

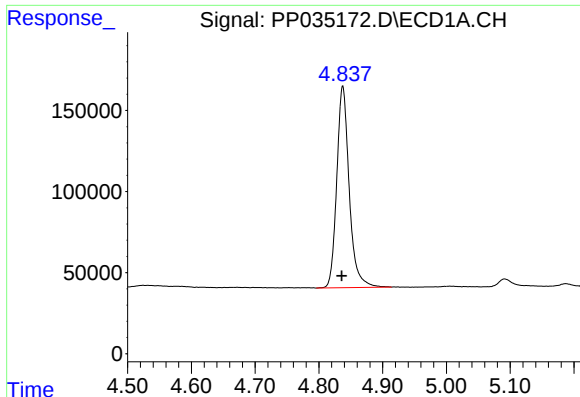


#1 Tetrachloro-m-xylene

R.T.: 4.837 min
Delta R.T.: 0.001 min
Response: 1686945
Conc: 20.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-28-0-2.0


Manual Integrations
APPROVED

Ankita
4/23/2021 4:44:43 PM

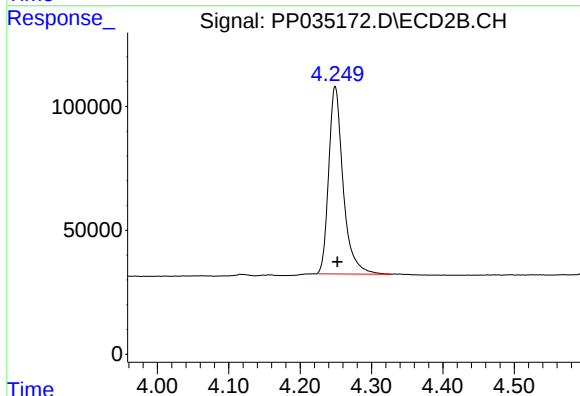


#1 Tetrachloro-m-xylene

R.T.: 4.249 min
Delta R.T.: -0.003 min
Response: 1063468
Conc: 20.65 ng/ml

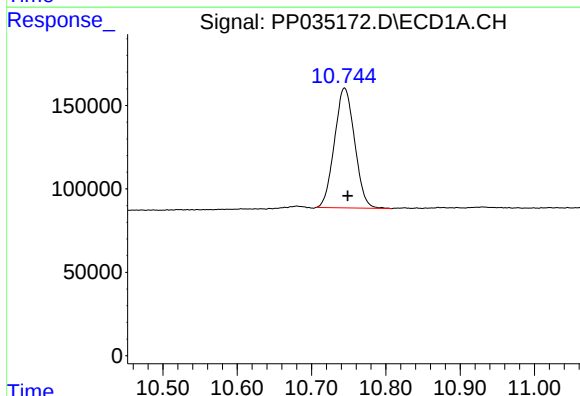


#2 Decachlorobiphenyl

R.T.: 10.744 min
Delta R.T.: -0.004 min
Response: 1355536
Conc: 21.45 ng/ml

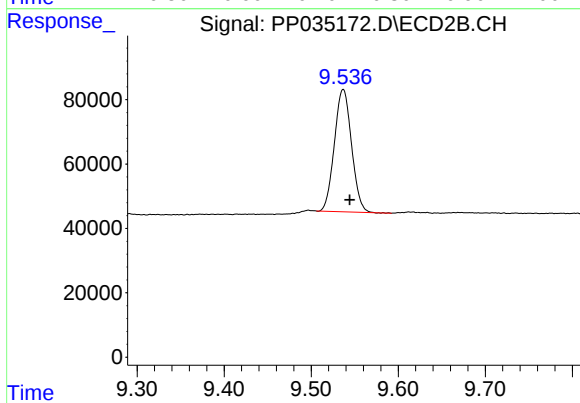

#2 Decachlorobiphenyl

R.T.: 9.537 min
Delta R.T.: -0.008 min
Response: 520931
Conc: 21.92 ng/ml

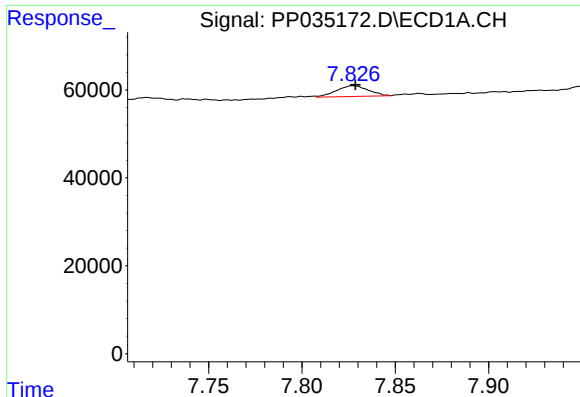


#31 AR-1260-1

R.T.: 7.826 min
Delta R.T.: -0.002 min
Response: 28996
Conc: 8.61 ng/ml m

Instrument :
ECD_P
ClientSampleId :
SB-28-0-2.0


Manual Integrations
APPROVED

Ankita
4/23/2021 4:44:43 PM

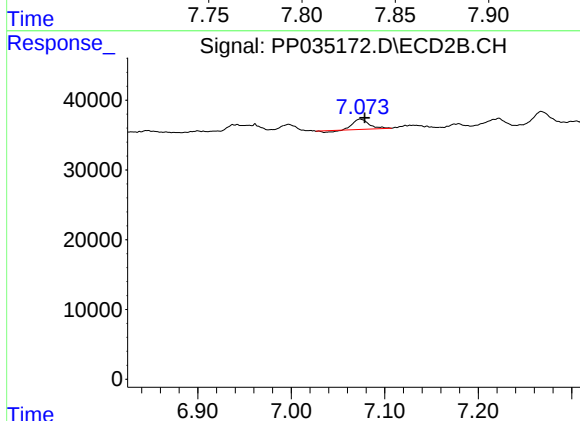


#31 AR-1260-1

R.T.: 7.074 min
Delta R.T.: -0.005 min
Response: 16225
Conc: 9.27 ng/ml

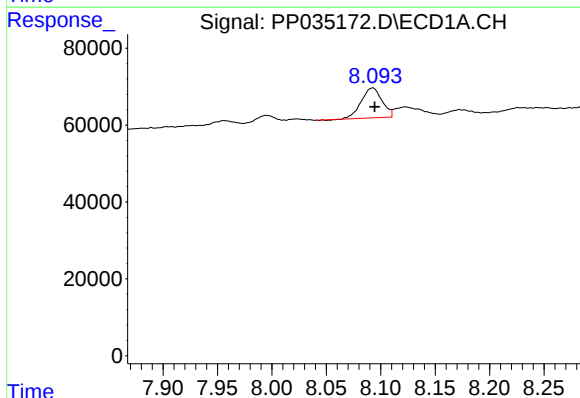


#32 AR-1260-2

R.T.: 8.093 min
Delta R.T.: -0.002 min
Response: 103419
Conc: 30.38 ng/ml

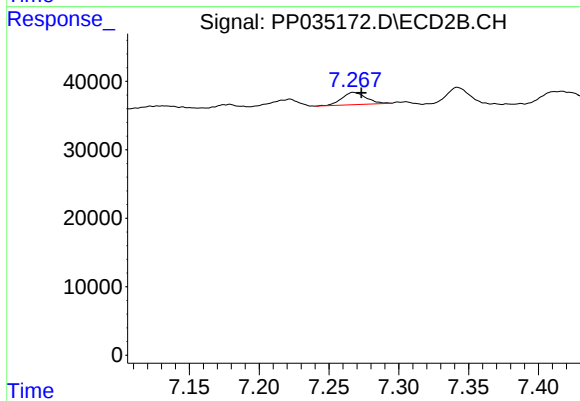

#32 AR-1260-2

R.T.: 7.267 min
Delta R.T.: -0.006 min
Response: 21469
Conc: 12.04 ng/ml

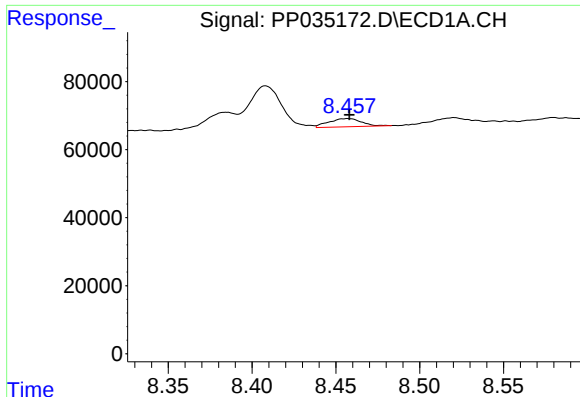


#33 AR-1260-3

R.T.: 8.457 min
Delta R.T.: 0.000 min
Response: 32849
Conc: 13.09 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-28-0-2.0


Manual Integrations
APPROVED

Ankita
4/23/2021 4:44:43 PM

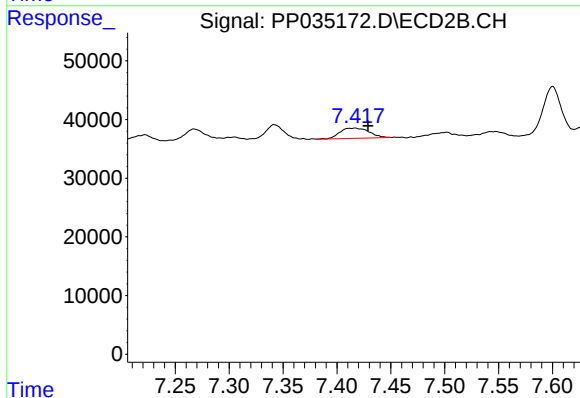


#33 AR-1260-3

R.T.: 7.417 min
Delta R.T.: -0.012 min
Response: 32836
Conc: 18.21 ng/ml

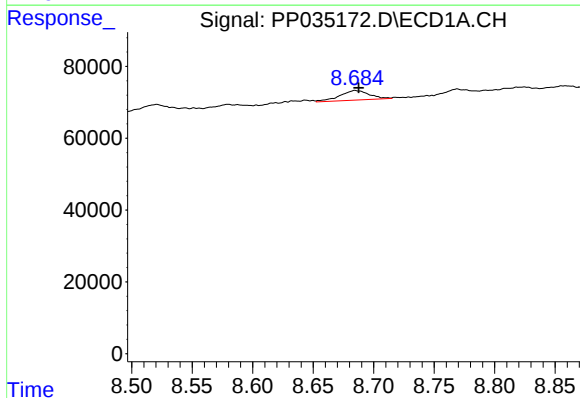


#34 AR-1260-4

R.T.: 8.684 min
Delta R.T.: -0.004 min
Response: 45550
Conc: 15.52 ng/ml m

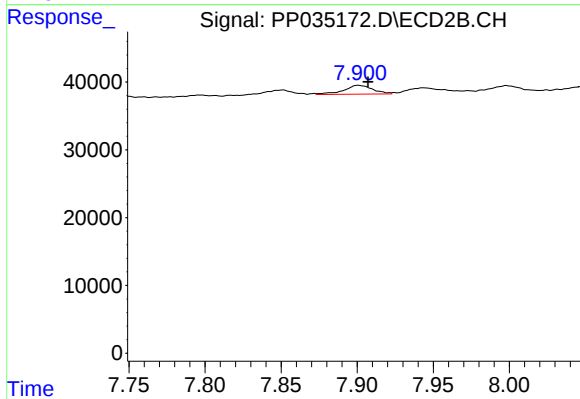

#34 AR-1260-4

R.T.: 7.900 min
Delta R.T.: -0.007 min
Response: 17102
Conc: 13.44 ng/ml m

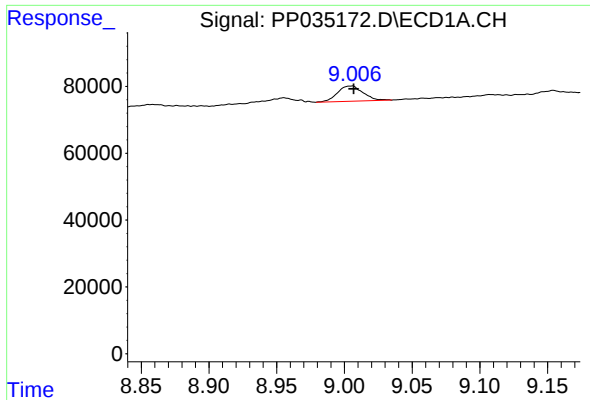


#35 AR-1260-5

R.T.: 9.005 min
Delta R.T.: -0.002 min
Response: 60225
Conc: 12.24 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-28-0-2.0

Manual Integrations
APPROVED

Ankita
4/23/2021 4:44:43 PM

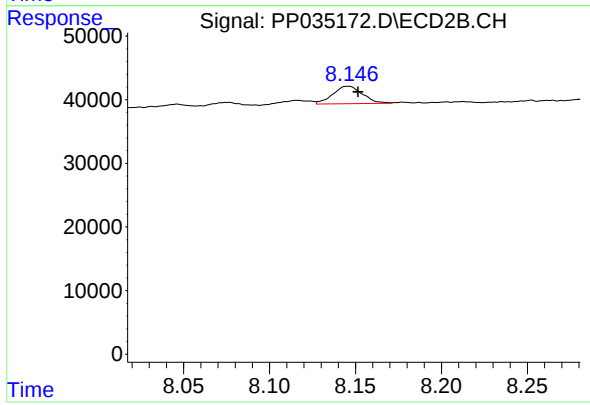

#35 AR-1260-5

R.T.: 8.146 min
Delta R.T.: -0.005 min
Response: 33193
Conc: 13.65 ng/ml m