

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042321\
 Data File : PP035231.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Apr 2021 20:27
 Operator : DD\AJ
 Sample : M2149-15
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SB-40-9.5-10.0

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 24 01:04:19 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 21 17:37:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.839	4.247	1643251	1069315	20.166	20.765
2)	SA Decachlor...	10.746	9.532	1116535	446442	17.669	18.790
Target Compounds							
8)	L2 AR-1221-1	5.090	0.000	373371	0	453.968	N.D. #
9)	L2 AR-1221-2	0.000	4.580f	0	149185	N.D.	392.444 #
28)	L6 AR-1254-3	7.687f	0.000	24376	0	6.534	N.D. #
32)	L7 AR-1260-2	8.124f	0.000	4281	0	1.258	N.D. #
34)	L7 AR-1260-4	8.665f	0.000	15971	0	5.441	N.D. #
35)	L7 AR-1260-5	9.030f	0.000	6640	0	1.350	N.D. #
37)	L8 AR-1262-2	9.030f	0.000	6640	0	1.143	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042321\
Data File : PP035231.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Apr 2021 20:27
Operator : DD\AJ
Sample : M2149-15
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
SB-40-9.5-10.0

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 24 01:04:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 21 17:37:28 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

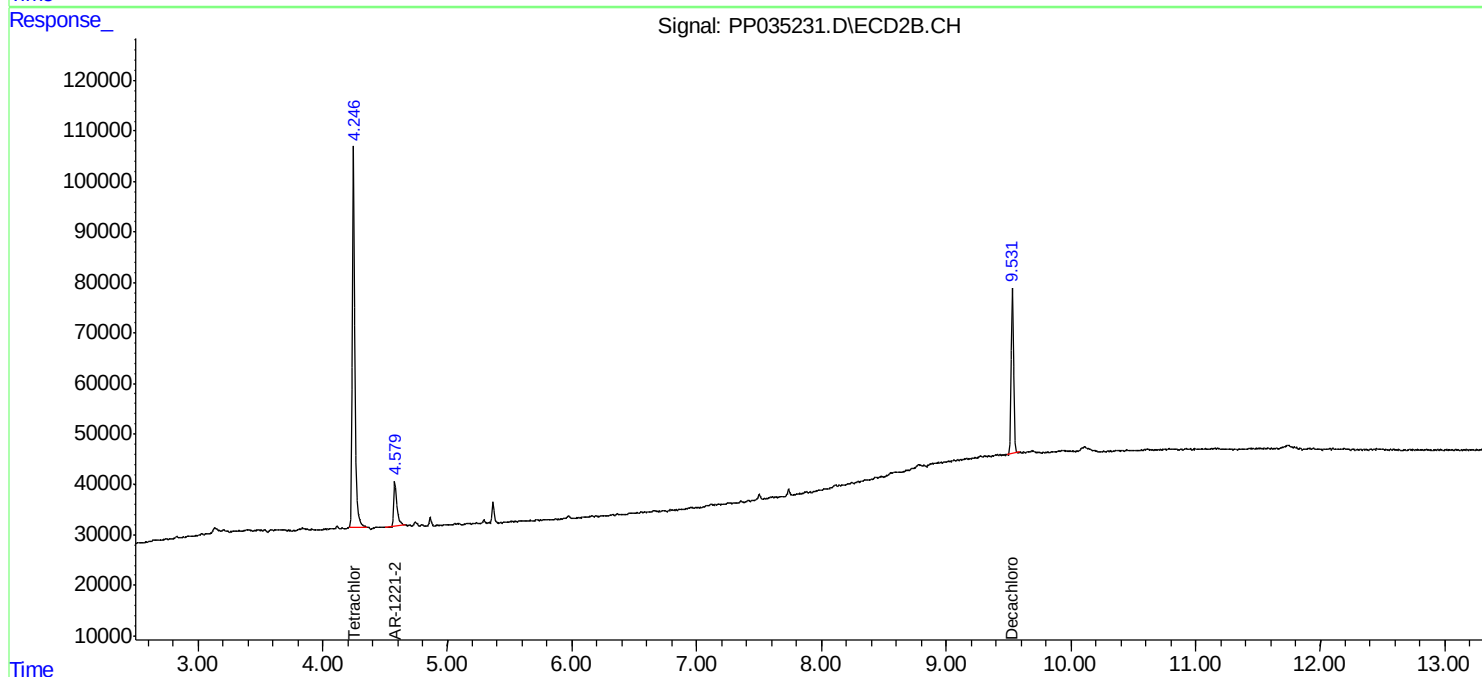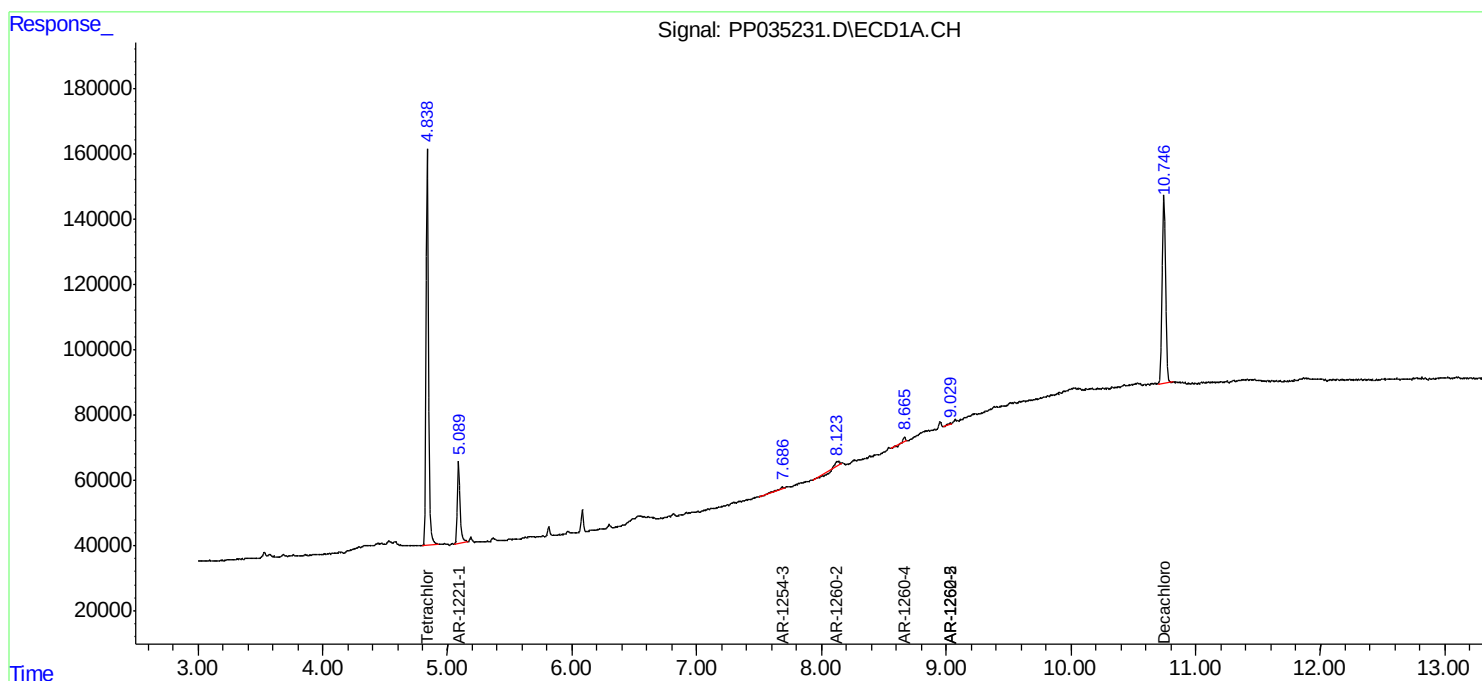


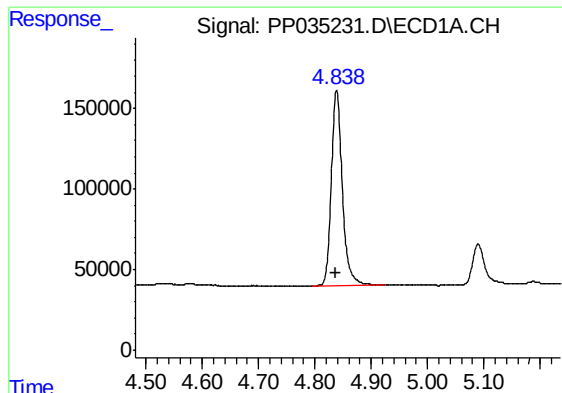

#1 Tetrachloro-m-xylene


R.T.: 4.839 min
Delta R.T.: 0.003 min
Response: 1643251
Conc: 20.17 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-40-9.5-10.0

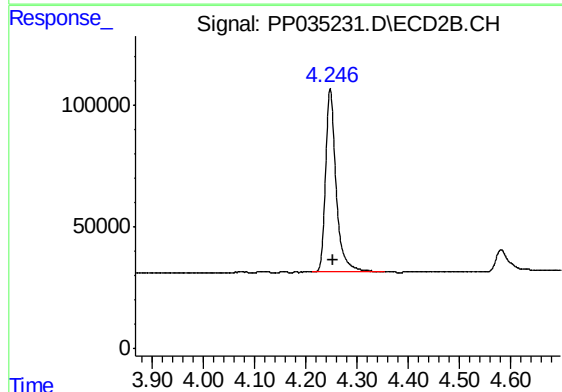


#1 Tetrachloro-m-xylene

R.T.: 4.247 min
Delta R.T.: -0.006 min
Response: 1069315
Conc: 20.76 ng/ml

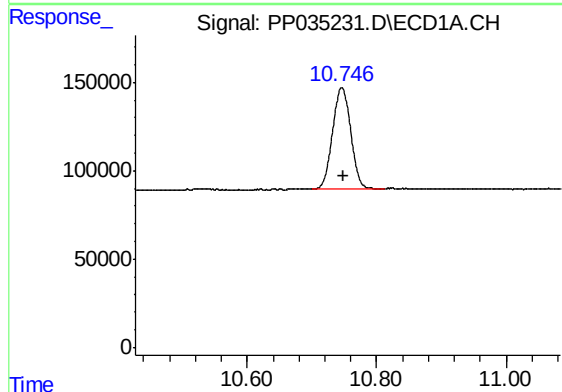


#2 Decachlorobiphenyl

R.T.: 10.746 min
Delta R.T.: -0.002 min
Response: 1116535
Conc: 17.67 ng/ml

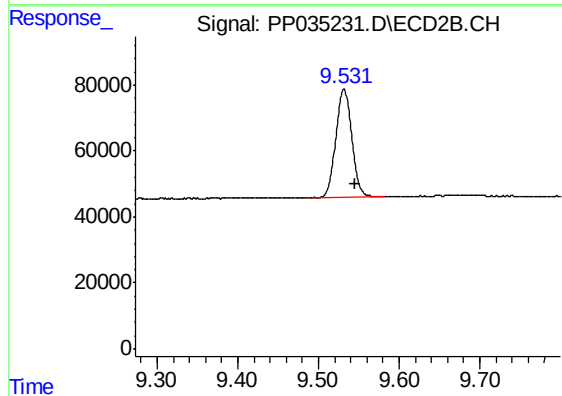

#2 Decachlorobiphenyl


R.T.: 9.532 min
Delta R.T.: -0.013 min
Response: 446442
Conc: 18.79 ng/ml

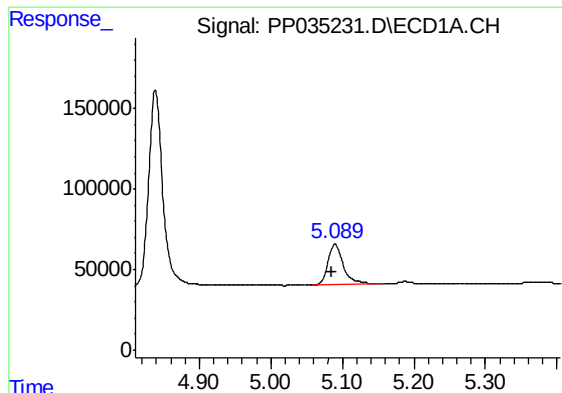

#8 AR-1221-1


R.T.: 5.090 min
Delta R.T.: 0.004 min
Response: 373371
Conc: 453.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-40-9.5-10.0

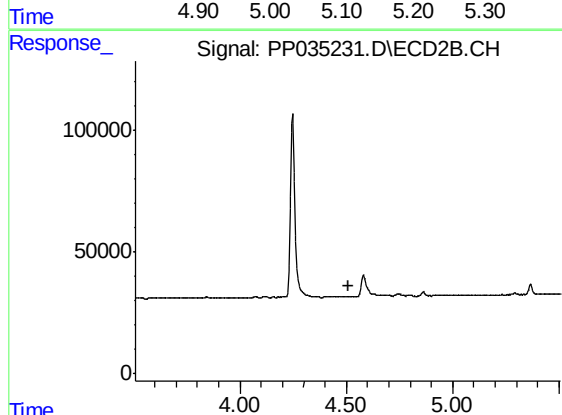


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.508 min
Response: 0
Conc: N.D.

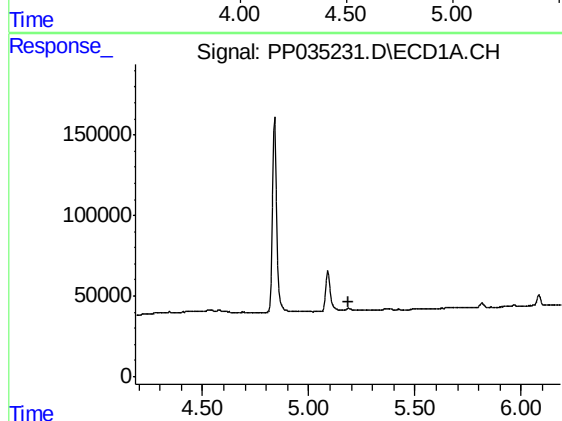


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 5.185 min
Response: 0
Conc: N.D.

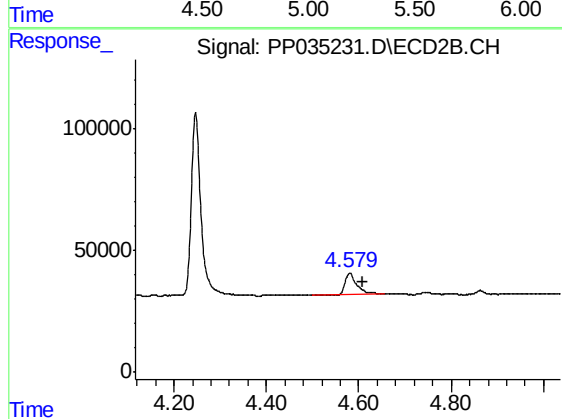

#9 AR-1221-2


R.T.: 4.580 min
Delta R.T.: -0.028 min
Response: 149185
Conc: 392.44 ng/ml

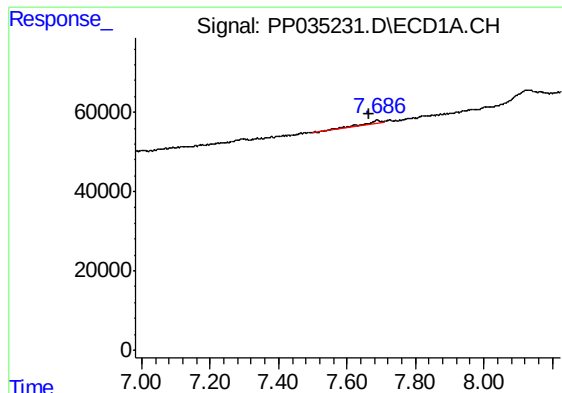

#28 AR-1254-3


R.T.: 7.687 min
Delta R.T.: 0.024 min
Response: 24376
Conc: 6.53 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-40-9.5-10.0

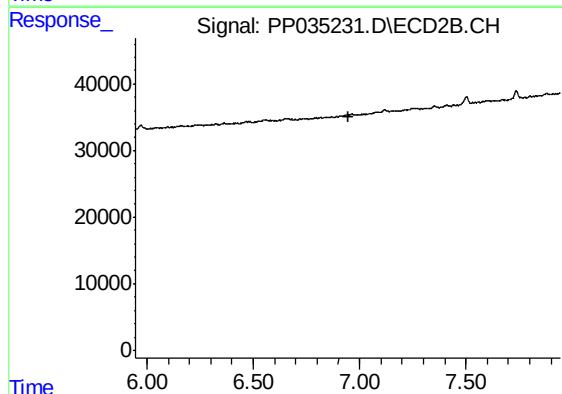


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.946 min
Response: 0
Conc: N.D.

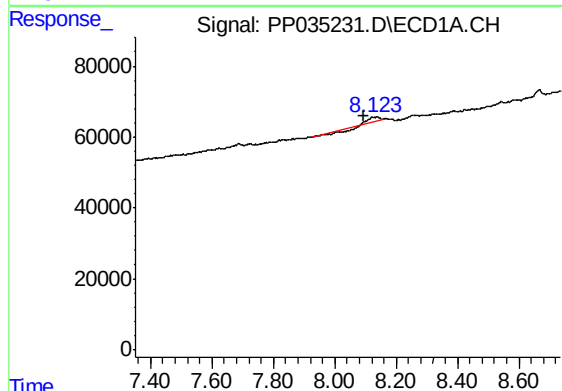


#32 AR-1260-2

R.T.: 8.124 min
Delta R.T.: 0.029 min
Response: 4281
Conc: 1.26 ng/ml

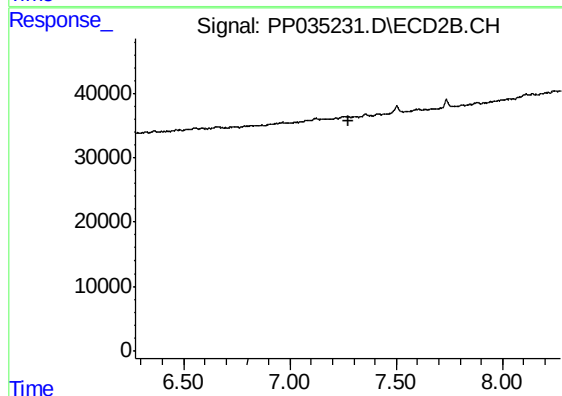

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 7.273 min
Response: 0
Conc: N.D.

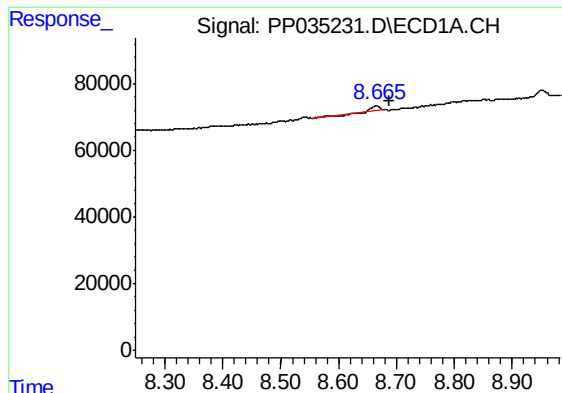

#34 AR-1260-4


R.T.: 8.665 min
Delta R.T.: -0.022 min
Response: 15971
Conc: 5.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-40-9.5-10.0

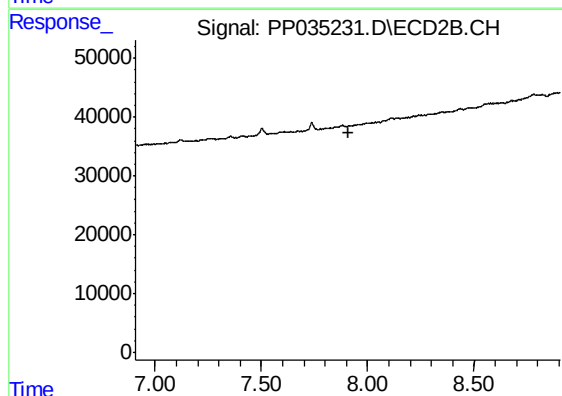


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.907 min
Response: 0
Conc: N.D.

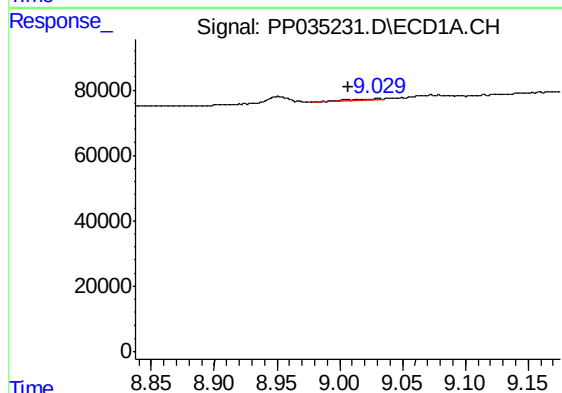


#35 AR-1260-5

R.T.: 9.030 min
Delta R.T.: 0.023 min
Response: 6640
Conc: 1.35 ng/ml

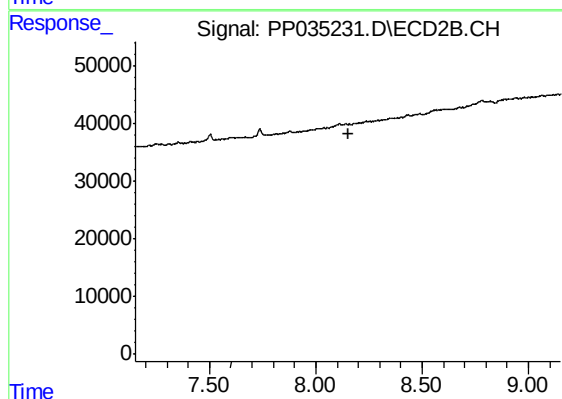

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 8.151 min
Response: 0
Conc: N.D.

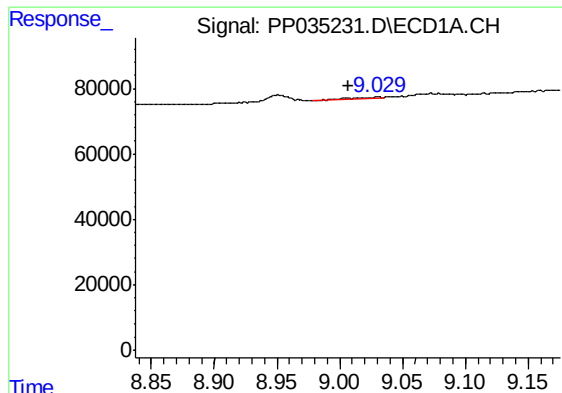

#37 AR-1262-2

R.T.: 9.030 min
Delta R.T.: 0.023 min
Response: 6640
Conc: 1.14 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-40-9.5-10.0

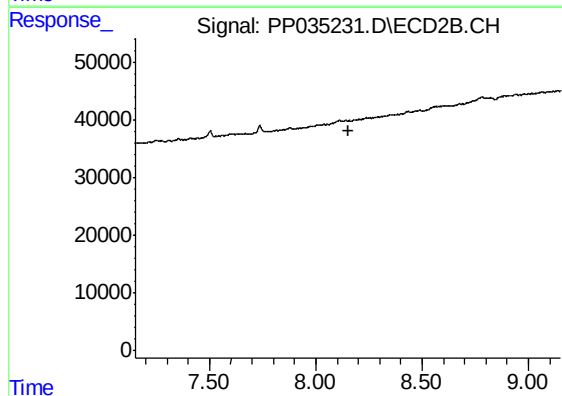

#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 8.151 min
Response: 0
Conc: N.D.