

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042321\
 Data File : PP035193.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Apr 2021 9:48
 Operator : DD\AJ
 Sample : M2106-03RE
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SB-22-14.5-15.0RE

Manual Integrations
 APPROVED

Ankita
 4/27/2021 10:41:37 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 16:43:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 21 17:37:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.837	4.247	1851581	1166117	22.723	22.644
2) SA Decachlor...	10.742	9.534	3567845	1356123	56.459	57.076
Target Compounds						
31) L7 AR-1260-1	7.824	7.073	77974	50152	23.153m	28.665
32) L7 AR-1260-2	8.091	7.267	464765	104837	136.518m	58.810 #
33) L7 AR-1260-3	8.456	7.421	83766	47776	33.373	26.496
34) L7 AR-1260-4	8.687	7.898	139452	48623	47.509	38.199
35) L7 AR-1260-5	9.003	8.144	163327	81332	33.199	33.452

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042321\
Data File : PP035193.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Apr 2021 9:48
Operator : DD\AJ
Sample : M2106-03RE
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
SB-22-14.5-15.0RE


Manual Integrations
APPROVED

Ankita
4/27/2021 10:41:37 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 16:43:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 21 17:37:28 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

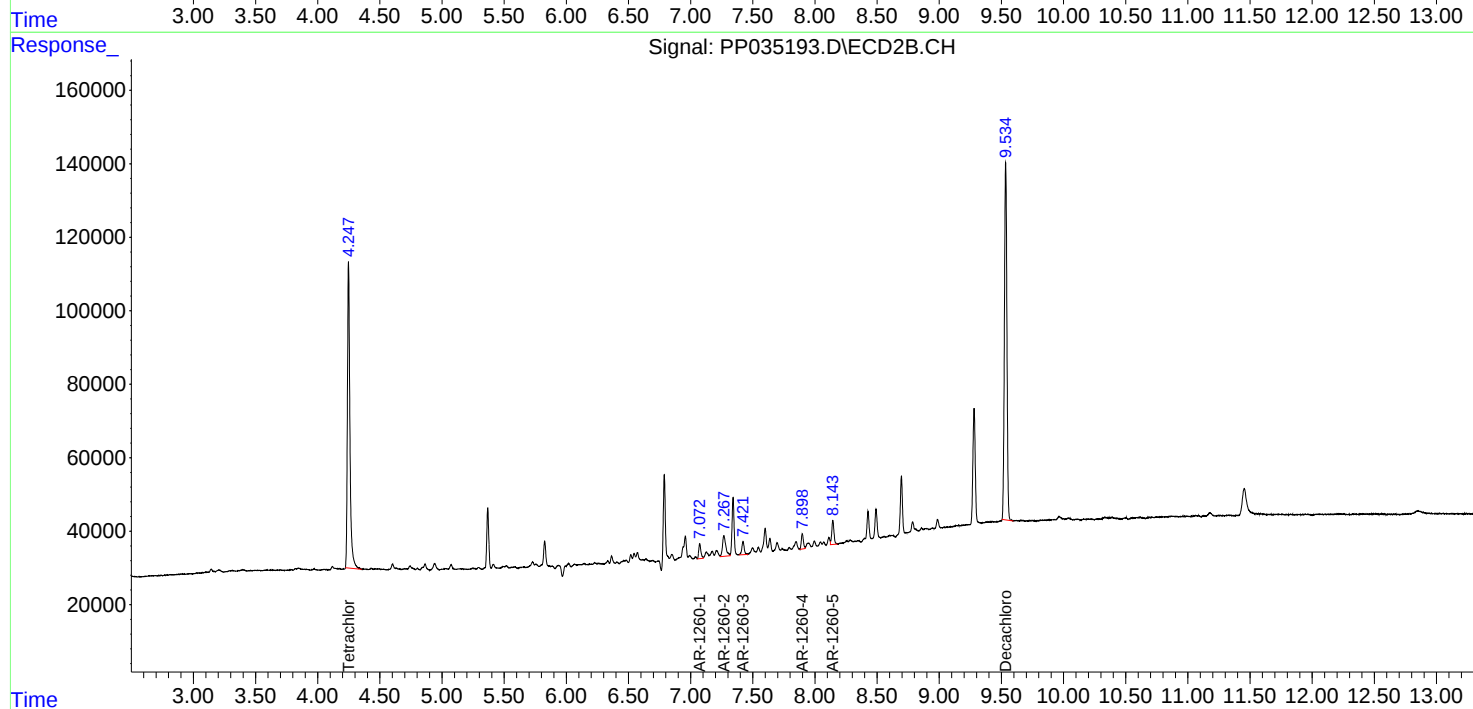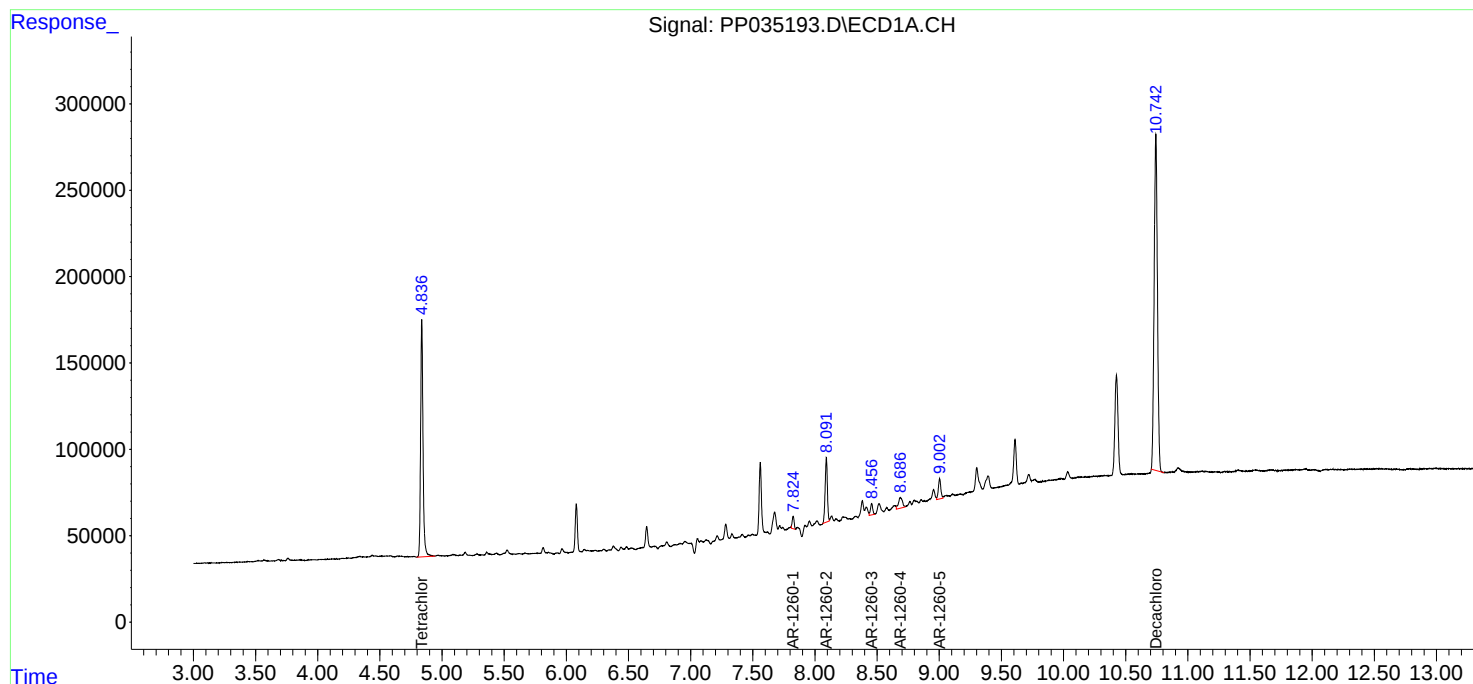

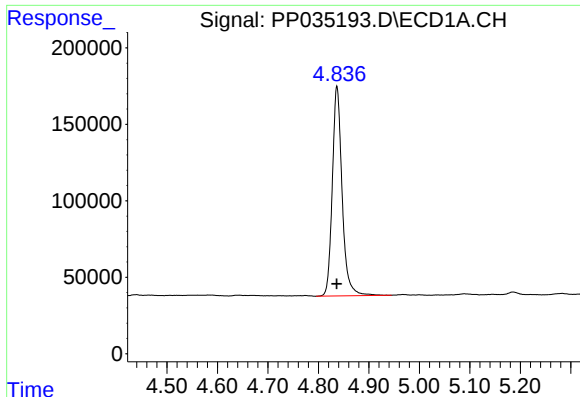


#1 Tetrachloro-m-xylene

R.T.: 4.837 min
Delta R.T.: 0.000 min
Response: 1851581
Conc: 22.72 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-22-14.5-15.0RE


Manual Integrations
APPROVED

Ankita
4/27/2021 10:41:37 AM

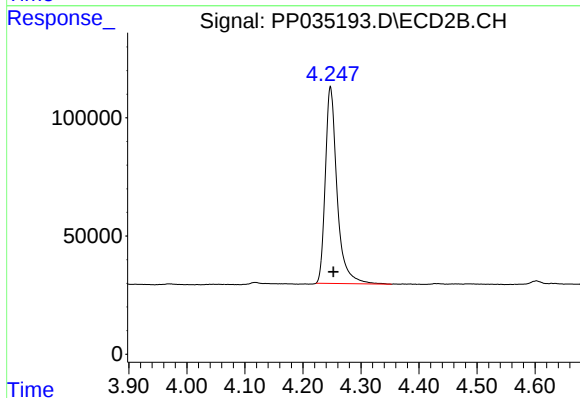


#1 Tetrachloro-m-xylene

R.T.: 4.247 min
Delta R.T.: -0.005 min
Response: 1166117
Conc: 22.64 ng/ml

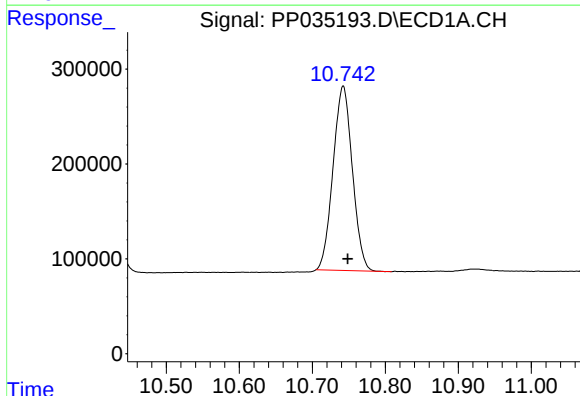


#2 Decachlorobiphenyl

R.T.: 10.742 min
Delta R.T.: -0.006 min
Response: 3567845
Conc: 56.46 ng/ml

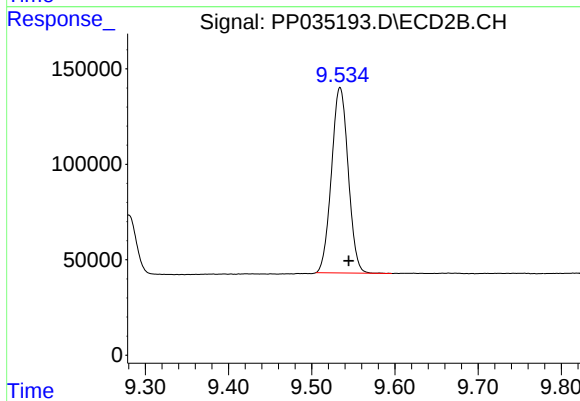

#2 Decachlorobiphenyl

R.T.: 9.534 min
Delta R.T.: -0.010 min
Response: 1356123
Conc: 57.08 ng/ml

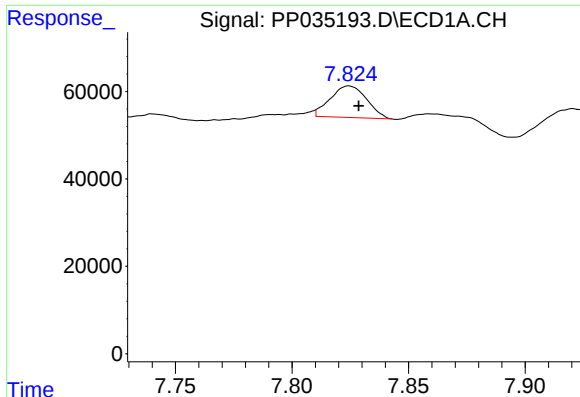


#31 AR-1260-1

R.T.: 7.824 min
Delta R.T.: -0.005 min
Response: 77974
Conc: 23.15 ng/ml m

Instrument :
ECD_P
ClientSampleId :
SB-22-14.5-15.0RE


Manual Integrations
APPROVED

Ankita
4/27/2021 10:41:37 AM

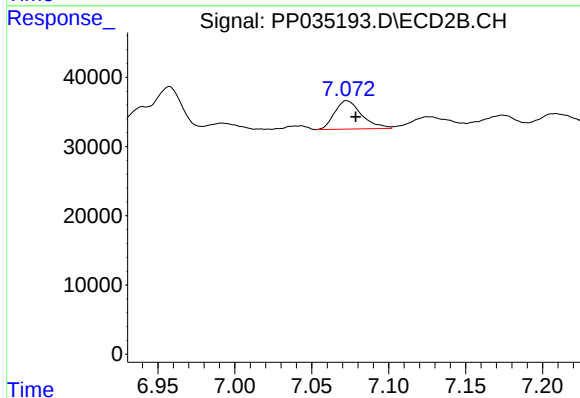


#31 AR-1260-1

R.T.: 7.073 min
Delta R.T.: -0.006 min
Response: 50152
Conc: 28.67 ng/ml

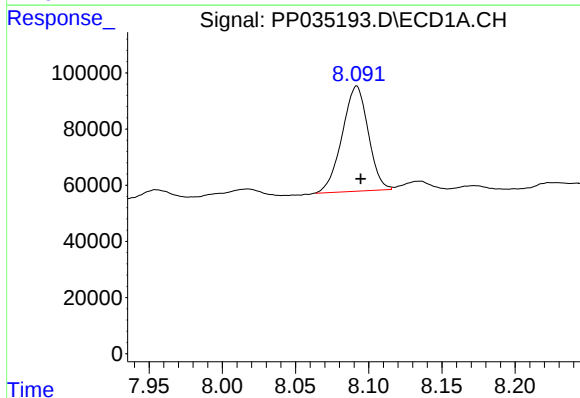


#32 AR-1260-2

R.T.: 8.091 min
Delta R.T.: -0.003 min
Response: 464765
Conc: 136.52 ng/ml m

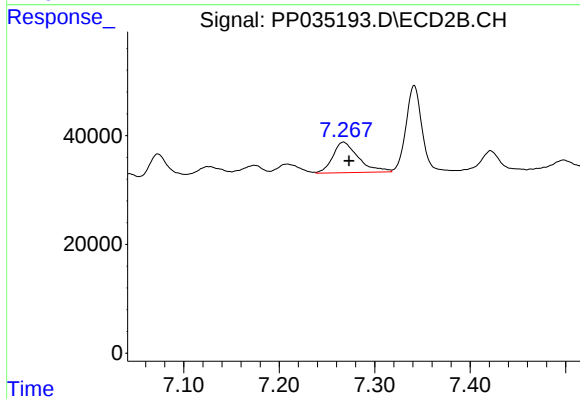

#32 AR-1260-2

R.T.: 7.267 min
Delta R.T.: -0.006 min
Response: 104837
Conc: 58.81 ng/ml

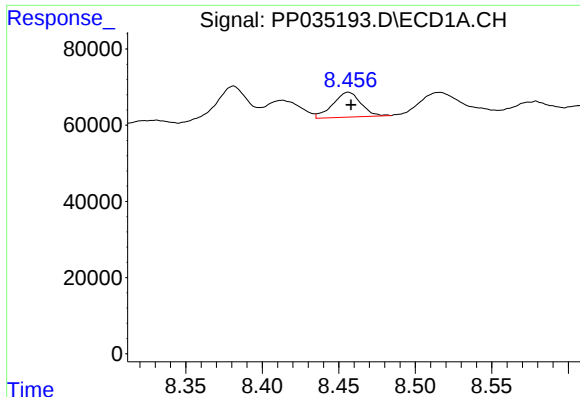


#33 AR-1260-3

R.T.: 8.456 min
Delta R.T.: -0.002 min
Response: 83766
Conc: 33.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-22-14.5-15.0RE


Manual Integrations
APPROVED

Ankita
4/27/2021 10:41:37 AM

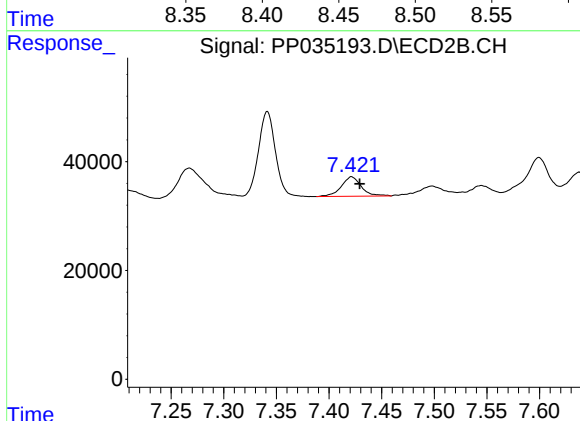


#33 AR-1260-3

R.T.: 7.421 min
Delta R.T.: -0.008 min
Response: 47776
Conc: 26.50 ng/ml

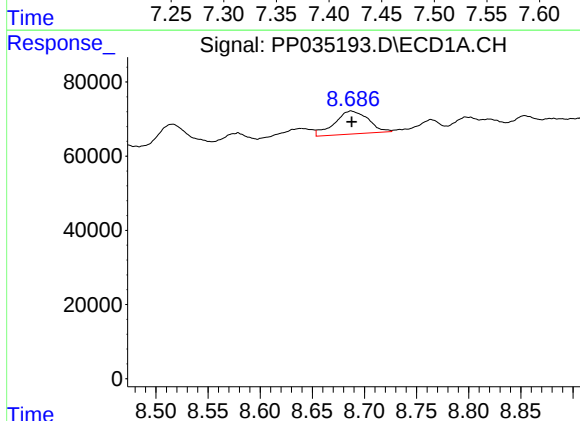


#34 AR-1260-4

R.T.: 8.687 min
Delta R.T.: 0.000 min
Response: 139452
Conc: 47.51 ng/ml

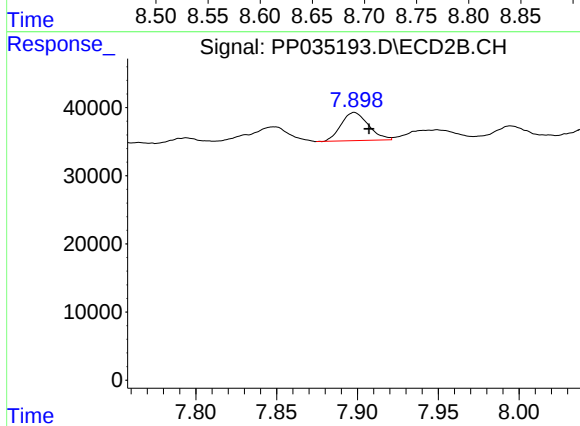

#34 AR-1260-4

R.T.: 7.898 min
Delta R.T.: -0.009 min
Response: 48623
Conc: 38.20 ng/ml

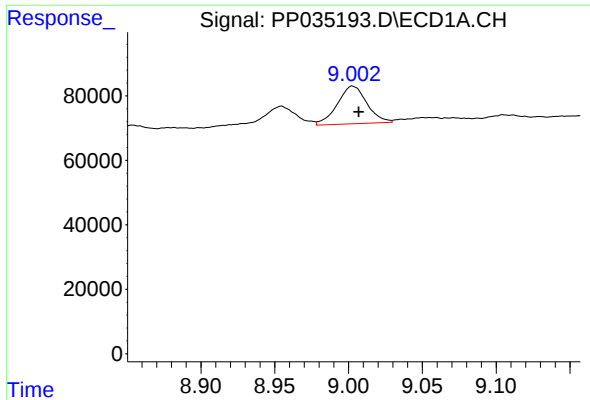


#35 AR-1260-5

R.T.: 9.003 min
Delta R.T.: -0.004 min
Response: 163327
Conc: 33.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-22-14.5-15.0RE

Manual Integrations
APPROVED

Ankita
4/27/2021 10:41:37 AM

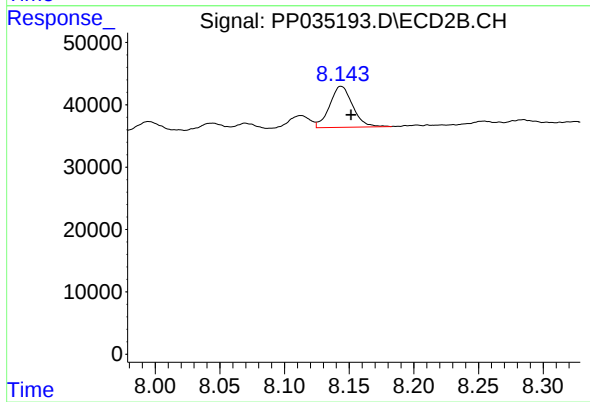

#35 AR-1260-5

R.T.: 8.144 min
Delta R.T.: -0.008 min
Response: 81332
Conc: 33.45 ng/ml