

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042321\
 Data File : PP035196.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Apr 2021 10:39
 Operator : DD\AJ
 Sample : M2107-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SB-29-0-2.0

Manual Integrations
 APPROVED

Ankita
 4/27/2021 10:41:38 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 16:44:19 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 21 17:37:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.837	4.248	1633542	1037131	20.047	20.140
2) SA Decachlor...	10.741	9.534	1473995	574251	23.325	24.169

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042321\
Data File : PP035196.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Apr 2021 10:39
Operator : DD\AJ
Sample : M2107-01
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
SB-29-0-2.0


Manual Integrations
APPROVED

Ankita
4/27/2021 10:41:38 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 16:44:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 21 17:37:28 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

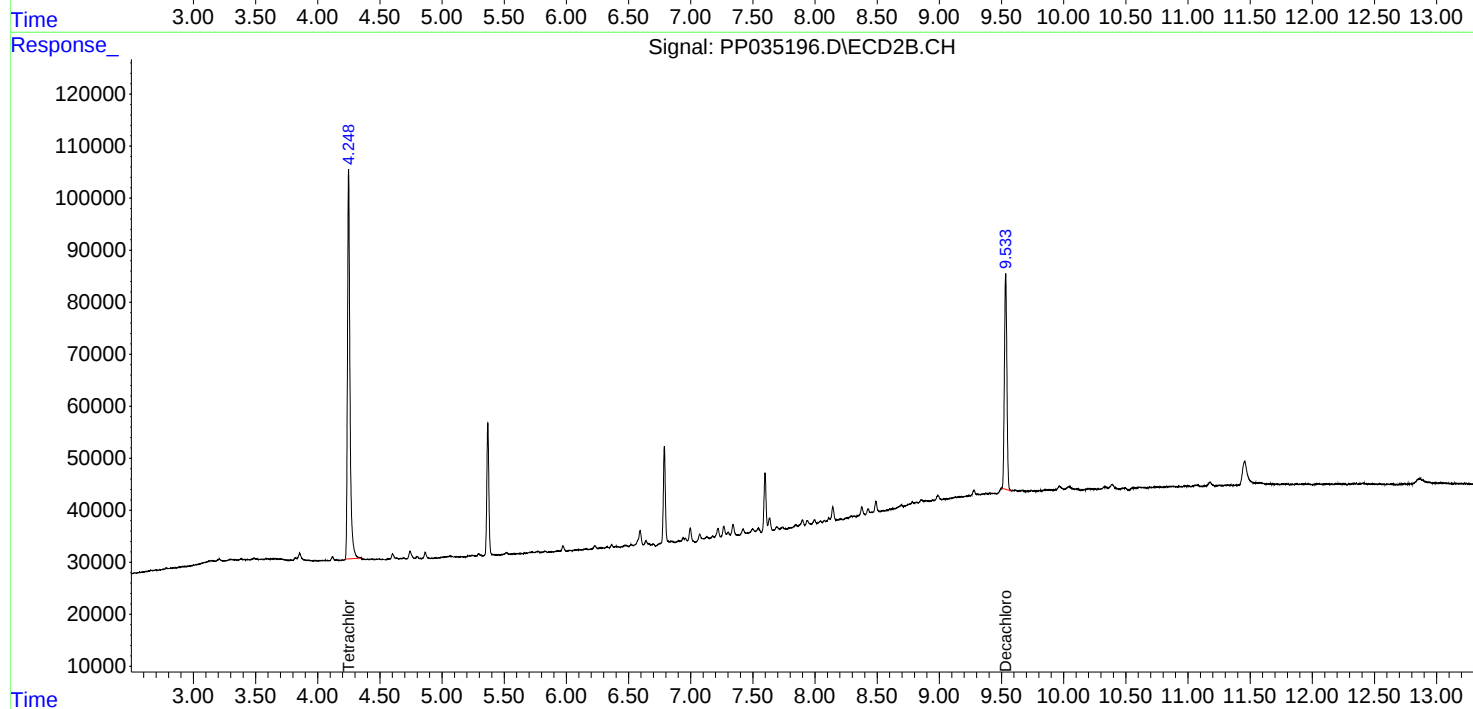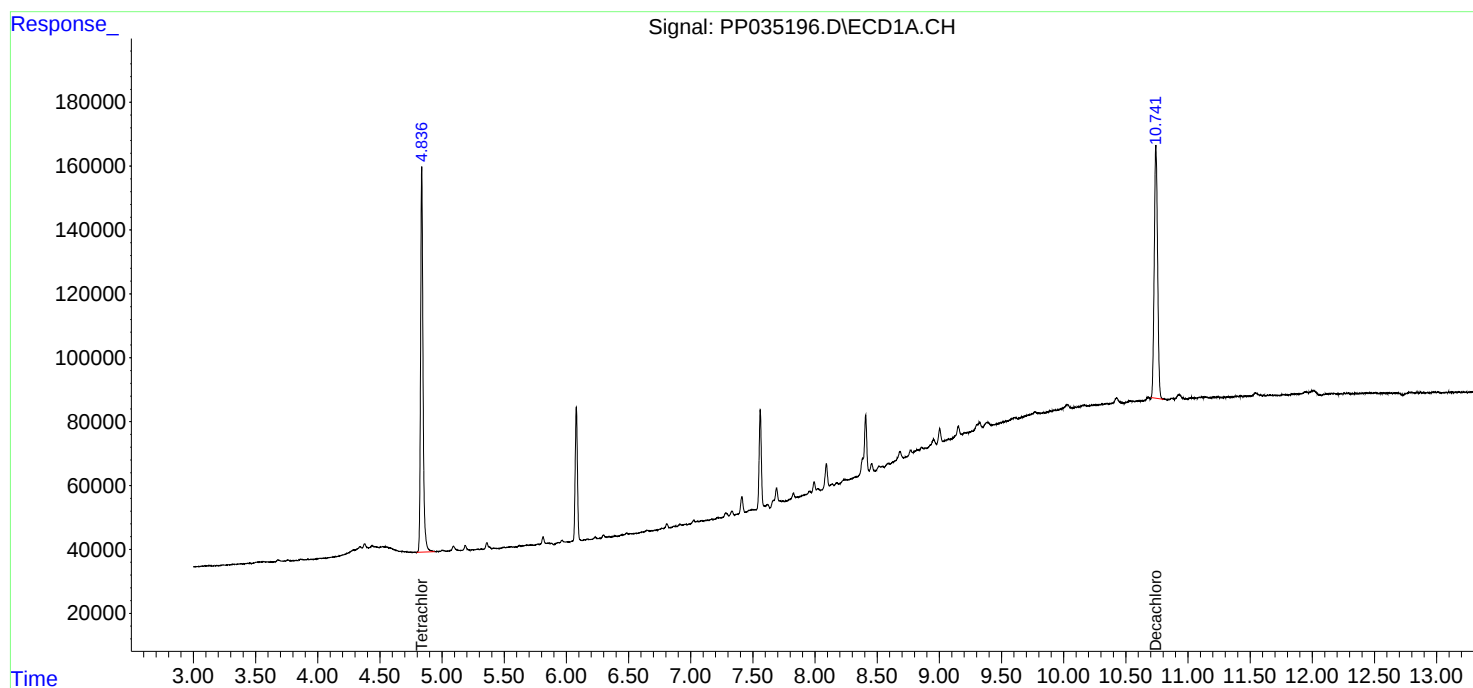

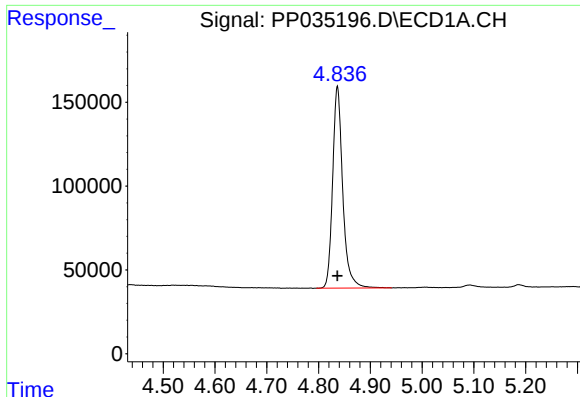


#1 Tetrachloro-m-xylene

R.T.: 4.837 min
Delta R.T.: 0.000 min
Response: 1633542
Conc: 20.05 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-29-0-2.0


Manual Integrations
APPROVED

Ankita
4/27/2021 10:41:38 AM

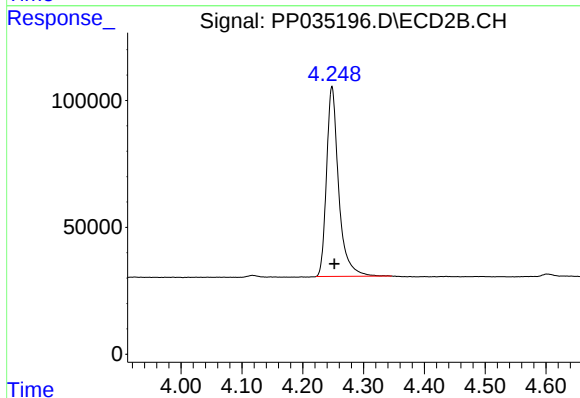


#1 Tetrachloro-m-xylene

R.T.: 4.248 min
Delta R.T.: -0.004 min
Response: 1037131
Conc: 20.14 ng/ml

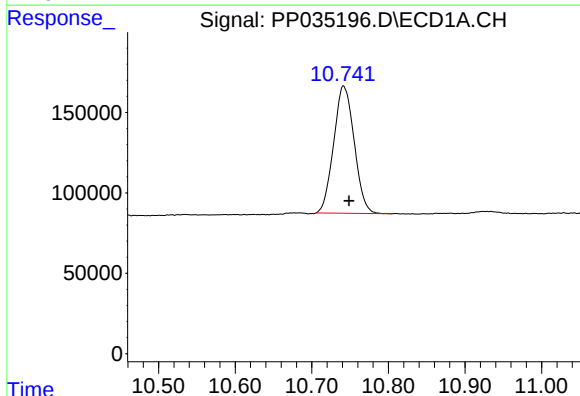

#2 Decachlorobiphenyl

R.T.: 10.741 min
Delta R.T.: -0.007 min
Response: 1473995
Conc: 23.33 ng/ml

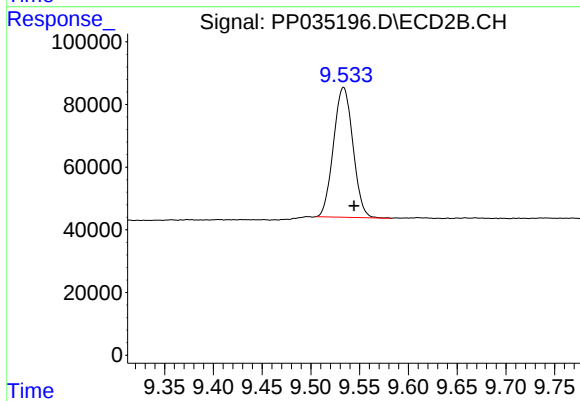

#2 Decachlorobiphenyl

R.T.: 9.534 min
Delta R.T.: -0.011 min
Response: 574251
Conc: 24.17 ng/ml