

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042321\
 Data File : PP035203.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Apr 2021 12:37
 Operator : DD\AJ
 Sample : M2107-08
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SB-31-0-2.0

Manual Integrations
 APPROVED

Ankita
 4/27/2021 10:41:42 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 16:46:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 21 17:37:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.837	4.248	2209036	1396472	27.110	27.118
2) SA Decachlor...	10.741	9.534	1955141	749086	30.939	31.527
Target Compounds						
31) L7 AR-1260-1	7.825	7.073	123765	99117	36.750	56.653 #
32) L7 AR-1260-2	8.090	7.267	396989	104610	116.610	58.683 #
33) L7 AR-1260-3	8.455	7.422	118913	61472	47.375	34.092 #
34) L7 AR-1260-4	8.684	7.899	130672	55843	44.518m	43.871
35) L7 AR-1260-5	9.003	8.144	216567	109017	44.021	44.840

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042321\
Data File : PP035203.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Apr 2021 12:37
Operator : DD\AJ
Sample : M2107-08
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
SB-31-0-2.0


Manual Integrations
APPROVED

Ankita
4/27/2021 10:41:42 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 16:46:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 21 17:37:28 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

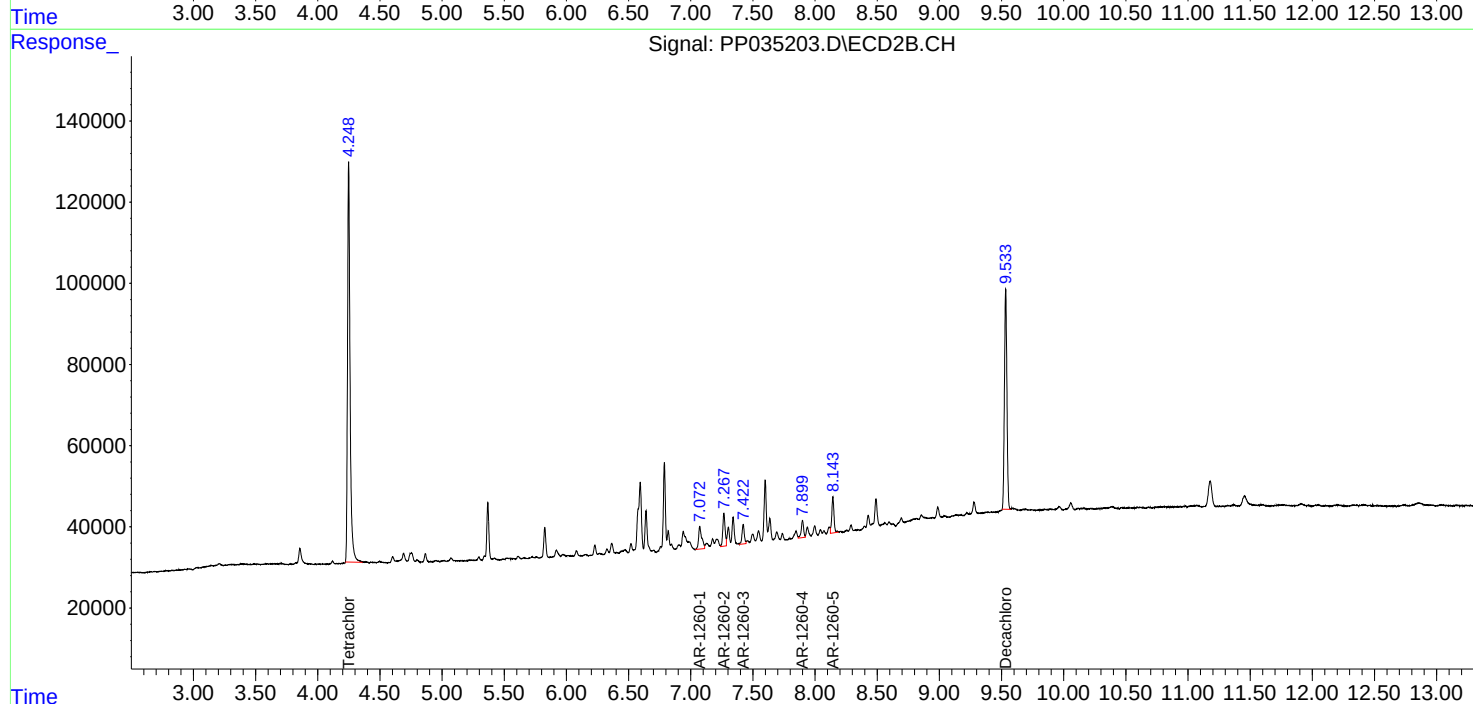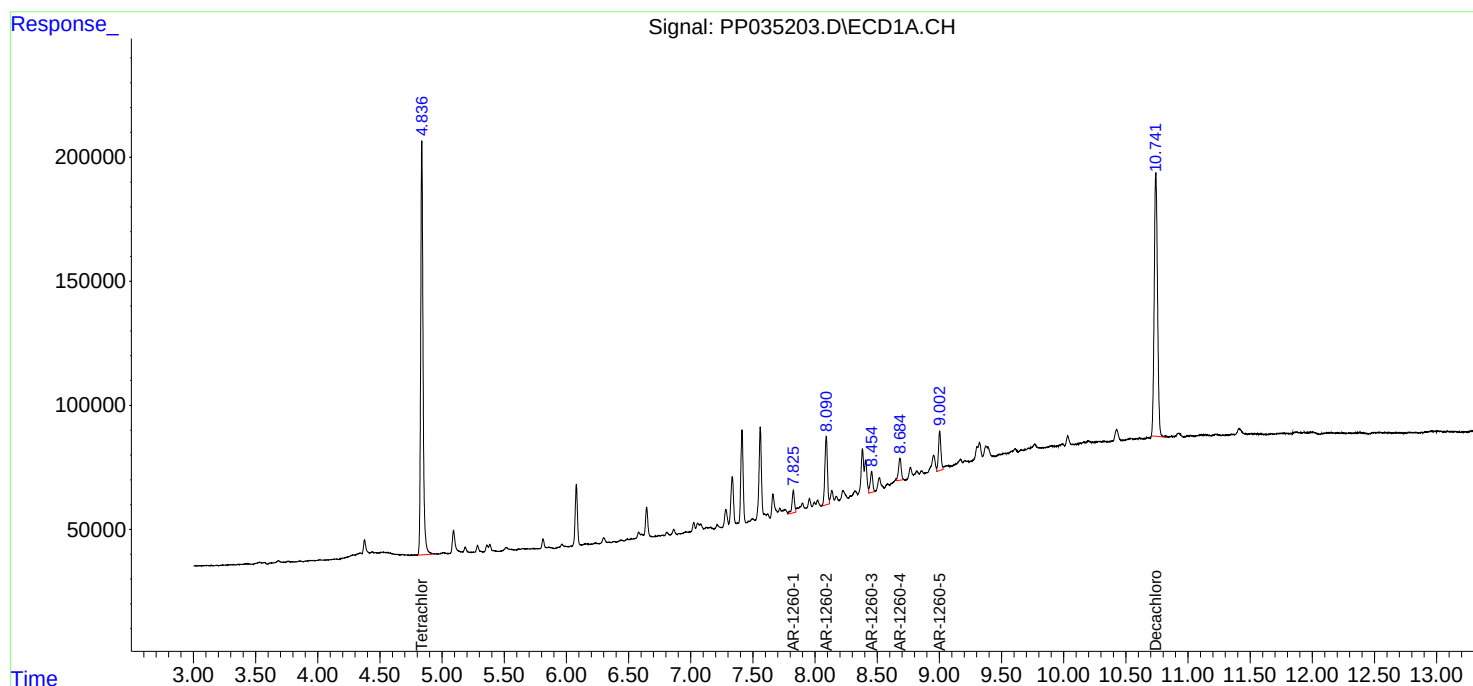

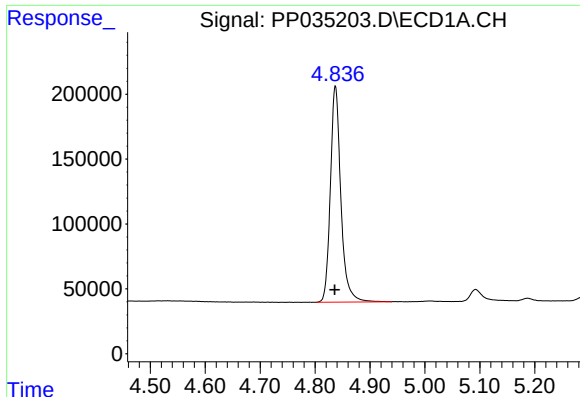


#1 Tetrachloro-m-xylene

R.T.: 4.837 min
Delta R.T.: 0.000 min
Response: 2209036
Conc: 27.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-31-0-2.0


Manual Integrations
APPROVED

Ankita
4/27/2021 10:41:42 AM

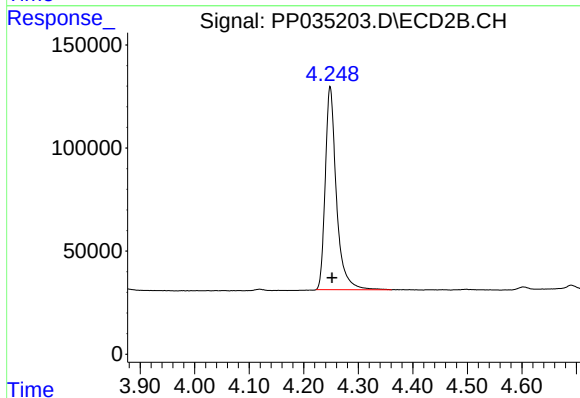


#1 Tetrachloro-m-xylene

R.T.: 4.248 min
Delta R.T.: -0.004 min
Response: 1396472
Conc: 27.12 ng/ml

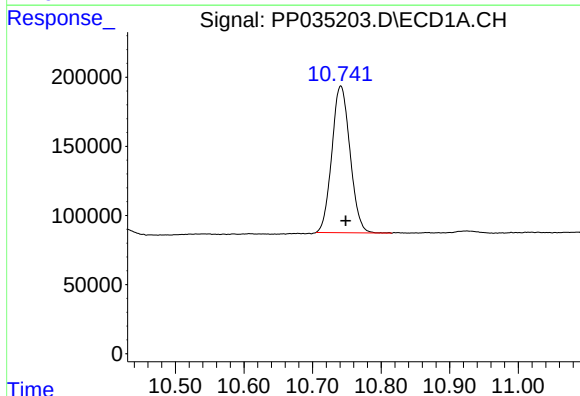


#2 Decachlorobiphenyl

R.T.: 10.741 min
Delta R.T.: -0.007 min
Response: 1955141
Conc: 30.94 ng/ml

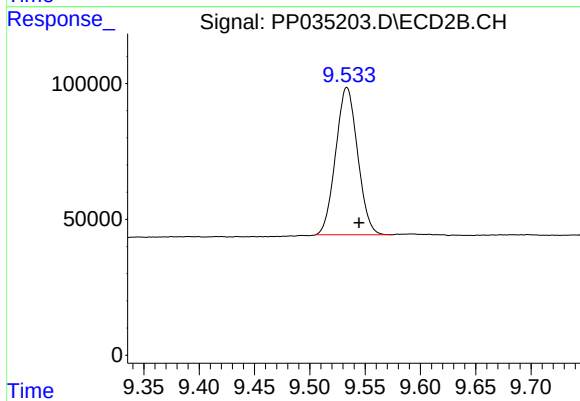

#2 Decachlorobiphenyl

R.T.: 9.534 min
Delta R.T.: -0.011 min
Response: 749086
Conc: 31.53 ng/ml

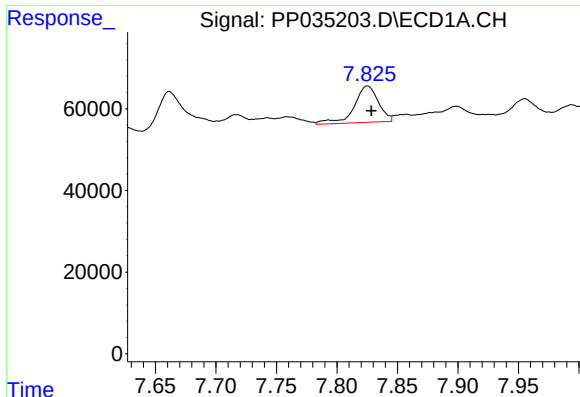


#31 AR-1260-1

R.T.: 7.825 min
Delta R.T.: -0.003 min
Response: 123765
Conc: 36.75 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-31-0-2.0


Manual Integrations
APPROVED

Ankita
4/27/2021 10:41:42 AM

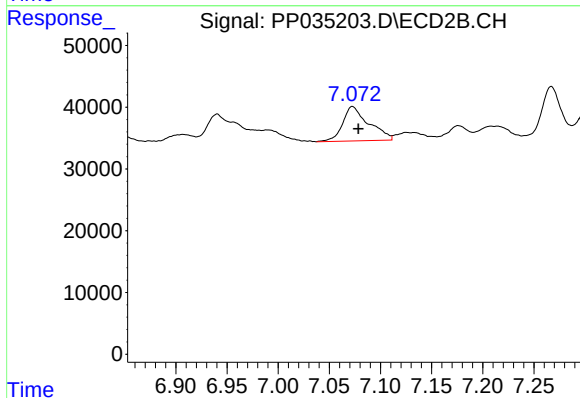


#31 AR-1260-1

R.T.: 7.073 min
Delta R.T.: -0.006 min
Response: 99117
Conc: 56.65 ng/ml

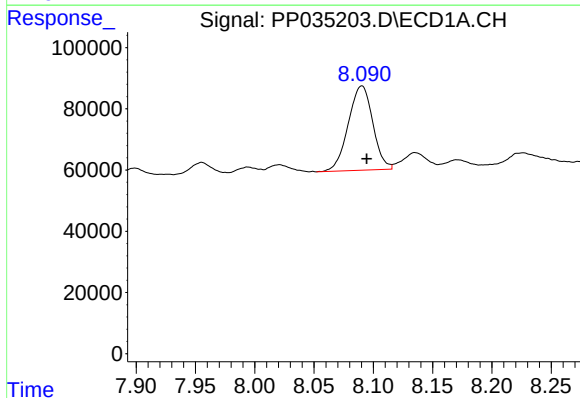


#32 AR-1260-2

R.T.: 8.090 min
Delta R.T.: -0.004 min
Response: 396989
Conc: 116.61 ng/ml

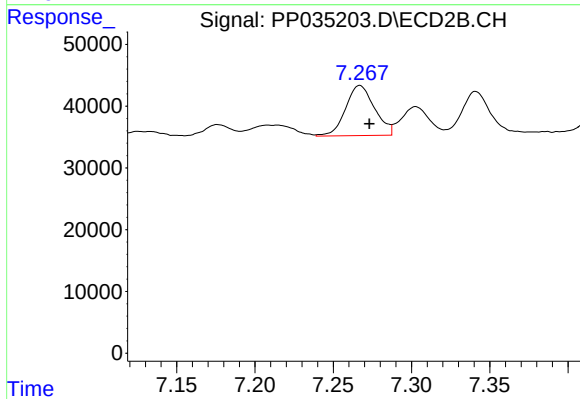

#32 AR-1260-2

R.T.: 7.267 min
Delta R.T.: -0.006 min
Response: 104610
Conc: 58.68 ng/ml

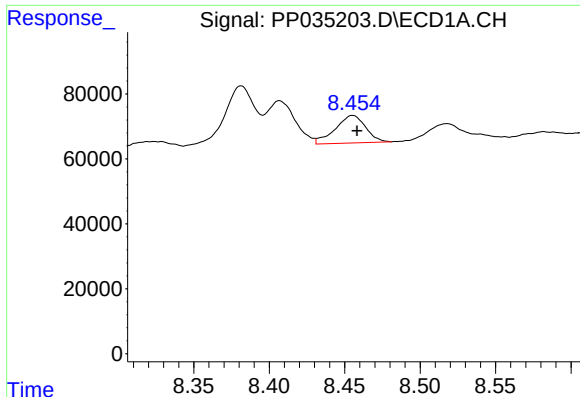


#33 AR-1260-3

R.T.: 8.455 min
Delta R.T.: -0.003 min
Response: 118913
Conc: 47.38 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-31-0-2.0


Manual Integrations
APPROVED

Ankita
4/27/2021 10:41:42 AM

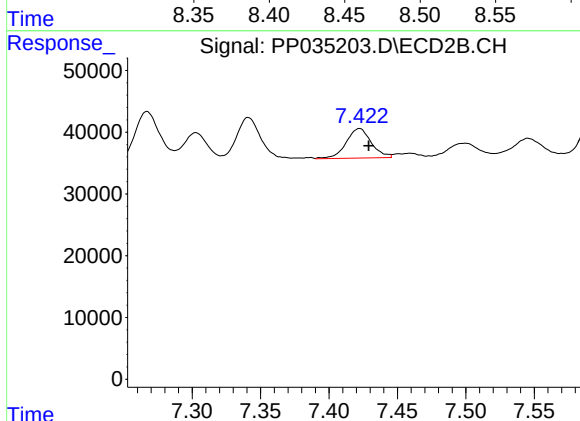


#33 AR-1260-3

R.T.: 7.422 min
Delta R.T.: -0.007 min
Response: 61472
Conc: 34.09 ng/ml

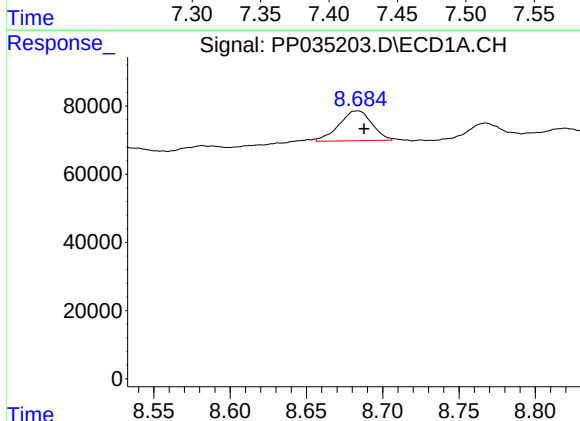


#34 AR-1260-4

R.T.: 8.684 min
Delta R.T.: -0.004 min
Response: 130672
Conc: 44.52 ng/ml m

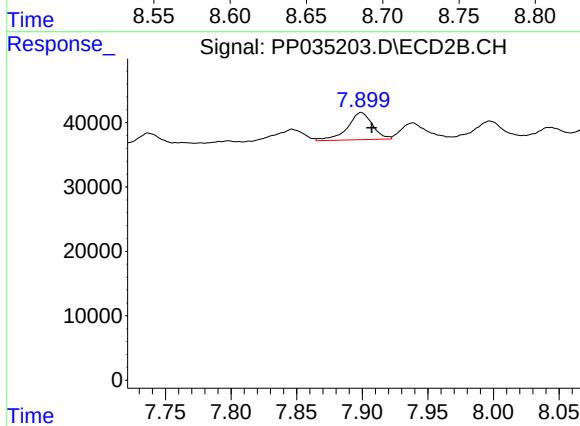

#34 AR-1260-4

R.T.: 7.899 min
Delta R.T.: -0.008 min
Response: 55843
Conc: 43.87 ng/ml

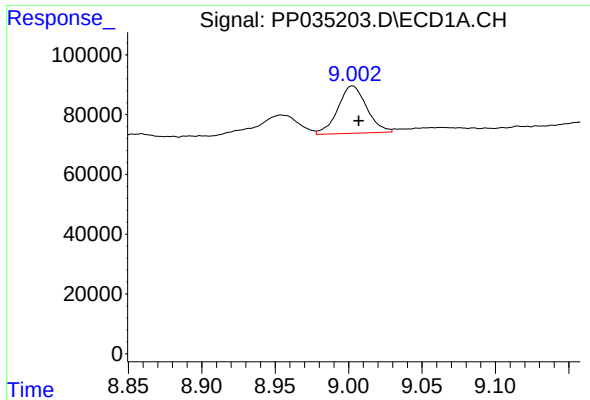


#35 AR-1260-5

R.T.: 9.003 min
Delta R.T.: -0.004 min
Response: 216567
Conc: 44.02 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-31-0-2.0

Manual Integrations
APPROVED

Ankita
4/27/2021 10:41:42 AM

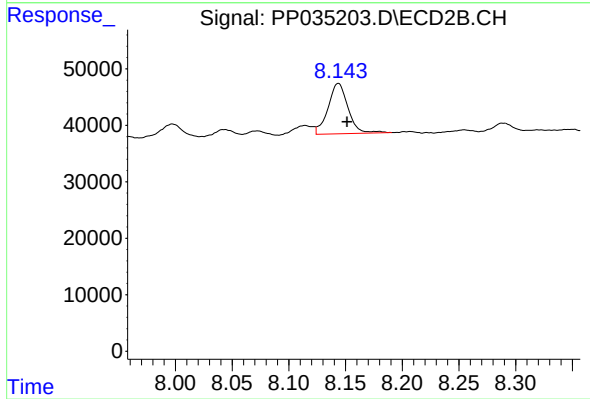

#35 AR-1260-5

R.T.: 8.144 min
Delta R.T.: -0.008 min
Response: 109017
Conc: 44.84 ng/ml