

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042321\
 Data File : PP035207.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Apr 2021 13:44
 Operator : DD\AJ
 Sample : M2107-14
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SB-33-0-2.0

Manual Integrations
 APPROVED

Ankita
 4/27/2021 10:41:45 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 16:48:21 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 21 17:37:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.837	4.248	1624111	1022687	19.931	19.859
2) SA Decachlor...	10.745	9.533	1331463	485570	21.070	20.436
Target Compounds						
31) L7 AR-1260-1	7.826	7.073	105429	71811	31.306	41.045 #
32) L7 AR-1260-2	8.089	7.267	299383	77213	87.939	43.314 #
33) L7 AR-1260-3	8.455	7.421	99654	37989	39.703	21.069 #
34) L7 AR-1260-4	8.681	7.900	113010	44237	38.501m	34.753
35) L7 AR-1260-5	9.003	8.144	191666	99936	38.959	41.104

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042321\
Data File : PP035207.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Apr 2021 13:44
Operator : DD\AJ
Sample : M2107-14
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
SB-33-0-2.0


Manual Integrations
APPROVED

Ankita
4/27/2021 10:41:45 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 16:48:21 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 21 17:37:28 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

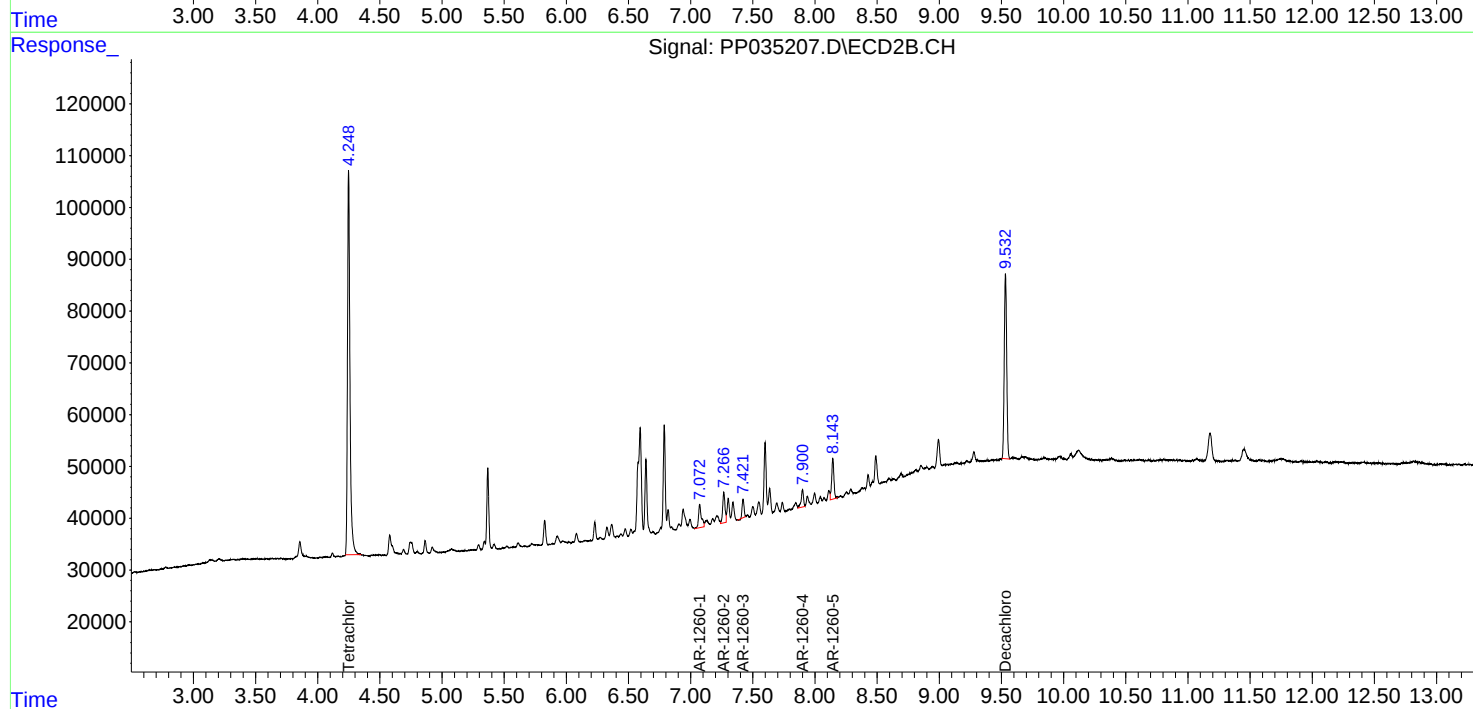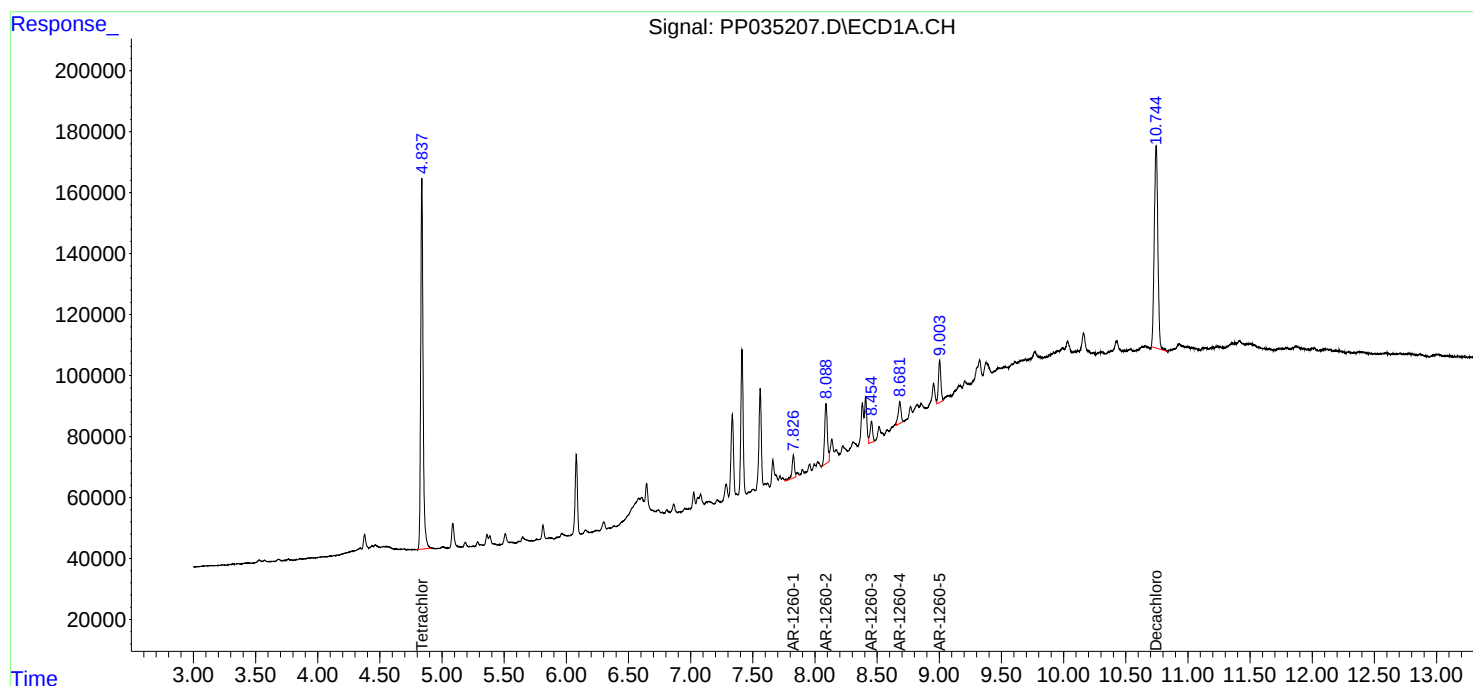

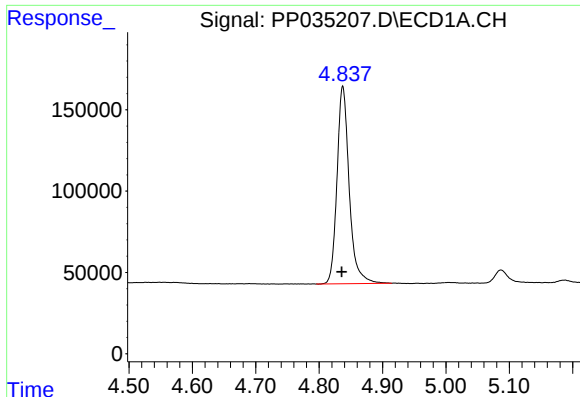


#1 Tetrachloro-m-xylene

R.T.: 4.837 min
Delta R.T.: 0.001 min
Response: 1624111
Conc: 19.93 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-33-0-2.0


Manual Integrations
APPROVED

Ankita
4/27/2021 10:41:45 AM

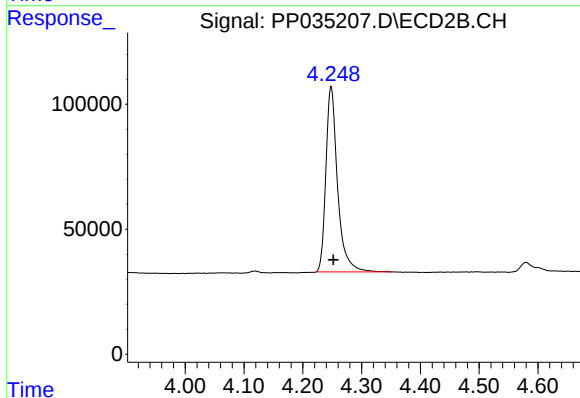


#1 Tetrachloro-m-xylene

R.T.: 4.248 min
Delta R.T.: -0.004 min
Response: 1022687
Conc: 19.86 ng/ml

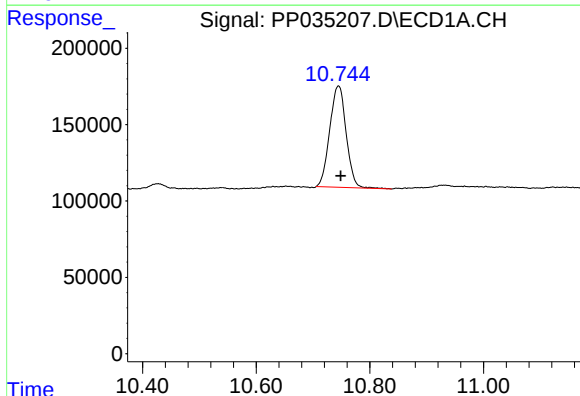


#2 Decachlorobiphenyl

R.T.: 10.745 min
Delta R.T.: -0.004 min
Response: 1331463
Conc: 21.07 ng/ml

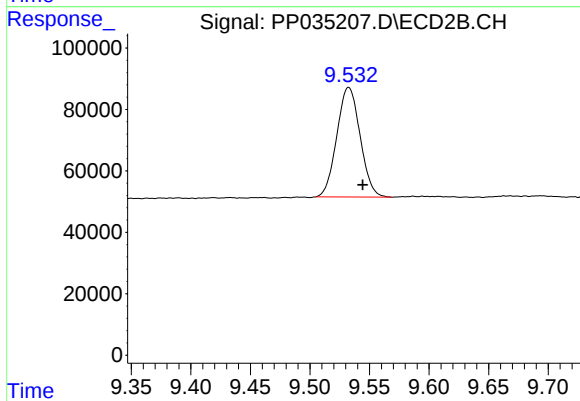

#2 Decachlorobiphenyl

R.T.: 9.533 min
Delta R.T.: -0.012 min
Response: 485570
Conc: 20.44 ng/ml

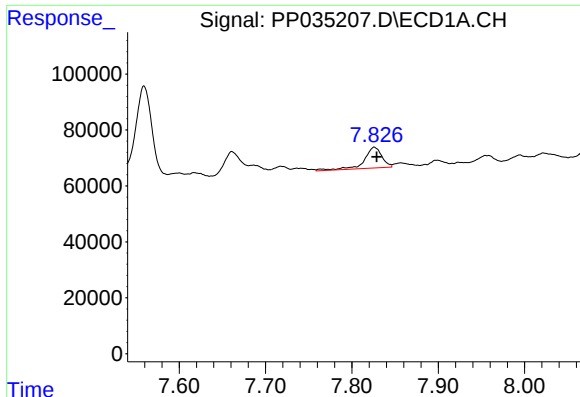


#31 AR-1260-1

R.T.: 7.826 min
Delta R.T.: -0.003 min
Response: 105429
Conc: 31.31 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-33-0-2.0


Manual Integrations
APPROVED

Ankita
4/27/2021 10:41:45 AM

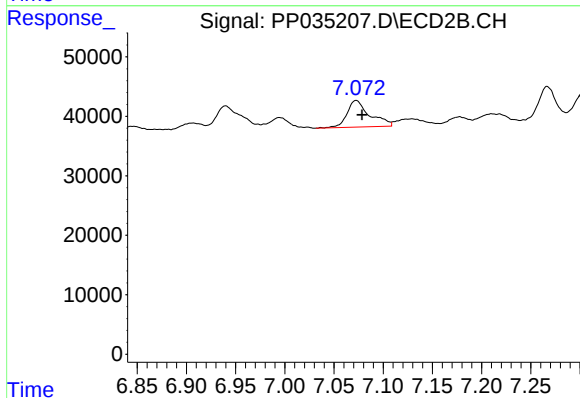


#31 AR-1260-1

R.T.: 7.073 min
Delta R.T.: -0.006 min
Response: 71811
Conc: 41.04 ng/ml

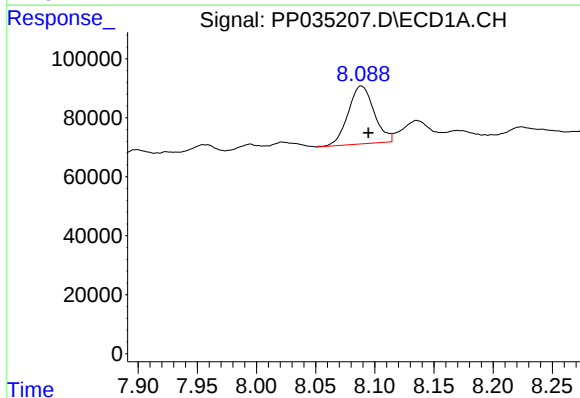


#32 AR-1260-2

R.T.: 8.089 min
Delta R.T.: -0.006 min
Response: 299383
Conc: 87.94 ng/ml

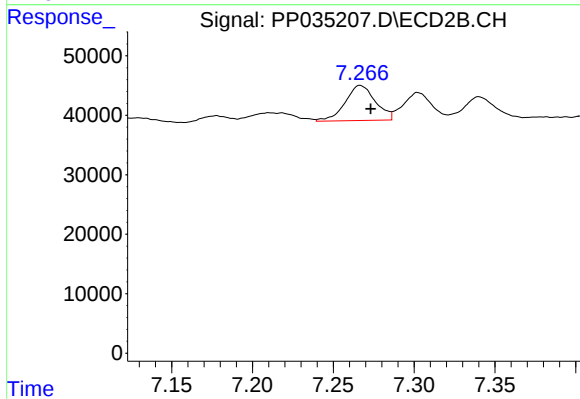

#32 AR-1260-2

R.T.: 7.267 min
Delta R.T.: -0.006 min
Response: 77213
Conc: 43.31 ng/ml

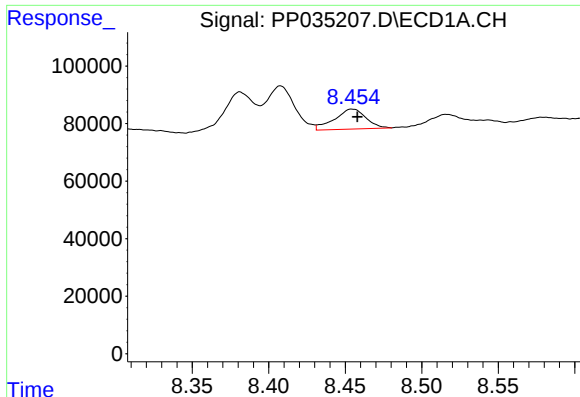


#33 AR-1260-3

R.T.: 8.455 min
Delta R.T.: -0.003 min
Response: 99654
Conc: 39.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-33-0-2.0


Manual Integrations
APPROVED

Ankita
4/27/2021 10:41:45 AM

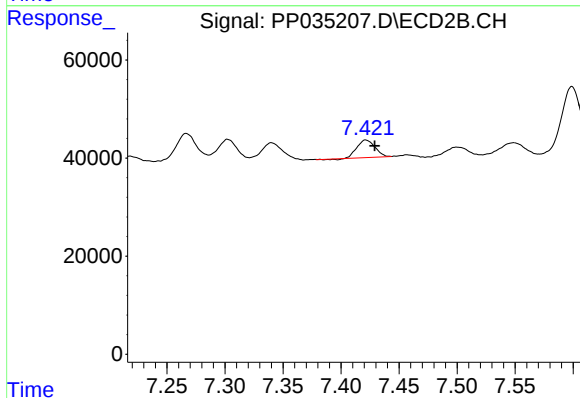


#33 AR-1260-3

R.T.: 7.421 min
Delta R.T.: -0.008 min
Response: 37989
Conc: 21.07 ng/ml

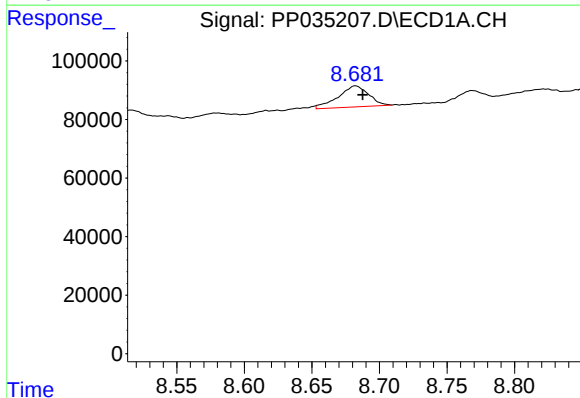


#34 AR-1260-4

R.T.: 8.681 min
Delta R.T.: -0.006 min
Response: 113010
Conc: 38.50 ng/ml m

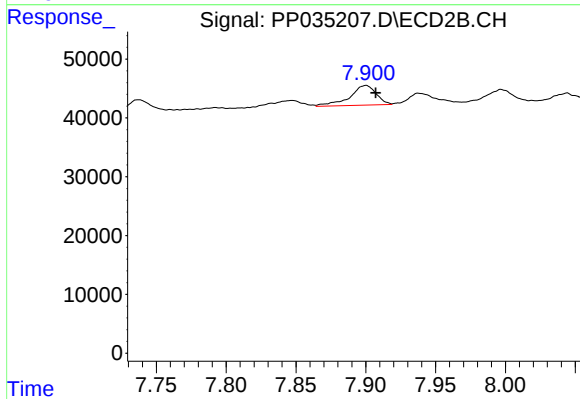

#34 AR-1260-4

R.T.: 7.900 min
Delta R.T.: -0.007 min
Response: 44237
Conc: 34.75 ng/ml

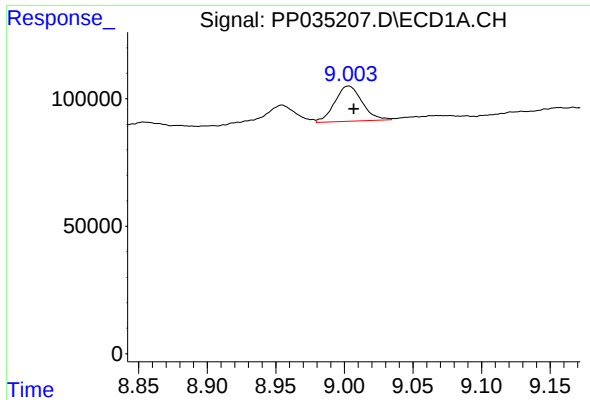


#35 AR-1260-5

R.T.: 9.003 min
Delta R.T.: -0.004 min
Response: 191666
Conc: 38.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-33-0-2.0

Manual Integrations
APPROVED

Ankita
4/27/2021 10:41:45 AM

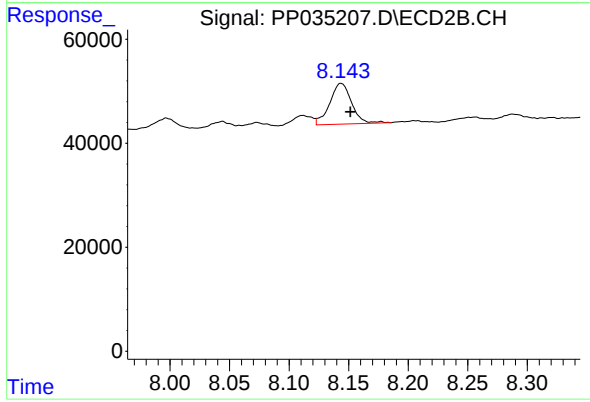

#35 AR-1260-5

R.T.: 8.144 min
Delta R.T.: -0.008 min
Response: 99936
Conc: 41.10 ng/ml