

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042321\
 Data File : PP035209.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Apr 2021 14:17
 Operator : DD\AJ
 Sample : M2107-17
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SB-34-0-2.0

Manual Integrations
 APPROVED

Ankita
 4/27/2021 10:41:46 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 16:49:10 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 21 17:37:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.839	4.246	1655939	1027420	20.322	19.951
2) SA Decachlor...	10.746	9.533	1417748	526567	22.435	22.162
Target Compounds						
31) L7 AR-1260-1	7.828	7.071	180080	136083	53.472	77.781 #
32) L7 AR-1260-2	8.093	7.265	902587	132230	265.121	74.178 #
33) L7 AR-1260-3	8.456	7.420	173243	114264	69.021	63.370
34) L7 AR-1260-4	8.685	7.898	206190	78839	70.246m	61.937
35) L7 AR-1260-5	9.005	8.143	339361	203236	68.981	83.592

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042321\
Data File : PP035209.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Apr 2021 14:17
Operator : DD\AJ
Sample : M2107-17
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
SB-34-0-2.0


Manual Integrations
APPROVED

Ankita
4/27/2021 10:41:46 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 16:49:10 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 21 17:37:28 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

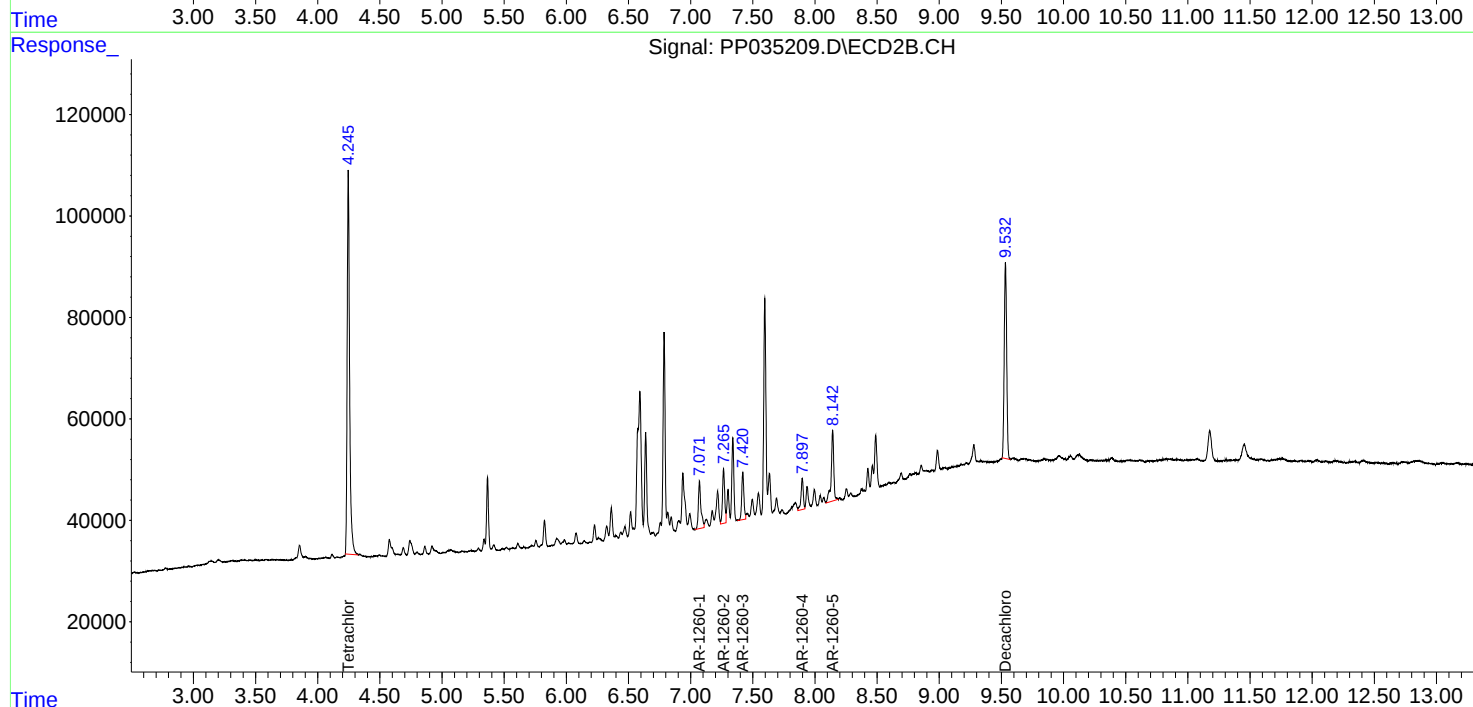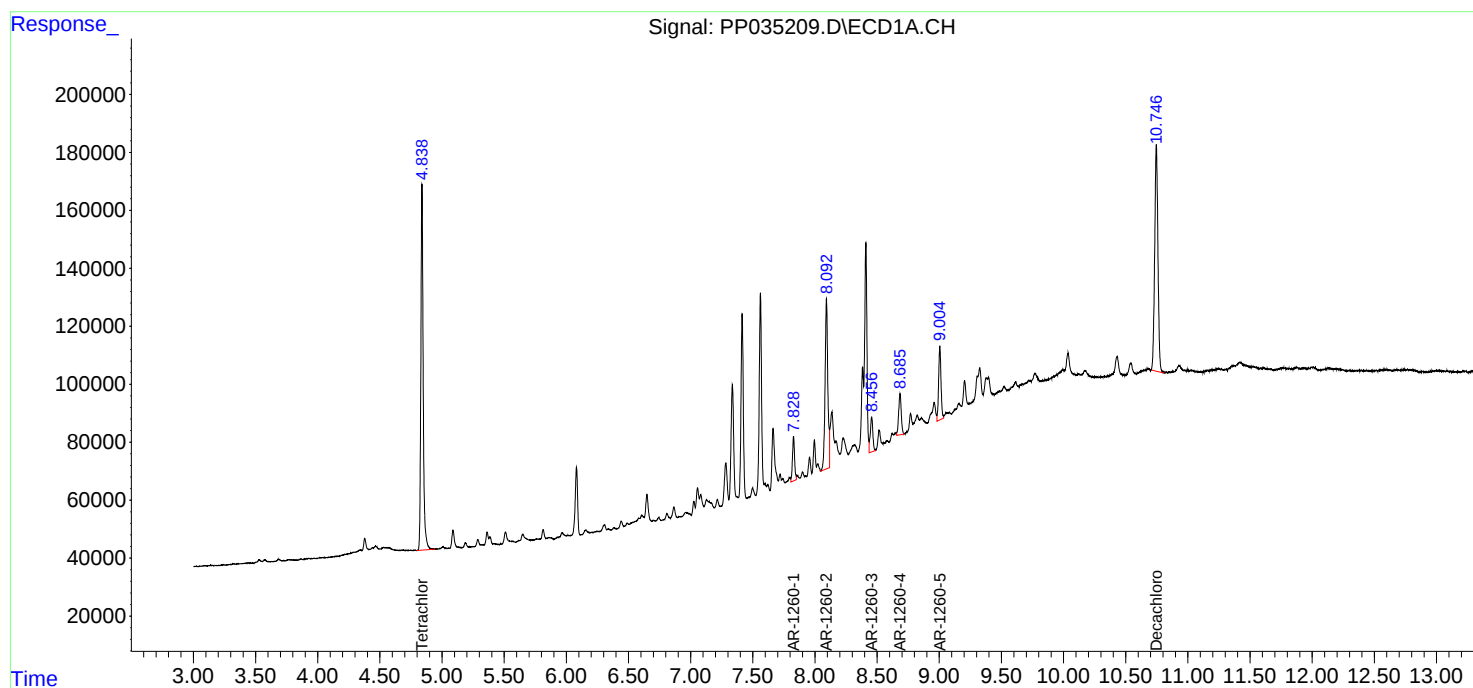

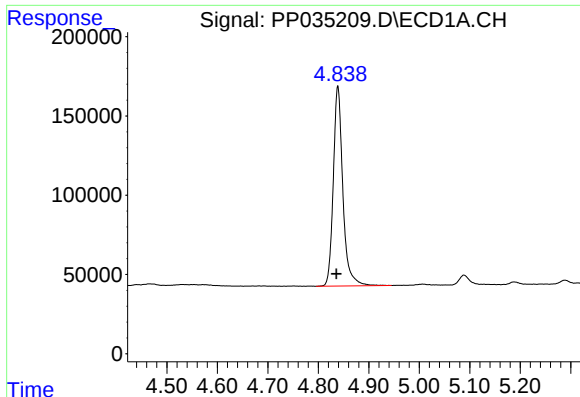


#1 Tetrachloro-m-xylene

R.T.: 4.839 min
Delta R.T.: 0.003 min
Response: 1655939
Conc: 20.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-34-0-2.0


Manual Integrations
APPROVED

Ankita
4/27/2021 10:41:46 AM

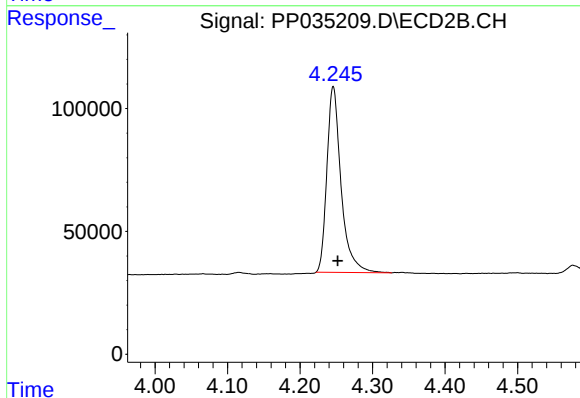


#1 Tetrachloro-m-xylene

R.T.: 4.246 min
Delta R.T.: -0.006 min
Response: 1027420
Conc: 19.95 ng/ml

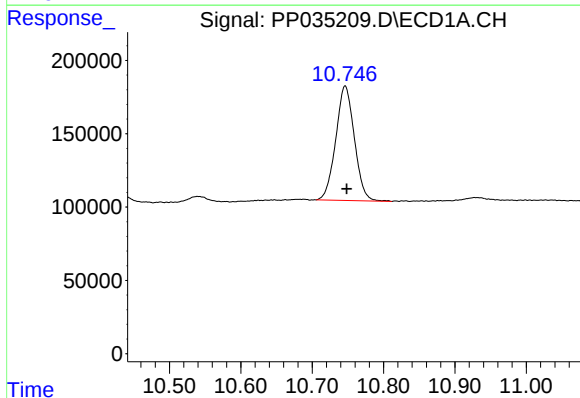


#2 Decachlorobiphenyl

R.T.: 10.746 min
Delta R.T.: -0.002 min
Response: 1417748
Conc: 22.44 ng/ml

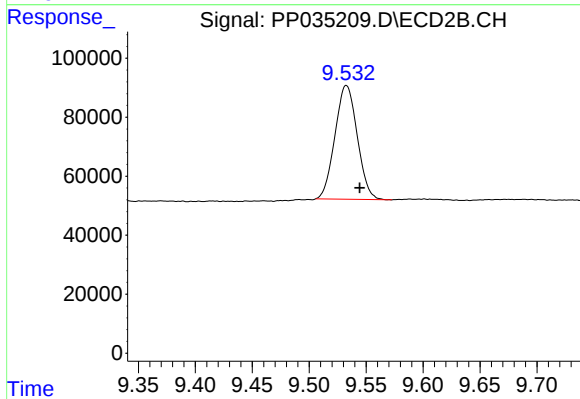

#2 Decachlorobiphenyl

R.T.: 9.533 min
Delta R.T.: -0.012 min
Response: 526567
Conc: 22.16 ng/ml

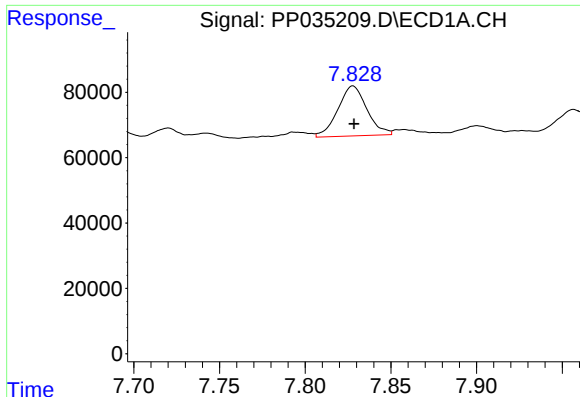


#31 AR-1260-1

R.T.: 7.828 min
Delta R.T.: 0.000 min
Response: 180080
Conc: 53.47 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-34-0-2.0


Manual Integrations
APPROVED

Ankita
4/27/2021 10:41:46 AM

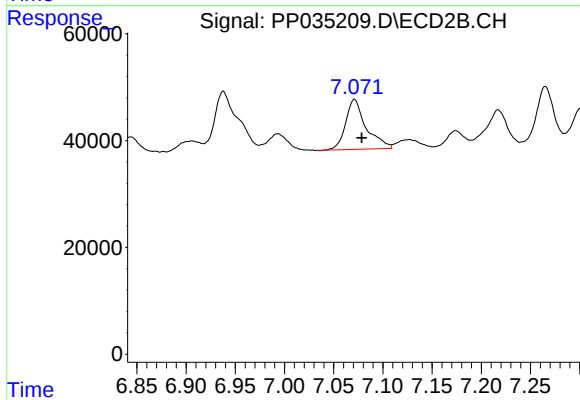


#31 AR-1260-1

R.T.: 7.071 min
Delta R.T.: -0.007 min
Response: 136083
Conc: 77.78 ng/ml

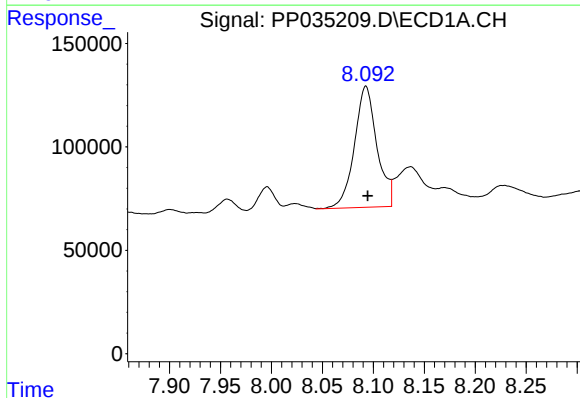


#32 AR-1260-2

R.T.: 8.093 min
Delta R.T.: -0.002 min
Response: 902587
Conc: 265.12 ng/ml

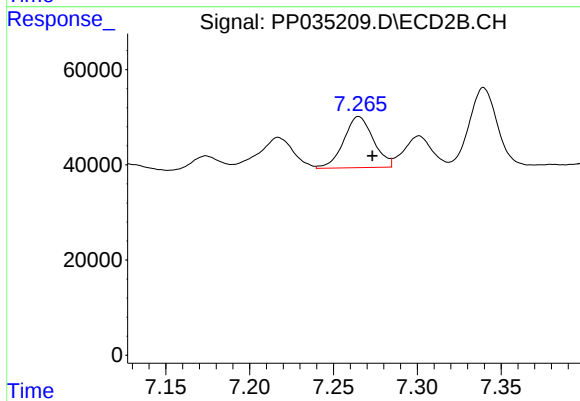

#32 AR-1260-2

R.T.: 7.265 min
Delta R.T.: -0.008 min
Response: 132230
Conc: 74.18 ng/ml

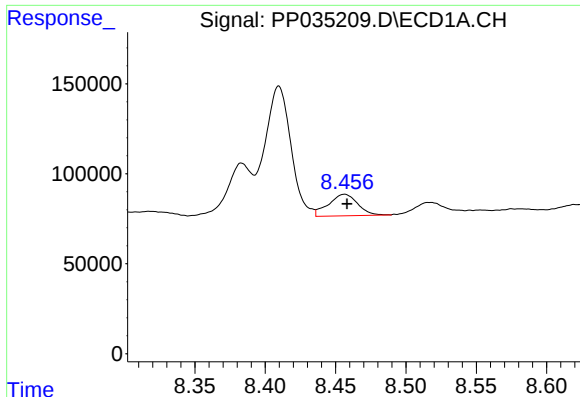


#33 AR-1260-3

R.T.: 8.456 min
Delta R.T.: -0.002 min
Response: 173243
Conc: 69.02 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-34-0-2.0


Manual Integrations
APPROVED

Ankita
4/27/2021 10:41:46 AM

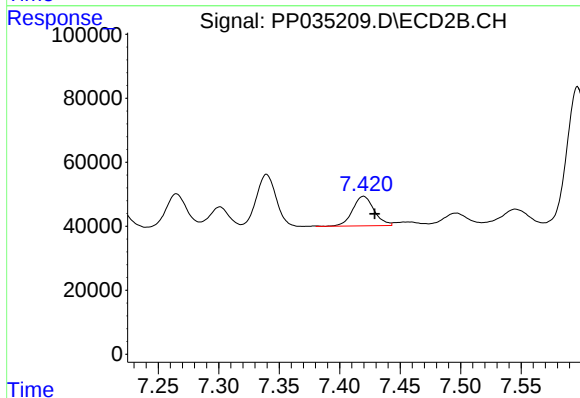


#33 AR-1260-3

R.T.: 7.420 min
Delta R.T.: -0.009 min
Response: 114264
Conc: 63.37 ng/ml

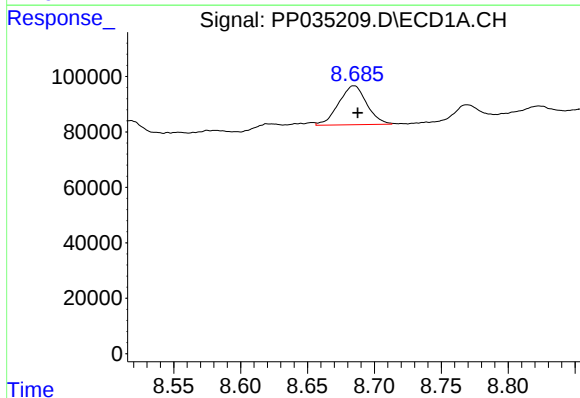


#34 AR-1260-4

R.T.: 8.685 min
Delta R.T.: -0.002 min
Response: 206190
Conc: 70.25 ng/ml m

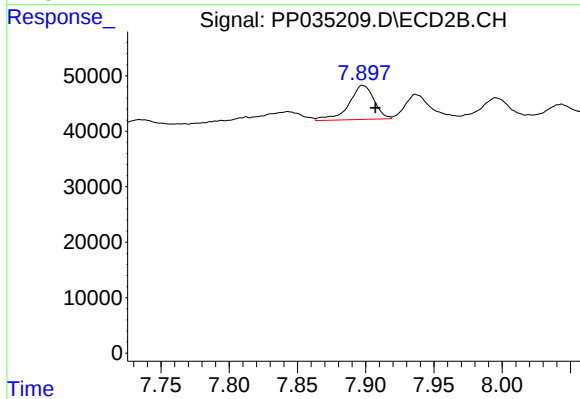

#34 AR-1260-4

R.T.: 7.898 min
Delta R.T.: -0.009 min
Response: 78839
Conc: 61.94 ng/ml

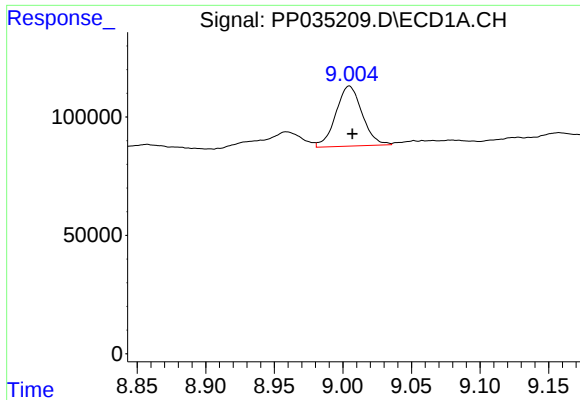


#35 AR-1260-5

R.T.: 9.005 min
Delta R.T.: -0.002 min
Response: 339361
Conc: 68.98 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-34-0-2.0

Manual Integrations
APPROVED

Ankita
4/27/2021 10:41:46 AM

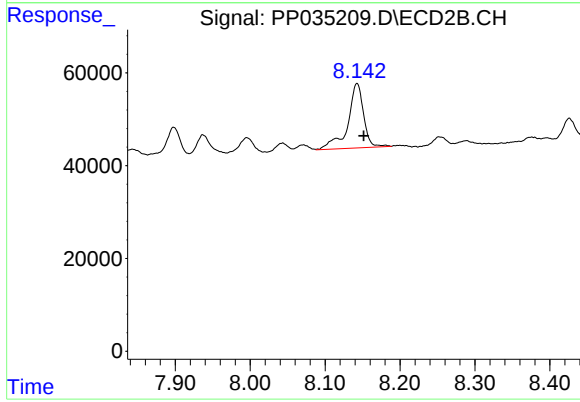

#35 AR-1260-5

R.T.: 8.143 min
Delta R.T.: -0.009 min
Response: 203236
Conc: 83.59 ng/ml