

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042321\
 Data File : PP035211.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Apr 2021 14:51
 Operator : DD\AJ
 Sample : M2107-20
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SB-35-0-2.0

Manual Integrations
 APPROVED

Ankita
 4/27/2021 10:41:48 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 16:50:02 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 21 17:37:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.839	4.247	1870912	1149557	22.960	22.323
2) SA Decachlor...	10.746	9.533	1839546	674138	29.110	28.373
Target Compounds						
31) L7 AR-1260-1	7.829	7.071	82096	58910	24.377	33.672 #
32) L7 AR-1260-2	8.093	7.266	284806	66782	83.658	37.463 #
33) L7 AR-1260-3	8.458	7.421	71076	35768	28.317	19.837 #
34) L7 AR-1260-4	8.685	7.899	102141	39624	34.798m	31.129
35) L7 AR-1260-5	9.006	8.143	150724	78157	30.637	32.147

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042321\
Data File : PP035211.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Apr 2021 14:51
Operator : DD\AJ
Sample : M2107-20
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
SB-35-0-2.0


Manual Integrations
APPROVED

Ankita
4/27/2021 10:41:48 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 16:50:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 21 17:37:28 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

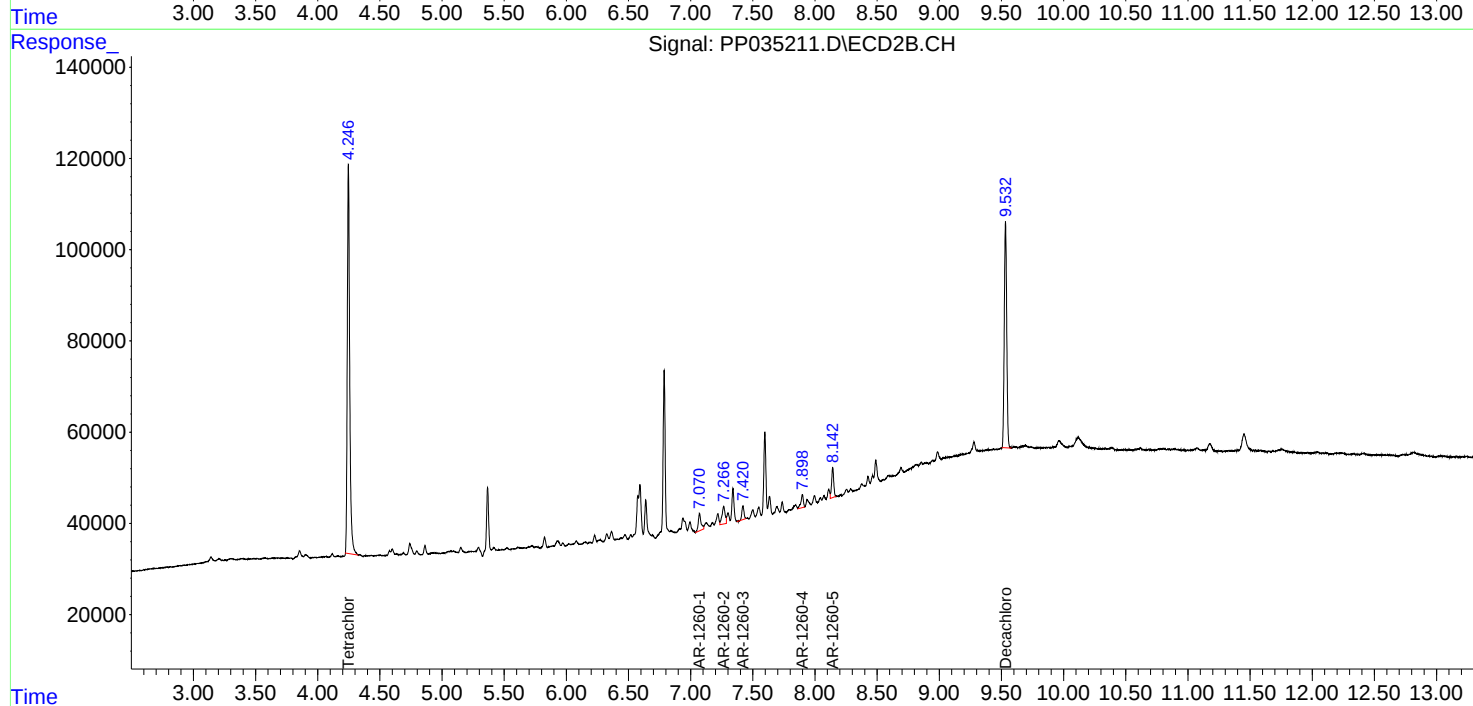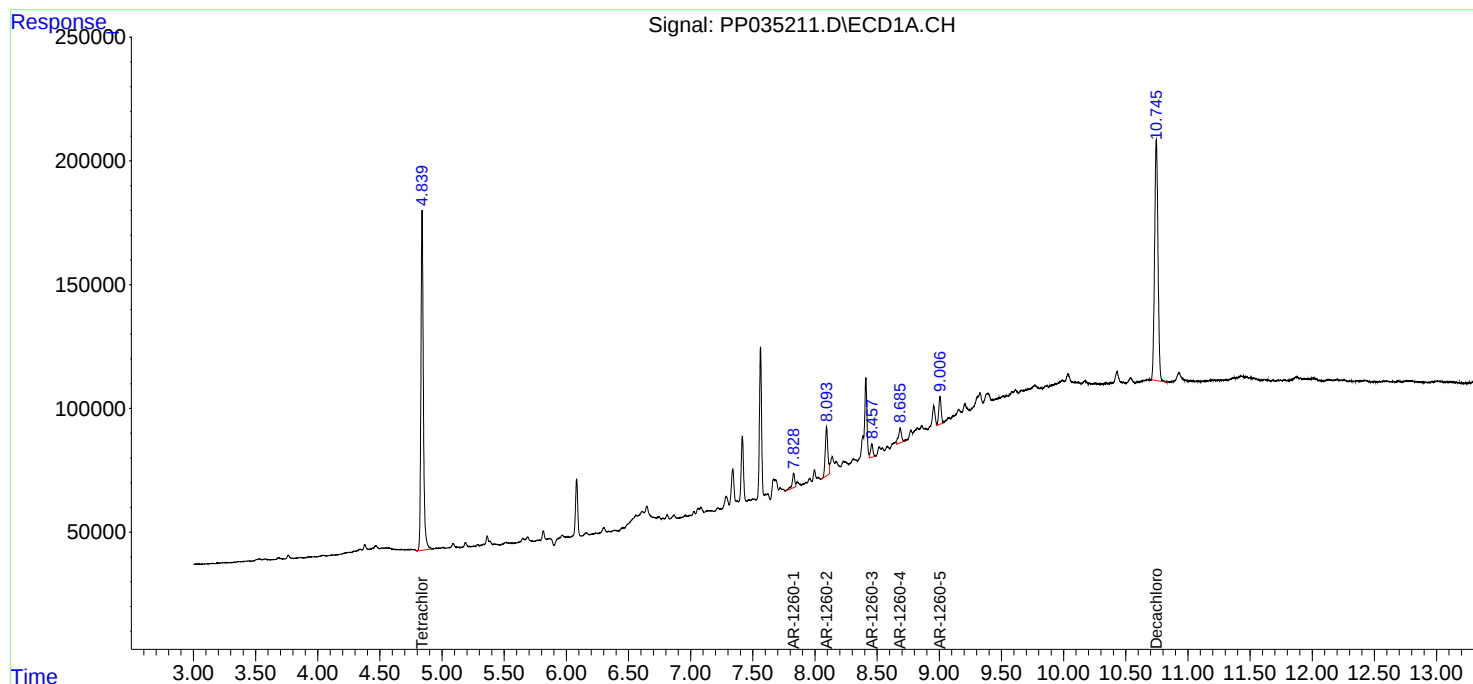

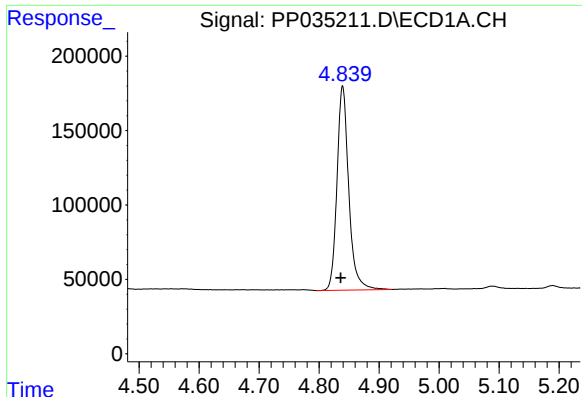


#1 Tetrachloro-m-xylene

R.T.: 4.839 min
Delta R.T.: 0.003 min
Response: 1870912
Conc: 22.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-35-0-2.0


Manual Integrations
APPROVED

Ankita
4/27/2021 10:41:48 AM

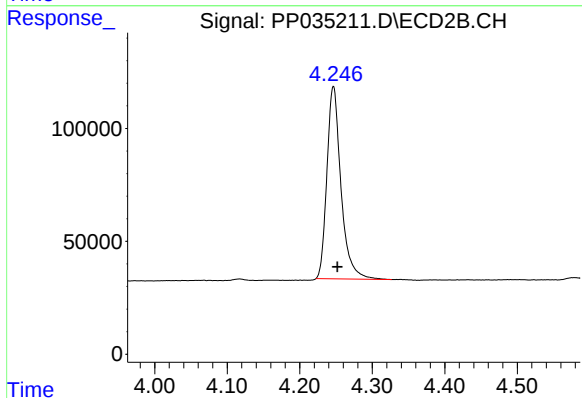


#1 Tetrachloro-m-xylene

R.T.: 4.247 min
Delta R.T.: -0.006 min
Response: 1149557
Conc: 22.32 ng/ml

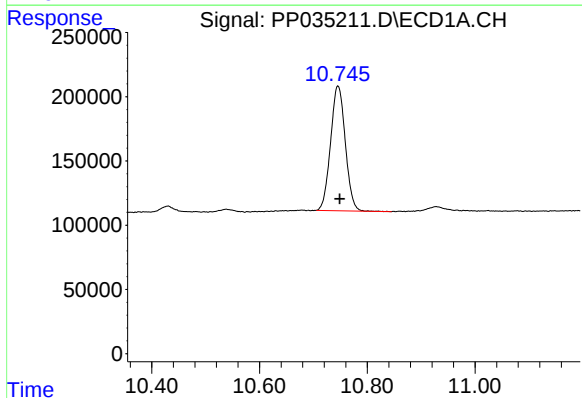


#2 Decachlorobiphenyl

R.T.: 10.746 min
Delta R.T.: -0.003 min
Response: 1839546
Conc: 29.11 ng/ml

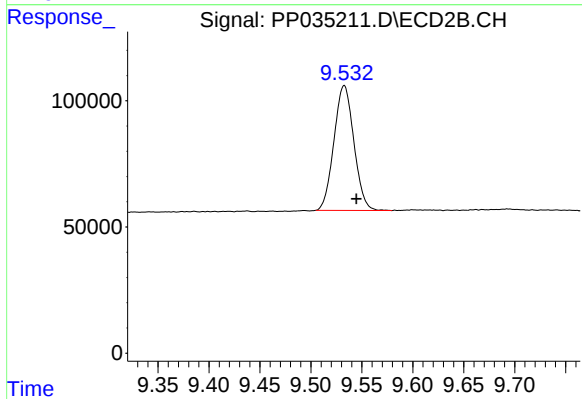

#2 Decachlorobiphenyl

R.T.: 9.533 min
Delta R.T.: -0.012 min
Response: 674138
Conc: 28.37 ng/ml

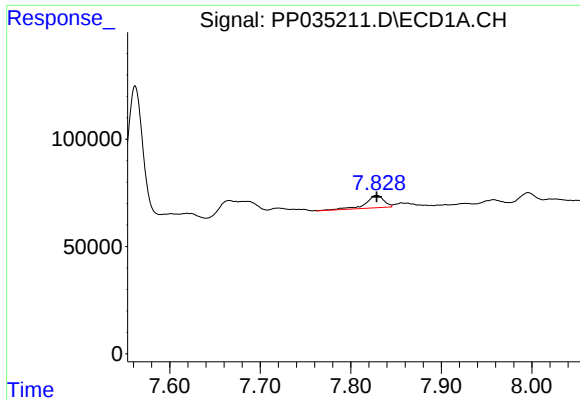


#31 AR-1260-1

R.T.: 7.829 min
Delta R.T.: 0.000 min
Response: 82096
Conc: 24.38 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-35-0-2.0


Manual Integrations
APPROVED

Ankita
4/27/2021 10:41:48 AM

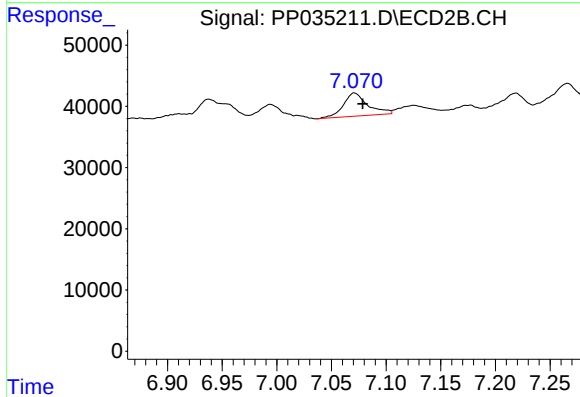


#31 AR-1260-1

R.T.: 7.071 min
Delta R.T.: -0.008 min
Response: 58910
Conc: 33.67 ng/ml

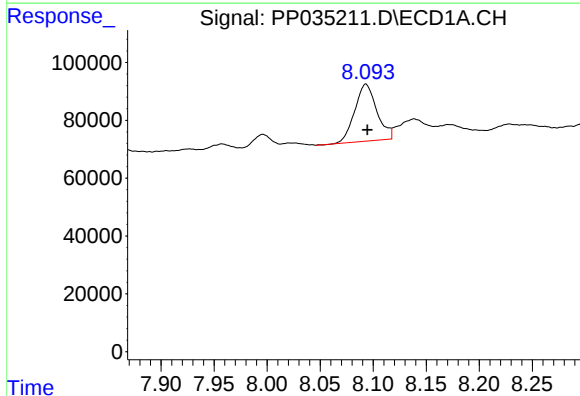


#32 AR-1260-2

R.T.: 8.093 min
Delta R.T.: -0.002 min
Response: 284806
Conc: 83.66 ng/ml

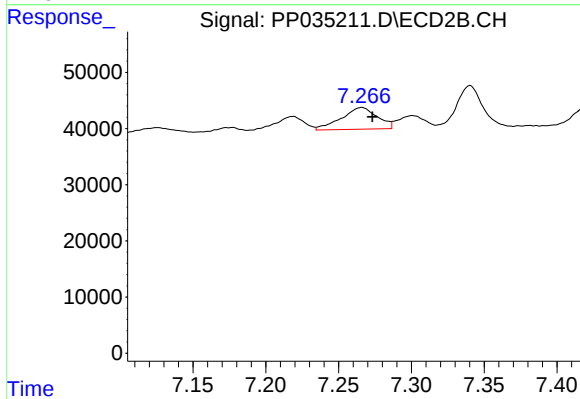

#32 AR-1260-2

R.T.: 7.266 min
Delta R.T.: -0.007 min
Response: 66782
Conc: 37.46 ng/ml

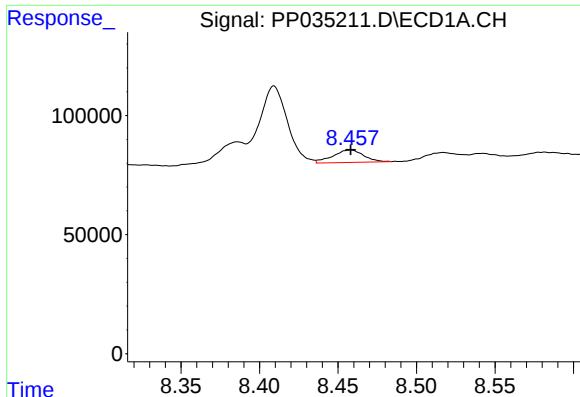


#33 AR-1260-3

R.T.: 8.458 min
Delta R.T.: 0.000 min
Response: 71076
Conc: 28.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-35-0-2.0


Manual Integrations
APPROVED

Ankita
4/27/2021 10:41:48 AM

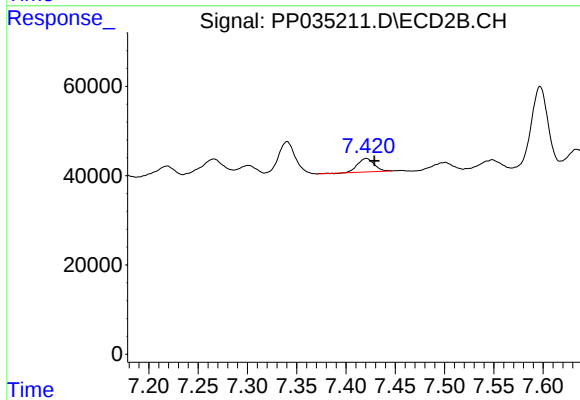


#33 AR-1260-3

R.T.: 7.421 min
Delta R.T.: -0.008 min
Response: 35768
Conc: 19.84 ng/ml

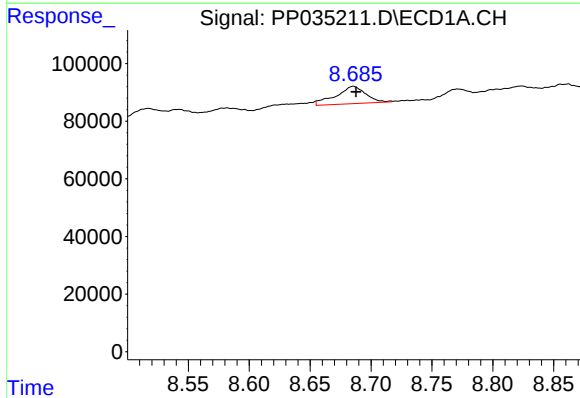


#34 AR-1260-4

R.T.: 8.685 min
Delta R.T.: -0.003 min
Response: 102141
Conc: 34.80 ng/ml m

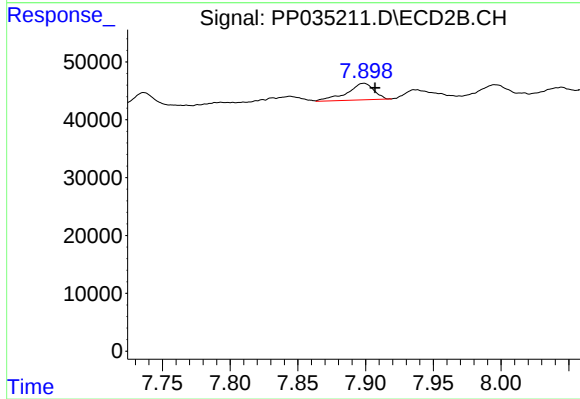

#34 AR-1260-4

R.T.: 7.899 min
Delta R.T.: -0.008 min
Response: 39624
Conc: 31.13 ng/ml

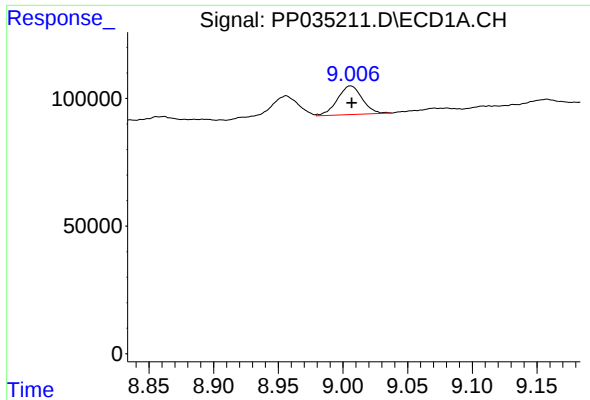


#35 AR-1260-5

R.T.: 9.006 min
Delta R.T.: 0.000 min
Response: 150724
Conc: 30.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-35-0-2.0

Manual Integrations
APPROVED

Ankita
4/27/2021 10:41:48 AM

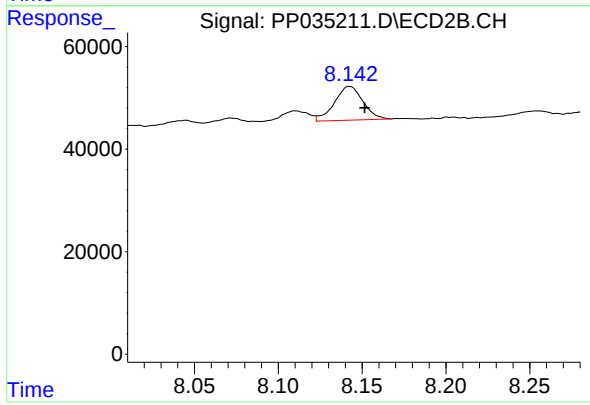

#35 AR-1260-5

R.T.: 8.143 min
Delta R.T.: -0.009 min
Response: 78157
Conc: 32.15 ng/ml