

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042321\
 Data File : PP035212.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Apr 2021 15:07
 Operator : DD\AJ
 Sample : M2107-22
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SB-35-10.5-11.0

Manual Integrations
 APPROVED

Ankita
 4/27/2021 10:41:50 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 16:50:25 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 21 17:37:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.839	4.247	1401656	887838	17.201	17.241
2) SA Decachlor...	10.747	9.533	3567403	1273968	56.452	53.618

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042321\
Data File : PP035212.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Apr 2021 15:07
Operator : DD\AJ
Sample : M2107-22
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
SB-35-10.5-11.0


Manual Integrations
APPROVED

Ankita
4/27/2021 10:41:50 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 16:50:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 21 17:37:28 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

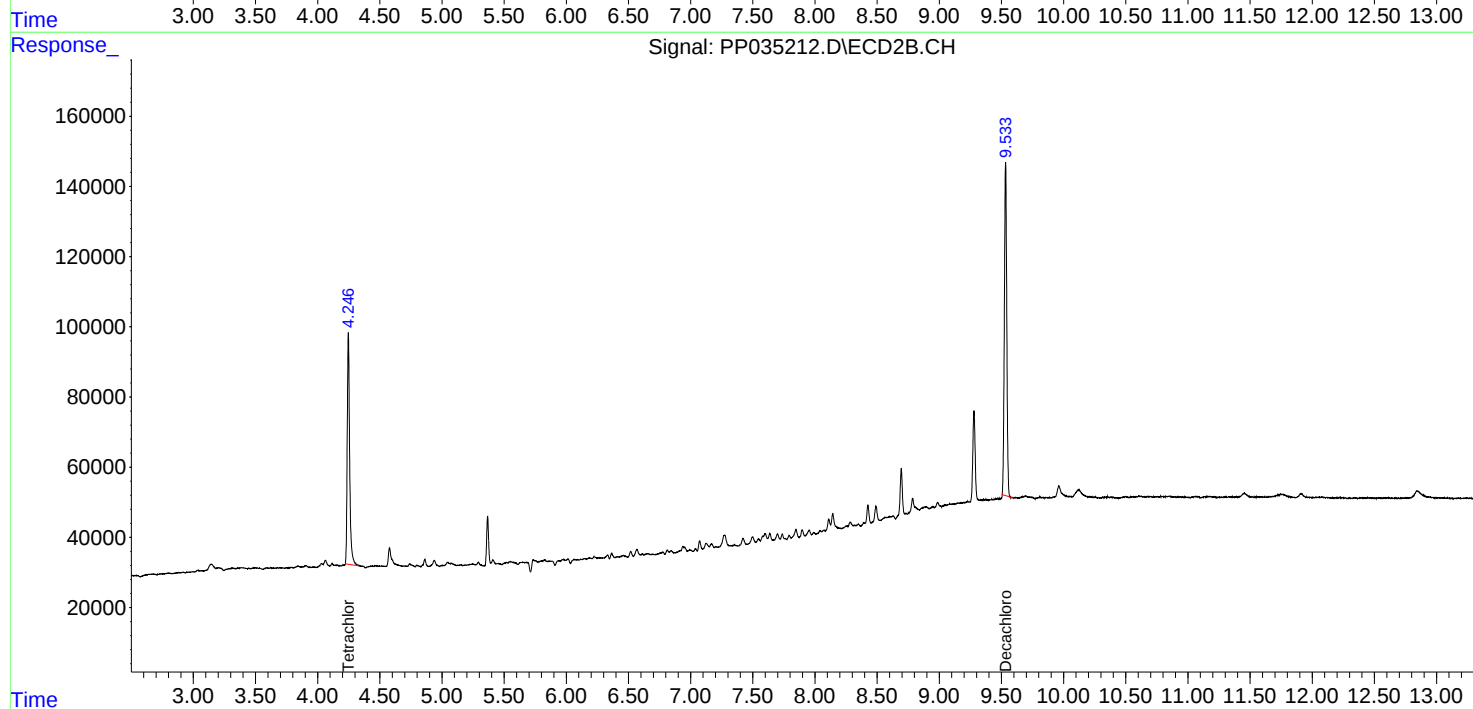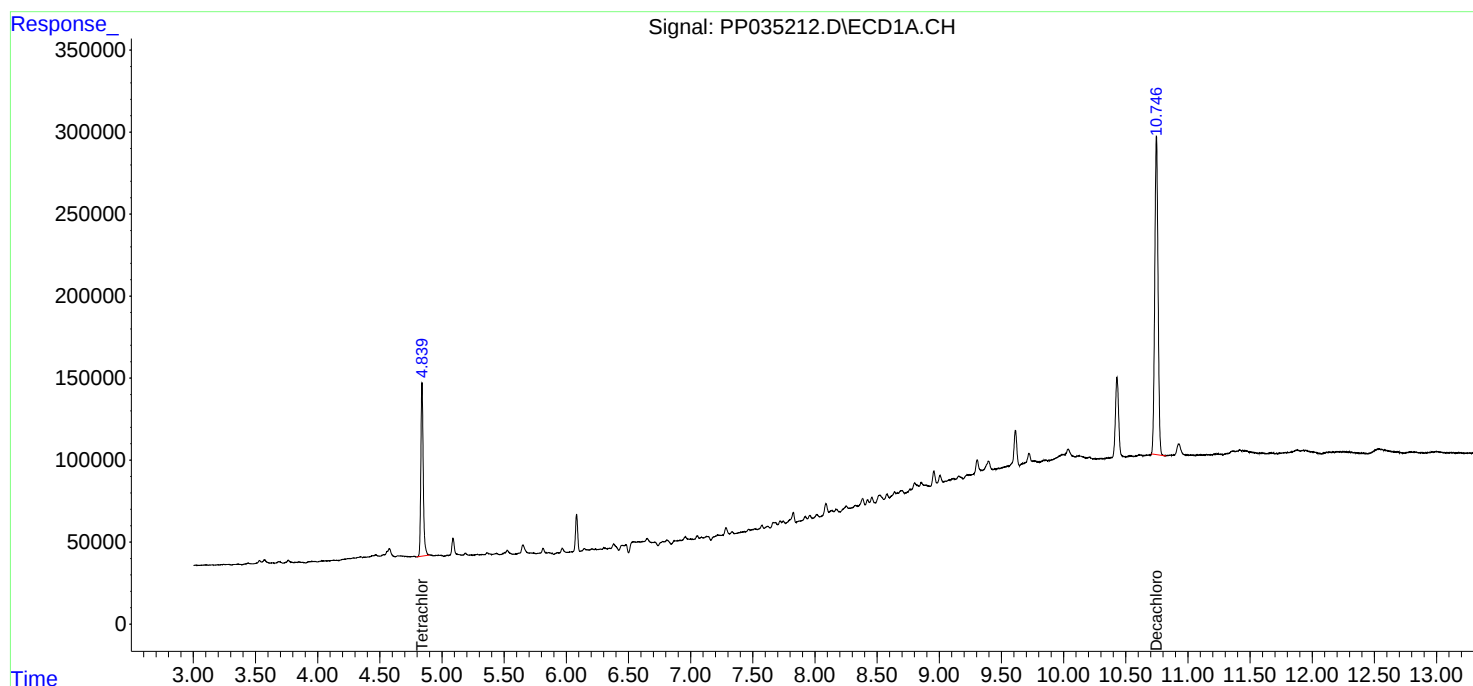

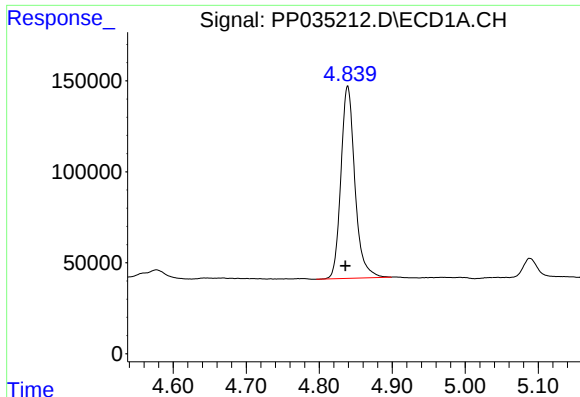


#1 Tetrachloro-m-xylene

R.T.: 4.839 min
Delta R.T.: 0.003 min
Response: 1401656
Conc: 17.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-35-10.5-11.0


Manual Integrations
APPROVED

Ankita
4/27/2021 10:41:50 AM

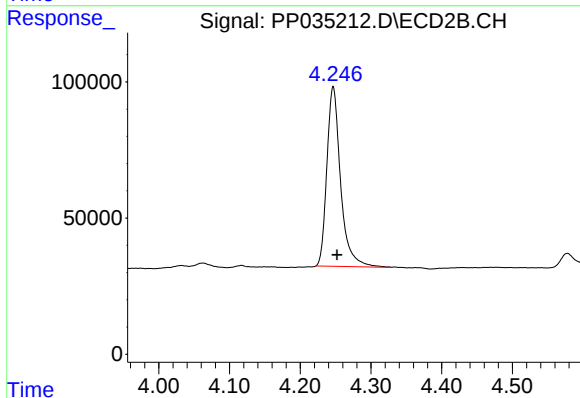


#1 Tetrachloro-m-xylene

R.T.: 4.247 min
Delta R.T.: -0.006 min
Response: 887838
Conc: 17.24 ng/ml

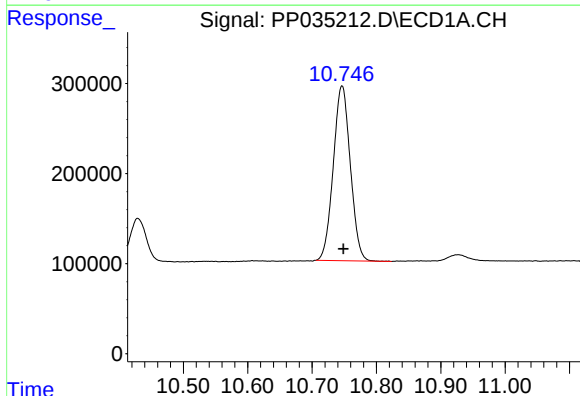

#2 Decachlorobiphenyl

R.T.: 10.747 min
Delta R.T.: -0.002 min
Response: 3567403
Conc: 56.45 ng/ml

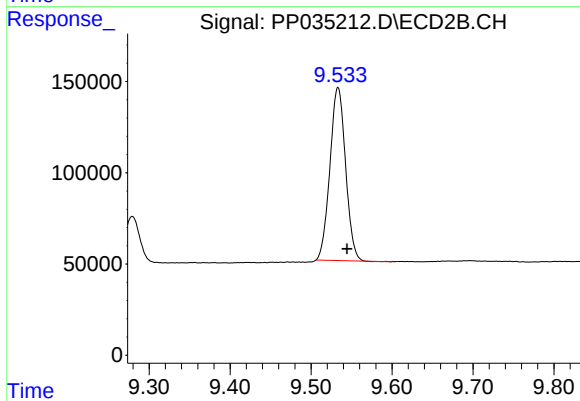

#2 Decachlorobiphenyl

R.T.: 9.533 min
Delta R.T.: -0.011 min
Response: 1273968
Conc: 53.62 ng/ml