

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042321\
 Data File : PP035217.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Apr 2021 16:32
 Operator : DD\AJ
 Sample : M2111-03
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 S-3

Manual Integrations
 APPROVED

Ankita
 4/27/2021 10:41:52 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 17:56:18 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 21 17:37:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.839	4.246	1804043	1105814	22.139	21.473
2) SA Decachlor...	10.745	9.532	1683702	624191	26.644	26.271
Target Compounds						
31) L7 AR-1260-1	7.825	7.071	67723	44247	20.109m	25.291m#
32) L7 AR-1260-2	8.092	7.265	235637	29505	69.215	16.552 #
33) L7 AR-1260-3	8.458	7.422	57199	33741	22.788	18.712
34) L7 AR-1260-4	8.686	7.899	70422	28028	23.992	22.019m
35) L7 AR-1260-5	9.004	8.143	117377	71289	23.859	29.322

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042321\
Data File : PP035217.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Apr 2021 16:32
Operator : DD\AJ
Sample : M2111-03
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
S-3


Manual Integrations
APPROVED

Ankita
4/27/2021 10:41:52 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 17:56:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 21 17:37:28 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

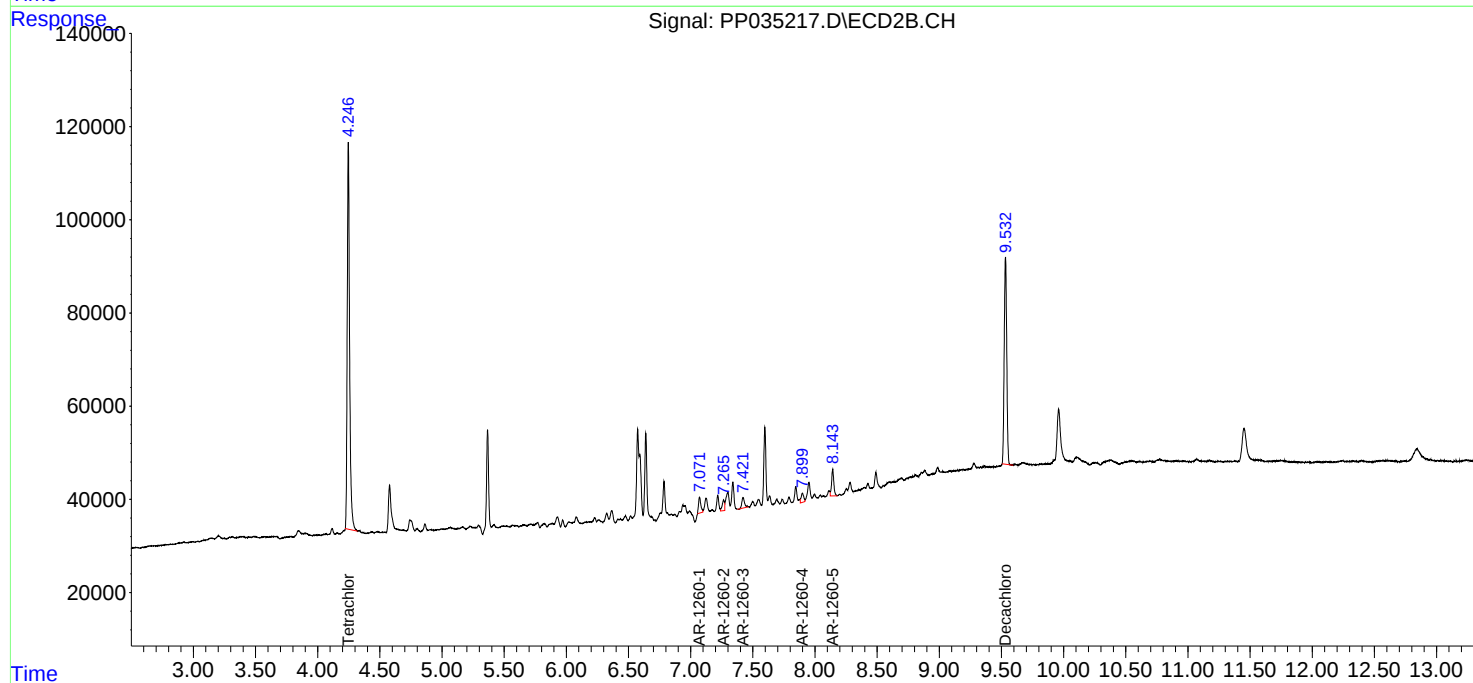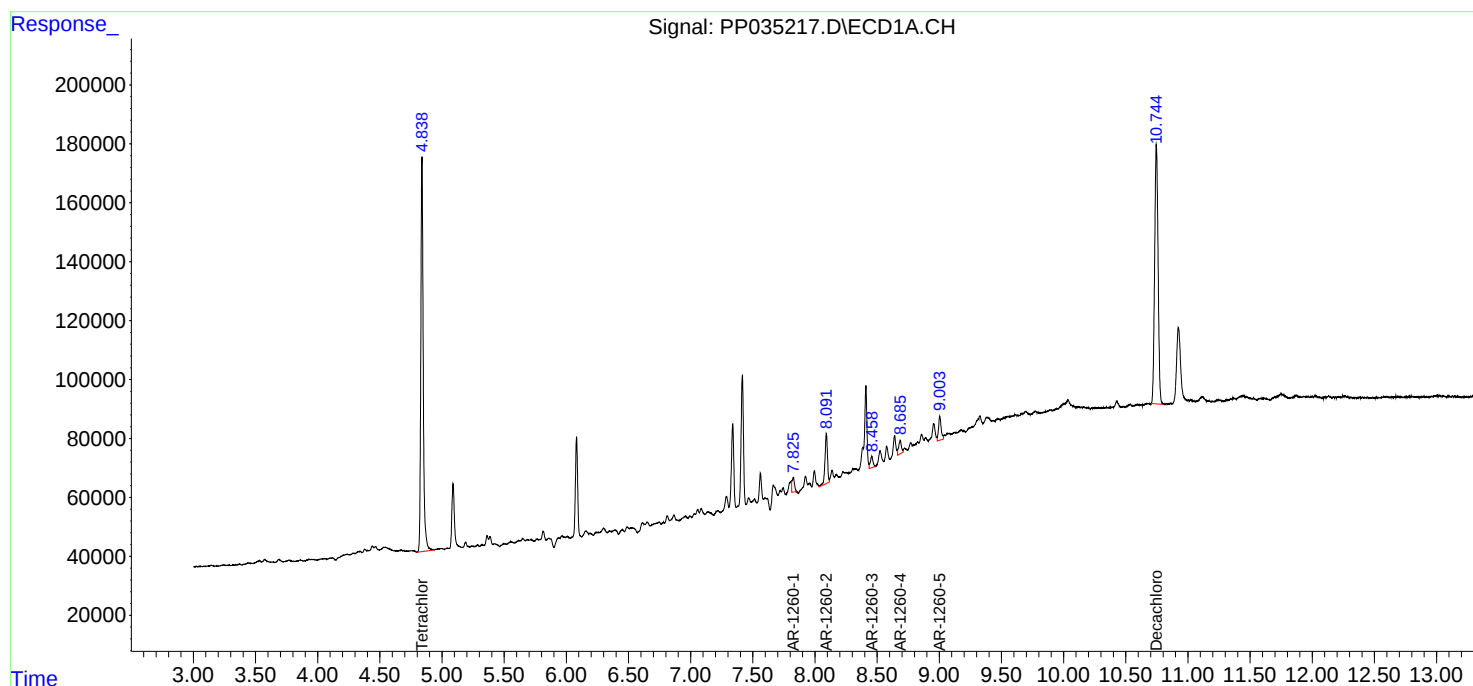

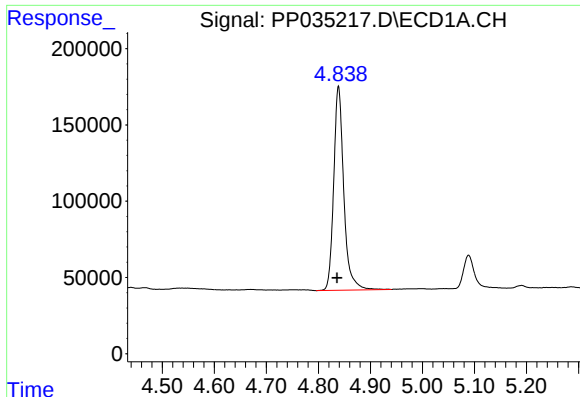


#1 Tetrachloro-m-xylene

R.T.: 4.839 min
Delta R.T.: 0.003 min
Response: 1804043
Conc: 22.14 ng/ml

Instrument :
ECD_P
ClientSampleId :
S-3


Manual Integrations
APPROVED

Ankita
4/27/2021 10:41:52 AM

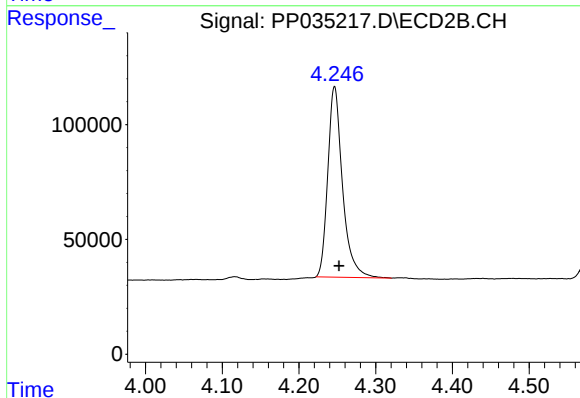


#1 Tetrachloro-m-xylene

R.T.: 4.246 min
Delta R.T.: -0.006 min
Response: 1105814
Conc: 21.47 ng/ml

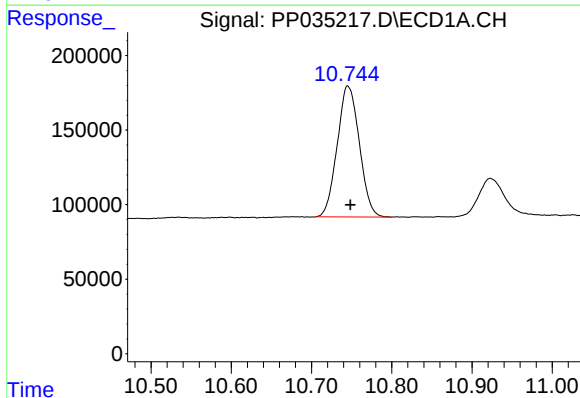


#2 Decachlorobiphenyl

R.T.: 10.745 min
Delta R.T.: -0.003 min
Response: 1683702
Conc: 26.64 ng/ml

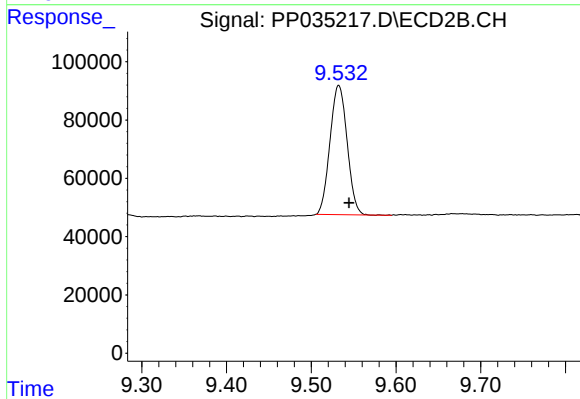

#2 Decachlorobiphenyl

R.T.: 9.532 min
Delta R.T.: -0.012 min
Response: 624191
Conc: 26.27 ng/ml

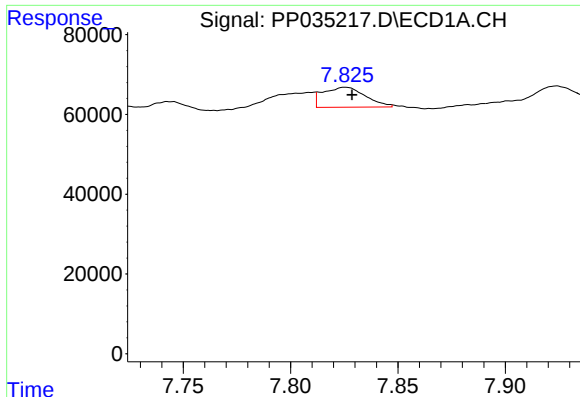


#31 AR-1260-1

R.T.: 7.825 min
Delta R.T.: -0.003 min
Response: 67723
Conc: 20.11 ng/ml m

Instrument :
ECD_P
ClientSampleId :
S-3


Manual Integrations
APPROVED

Ankita
4/27/2021 10:41:52 AM

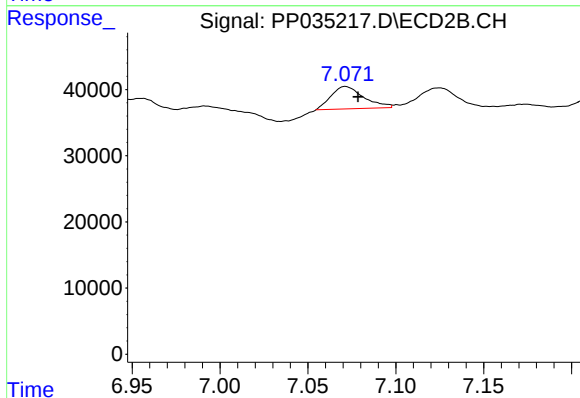


#31 AR-1260-1

R.T.: 7.071 min
Delta R.T.: -0.008 min
Response: 44247
Conc: 25.29 ng/ml m

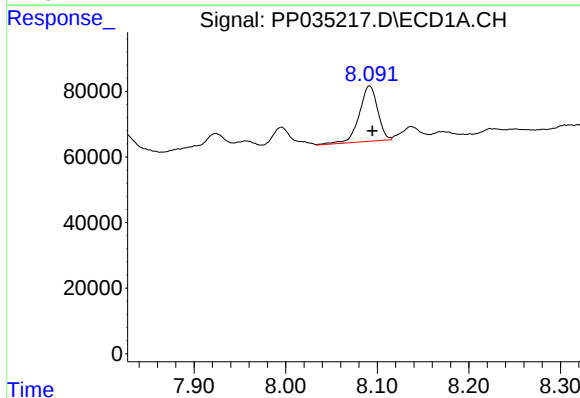


#32 AR-1260-2

R.T.: 8.092 min
Delta R.T.: -0.003 min
Response: 235637
Conc: 69.21 ng/ml

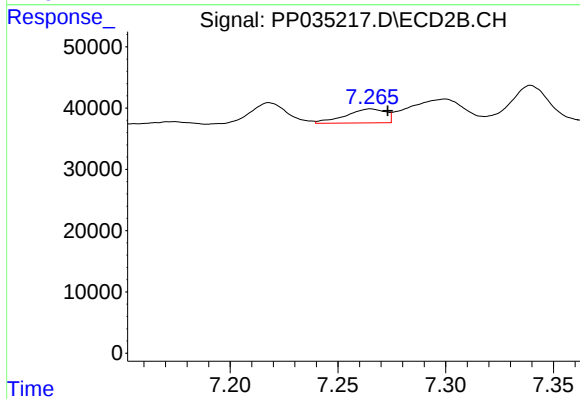

#32 AR-1260-2

R.T.: 7.265 min
Delta R.T.: -0.008 min
Response: 29505
Conc: 16.55 ng/ml

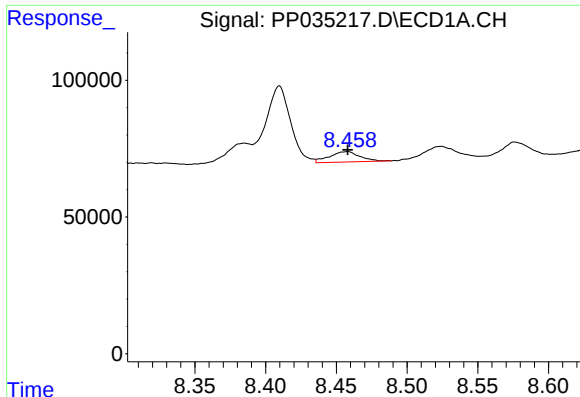


#33 AR-1260-3

R.T.: 8.458 min
Delta R.T.: 0.000 min
Response: 57199
Conc: 22.79 ng/ml

Instrument :
ECD_P
ClientSampleId :
S-3


Manual Integrations
APPROVED

Ankita
4/27/2021 10:41:52 AM

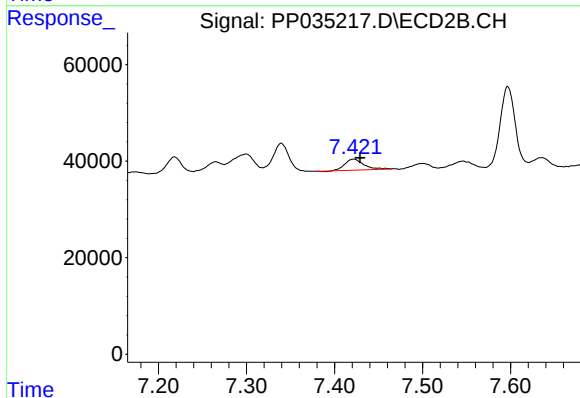


#33 AR-1260-3

R.T.: 7.422 min
Delta R.T.: -0.007 min
Response: 33741
Conc: 18.71 ng/ml

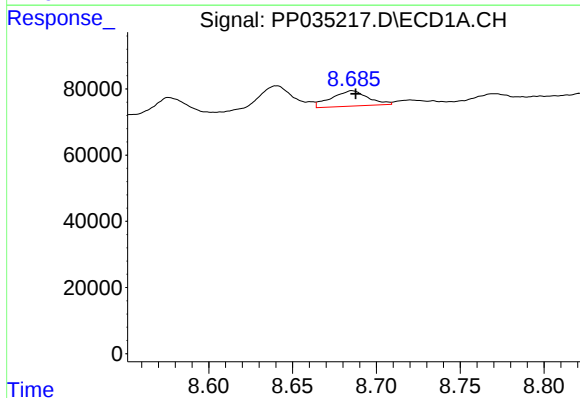


#34 AR-1260-4

R.T.: 8.686 min
Delta R.T.: -0.002 min
Response: 70422
Conc: 23.99 ng/ml

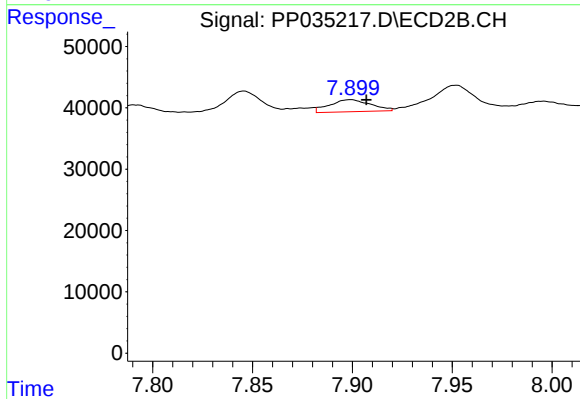

#34 AR-1260-4

R.T.: 7.899 min
Delta R.T.: -0.008 min
Response: 28028
Conc: 22.02 ng/ml m

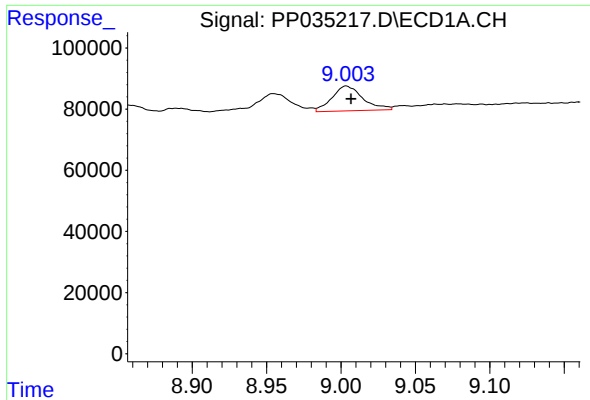


#35 AR-1260-5

R.T.: 9.004 min
Delta R.T.: -0.003 min
Response: 117377
Conc: 23.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
S-3

Manual Integrations
APPROVED

Ankita
4/27/2021 10:41:52 AM

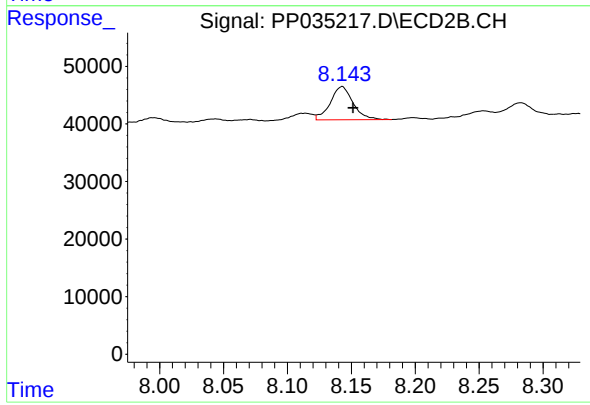

#35 AR-1260-5

R.T.: 8.143 min
Delta R.T.: -0.009 min
Response: 71289
Conc: 29.32 ng/ml