

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042321\
 Data File : PP035232.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Apr 2021 20:44
 Operator : DD\AJ
 Sample : M2149-16
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SB-40-9.5-10.0-DUP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 24 01:04:39 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 21 17:37:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.839	4.246	1631749	1041229	20.025	20.219
2) SA Decachlor...	10.746	9.532	896097	365596	14.180	15.387

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042321\
Data File : PP035232.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Apr 2021 20:44
Operator : DD\AJ
Sample : M2149-16
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
SB-40-9.5-10.0-DUP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 24 01:04:39 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 21 17:37:28 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

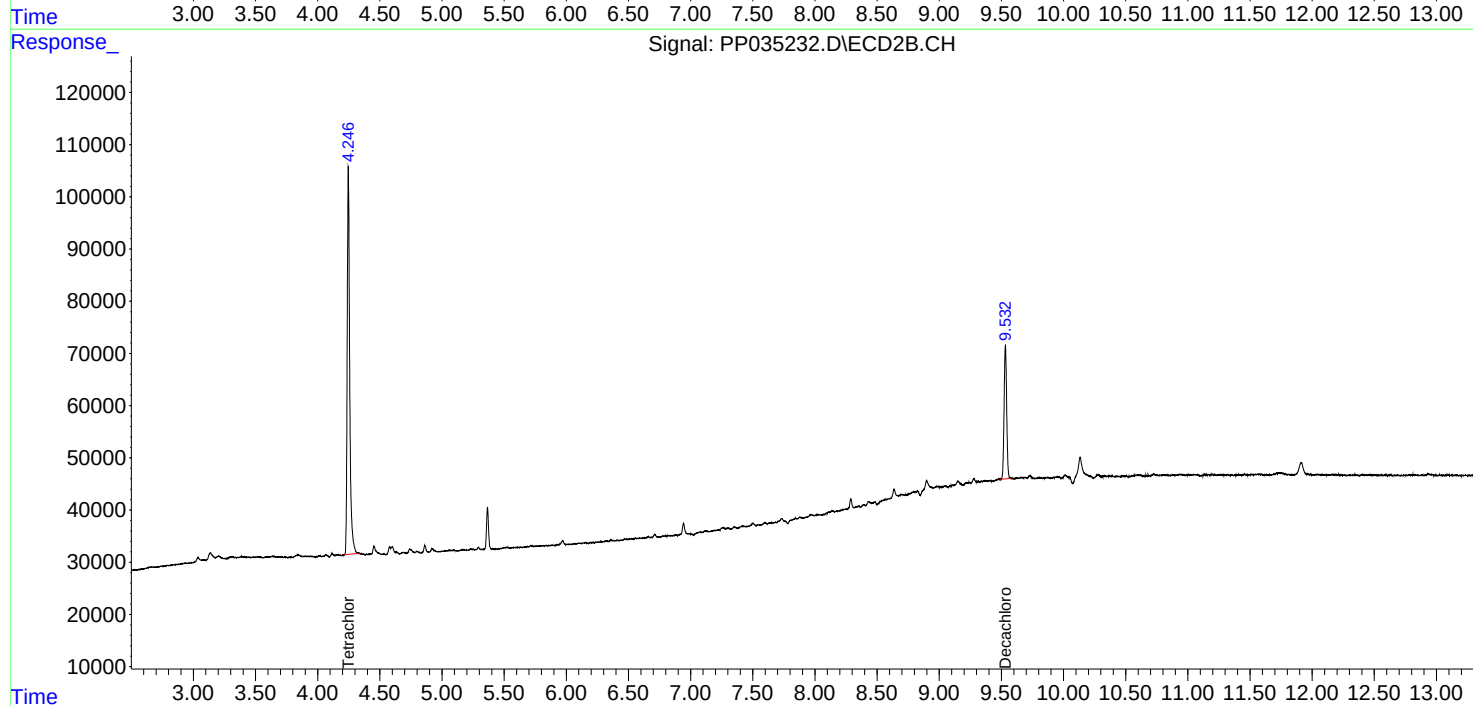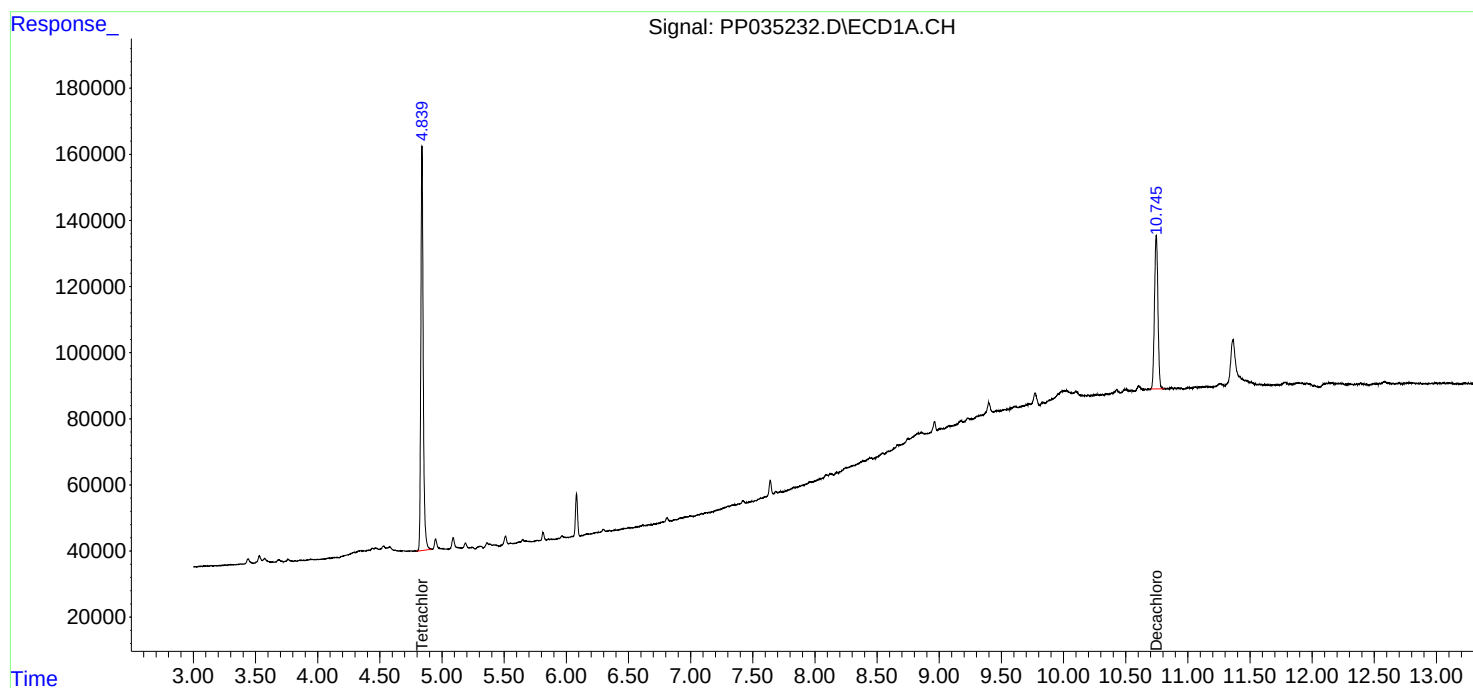


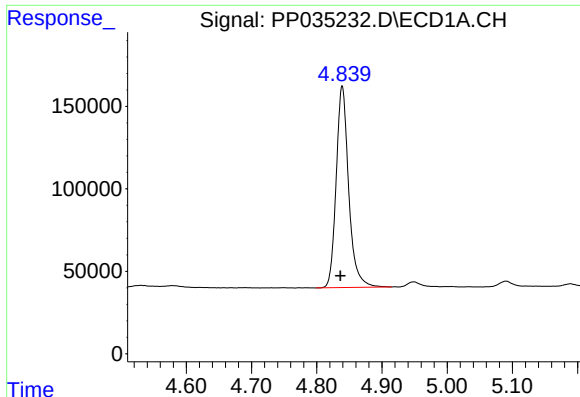

#1 Tetrachloro-m-xylene


R.T.: 4.839 min
Delta R.T.: 0.003 min
Response: 1631749
Conc: 20.03 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-40-9.5-10.0-DUP

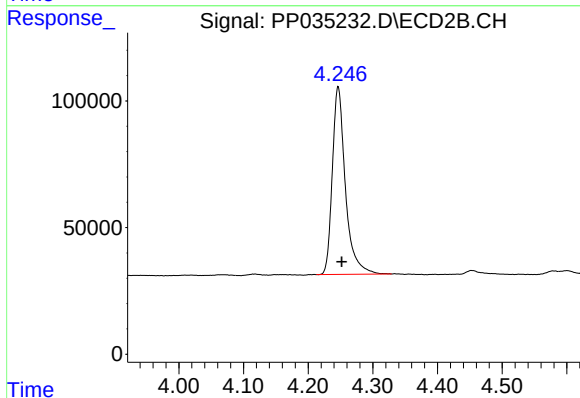


#1 Tetrachloro-m-xylene

R.T.: 4.246 min
Delta R.T.: -0.006 min
Response: 1041229
Conc: 20.22 ng/ml

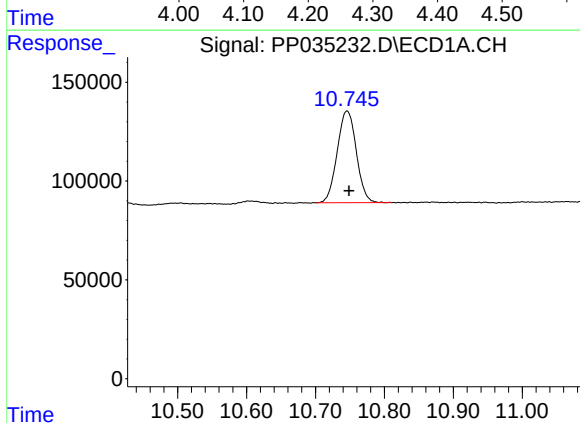

#2 Decachlorobiphenyl

R.T.: 10.746 min
Delta R.T.: -0.003 min
Response: 896097
Conc: 14.18 ng/ml

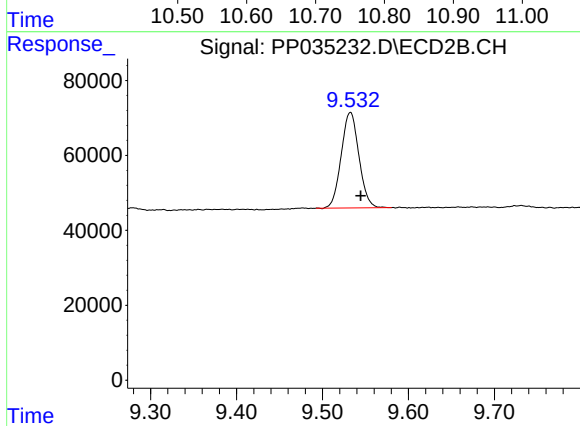

#2 Decachlorobiphenyl

R.T.: 9.532 min
Delta R.T.: -0.012 min
Response: 365596
Conc: 15.39 ng/ml