

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042421\
 Data File : PP035252.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Apr 2021 11:31
 Operator : DD\AJ
 Sample : M2150-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TWP-20

Manual Integrations
 APPROVED

Ankita
 4/27/2021 10:54:36 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 02:12:01 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 21 17:37:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.839	4.259	785083	6521314	9.635	126.635m#
2) SA Decachlor...	10.743	9.527	899276	327352	14.231	13.777

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042421\
Data File : PP035252.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Apr 2021 11:31
Operator : DD\AJ
Sample : M2150-01
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
TWP-20


Manual Integrations
APPROVED

Ankita
4/27/2021 10:54:36 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 02:12:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 21 17:37:28 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

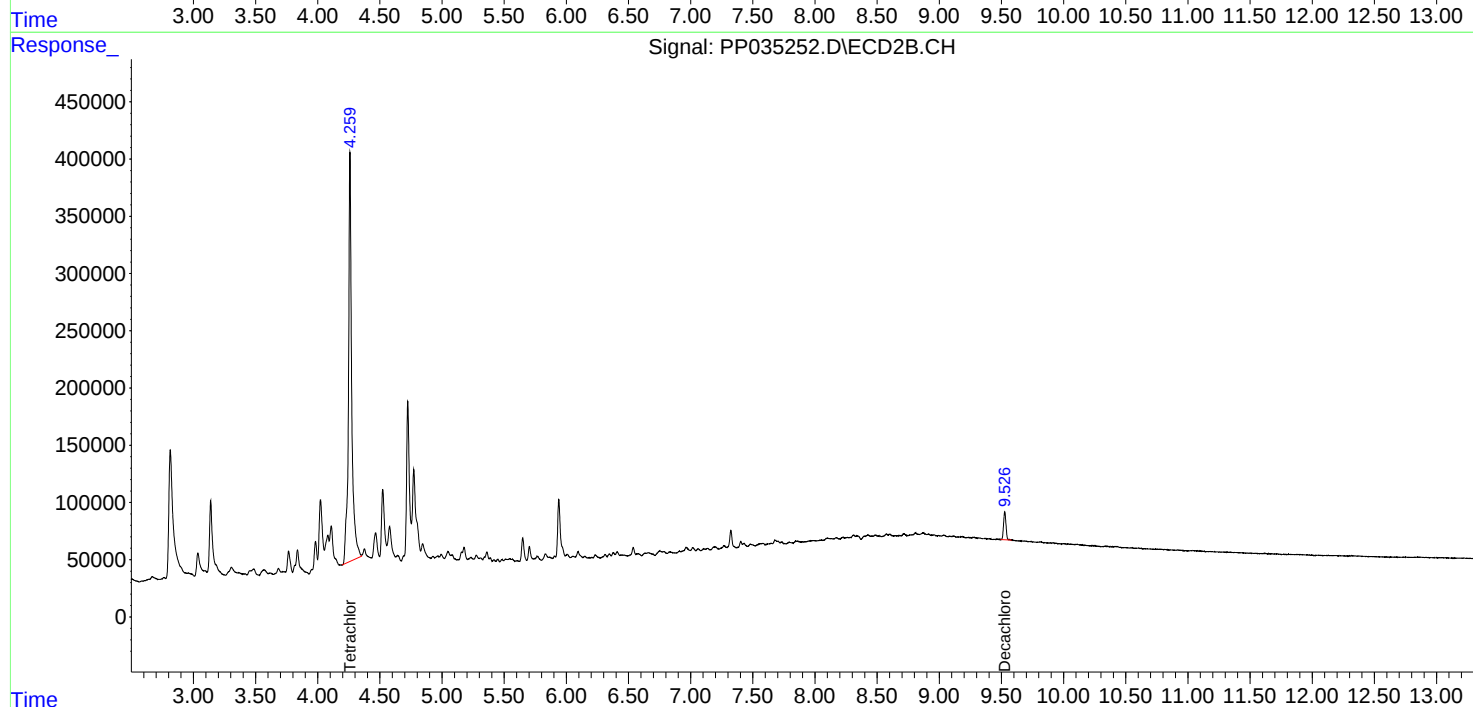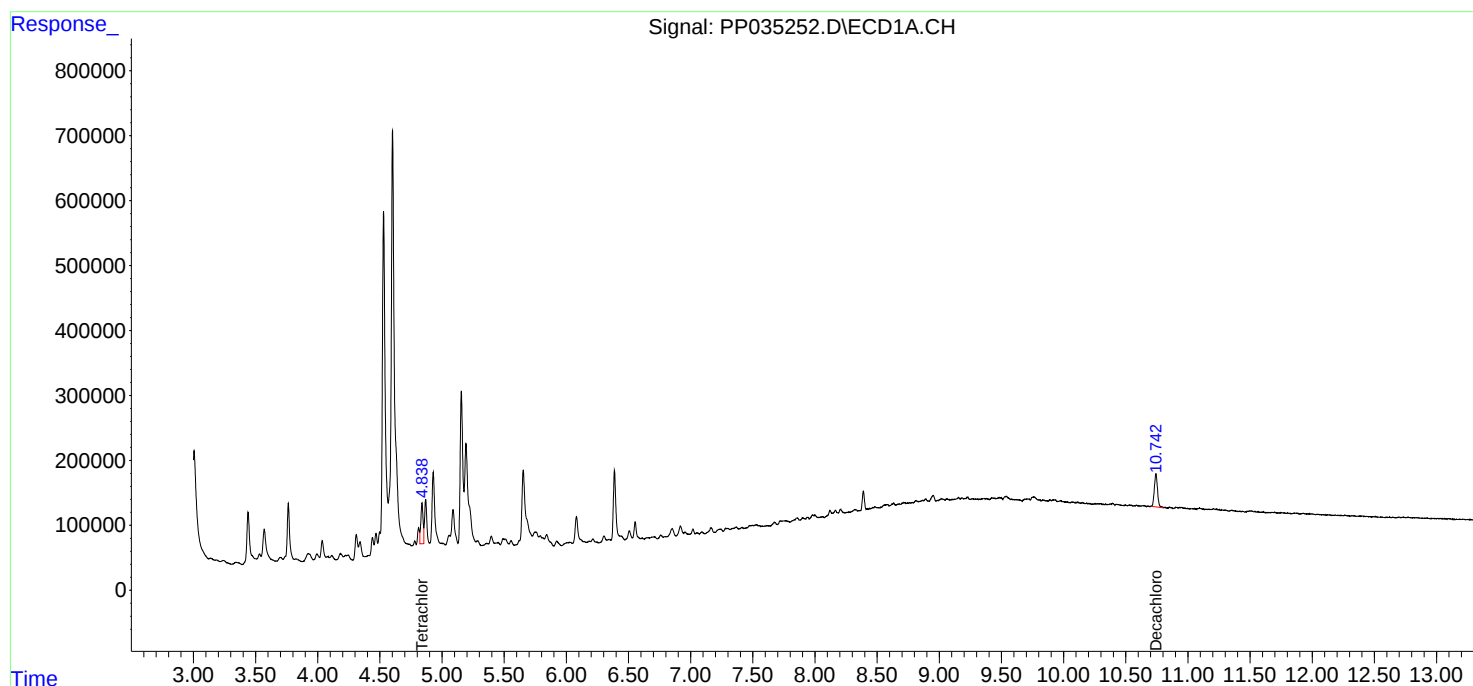

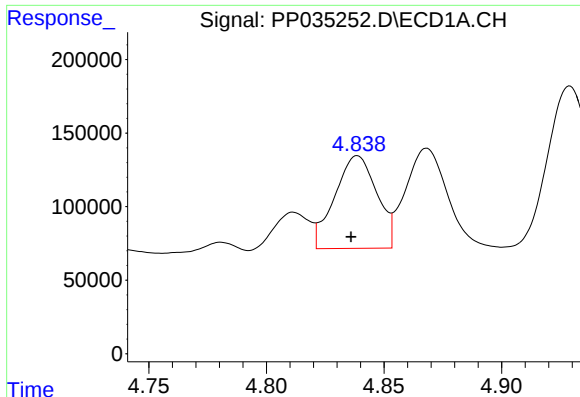


#1 Tetrachloro-m-xylene

R.T.: 4.839 min
Delta R.T.: 0.003 min
Response: 785083
Conc: 9.63 ng/ml

Instrument :
ECD_P
ClientSampleId :
TWP-20


Manual Integrations
APPROVED

Ankita
4/27/2021 10:54:36 AM

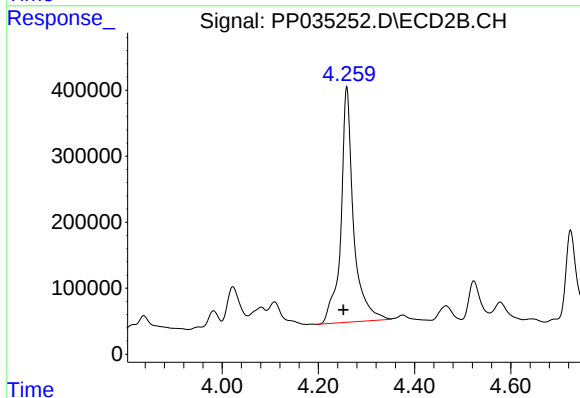


#1 Tetrachloro-m-xylene

R.T.: 4.259 min
Delta R.T.: 0.007 min
Response: 6521314
Conc: 126.64 ng/ml m

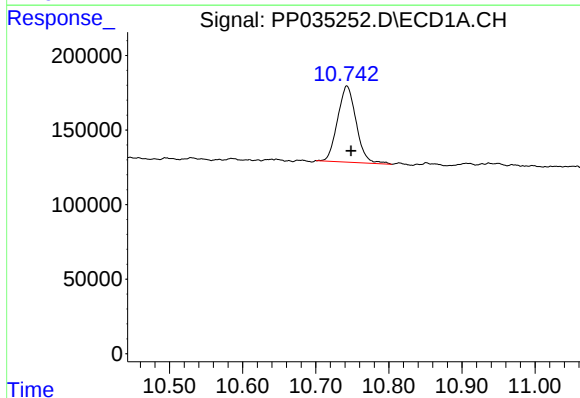

#2 Decachlorobiphenyl

R.T.: 10.743 min
Delta R.T.: -0.006 min
Response: 899276
Conc: 14.23 ng/ml

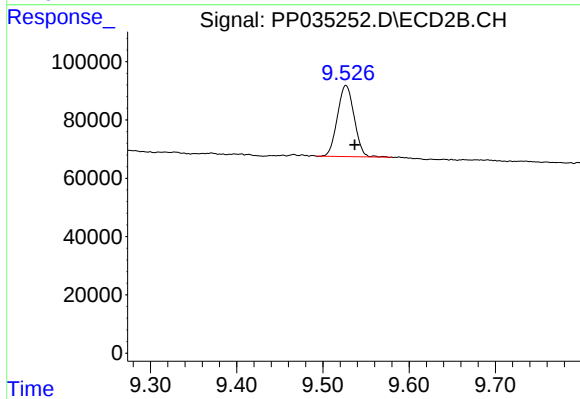

#2 Decachlorobiphenyl

R.T.: 9.527 min
Delta R.T.: -0.010 min
Response: 327352
Conc: 13.78 ng/ml